

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049515.D
 Acq On : 29 Jan 2025 22:11
 Operator : RC/JU
 Sample : Q1184-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2960

Quant Time: Jan 30 07:34:53 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 28 14:45:18 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	214373	20.000	ng/ul	0.00
20) Naphthalene-d8	10.269	136	794748	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.151	164	512108	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	1060423	20.000	ng/ul	0.00
79) Chrysene-d12	21.133	240	1108387	20.000	ng/ul	0.00
88) Perylene-d12	23.915	264	1193102	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	29539	5.105	ng/uL	0.00
4) Pyridine-d5	3.510	84	169626	9.978	ng/ul	0.00
7) Phenol-d5	6.734	99	191821	11.027	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.863	67	410108	34.476	ng/ul	0.00
11) 2-Chlorophenol-d4	7.057	132	458994	34.097	ng/ul	0.00
15) 4-Methylphenol-d8	8.239	113	327021	25.658	ng/ul	0.01
21) Nitrobenzene-d5	8.657	128	225327	37.060	ng/ul	0.00
24) 2-Nitrophenol-d4	9.369	143	264003	39.808	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.922	165	489268	36.152	ng/ul	0.02
31) 4-Chloroaniline-d4	10.422	131	462676	26.652	ng/ul	0.00
46) Dimethylphthalate-d6	13.574	166	1509108	40.191	ng/ul	0.00
49) Acenaphthylene-d8	13.839	160	1658570	37.595	ng/ul	0.00
54) 4-Nitrophenol-d4	14.445	143	41201	6.689	ng/ul	0.06
60) Fluorene-d10	15.151	176	1335797	40.454	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.280	200	226707	33.926	ng/ul	0.00
73) Anthracene-d10	17.004	188	2199052	41.527	ng/ul	0.00
81) Pyrene-d10	19.309	212	2777490	42.866	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	2724179	42.810	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.645	107	189000	16.079	ng/ul#	Qvalue 17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049515.D
Acq On : 29 Jan 2025 22:11
Operator : RC/JU
Sample : Q1184-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2960

Quant Time: Jan 30 07:34:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

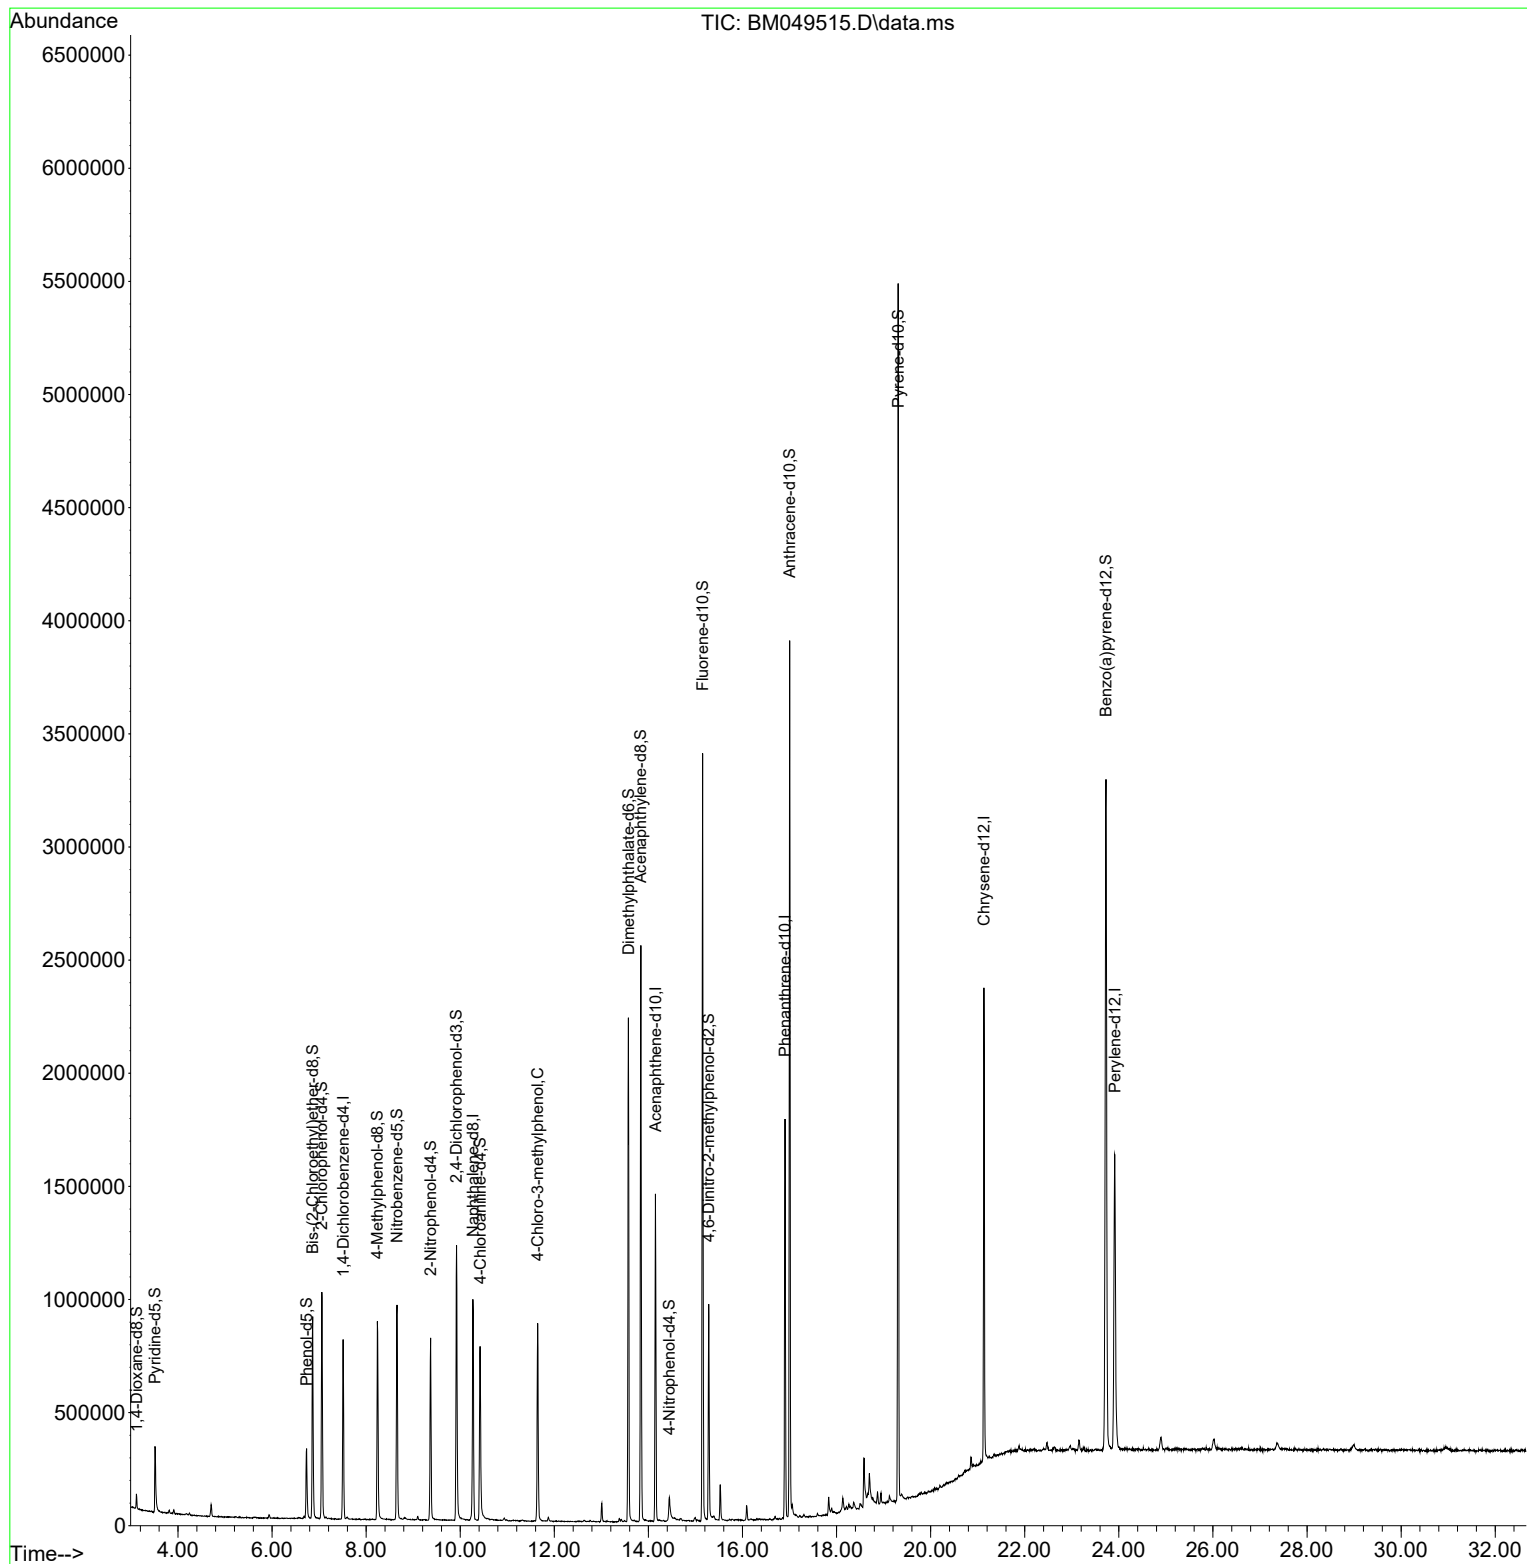

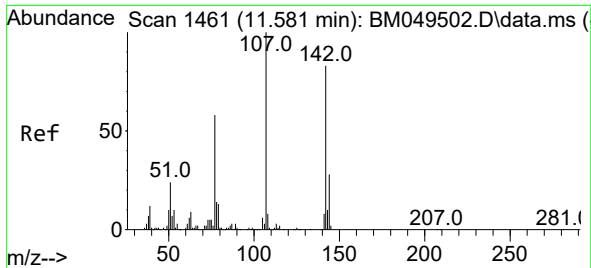

#35
 4-Chloro-3-methylphenol
 Concen: 16.079 ng/ul
 RT: 11.645 min Scan# 14
 Delta R.T. 0.065 min
 Lab File: BM049515.D
 Acq: 29 Jan 2025 22:11

Instrument :
 BNA_M
 ClientSampleId :
 E2960

Tgt Ion:107 Resp: 189000
 Ion Ratio Lower Upper
 107 100
 144 0.0 22.6 34.0#
 142 0.0 67.5 101.3#

