

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049516.D
 Acq On : 29 Jan 2025 22:50
 Operator : RC/JU
 Sample : PB166284BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS284

Quant Time: Jan 30 07:35:03 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 28 14:45:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	191013	20.000	ng/u1	0.00
20) Naphthalene-d8	10.269	136	709465	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.151	164	459247	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.904	188	929566	20.000	ng/u1	0.00
79) Chrysene-d12	21.133	240	949160	20.000	ng/u1	0.00
88) Perylene-d12	23.909	264	1030664	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.122	96	27316	5.299	ng/uL	0.00
4) Pyridine-d5	3.510	84	430171	28.400	ng/u1	0.00
7) Phenol-d5	6.728	99	481023	31.033	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	6.863	67	296619	27.985	ng/u1	0.00
11) 2-Chlorophenol-d4	7.063	132	383030	31.934	ng/u1	0.01
15) 4-Methylphenol-d8	8.245	113	344994	30.379	ng/u1	0.02
21) Nitrobenzene-d5	8.657	128	163277	30.083	ng/u1	0.00
24) 2-Nitrophenol-d4	9.369	143	186390	31.483	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.922	165	379542	31.416	ng/u1	0.02
31) 4-Chloroaniline-d4	10.422	131	387715	25.019	ng/u1	0.00
46) Dimethylphthalate-d6	13.574	166	979250	29.081	ng/u1	0.00
49) Acenaphthylene-d8	13.839	160	1171056	29.600	ng/u1	0.00
54) 4-Nitrophenol-d4	14.427	143	134271	24.308	ng/u1	0.05
60) Fluorene-d10	15.151	176	870311	29.391	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.286	200	166434	28.413	ng/u1	0.00
73) Anthracene-d10	17.004	188	1375584	29.634	ng/u1	0.00
81) Pyrene-d10	19.309	212	1613191	29.073	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.727	264	1683929	30.633	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.152	88	57718	10.654	ng/uL	98
5) Pyridine	3.534	79	447920	28.835	ng/u1	95
6) Benzaldehyde	6.675	77	25236	2.964	ng/u1	98
8) Phenol	6.757	94	506609	31.139	ng/u1	99
10) Bis(2-Chloroethyl)ether	6.951	93	383791	28.928	ng/u1	98
12) 2-Chlorophenol	7.092	128	397606	32.100	ng/u1	98
13) 2-Methylphenol	7.981	108	354606	31.103	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.034	45	595561	29.142	ng/u1	100
16) Acetophenone	8.328	105	552889	29.277	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.316	70	300665	30.357	ng/u1	97
18) 4-Methylphenol	8.304	108	386592	31.417	ng/u1	100
19) Hexachloroethane	8.569	117	158654	29.152	ng/u1	98
22) Nitrobenzene	8.698	77	416929	28.760	ng/u1	98
23) Isophorone	9.222	82	777122	29.978	ng/u1	99
25) 2-Nitrophenol	9.398	139	205860	31.316	ng/u1	98
26) 2,4-Dimethylphenol	9.486	107	369961	30.583	ng/u1	99
27) Bis(2-Chloroethoxy)met...	9.704	93	475806	29.305	ng/u1	98
29) 2,4-Dichlorophenol	9.945	162	381885	31.444	ng/u1	99
30) Naphthalene	10.322	128	1110897	29.410	ng/u1	99
32) 4-Chloroaniline	10.445	127	224610	15.148	ng/u1	98
33) Hexachlorobutadiene	10.610	225	265479	29.161	ng/u1	99
34) Caprolactam	11.227	113	97231	29.023	ng/u1	99
35) 4-Chloro-3-methylphenol	11.604	107	340894	32.488	ng/u1	99
36) 2-Methylnaphthalene	11.939	142	771455	29.946	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049516.D
 Acq On : 29 Jan 2025 22:50
 Operator : RC/JU
 Sample : PB166284BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SLCS284


Quant Time: Jan 30 07:35:03 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 28 14:45:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.163	142	772746	30.427	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.316	216	485656	28.689	ng/ul	99
40) Hexachlorocyclopentadiene	12.298	237	219457	22.098	ng/ul	99
41) 2,4,6-Trichlorophenol	12.580	196	312811	31.333	ng/ul	95
42) 2,4,5-Trichlorophenol	12.669	196	328039	31.264	ng/ul	98
43) 1,1'-Biphenyl	12.974	154	1011829	29.039	ng/ul	99
44) 2-Chloronaphthalene	13.010	162	823918	29.166	ng/ul	99
45) 2-Nitroaniline	13.233	65	221769	31.250	ng/ul	97
47) Dimethylphthalate	13.621	163	980084	29.300	ng/ul	100
48) 2,6-Dinitrotoluene	13.739	165	190379	31.646	ng/ul	99
50) Acenaphthylene	13.868	152	1194232	29.381	ng/ul	100
51) 3-Nitroaniline	14.074	138	179462	30.031	ng/ul	98
52) Acenaphthene	14.216	153	849122	29.261	ng/ul	99
53) 2,4-Dinitrophenol	14.280	184	102003	27.421	ng/ul	92
55) 4-Nitrophenol	14.439	109	121344	30.024	ng/ul	98
56) Dibenzofuran	14.557	168	1216979	29.412	ng/ul	98
57) 2,4-Dinitrotoluene	14.533	165	289980	32.234	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	14.792	232	269232	31.508	ng/ul	97
59) Diethylphthalate	14.998	149	958437	30.183	ng/ul	100
61) Fluorene	15.210	166	1002052	29.970	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.210	204	536651	29.590	ng/ul	95
63) 4-Nitroaniline	15.245	138	179826	32.587	ng/ul	92
66) 4,6-Dinitro-2-methylph...	15.298	198	183837	28.633	ng/ul	97
67) N-Nitrosodiphenylamine	15.427	169	823122	29.705	ng/ul	98
68) 4-Bromophenyl-phenylether	16.104	248	320775	30.221	ng/ul	96
69) Hexachlorobenzene	16.209	284	368640	30.076	ng/ul	97
70) Atrazine	16.392	200	299610	27.469	ng/ul	100
71) Pentachlorophenol	16.568	266	201868	26.156	ng/ul	99
72) Phenanthrene	16.945	178	1549405	29.611	ng/ul	99
74) Anthracene	17.039	178	1579729	29.973	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	12.933	216	470243	27.989	ng/ul	98
76) Pentachlorobenzene	14.474	250	446130	27.770	ng/ul	98
77) Carbazole	17.315	167	1394279	29.599	ng/ul	99
78) Di-n-butylphthalate	17.892	149	1642882	30.535	ng/ul	99
80) Fluoranthene	18.974	202	1877860	29.631	ng/ul	100
82) Pyrene	19.339	202	2024730	29.693	ng/ul	99
83) Butylbenzylphthalate	20.268	149	730581	31.813	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.056	252	583948	32.402	ng/ul	99
85) Benzo(a)anthracene	21.121	228	2025754	30.383	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.068	149	1086131	32.188	ng/ul	100
87) Chrysene	21.174	228	1891736	30.552	ng/ul	99
89) Di-n-octyl phthalate	22.133	149	1828196	28.998	ng/ul	100
90) Benzo(b)fluoranthene	23.044	252	2044221	30.599	ng/ul	99
91) Benzo(k)fluoranthene	23.103	252	2017711	29.889	ng/ul	99
93) Benzo(a)pyrene	23.785	252	1916209	30.576	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.997	276	2470008	31.798	ng/ul	99
95) Dibenzo(a,h)anthracene	27.050	278	2015205	32.016	ng/ul	99
96) Benzo(g,h,i)perylene	27.956	276	1912410	32.380	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 30 07:35:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration




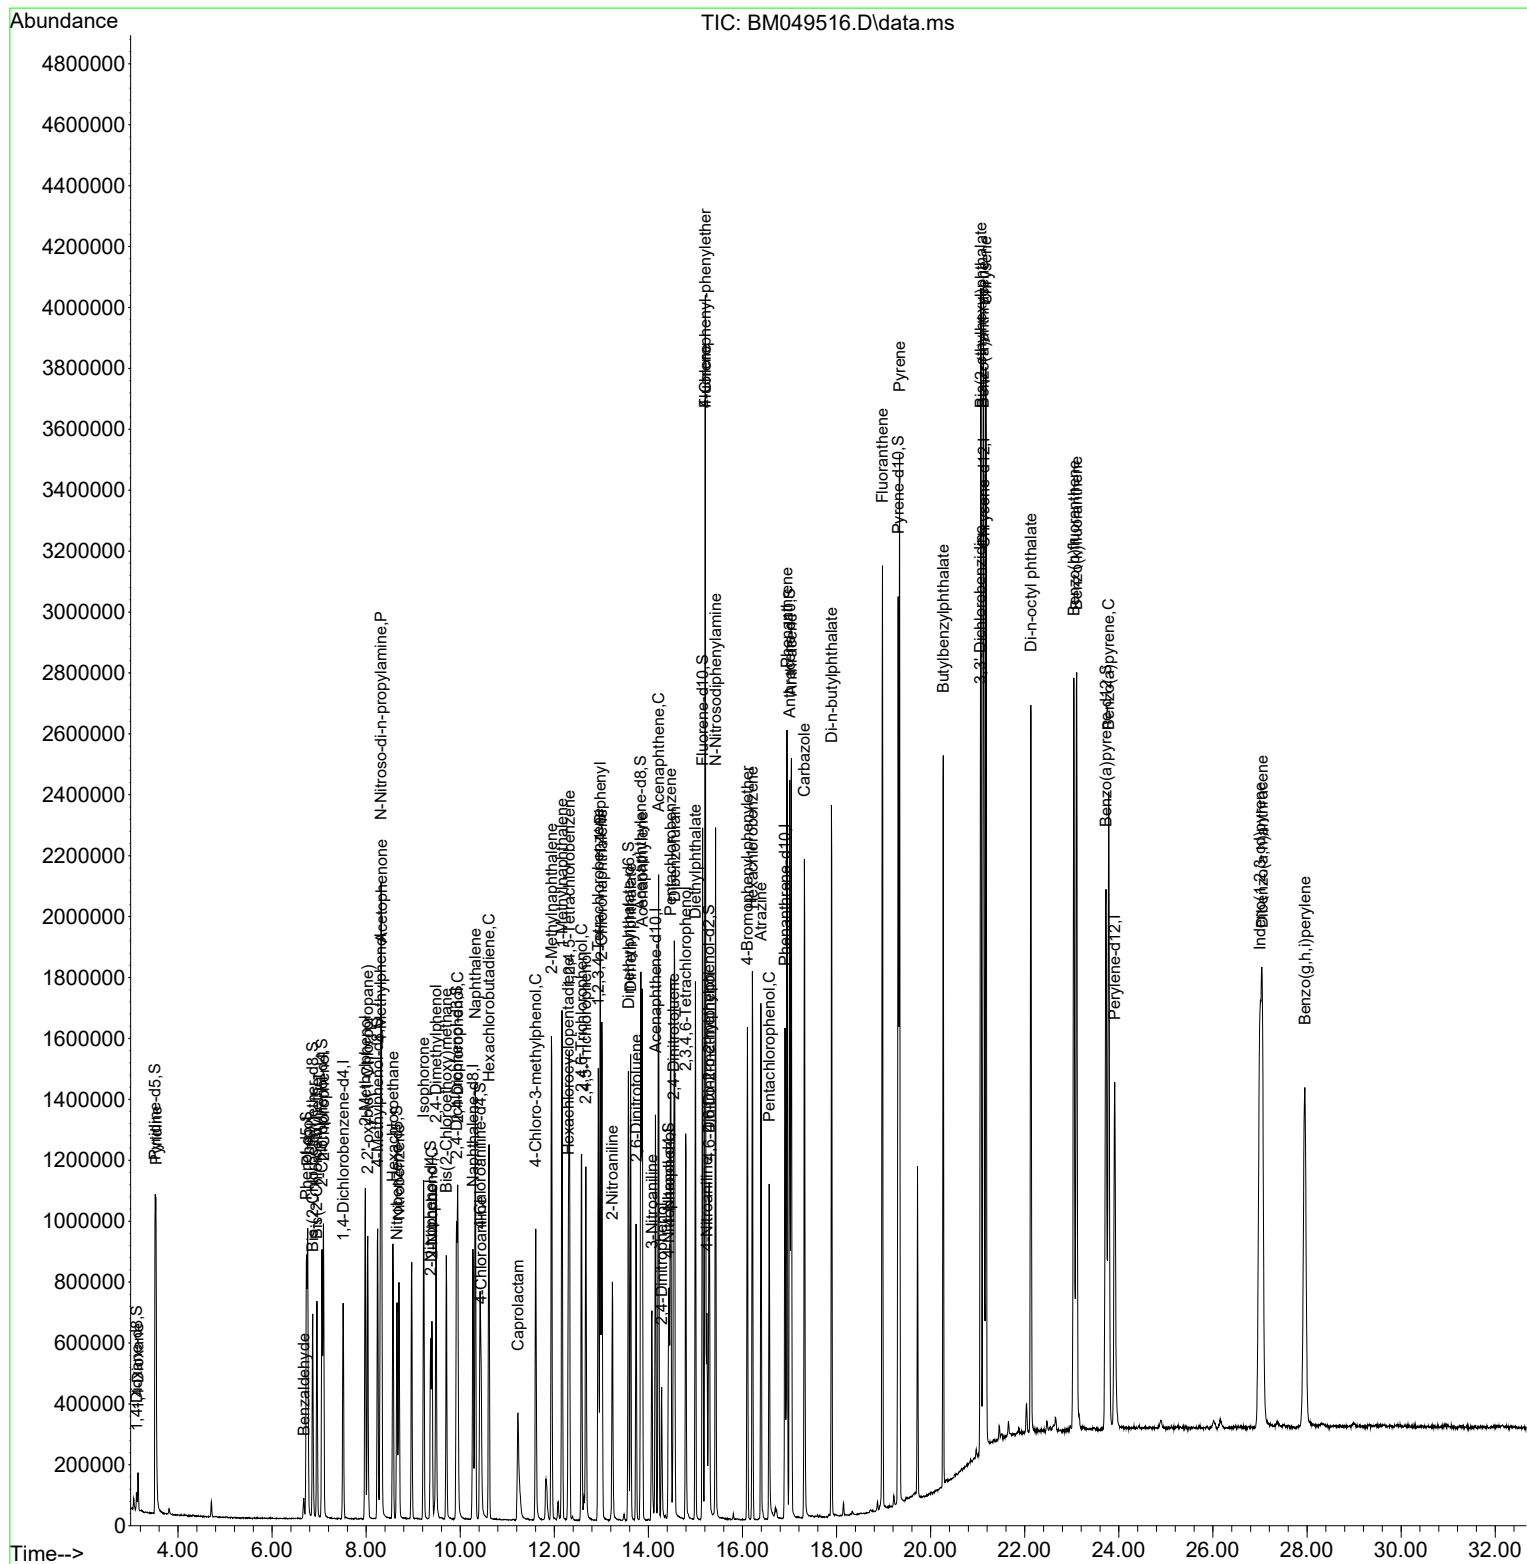




#2
1,4-Dioxane
Concen: 10.654 ng/uL
RT: 3.152 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion: 88 Resp: 57718
Ion Ratio Lower Upper
88 100
43 31.7 23.4 35.0
58 72.6 57.3 85.9



#5
Pyridine
Concen: 28.835 ng/uL
RT: 3.534 min Scan# 93
Delta R.T. 0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion: 79 Resp: 447920
Ion Ratio Lower Upper
79 100
52 71.6 60.7 91.1
51 33.5 29.3 43.9







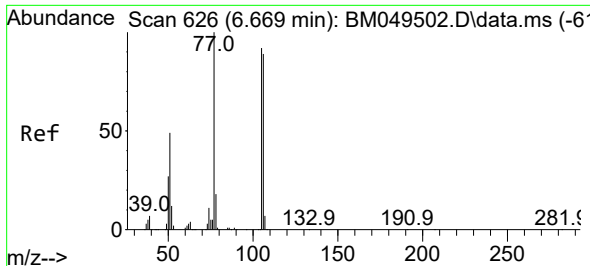

#6
Benzaldehyde
Concen: 2.964 ng/ul
RT: 6.675 min Scan# 61
Delta R.T. 0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion: 77 Resp: 25236
Ion Ratio Lower Upper
77 100
105 95.6 74.2 111.4
106 92.0 72.7 109.1

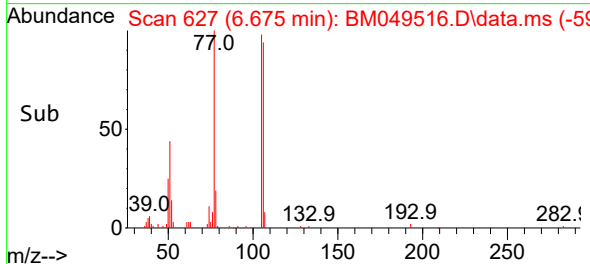

#8
Phenol
Concen: 31.139 ng/ul
RT: 6.757 min Scan# 641
Delta R.T. 0.023 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion: 94 Resp: 506609
Ion Ratio Lower Upper
94 100
65 27.9 23.4 35.0
66 34.5 27.8 41.8


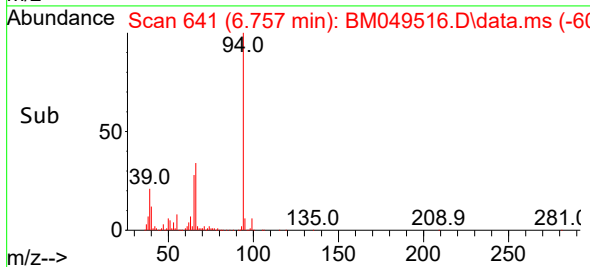

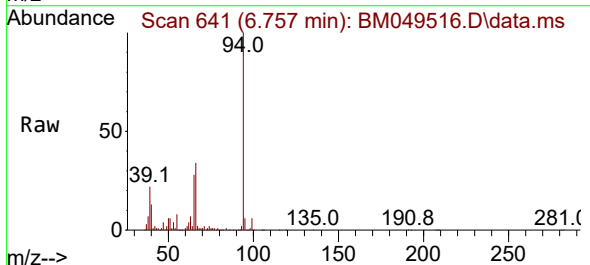




#10
Bis(2-Chloroethyl)ether
Concen: 28.928 ng/ul
RT: 6.951 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion: 93 Resp: 383791
Ion Ratio Lower Upper
93 100
63 80.6 66.3 99.5
95 31.8 25.0 37.6



#12
2-Chlorophenol
Concen: 32.100 ng/ul
RT: 7.092 min Scan# 698
Delta R.T. 0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:128 Resp: 397606
Ion Ratio Lower Upper
128 100
64 48.9 40.3 60.5
130 33.2 26.2 39.4









#13
2-Methylphenol
Concen: 31.103 ng/ul
RT: 7.981 min Scan# 845
Delta R.T. 0.017 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:108 Resp: 354606
Ion Ratio Lower Upper
108 100
107 85.9 69.7 104.5



#14
2,2'-oxybis(1-Chloropropane)
Concen: 29.142 ng/ul
RT: 8.034 min Scan# 858
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion: 45 Resp: 595561
Ion Ratio Lower Upper
45 100
77 13.2 10.6 15.8
79 10.1 7.8 11.6









#16
Acetophenone
Concen: 29.277 ng/ul
RT: 8.328 min Scan# 907
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:105 Resp: 552889
Ion Ratio Lower Upper
105 100
77 83.5 64.6 97.0
51 27.7 23.3 34.9



#17
N-Nitroso-di-n-propylamine
Concen: 30.357 ng/ul
RT: 8.316 min Scan# 906
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion: 70 Resp: 300665
Ion Ratio Lower Upper
70 100
42 55.8 47.0 70.6
101 9.0 7.2 10.8
130 18.9 14.6 21.8









#18
4-Methylphenol
Concen: 31.417 ng/ul
RT: 8.304 min Scan# 901
Delta R.T. 0.017 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:108 Resp: 386592
Ion Ratio Lower Upper
108 100
107 112.7 90.0 135.0



#19
Hexachloroethane
Concen: 29.152 ng/ul
RT: 8.569 min Scan# 949
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:117 Resp: 158654
Ion Ratio Lower Upper
117 100
201 117.5 94.9 142.3
199 75.6 57.3 85.9





#22

Nitrobenzene

Concen: 28.760 ng/ul

RT: 8.698 min Scan# 91

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion: 77 Resp: 416929

Ion Ratio Lower Upper

77 100

123 44.4 33.9 50.9

65 13.3 10.6 16.0



#23

Isophorone

Concen: 29.978 ng/ul

RT: 9.222 min Scan# 1060

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion: 82 Resp: 777122


Ion Ratio Lower Upper

82 100

95 6.2 5.1 7.7

138 17.1 13.3 19.9



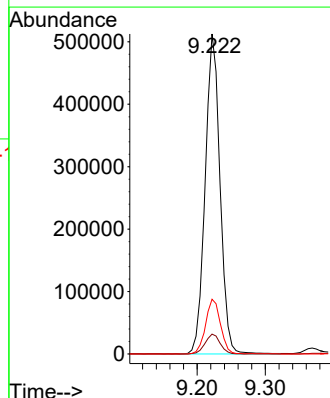





#25
2-Nitrophenol
Concen: 31.316 ng/ul
RT: 9.398 min Scan# 1105
Delta R.T. -0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:139 Resp: 205860
Ion Ratio Lower Upper
139 100
65 52.3 40.6 60.8
109 25.0 20.7 31.1

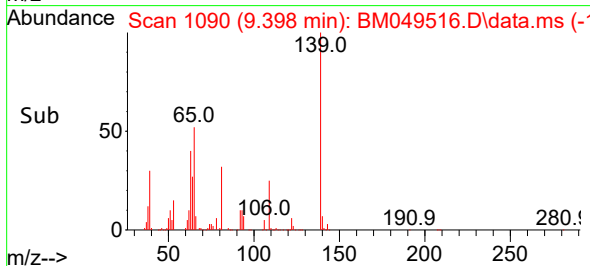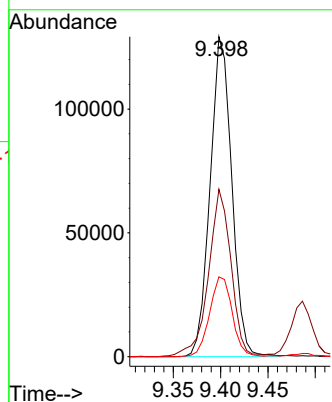

#26
2,4-Dimethylphenol
Concen: 30.583 ng/ul
RT: 9.486 min Scan# 1105
Delta R.T. 0.012 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:107 Resp: 369961
Ion Ratio Lower Upper
107 100
121 49.5 39.6 59.4
122 87.5 68.7 103.1


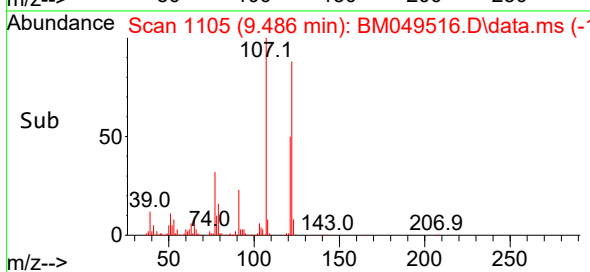
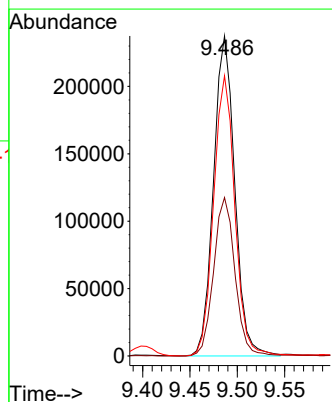
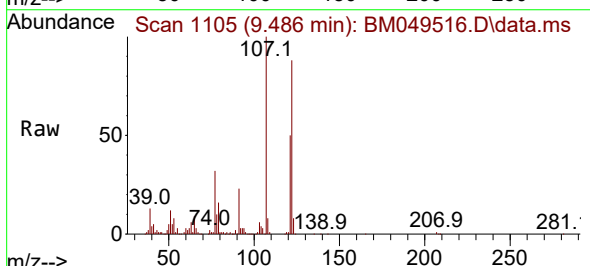


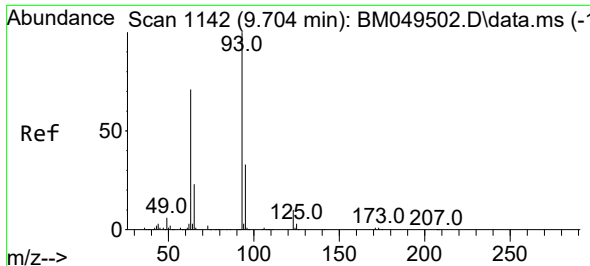

#27
 Bis(2-Chloroethoxy)methane
 Concen: 29.305 ng/ul
 RT: 9.704 min Scan# 1142
 Delta R.T. -0.000 min
 Lab File: BM049516.D
 Acq: 29 Jan 2025 22:50




Instrument :
 BNA_M
 ClientSampleId :
 SLCS284


Tgt Ion: 93 Resp: 475806
 Ion Ratio Lower Upper
 93 100
 95 32.4 25.0 37.6
 123 10.8 8.6 13.0

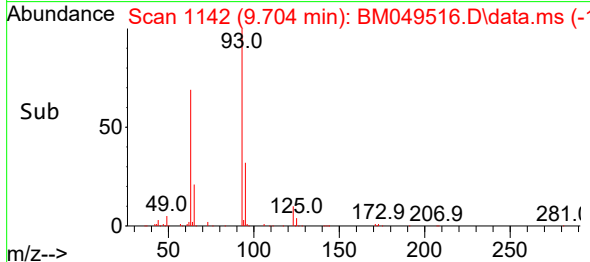

#29
 2,4-Dichlorophenol
 Concen: 31.444 ng/ul
 RT: 9.945 min Scan# 1183
 Delta R.T. 0.012 min
 Lab File: BM049516.D
 Acq: 29 Jan 2025 22:50

Tgt Ion: 162 Resp: 381885
 Ion Ratio Lower Upper
 162 100
 164 65.9 53.7 80.5
 98 33.4 27.2 40.8

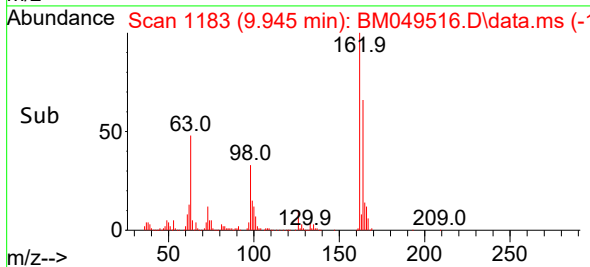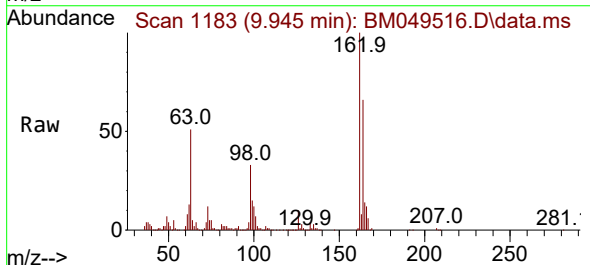



#30

Naphthalene

Concen: 29.410 ng/ul

RT: 10.322 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:128 Resp: 1110897

Ion Ratio Lower Upper

128 100

129 10.9 8.8 13.2

127 12.7 10.6 15.8



#32

4-Chloroaniline

Concen: 15.148 ng/ul

RT: 10.445 min Scan# 1268

Delta R.T. -0.000 min

Lab File: BM049516.D




Acq: 29 Jan 2025 22:50


Tgt Ion:127 Resp: 224610

Ion Ratio Lower Upper

127 100

129 33.0 25.4 38.2









#33
Hexachlorobutadiene
Concen: 29.161 ng/ul
RT: 10.610 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:225 Resp: 265479
Ion Ratio Lower Upper
225 100
223 63.6 50.1 75.1
227 64.0 50.2 75.4



#34
Caprolactam
Concen: 29.023 ng/ul
RT: 11.227 min Scan# 1401
Delta R.T. 0.012 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:113 Resp: 97231
Ion Ratio Lower Upper
113 100
55 179.5 146.0 219.0
56 135.1 107.8 161.8









#35
4-Chloro-3-methylphenol
Concen: 32.488 ng/ul
RT: 11.604 min Scan# 1465
Delta R.T. 0.023 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:107 Resp: 340894
Ion Ratio Lower Upper
107 100
144 27.7 22.6 34.0
142 85.6 67.5 101.3

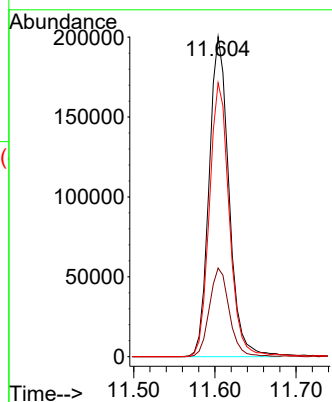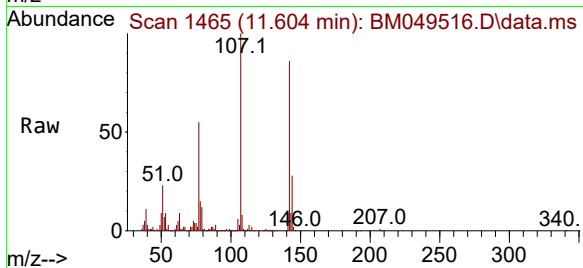

#36
2-Methylnaphthalene
Concen: 29.946 ng/ul
RT: 11.939 min Scan# 1522
Delta R.T. -0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:142 Resp: 771455
Ion Ratio Lower Upper
142 100
141 86.2 70.4 105.6

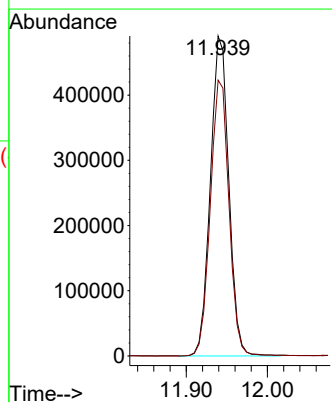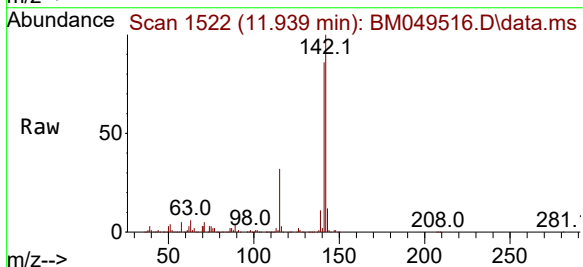



#37

1-Methylnaphthalene

Concen: 30.427 ng/ul

RT: 12.163 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:142 Resp: 772746

Ion Ratio Lower Upper

142 100

141 89.7 72.8 109.2

116 3.5 3.0 4.6

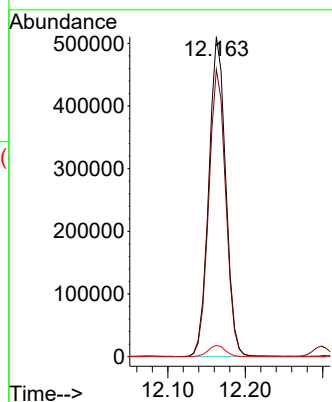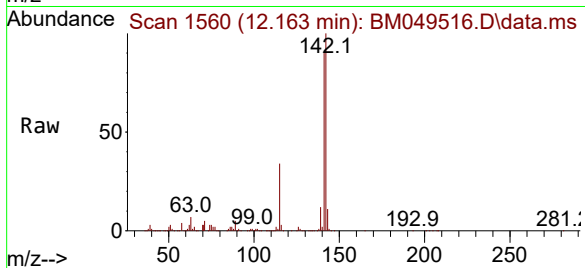

#39

1,2,4,5-Tetrachlorobenzene

Concen: 28.689 ng/ul

RT: 12.316 min Scan# 1586

Delta R.T. -0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Tgt Ion:216 Resp: 485656




Ion Ratio Lower Upper


216 100

214 78.1 61.7 92.5

179 20.0 15.4 23.2

108 14.0 11.2 16.8


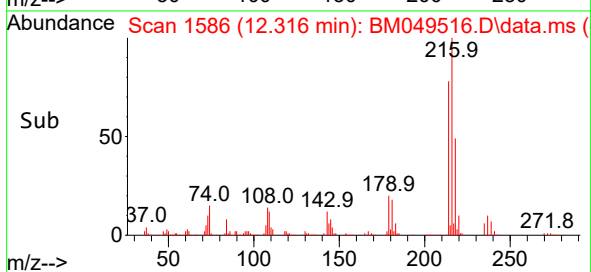

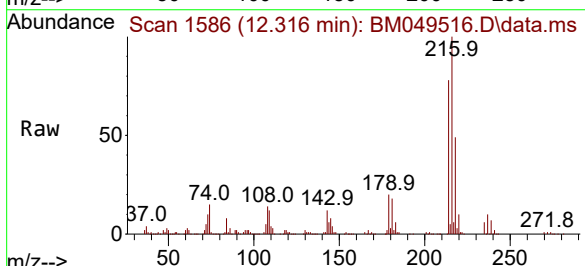




#40
Hexachlorocyclopentadiene
Concen: 22.098 ng/ul
RT: 12.298 min Scan# 1583
Delta R.T. -0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:237 Resp: 219457
Ion Ratio Lower Upper
237 100
235 63.4 50.1 75.1
272 12.5 10.6 15.8



#41
2,4,6-Trichlorophenol
Concen: 31.333 ng/ul
RT: 12.580 min Scan# 1631
Delta R.T. 0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:196 Resp: 312811
Ion Ratio Lower Upper
196 100
198 98.5 74.9 112.3
200 32.7 24.3 36.5





#42

2,4,5-Trichlorophenol

Concen: 31.264 ng/ul

RT: 12.669 min Scan# 1

Delta R.T. 0.023 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:196 Resp: 328039

Ion Ratio Lower Upper

196 100

198 96.2 79.4 119.0

200 31.0 25.1 37.7



#43

1,1'-Biphenyl

Concen: 29.039 ng/ul

RT: 12.974 min Scan# 1698

Delta R.T. -0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion:154 Resp: 1011829


Ion Ratio Lower Upper

154 100

153 39.0 31.7 47.5

76 12.3 9.8 14.8





#44

2-Chloronaphthalene

Concen: 29.166 ng/ul

RT: 13.010 min Scan# 11

Delta R.T. -0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:162 Resp: 823918

Ion Ratio Lower Upper

162 100

164 32.6 26.5 39.7

127 33.9 26.8 40.2

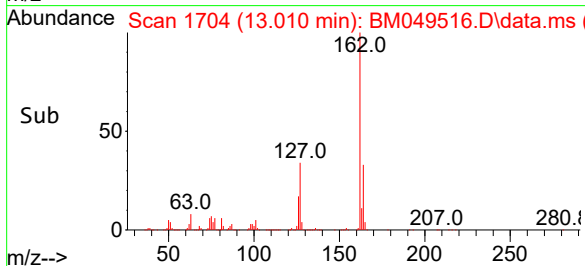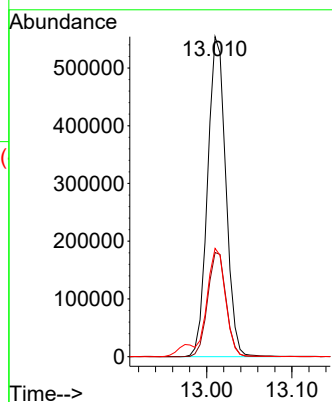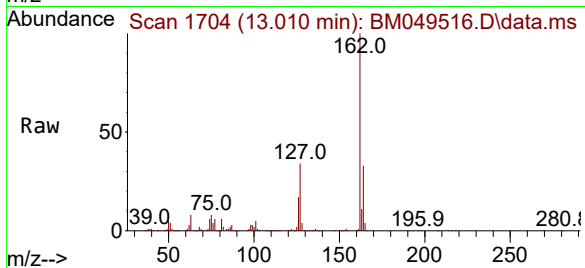

#45

2-Nitroaniline

Concen: 31.250 ng/ul

RT: 13.233 min Scan# 1742

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion: 65 Resp: 221769


Ion Ratio Lower Upper

65 100

92 67.5 52.6 79.0

138 102.5 79.6 119.4


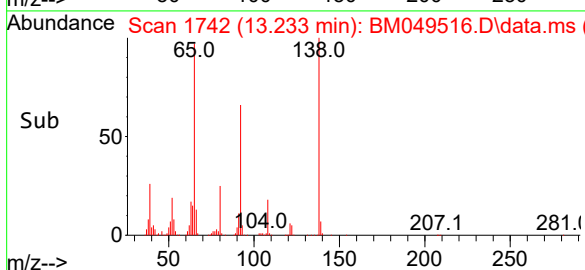

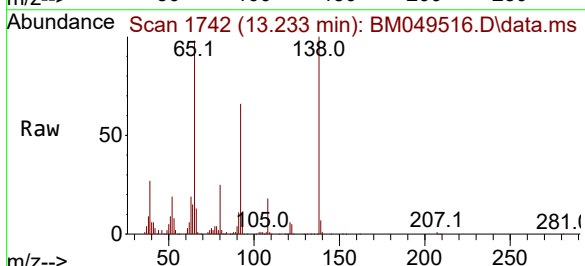


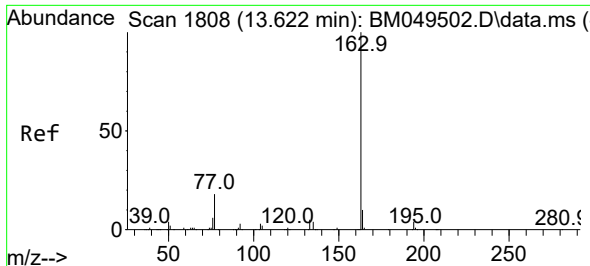

#47
Dimethylphthalate
Concen: 29.300 ng/ul
RT: 13.621 min Scan# 1808
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:163 Resp: 980084
Ion Ratio Lower Upper
163 100
194 4.3 3.3 4.9
164 10.0 8.0 12.0

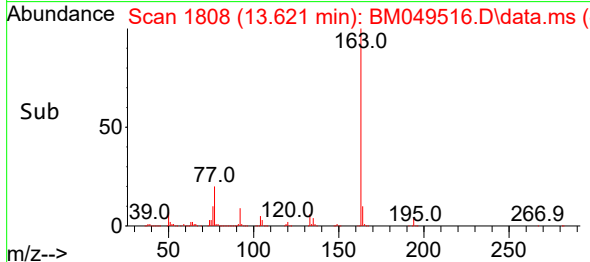

#48
2,6-Dinitrotoluene
Concen: 31.646 ng/ul
RT: 13.739 min Scan# 1828
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:165 Resp: 190379
Ion Ratio Lower Upper
165 100
89 55.1 44.5 66.7
121 19.6 16.3 24.5


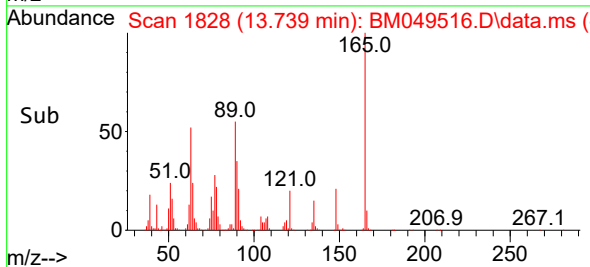

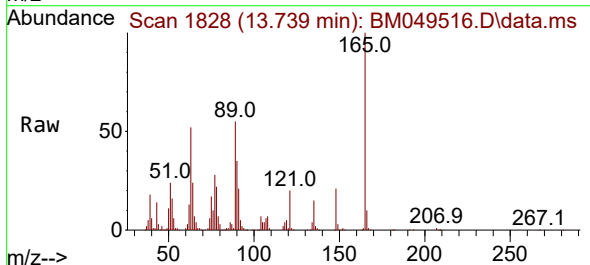




#50
Acenaphthylene
Concen: 29.381 ng/ul
RT: 13.868 min Scan# 1850
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:152 Resp: 1194232
Ion Ratio Lower Upper
152 100
151 20.1 16.0 24.0
153 13.0 10.4 15.6



#51
3-Nitroaniline
Concen: 30.031 ng/ul
RT: 14.074 min Scan# 1885
Delta R.T. 0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:138 Resp: 179462
Ion Ratio Lower Upper
138 100
108 10.6 9.0 13.6
92 114.3 93.7 140.5





#52

Acenaphthene

Concen: 29.261 ng/ul

RT: 14.216 min Scan# 1909

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:153 Resp: 849122

Ion Ratio Lower Upper

153 100

152 49.3 39.0 58.4

154 88.6 71.5 107.3

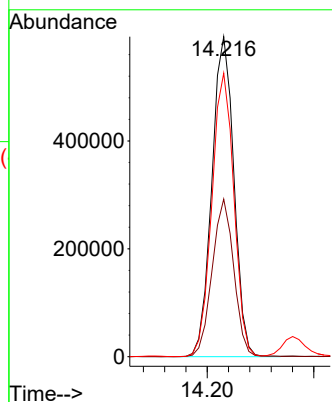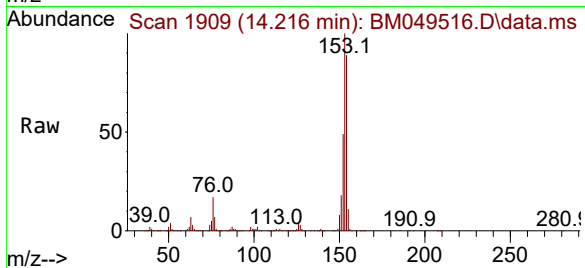

#53

2,4-Dinitrophenol

Concen: 27.421 ng/ul

RT: 14.280 min Scan# 1920

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion:184 Resp: 102003


Ion Ratio Lower Upper

184 100

63 57.3 51.0 76.6

154 56.2 49.8 74.6




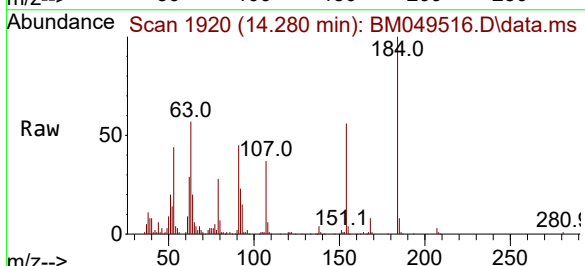




#55
4-Nitrophenol
Concen: 30.024 ng/ul
RT: 14.439 min Scan# 1939
Delta R.T. 0.047 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:109 Resp: 121344
Ion Ratio Lower Upper
109 100
139 144.9 115.4 173.2
65 153.5 118.6 178.0

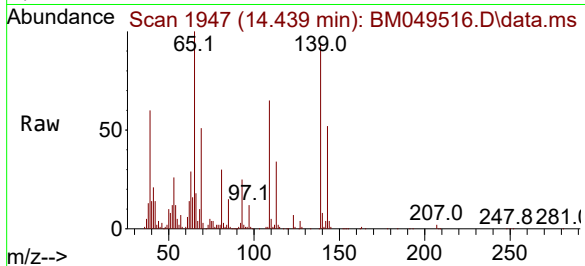

#56
Dibenzofuran
Concen: 29.412 ng/ul
RT: 14.557 min Scan# 1967
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:168 Resp: 1216979
Ion Ratio Lower Upper
168 100
139 33.1 27.4 41.0




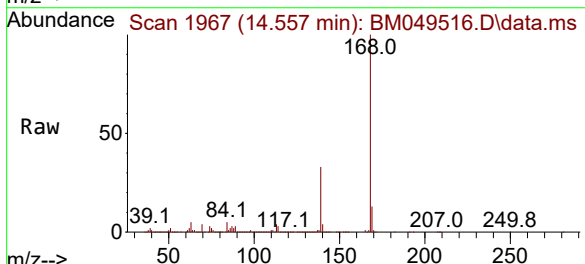




#57
2,4-Dinitrotoluene
Concen: 32.234 ng/ul
RT: 14.533 min Scan# 1963
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:165 Resp: 289980
Ion Ratio Lower Upper
165 100
63 41.1 35.5 53.3
182 2.6 1.9 2.9

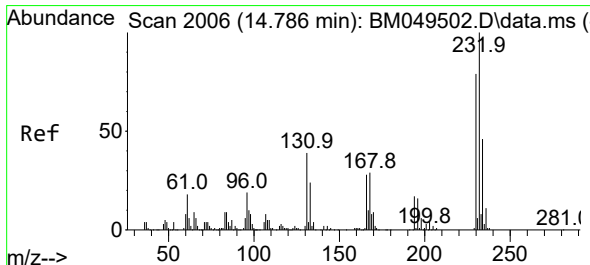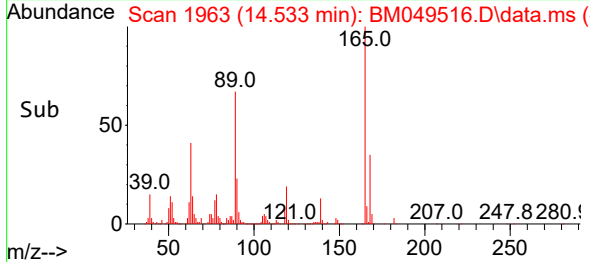

#58
2,3,4,6-Tetrachlorophenol
Concen: 31.508 ng/ul
RT: 14.792 min Scan# 2007
Delta R.T. 0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:232 Resp: 269232
Ion Ratio Lower Upper
232 100
131 38.4 32.8 49.2
130 2.2 1.5 2.3
166 29.1 24.3 36.5

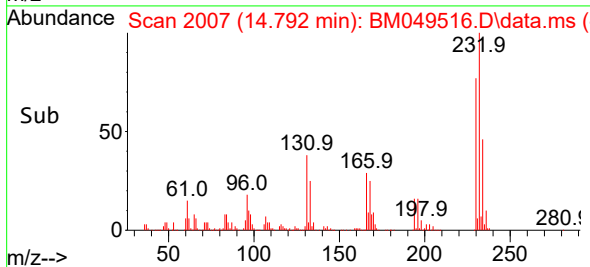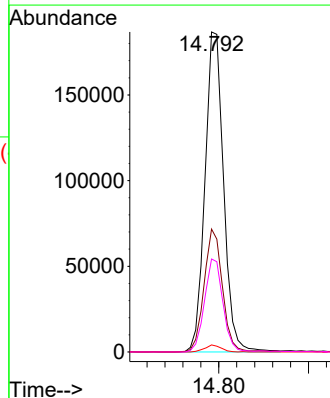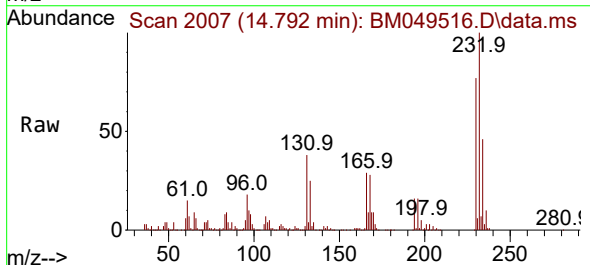



#59

Diethylphthalate

Concen: 30.183 ng/ul

RT: 14.998 min Scan# 2042

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:149 Resp: 958437

Ion Ratio Lower Upper

149 100

177 23.0 18.3 27.5

150 12.2 9.9 14.9

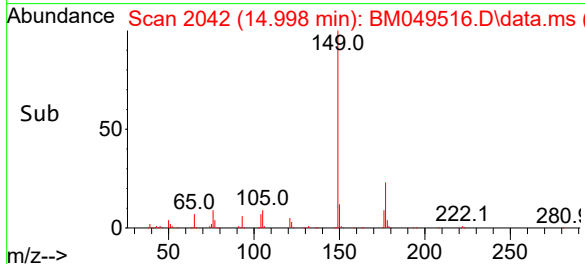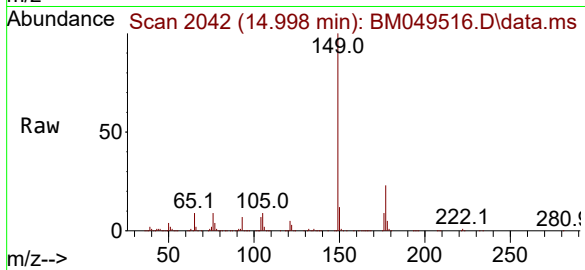

#61

Fluorene

Concen: 29.970 ng/ul

RT: 15.210 min Scan# 2078

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion:166 Resp: 1002052


Ion Ratio Lower Upper

166 100

165 96.8 78.5 117.7

167 13.5 10.7 16.1


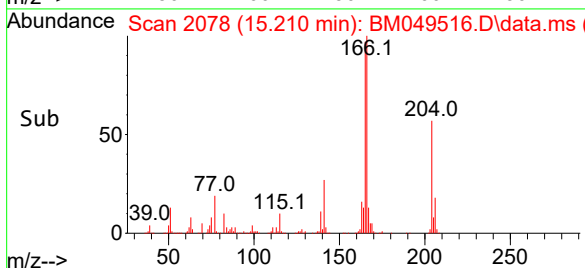

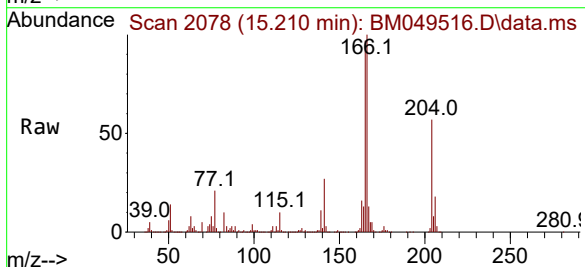




#62
4-Chlorophenyl-phenylether
Concen: 29.590 ng/ul
RT: 15.210 min Scan# 2078
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:204 Resp: 536651
Ion Ratio Lower Upper
204 100
206 32.2 27.0 40.6
141 46.8 41.2 61.8

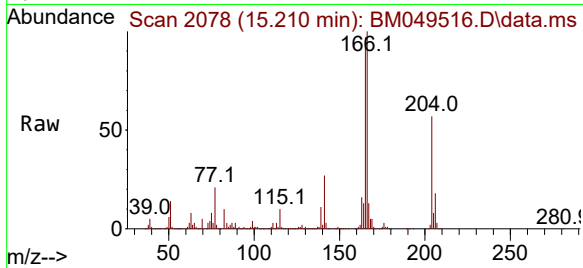

#63
4-Nitroaniline
Concen: 32.587 ng/ul
RT: 15.245 min Scan# 2084
Delta R.T. 0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:138 Resp: 179826
Ion Ratio Lower Upper
138 100
92 49.2 42.7 64.1
108 70.9 63.9 95.9




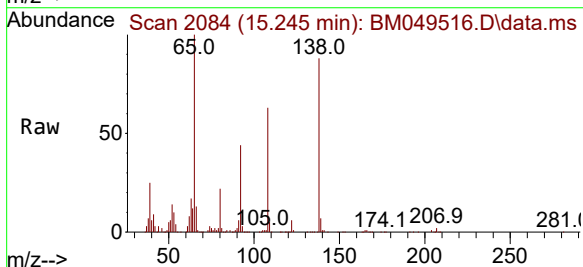




#66
4,6-Dinitro-2-methylphenol
Concen: 28.633 ng/ul
RT: 15.298 min Scan# 2092
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:198 Resp: 183837
Ion Ratio Lower Upper
198 100
182 4.7 4.2 6.4
77 20.5 17.7 26.5



#67
N-Nitrosodiphenylamine
Concen: 29.705 ng/ul
RT: 15.427 min Scan# 2115
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:169 Resp: 823122
Ion Ratio Lower Upper
169 100
168 66.9 55.1 82.7
167 36.9 29.9 44.9









#68
4-Bromophenyl-phenylether
Concen: 30.221 ng/ul
RT: 16.104 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:248 Resp: 320775
Ion Ratio Lower Upper
248 100
250 97.8 75.9 113.9
141 58.3 43.8 65.8

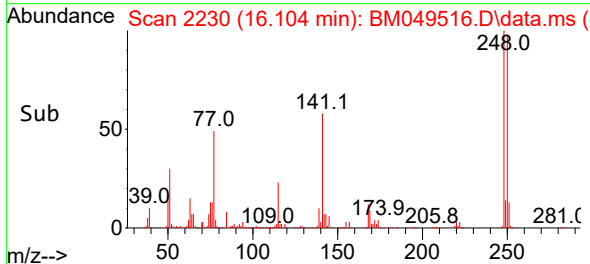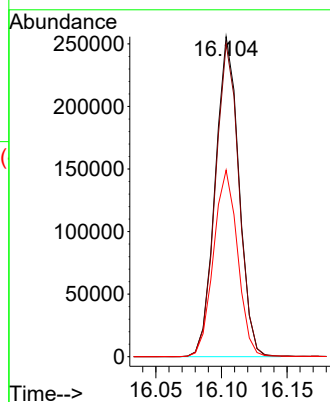

#69
Hexachlorobenzene
Concen: 30.076 ng/ul
RT: 16.209 min Scan# 2248
Delta R.T. -0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:284 Resp: 368640
Ion Ratio Lower Upper
284 100
142 32.1 24.4 36.6
249 31.0 23.4 35.2

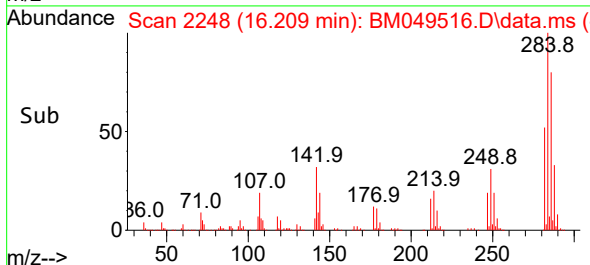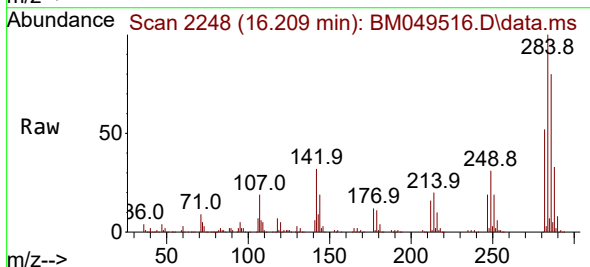



#70

Atrazine

Concen: 27.469 ng/ul

RT: 16.392 min Scan# 21

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:200 Resp: 299610

Ion Ratio Lower Upper

200 100

173 24.8 19.8 29.8

215 48.5 38.7 58.1



#71

Pentachlorophenol

Concen: 26.156 ng/ul

RT: 16.568 min Scan# 2309

Delta R.T. 0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion:266 Resp: 201868


Ion Ratio Lower Upper

266 100

264 62.6 50.5 75.7

268 64.6 52.0 78.0









#72
Phenanthrene
Concen: 29.611 ng/ul
RT: 16.945 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:178 Resp: 1549405
Ion Ratio Lower Upper
178 100
179 15.8 12.4 18.6
176 19.9 15.6 23.4

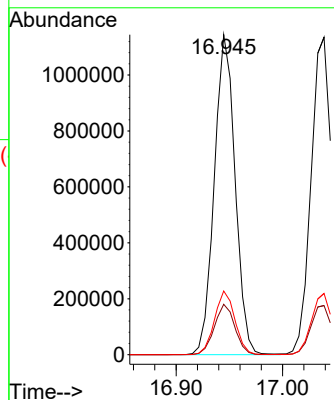

#74
Anthracene
Concen: 29.973 ng/ul
RT: 17.039 min Scan# 2389
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:178 Resp: 1579729
Ion Ratio Lower Upper
178 100
179 15.5 12.2 18.4
176 19.3 15.0 22.4

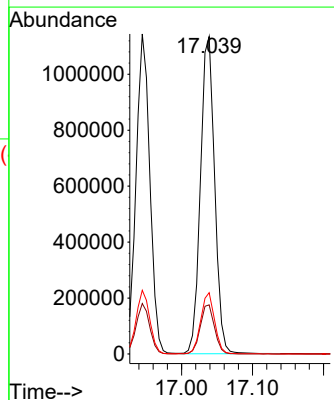



#75

1,2,3,4-Tetrachlorobenzene

Concen: 27.989 ng/uL

RT: 12.933 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:216 Resp: 470243

Ion Ratio Lower Upper

216 100

214 80.3 62.5 93.7

218 48.2 38.4 57.6

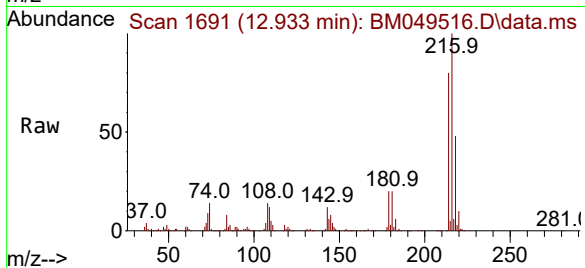

#76

Pentachlorobenzene

Concen: 27.770 ng/uL

RT: 14.474 min Scan# 1953

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion:250 Resp: 446130


Ion Ratio Lower Upper

250 100

248 62.0 50.8 76.2

252 62.4 51.7 77.5




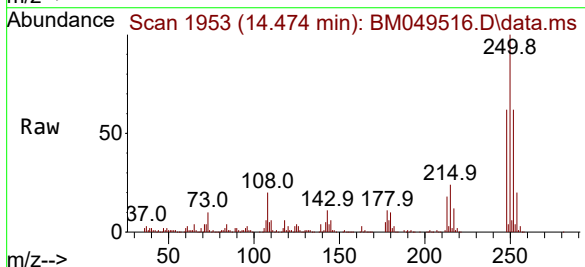


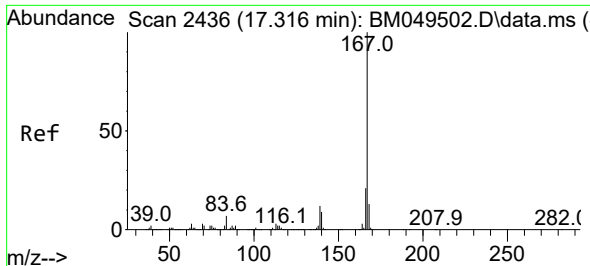

#77
 Carbazole
 Concen: 29.599 ng/ul
 RT: 17.315 min Scan# 2436
 Delta R.T. -0.000 min
 Lab File: BM049516.D
 Acq: 29 Jan 2025 22:50




Instrument :
 BNA_M
 ClientSampleId :
 SLCS284


Tgt Ion:167 Resp: 1394279
 Ion Ratio Lower Upper
 167 100
 166 21.1 17.2 25.8
 139 11.8 9.3 13.9

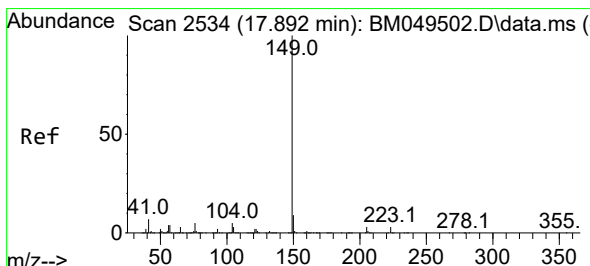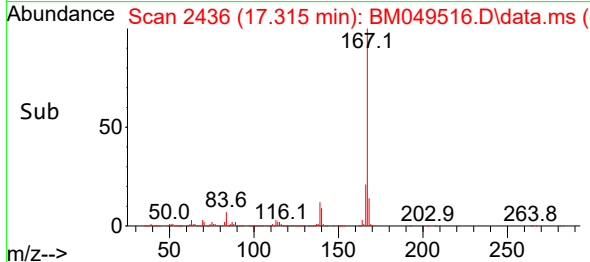

#78
 Di-n-butylphthalate
 Concen: 30.535 ng/ul
 RT: 17.892 min Scan# 2534
 Delta R.T. -0.006 min
 Lab File: BM049516.D
 Acq: 29 Jan 2025 22:50

Tgt Ion:149 Resp: 1642882
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.2 10.8
 104 4.7 3.8 5.6


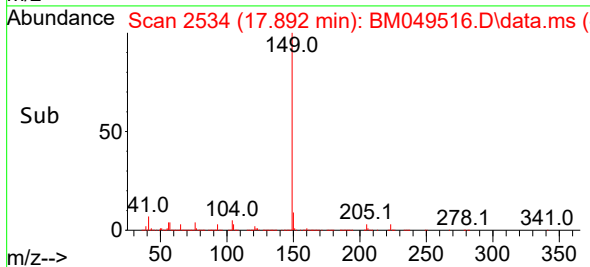

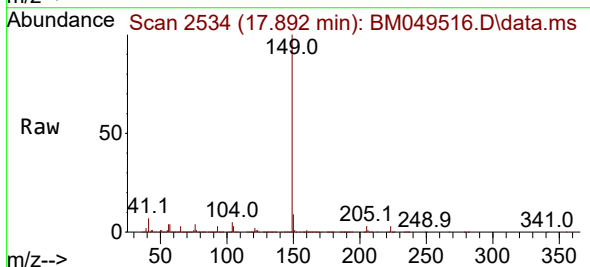




#80
Fluoranthene
Concen: 29.631 ng/ul
RT: 18.974 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:202 Resp: 1877860
Ion Ratio Lower Upper
202 100
101 8.5 6.9 10.3
100 6.4 5.1 7.7



#82
Pyrene
Concen: 29.693 ng/ul
RT: 19.339 min Scan# 2780
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:202 Resp: 2024730
Ion Ratio Lower Upper
202 100
101 10.1 8.3 12.5
100 8.0 6.6 9.8





#83

Butylbenzylphthalate

Concen: 31.813 ng/ul

RT: 20.268 min Scan# 2938

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:149 Resp: 730581

Ion Ratio Lower Upper

149 100

91 66.2 55.3 82.9

206 23.1 17.8 26.8

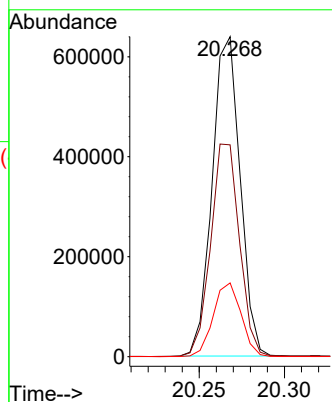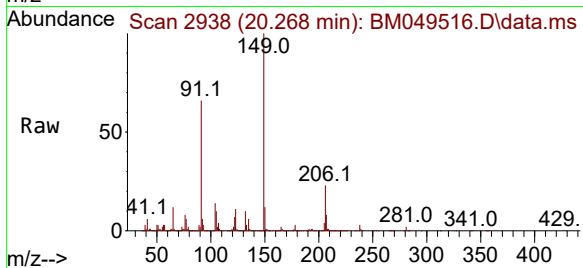

#84

3,3'-Dichlorobenzidine

Concen: 32.402 ng/ul

RT: 21.056 min Scan# 3072

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion:252 Resp: 583948


Ion Ratio Lower Upper

252 100

254 64.6 51.1 76.7

126 9.2 7.4 11.0

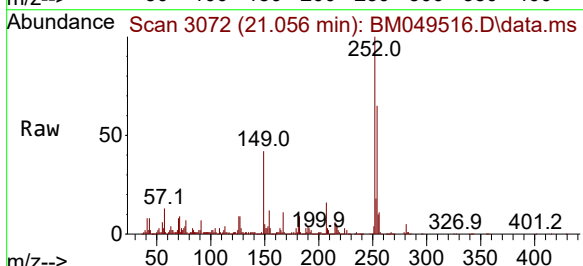



#85

Benzo(a)anthracene

Concen: 30.383 ng/ul

RT: 21.121 min Scan# 3082

Delta R.T. 0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:228 Resp: 2025754

Ion Ratio Lower Upper

228 100

229 19.6 15.7 23.5

226 27.2 22.1 33.1

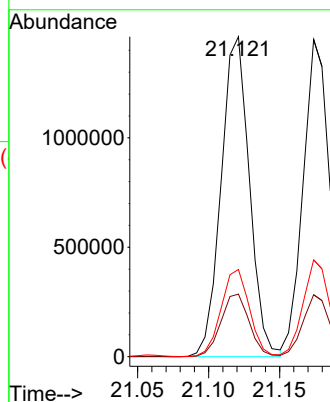

#86

Bis(2-ethylhexyl)phthalate

Concen: 32.188 ng/ul

RT: 21.068 min Scan# 3074

Delta R.T. -0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion:149 Resp: 1086131


Ion Ratio Lower Upper

149 100

167 28.9 23.0 34.4

279 4.0 3.3 4.9





#87

Chrysene

Concen: 30.552 ng/ul

RT: 21.174 min Scan# 3092

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:228 Resp: 1891736

Ion Ratio Lower Upper

228 100

226 30.5 24.6 37.0

229 19.5 15.9 23.9

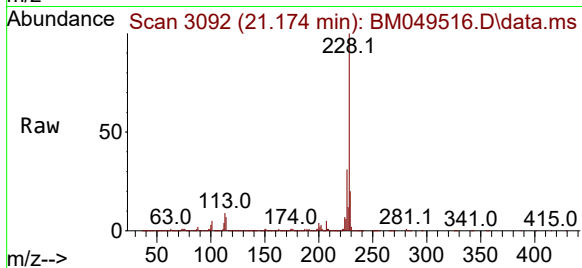

#89

Di-n-octyl phthalate

Concen: 28.998 ng/ul




RT: 22.133 min Scan# 3255


Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Tgt Ion:149 Resp: 1828196




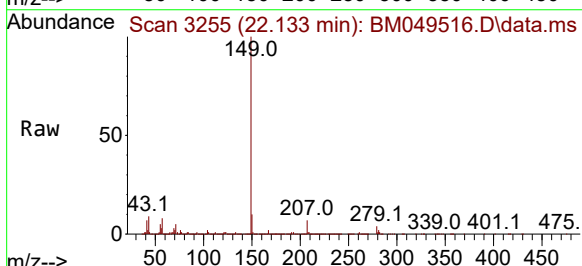




#90
Benzo(b)fluoranthene
Concen: 30.599 ng/ul
RT: 23.044 min Scan# 3410
Delta R.T. -0.000 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50




Instrument :
BNA_M
ClientSampleId :
SLCS284


Tgt Ion:252 Resp: 2044221
Ion Ratio Lower Upper
252 100
253 22.2 17.6 26.4
125 7.5 6.3 9.5

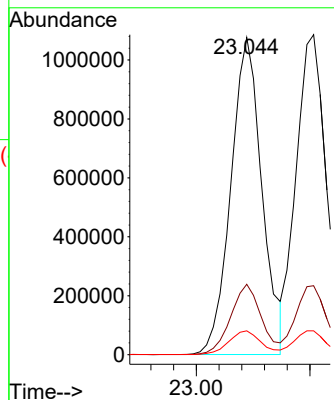

#91
Benzo(k)fluoranthene
Concen: 29.889 ng/ul
RT: 23.103 min Scan# 3420
Delta R.T. 0.006 min
Lab File: BM049516.D
Acq: 29 Jan 2025 22:50

Tgt Ion:252 Resp: 2017711
Ion Ratio Lower Upper
252 100
253 21.6 17.5 26.3
125 7.4 6.5 9.7

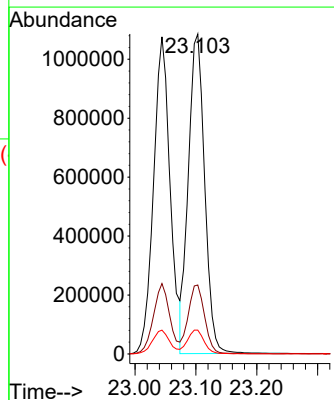



#93

Benzo(a)pyrene

Concen: 30.576 ng/ul

RT: 23.785 min Scan# 3

Delta R.T. 0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:252 Resp: 1916209

Ion Ratio Lower Upper

252 100

253 21.4 17.3 25.9

125 8.2 7.0 10.6



#94

Indeno(1,2,3-cd)pyrene

Concen: 31.798 ng/ul

RT: 26.997 min Scan# 4082

Delta R.T. 0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50




Tgt Ion:276 Resp: 2470008


Ion Ratio Lower Upper

276 100

138 16.3 13.8 20.6

277 24.0 19.0 28.6





#95

Dibenzo(a,h)anthracene

Concen: 32.016 ng/ul

RT: 27.050 min Scan# 4091

Delta R.T. -0.000 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Instrument :

BNA_M

ClientSampleId :

SLCS284





Tgt Ion:278 Resp: 2015205

Ion Ratio Lower Upper

278 100

139 12.2 10.5 15.7

279 23.6 19.3 28.9



#96

Benzo(g,h,i)perylene

Concen: 32.380 ng/ul

RT: 27.956 min Scan# 4245

Delta R.T. 0.006 min

Lab File: BM049516.D

Acq: 29 Jan 2025 22:50

Tgt Ion:276 Resp: 1912410

Ion Ratio Lower Upper

276 100

138 16.7 14.1 21.1

277 23.4 19.1 28.7

