

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049509.D
 Acq On : 29 Jan 2025 18:16
 Operator : RC/JU
 Sample : Q1189-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A44R0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/30/2025
 Supervised By :mohammad ahmed 02/05/2025

Quant Time: Jan 30 08:09:13 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 28 14:45:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	217843	20.000	ng/u1	0.00
20) Naphthalene-d8	10.269	136	818671	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.151	164	524785	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.904	188	1069898	20.000	ng/u1	0.00
79) Chrysene-d12	21.133	240	1192808	20.000	ng/u1	0.00
88) Perylene-d12	23.915	264	1298589	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	20508	3.488	ng/uL	0.00
4) Pyridine-d5	3.510	84	265315	15.359	ng/u1	0.00
7) Phenol-d5	6.734	99	345522	19.546	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	6.863	67	210876	17.445	ng/u1	0.00
11) 2-Chlorophenol-d4	7.063	132	278275	20.343	ng/u1	0.01
15) 4-Methylphenol-d8	8.245	113	246485	19.031	ng/u1	0.02
21) Nitrobenzene-d5	8.657	128	122609	19.576	ng/u1	0.00
24) 2-Nitrophenol-d4	9.369	143	139170	20.372	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.922	165	259678	18.627	ng/u1	0.02
31) 4-Chloroaniline-d4	10.422	131	256068	14.320	ng/u1	0.00
46) Dimethylphthalate-d6	13.574	166	790245	20.538	ng/u1	0.00
49) Acenaphthylene-d8	13.839	160	768927	17.008	ng/u1	0.00
54) 4-Nitrophenol-d4	14.445	143	78383m	12.418	ng/u1	0.06
60) Fluorene-d10	15.151	176	536331	15.850	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.286	200	94212	13.974	ng/u1	0.00
73) Anthracene-d10	17.004	188	787416	14.738	ng/u1	0.00
81) Pyrene-d10	19.309	212	875740	12.559	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.727	264	673255	9.721	ng/u1	0.00
Target Compounds						
8) Phenol	6.757	94	21872	1.179	ng/u1#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049509.D
Acq On : 29 Jan 2025 18:16
Operator : RC/JU
Sample : Q1189-07
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A44R0

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/30/2025
Supervised By :mohammad ahmed 02/05/2025


Quant Time: Jan 30 08:09:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

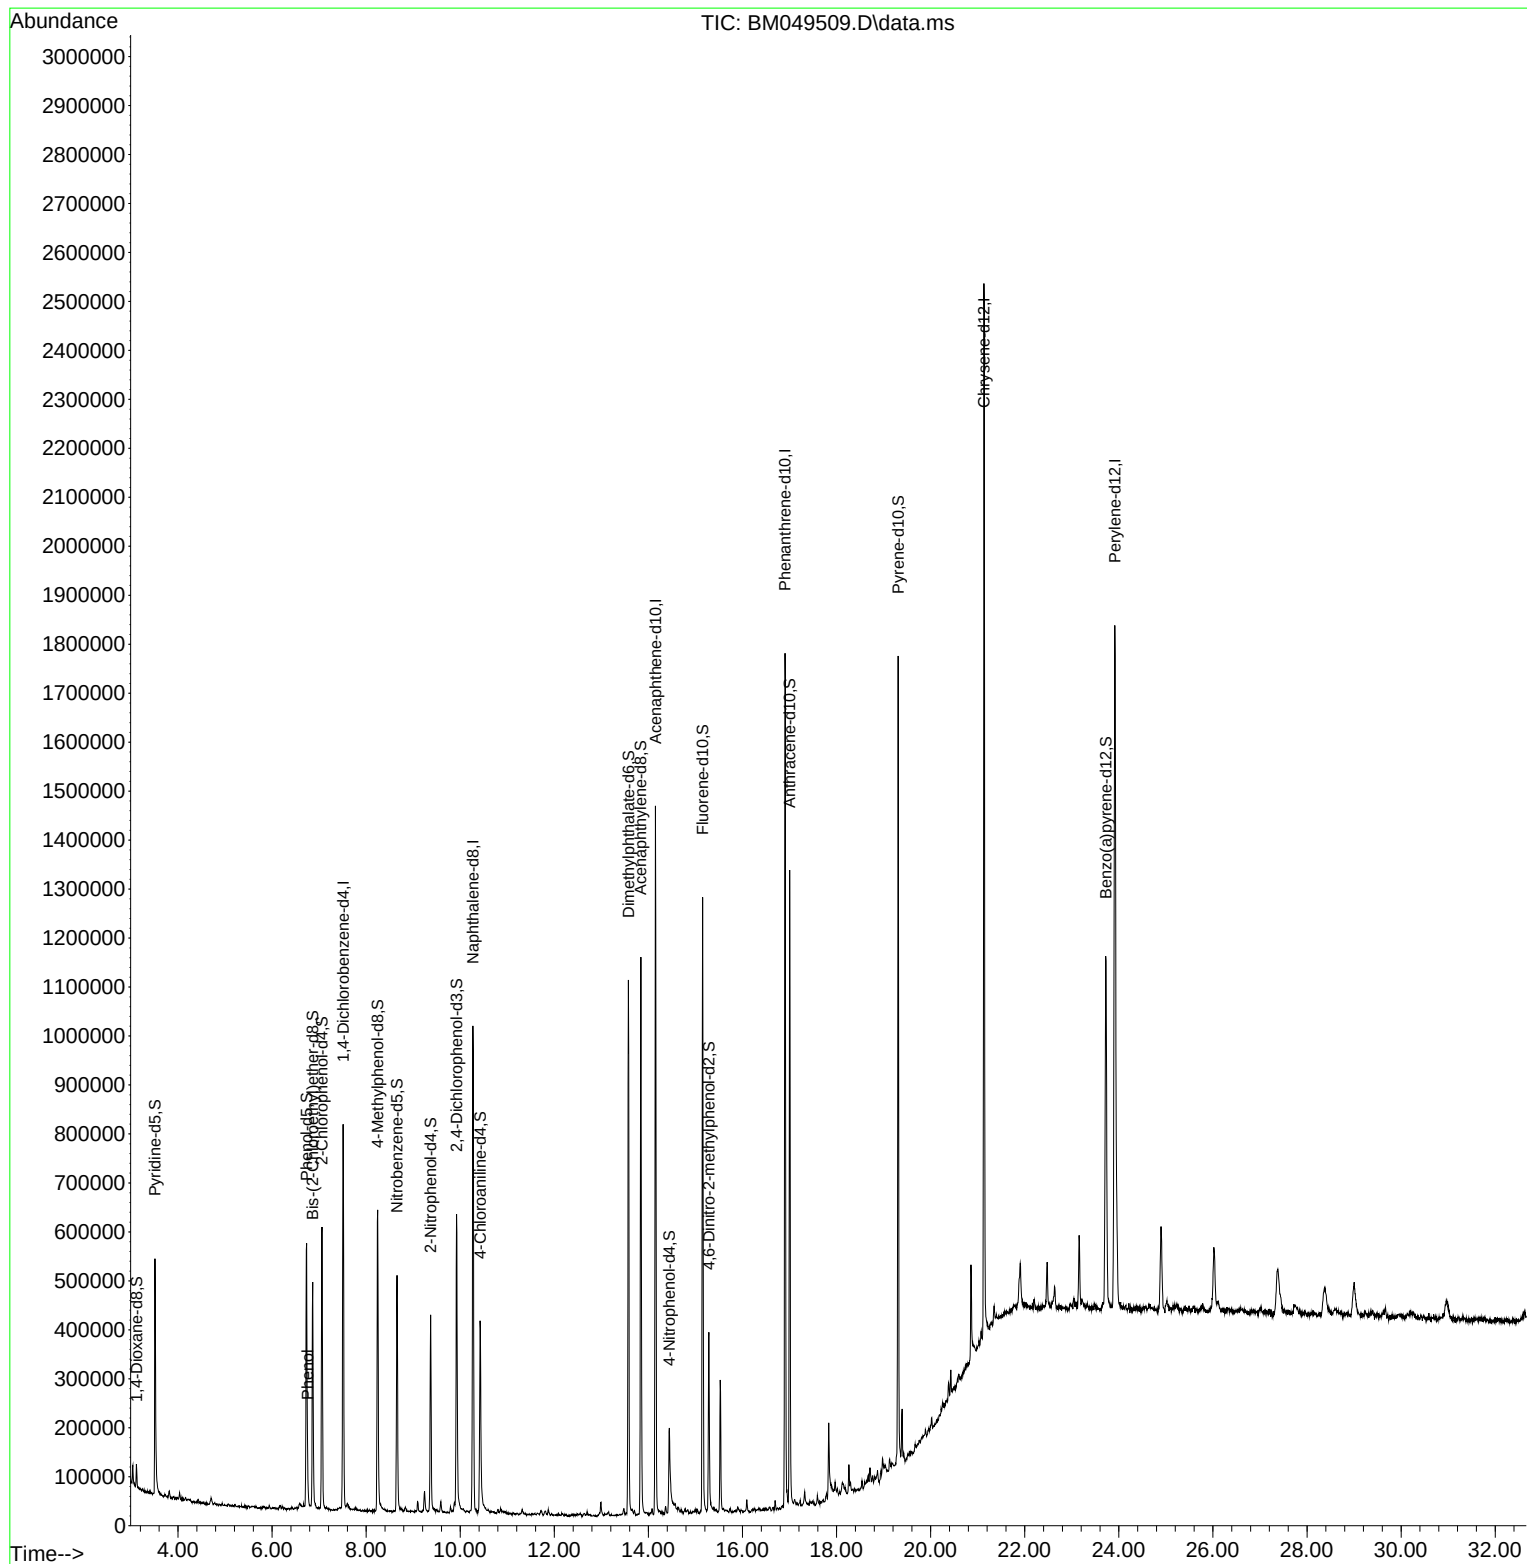

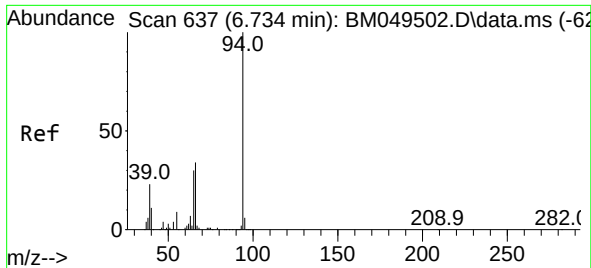

#8
Phenol
Concen: 1.179 ng/ul
RT: 6.757 min Scan# 641
Delta R.T. 0.023 min
Lab File: BM049509.D
Acq: 29 Jan 2025 18:16

Instrument :
BNA_M
ClientSampleId :
A44R0

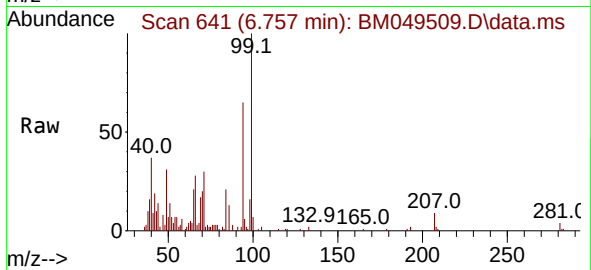

Tgt Ion: 94 Resp: 21872
Ion Ratio Lower Upper
94 100
65 32.7 23.4 35.0
66 42.8 27.8 41.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/30/2025
Supervised By :mohammad ahmed 02/05/2025

