

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049470.D
 Acq On : 28 Jan 2025 15:27
 Operator : RC/JU
 Sample : PB166286BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK286

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	19	22	29	rBV	61133	74377	2.36%	0.211%
2	3.510	84	89	102	rBV	711065	1074594	34.06%	3.053%
3	3.816	137	141	144	rVB3	12887	17578	0.56%	0.050%
4	5.916	496	498	502	rBV4	3714	5226	0.17%	0.015%
5	6.710	626	633	646	rBV	686987	1102637	34.95%	3.132%
6	6.863	653	659	669	rBV	573023	876434	27.78%	2.490%
7	7.051	685	691	700	rBV	707587	1104447	35.00%	3.137%
8	7.510	763	769	778	rVB	627068	970267	30.75%	2.756%
9	8.069	860	864	865	rBV4	3030	3493	0.11%	0.010%
10	8.228	884	891	906	rBV	753547	1248163	39.56%	3.546%
11	8.575	948	950	956	rVB5	3183	3445	0.11%	0.010%
12	8.657	956	964	978	rBV	583886	971281	30.78%	2.759%
13	9.369	1077	1085	1095	rBV	456217	754365	23.91%	2.143%
14	9.904	1168	1176	1193	rBV	690806	1225297	38.83%	3.481%
15	10.269	1231	1238	1250	rBV	748961	1232866	39.07%	3.502%
16	10.422	1254	1264	1281	rBV	549442	1114750	35.33%	3.167%
17	11.204	1394	1397	1401	rBV4	1925	3181	0.10%	0.009%
18	11.410	1431	1432	1436	rVB3	3461	4094	0.13%	0.012%
19	11.875	1508	1511	1512	rBV3	6162	5450	0.17%	0.015%
20	13.574	1794	1800	1812	rBV	1117498	1592213	50.46%	4.523%
21	13.657	1812	1814	1821	rVV6	4838	8383	0.27%	0.024%
22	13.739	1825	1828	1833	rBV5	2180	3535	0.11%	0.010%
23	13.839	1838	1845	1859	rBV	1364138	1989380	63.05%	5.651%
24	14.022	1871	1876	1879	rBV7	2316	3479	0.11%	0.010%
25	14.151	1891	1898	1912	rBV	1071752	1531273	48.53%	4.350%
26	14.386	1932	1938	1956	rBV	208189	546832	17.33%	1.553%
27	14.563	1967	1968	1975	rVB6	4013	5636	0.18%	0.016%
28	15.151	2060	2068	2083	rBV	1673340	2448756	77.61%	6.956%
29	15.280	2084	2090	2105	rVV	408631	602721	19.10%	1.712%
30	15.392	2105	2109	2118	rVB5	8550	18912	0.60%	0.054%
31	15.939	2199	2202	2205	rVB4	2593	3227	0.10%	0.009%
32	16.692	2326	2330	2333	rBV2	6043	6559	0.21%	0.019%
33	16.904	2360	2366	2376	rBV2	1258315	1729818	54.82%	4.914%
34	17.004	2376	2383	2401	rVB	1830349	2583524	81.88%	7.339%
35	17.598	2480	2484	2488	rVB6	2673	4148	0.13%	0.012%
36	17.674	2495	2497	2501	rBV4	2824	3782	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049470.D
Acq On : 28 Jan 2025 15:27
Operator : RC/JU
Sample : PB166286BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK286

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Title : SVOA CALIBRATION

37	17.833	2518	2524	2533	rBV8	19319	42412	1.34%	0.120%
38	18.874	2697	2701	2707	rBV4	19455	27098	0.86%	0.077%
39	18.945	2709	2713	2717	rVV2	15843	20782	0.66%	0.059%
40	19.127	2741	2744	2746	rBV3	7025	7434	0.24%	0.021%
41	19.309	2769	2775	2786	rBV	2429016	3155248	100.00%	8.963%
42	21.133	3080	3085	3097	rBV	1369852	1919567	60.84%	5.453%
43	23.727	3518	3526	3541	rVB	1365056	3058488	96.93%	8.688%
44	23.915	3550	3558	3574	rVB	850561	2096906	66.46%	5.957%




Sum of corrected areas: 35202058

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049470.D
Acq On : 28 Jan 2025 15:27
Operator : RC/JU
Sample : PB166286BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK286

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

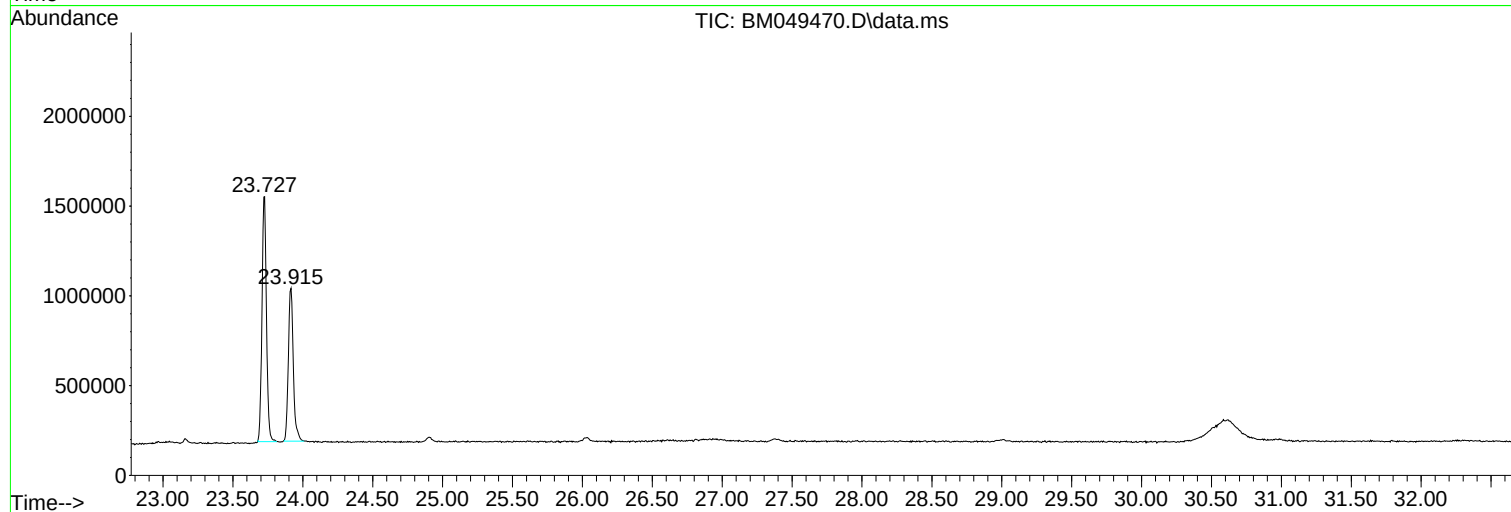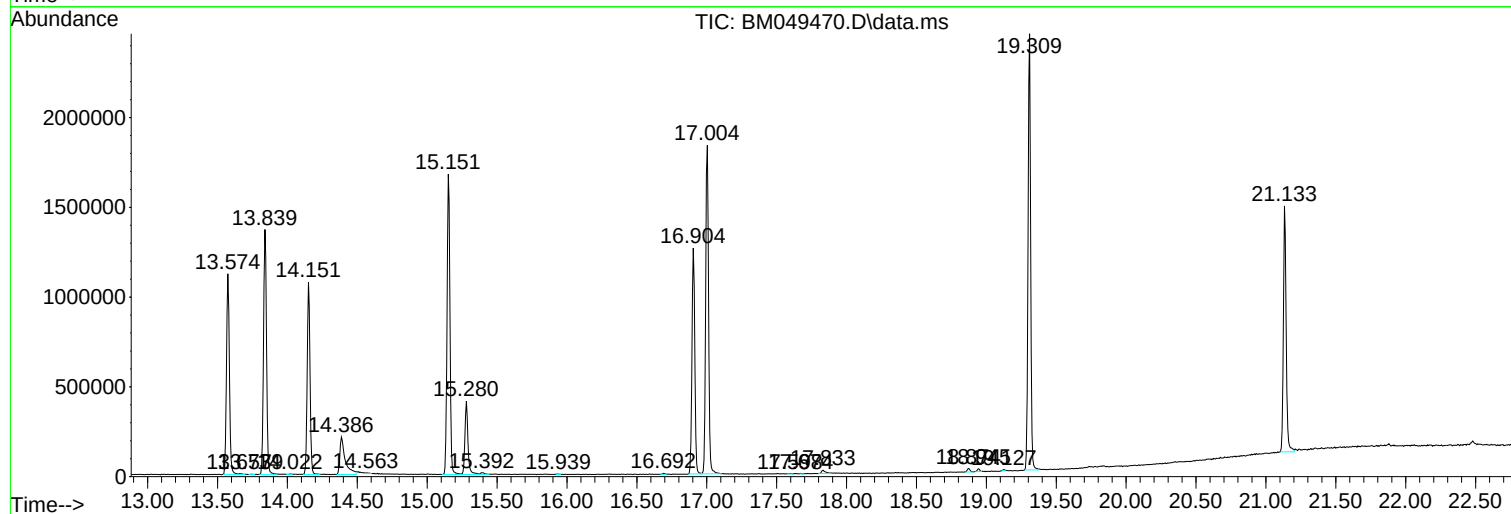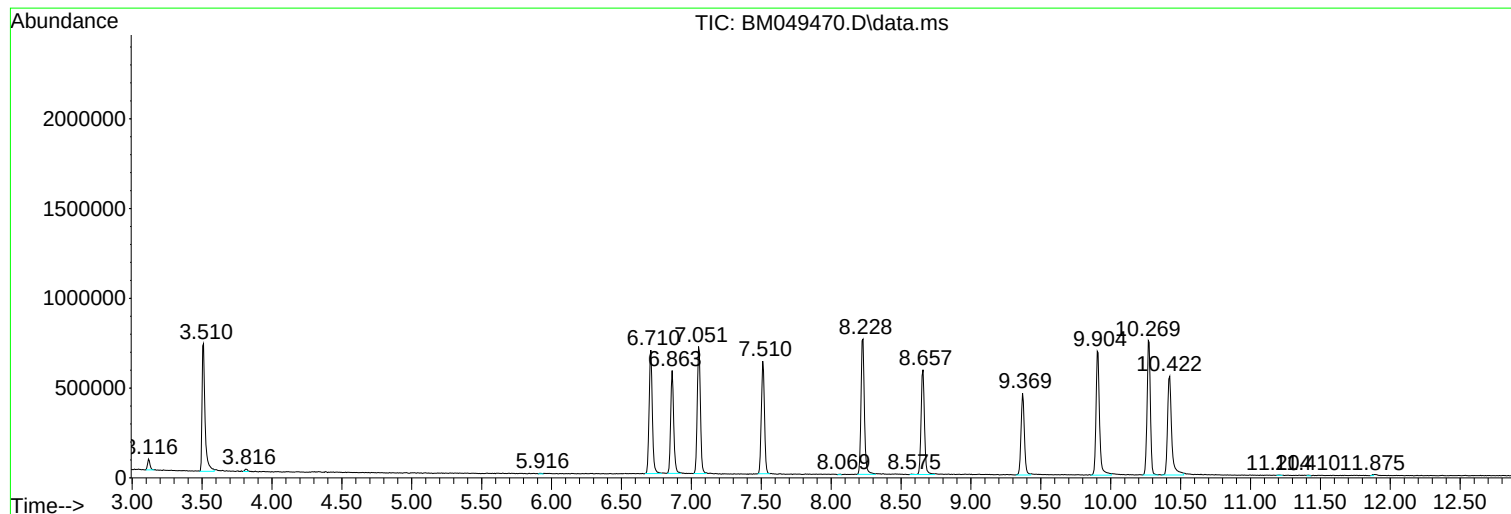

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049470.D
Acq On : 28 Jan 2025 15:27
Operator : RC/JU
Sample : PB166286BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK286

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049470.D
Acq On : 28 Jan 2025 15:27
Operator : RC/JU
Sample : PB166286BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK286

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc