

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049487.D
 Acq On : 29 Jan 2025 03:52
 Operator : RC/JU
 Sample : PB166304BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK304

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	30	rVB	83681	107483	2.29%	0.210%
2	3.504	84	88	108	rBV	1165540	1632537	34.82%	3.196%
3	3.810	137	140	146	rVB2	13132	19577	0.42%	0.038%
4	6.704	625	632	647	rBV	1071019	1695888	36.17%	3.320%
5	6.863	652	659	676	rVB	835642	1310072	27.94%	2.564%
6	7.051	685	691	702	rBV	1130080	1678981	35.81%	3.287%
7	7.510	762	769	777	rBV	831237	1266644	27.02%	2.479%
8	8.222	883	890	907	rBV	1187424	1900908	40.55%	3.721%
9	8.651	956	963	981	rBV	868230	1450353	30.94%	2.839%
10	9.369	1077	1085	1094	rBV	699141	1128423	24.07%	2.209%
11	9.904	1169	1176	1193	rBV	1102549	1853520	39.54%	3.628%
12	10.269	1231	1238	1248	rVB	1003150	1591997	33.96%	3.116%
13	10.416	1255	1263	1283	rBV	892463	1699410	36.25%	3.327%
14	11.886	1508	1513	1521	rBV5	10332	22870	0.49%	0.045%
15	13.574	1794	1800	1811	rBV	1732743	2373199	50.62%	4.645%
16	13.839	1837	1845	1858	rBV	2185615	3047826	65.01%	5.966%
17	14.151	1891	1898	1908	rBV	1397088	2006048	42.79%	3.927%
18	14.380	1930	1937	1959	rBV	354714	892309	19.03%	1.747%
19	15.151	2061	2068	2079	rBV	2682126	3682267	78.54%	7.208%
20	15.280	2084	2090	2105	rVV	639660	912226	19.46%	1.786%
21	15.398	2106	2110	2115	rVB3	9579	15875	0.34%	0.031%
22	16.692	2324	2330	2333	rBV3	5705	8516	0.18%	0.017%
23	16.903	2357	2366	2377	rBV	1773051	2311746	49.31%	4.525%
24	17.003	2377	2383	2398	rVV	2897767	3934413	83.92%	7.701%
25	17.845	2521	2526	2528	rBV5	4604	6712	0.14%	0.013%
26	18.874	2697	2701	2706	rBV2	26699	35814	0.76%	0.070%
27	18.945	2708	2713	2717	rBV	25679	35438	0.76%	0.069%
28	19.309	2769	2775	2789	rBV	3734546	4688128	100.00%	9.177%
29	21.138	3080	3086	3098	rBV	1679898	2465187	52.58%	4.825%
30	23.727	3517	3526	3544	rBV	2087750	4594784	98.01%	8.994%
31	23.915	3550	3558	3577	rVB	1129932	2717648	57.97%	5.320%




Sum of corrected areas: 51086799

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049487.D
Acq On : 29 Jan 2025 03:52
Operator : RC/JU
Sample : PB166304BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK304

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

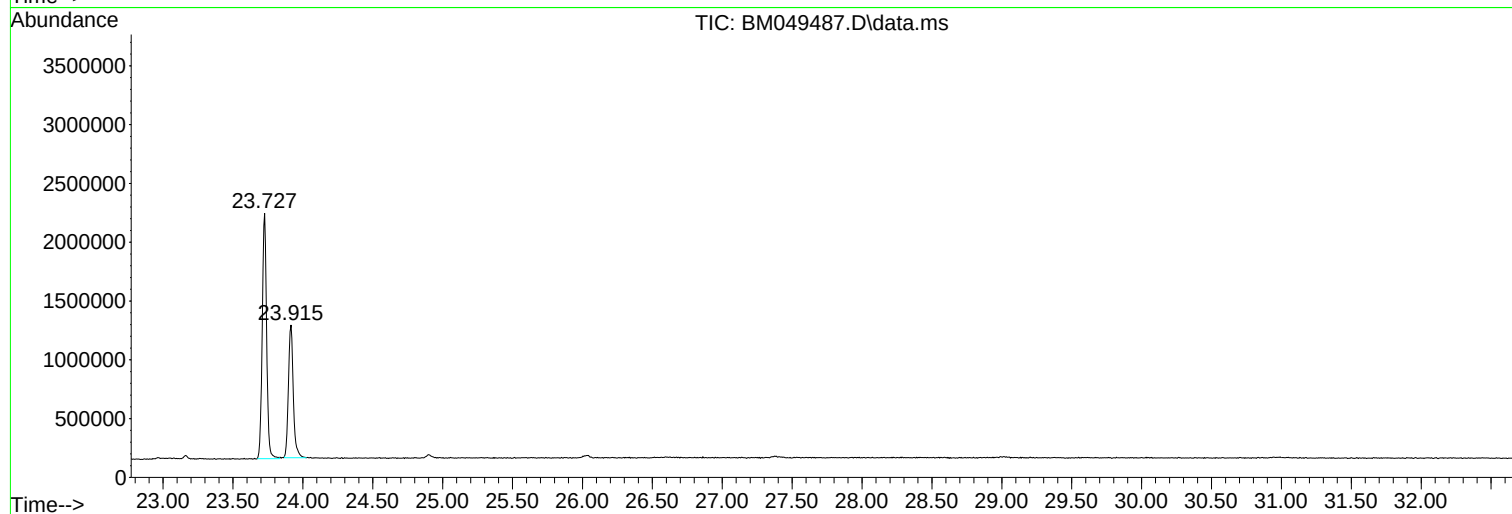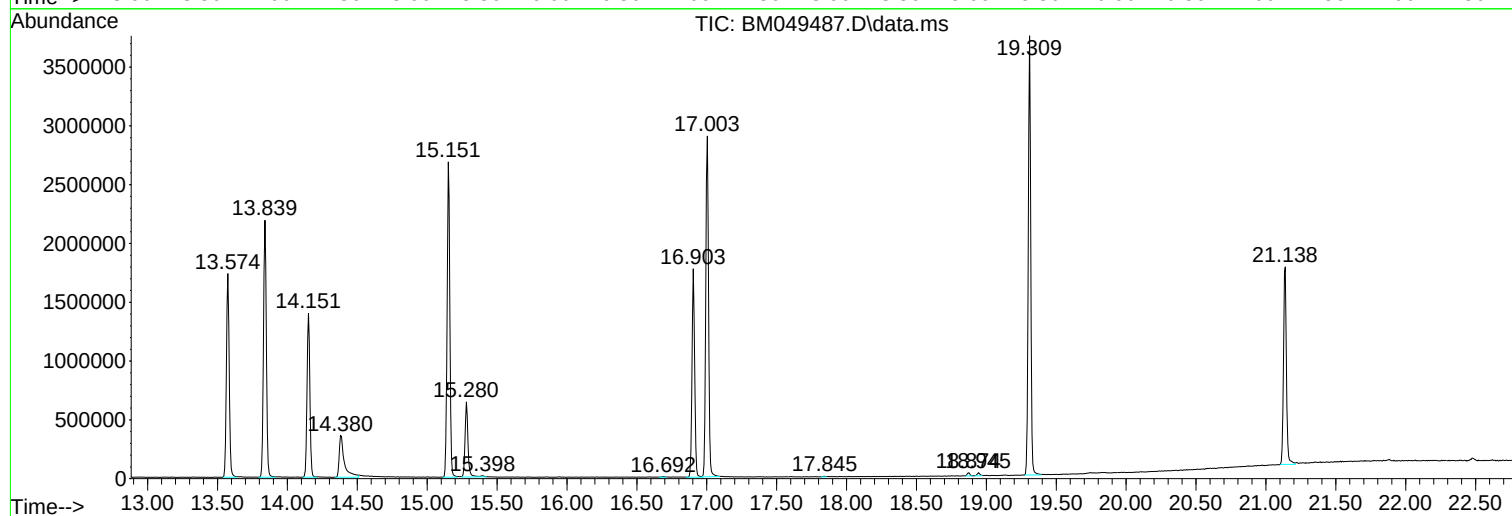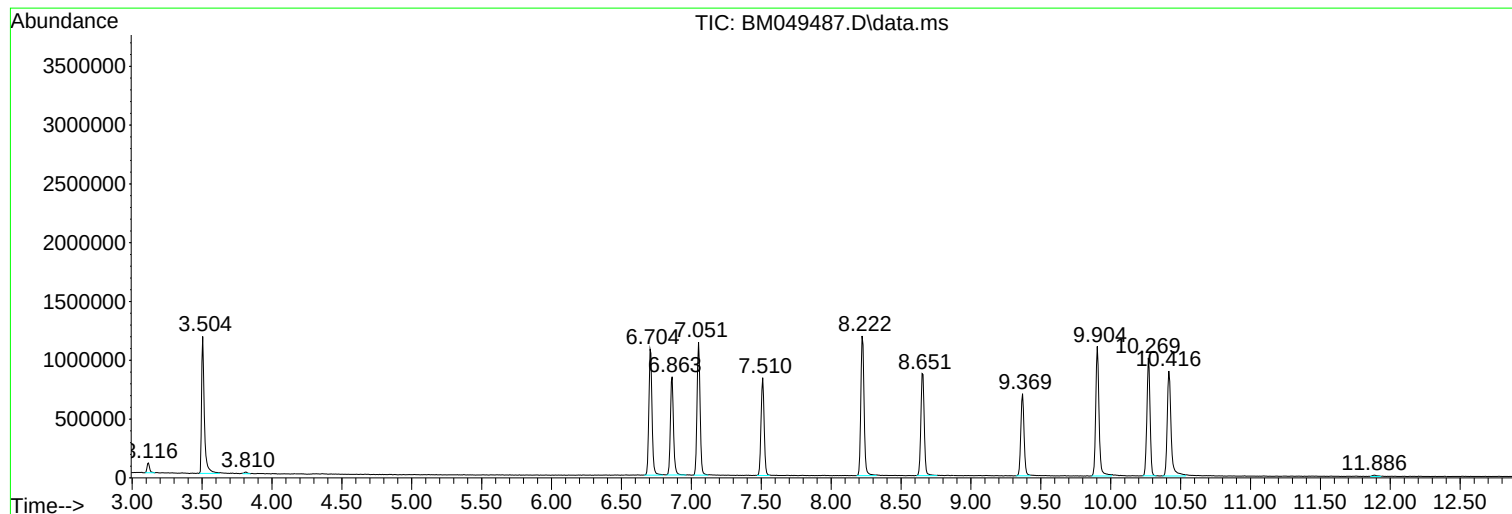

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049487.D
Acq On : 29 Jan 2025 03:52
Operator : RC/JU
Sample : PB166304BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK304

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049487.D
Acq On : 29 Jan 2025 03:52
Operator : RC/JU
Sample : PB166304BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK304

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc