

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049490.D
 Acq On : 29 Jan 2025 05:49
 Operator : RC/JU
 Sample : Q1184-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2949

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	19	22	26	rBV	57913	64363	1.27%	0.139%
2	3.510	85	89	101	rBV	241534	379636	7.47%	0.820%
3	3.810	138	140	146	rVB2	13367	17649	0.35%	0.038%
4	3.910	154	157	162	rVB3	17622	23112	0.45%	0.050%
5	4.705	286	292	304	rVB2	30648	56523	1.11%	0.122%
6	5.228	377	381	384	rVB4	5855	8340	0.16%	0.018%
7	5.934	498	501	508	rVB5	13255	19672	0.39%	0.042%
8	6.704	624	632	647	rBV	258386	436218	8.58%	0.942%
9	6.863	652	659	673	rBV	738177	1170630	23.02%	2.527%
10	7.051	685	691	701	rBV	852209	1278976	25.16%	2.761%
11	7.510	762	769	780	rBV	779786	1178704	23.18%	2.545%
12	7.593	780	783	788	rVB6	6136	8587	0.17%	0.019%
13	7.951	841	844	850	rVB6	4834	8269	0.16%	0.018%
14	8.222	883	890	902	rBV	678964	1079509	21.23%	2.331%
15	8.651	956	963	975	rBV	783587	1286451	25.30%	2.777%
16	9.098	1035	1039	1043	rBV	14630	19764	0.39%	0.043%
17	9.369	1078	1085	1097	rBV	622261	1008405	19.83%	2.177%
18	9.904	1169	1176	1197	rBV	975388	1620957	31.88%	3.500%
19	10.269	1231	1238	1247	rBV	955936	1503442	29.57%	3.246%
20	10.416	1255	1263	1287	rBV	691219	1314775	25.86%	2.839%
21	11.104	1379	1380	1386	rBV5	3380	5552	0.11%	0.012%
22	11.586	1457	1462	1468	rVB8	5054	8765	0.17%	0.019%
23	11.881	1506	1512	1519	rBV7	8399	19231	0.38%	0.042%
24	12.757	1656	1661	1668	rBV6	4934	10529	0.21%	0.023%
25	13.575	1793	1800	1812	rBV	1674323	2275682	44.76%	4.913%
26	13.839	1836	1845	1857	rBV	1815480	2641183	51.95%	5.702%
27	13.992	1870	1871	1876	rVB4	5398	5112	0.10%	0.011%
28	14.151	1891	1898	1907	rBV	1336453	1893366	37.24%	4.088%
29	14.251	1910	1915	1918	rVB6	4428	7391	0.15%	0.016%
30	14.392	1933	1939	1950	rBV2	65652	178447	3.51%	0.385%
31	14.516	1958	1960	1965	rVB5	4133	6982	0.14%	0.015%
32	14.980	2036	2039	2040	rBV2	5648	5816	0.11%	0.013%
33	15.151	2060	2068	2083	rBV	2693552	3545838	69.74%	7.655%
34	15.280	2083	2090	2104	rVV	678239	950331	18.69%	2.052%
35	15.392	2106	2109	2115	rVB3	10883	16550	0.33%	0.036%
36	15.527	2127	2132	2138	rBV	70612	105389	2.07%	0.228%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049490.D
 Acq On : 29 Jan 2025 05:49
 Operator : RC/JU
 Sample : Q1184-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2949

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

37	16.692	2327	2330	2335	rBV4	6313	8441	0.17%	0.018%
38	16.904	2360	2366	2376	rBV2	1632770	2190359	43.08%	4.729%
39	17.004	2376	2383	2398	rVV	3011701	4059699	79.85%	8.765%
40	17.698	2498	2501	2504	rBV5	3572	5971	0.12%	0.013%
41	17.827	2518	2523	2530	rBV3	65997	103069	2.03%	0.223%
42	17.892	2533	2534	2540	rVB4	6428	8115	0.16%	0.018%
43	18.304	2601	2604	2607	rBV4	4081	5451	0.11%	0.012%
44	18.868	2696	2700	2708	rBV2	31699	48952	0.96%	0.106%
45	18.939	2708	2712	2720	rBV	29104	46389	0.91%	0.100%
46	19.121	2739	2743	2747	rBV2	31830	39936	0.79%	0.086%
47	19.309	2769	2775	2786	rBV	4077870	5034603	99.02%	10.870%
48	21.133	3080	3085	3094	rBV	1762749	2507337	49.32%	5.413%
49	23.162	3426	3430	3437	rVB3	61455	106363	2.09%	0.230%
50	23.727	3517	3526	3541	rBV	2359946	5084199	100.00%	10.977%
51	23.915	3550	3558	3573	rVB	1238107	2909197	57.22%	6.281%




Sum of corrected areas: 46318227

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049490.D
Acq On : 29 Jan 2025 05:49
Operator : RC/JU
Sample : Q1184-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2949

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

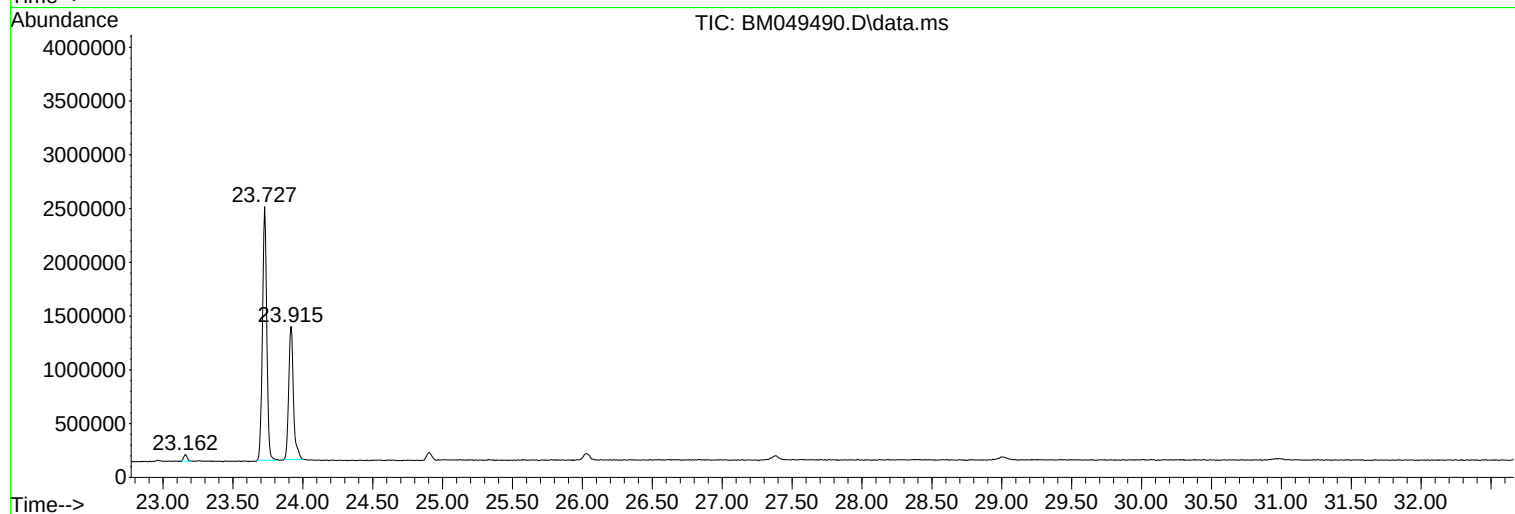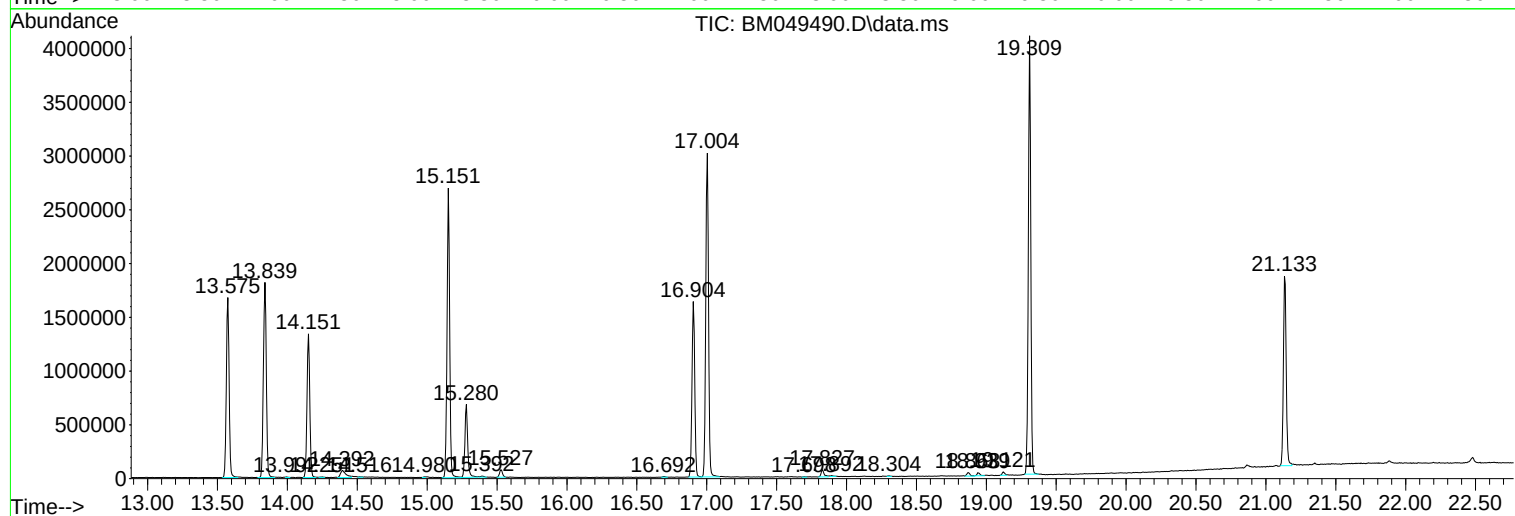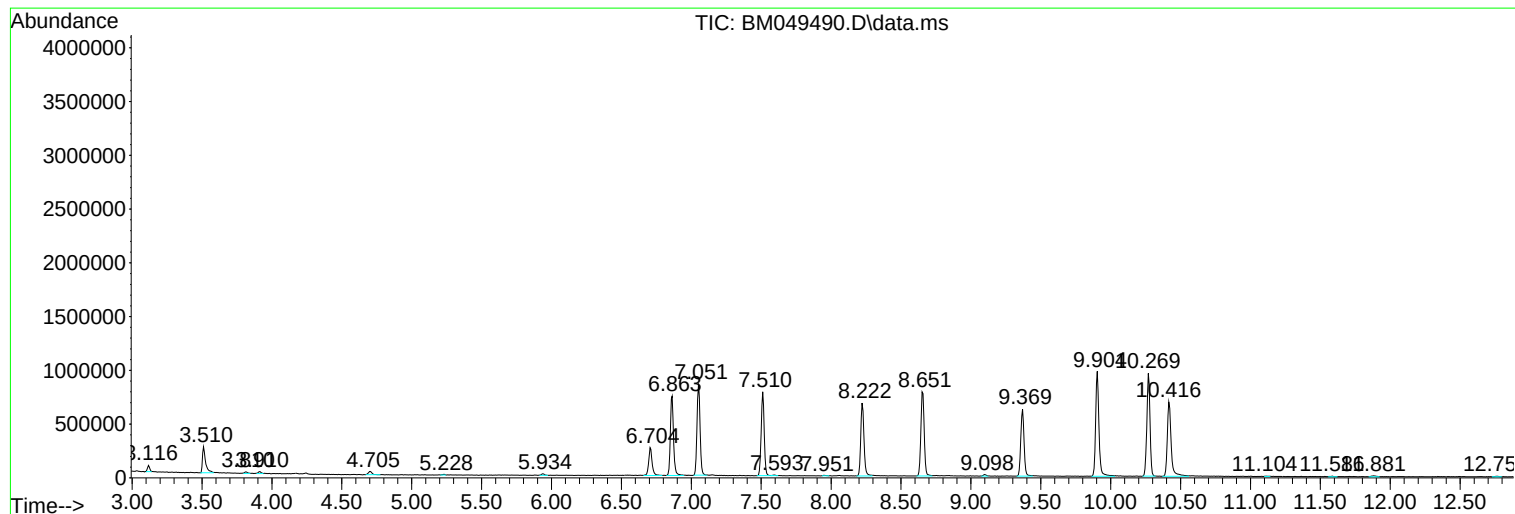

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049490.D
Acq On : 29 Jan 2025 05:49
Operator : RC/JU
Sample : Q1184-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2949

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049490.D
Acq On : 29 Jan 2025 05:49
Operator : RC/JU
Sample : Q1184-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2949

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------