

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049491.D
 Acq On : 29 Jan 2025 06:28
 Operator : RC/JU
 Sample : Q1184-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2955

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	19	22	27	rVB	55199	59519	1.09%	0.125%
2	3.511	86	89	108	rBV	169680	287310	5.28%	0.604%
3	3.817	137	141	149	rVB5	16956	25564	0.47%	0.054%
4	3.911	154	157	162	rVB4	19416	23991	0.44%	0.050%
5	4.705	287	292	300	rVB2	35780	63101	1.16%	0.133%
6	5.228	377	381	389	rVB7	9445	14061	0.26%	0.030%
7	5.940	498	502	507	rVB3	13252	17811	0.33%	0.037%
8	6.705	625	632	643	rBV	237067	394494	7.25%	0.829%
9	6.864	653	659	669	rBV	776914	1228935	22.60%	2.582%
10	7.052	684	691	703	rBV	894734	1349574	24.82%	2.835%
11	7.511	762	769	780	rVV	772094	1184996	21.79%	2.489%
12	7.587	780	782	788	rVB5	4490	7716	0.14%	0.016%
13	8.222	883	890	905	rBV	673320	1068043	19.64%	2.244%
14	8.652	956	963	976	rBV	824761	1360527	25.02%	2.858%
15	9.099	1034	1039	1042	rBV5	10510	16749	0.31%	0.035%
16	9.369	1077	1085	1094	rBV	672316	1066509	19.61%	2.240%
17	9.434	1094	1096	1103	rVB4	6872	8619	0.16%	0.018%
18	9.905	1168	1176	1190	rBV	1005367	1700140	31.26%	3.572%
19	10.269	1230	1238	1246	rBV	950776	1505511	27.68%	3.163%
20	10.416	1255	1263	1274	rBV	593024	1111727	20.44%	2.335%
21	11.587	1459	1462	1468	rVB5	3640	5556	0.10%	0.012%
22	11.875	1506	1511	1523	rVB2	9173	18764	0.35%	0.039%
23	13.575	1793	1800	1810	rBV	1791448	2448422	45.02%	5.144%
24	13.704	1819	1822	1827	rVB7	4733	6147	0.11%	0.013%
25	13.840	1837	1845	1856	rBV	2030904	2874347	52.85%	6.038%
26	14.151	1891	1898	1908	rBV	1361733	1883420	34.63%	3.957%
27	14.393	1934	1939	1952	rBV2	55799	166876	3.07%	0.351%
28	14.981	2035	2039	2041	rBV2	8494	11627	0.21%	0.024%
29	15.151	2062	2068	2081	rBV	2752465	3780774	69.52%	7.942%
30	15.281	2084	2090	2103	rVV	710527	1018567	18.73%	2.140%
31	15.398	2105	2110	2121	rVB5	12942	25897	0.48%	0.054%
32	15.528	2127	2132	2140	rBV	22424	36591	0.67%	0.077%
33	15.598	2140	2144	2148	rVB6	5766	7551	0.14%	0.016%
34	16.686	2326	2329	2335	rVB5	6866	9697	0.18%	0.020%
35	16.904	2360	2366	2375	rBV2	1598219	2165316	39.82%	4.549%
36	17.004	2377	2383	2399	rVB	3194380	4300872	79.08%	9.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049491.D
Acq On : 29 Jan 2025 06:28
Operator : RC/JU
Sample : Q1184-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2955

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Title : SVOA CALIBRATION

37	17.828	2517	2523	2530	rBV5	21980	40747	0.75%	0.086%
38	17.892	2532	2534	2541	rVB5	5220	9662	0.18%	0.020%
39	18.298	2600	2603	2606	rVB4	5483	6062	0.11%	0.013%
40	18.869	2696	2700	2707	rVB	32385	46390	0.85%	0.097%
41	18.945	2708	2713	2717	rBV2	31160	43130	0.79%	0.091%
42	19.122	2740	2743	2747	rBV5	13682	19083	0.35%	0.040%
43	19.310	2769	2775	2787	rVB	4366100	5392101	99.15%	11.327%
44	21.139	3080	3086	3100	rBV	1875772	2553637	46.96%	5.365%
45	23.727	3517	3526	3541	rBV	2458015	5438381	100.00%	11.425%
46	23.915	3550	3558	3574	rBV	1203209	2797610	51.44%	5.877%




Sum of corrected areas: 47602124

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049491.D
Acq On : 29 Jan 2025 06:28
Operator : RC/JU
Sample : Q1184-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2955

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

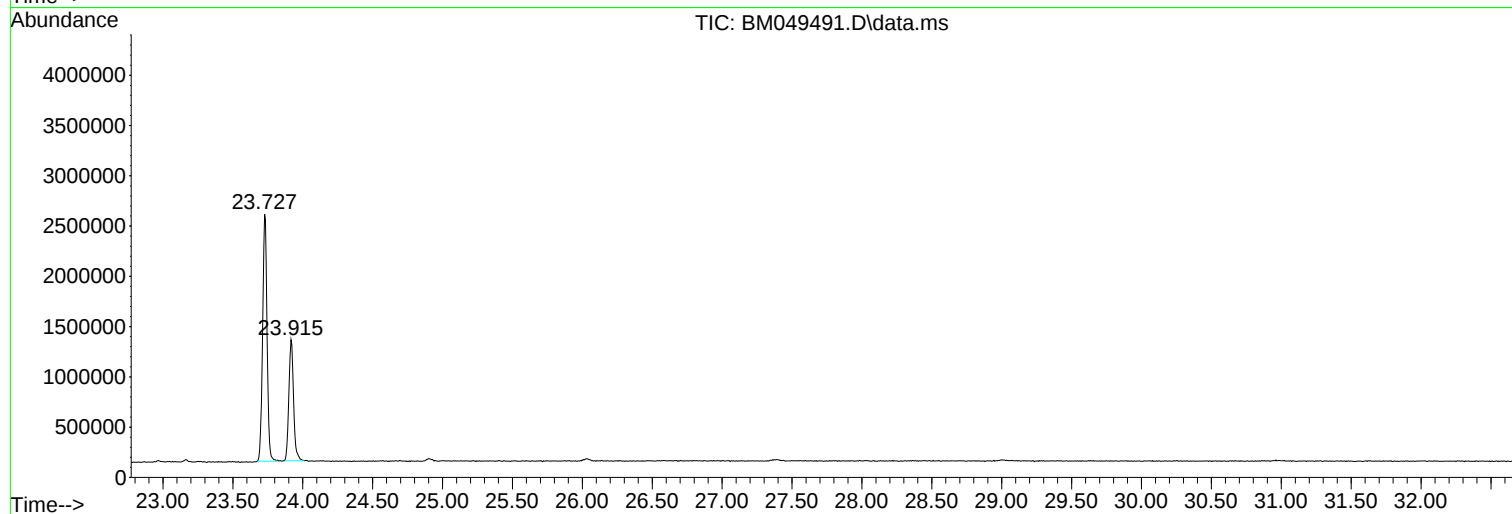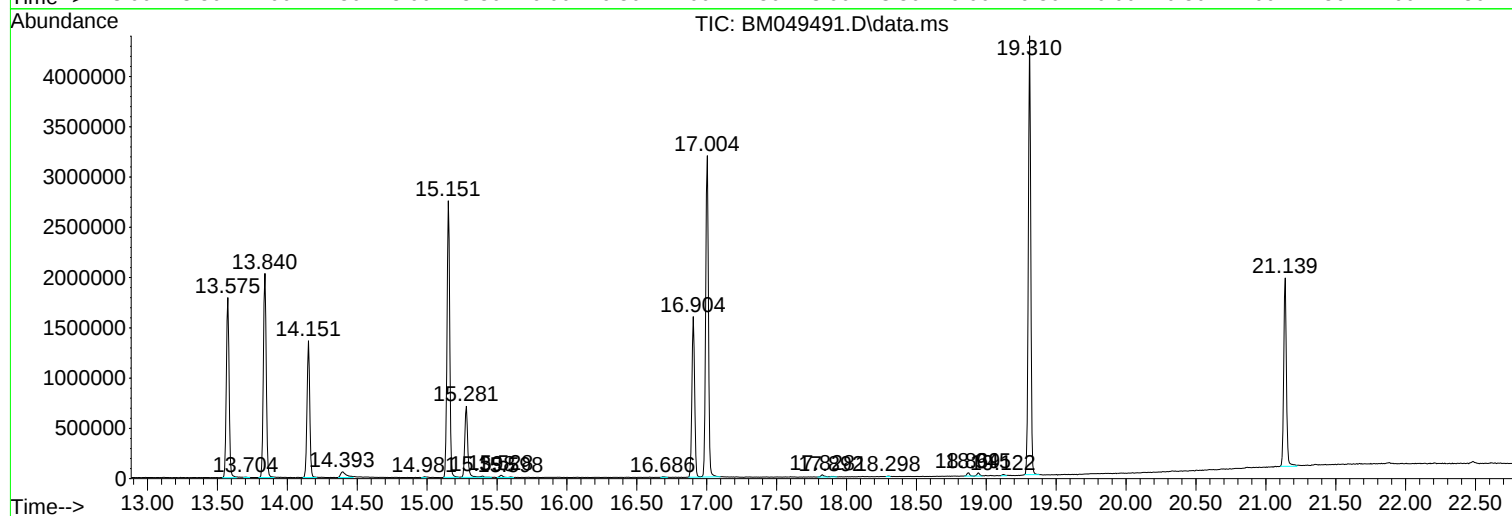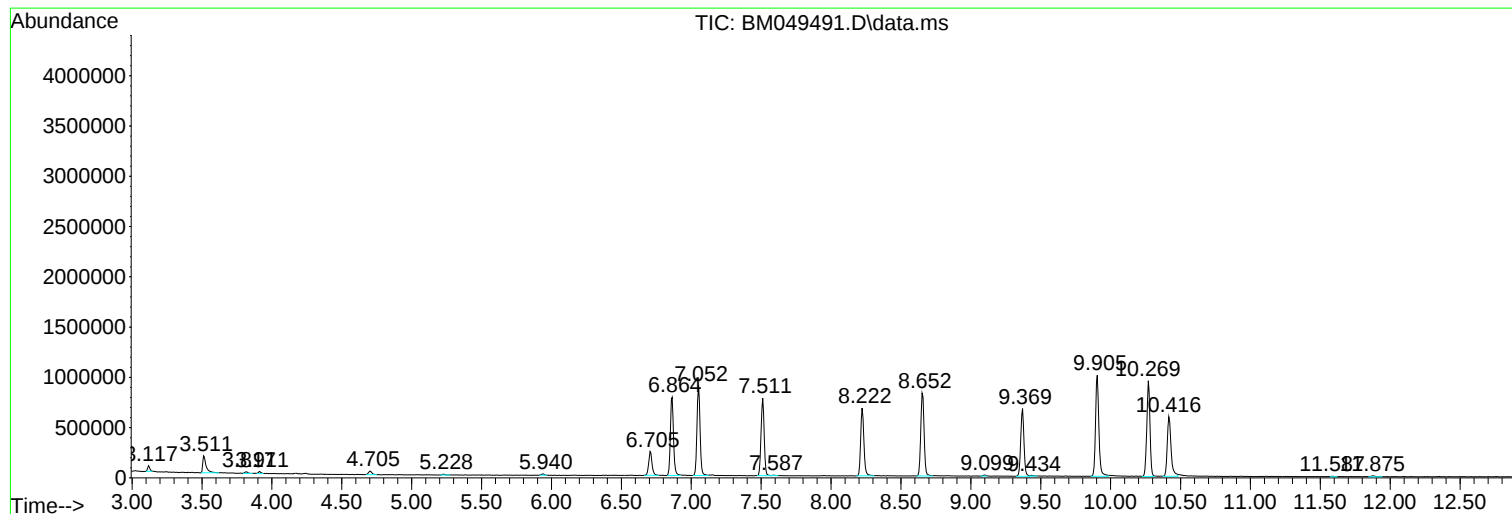

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049491.D
Acq On : 29 Jan 2025 06:28
Operator : RC/JU
Sample : Q1184-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2955

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049491.D
Acq On : 29 Jan 2025 06:28
Operator : RC/JU
Sample : Q1184-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2955

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc