

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049500.D
 Acq On : 29 Jan 2025 12:22
 Operator : RC/JU
 Sample : PB166286BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK286

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	30	rVB	51944	69529	2.40%	0.220%
2	3.505	84	88	102	rBV	682200	974940	33.59%	3.081%
3	3.810	136	140	146	rVB5	12014	19993	0.69%	0.063%
4	6.034	515	518	521	rBV5	2476	3152	0.11%	0.010%
5	6.704	626	632	647	rBV	630799	1015565	34.99%	3.210%
6	6.857	652	658	668	rBV	490944	779117	26.84%	2.462%
7	7.051	684	691	703	rBV	670352	1015311	34.98%	3.209%
8	7.510	762	769	776	rBV	530771	821782	28.31%	2.597%
9	8.222	883	890	906	rBV	685012	1129272	38.91%	3.569%
10	8.369	913	915	919	rVB5	2418	3648	0.13%	0.012%
11	8.540	940	944	948	rBV6	2964	5514	0.19%	0.017%
12	8.651	956	963	977	rBV	527657	862484	29.72%	2.726%
13	9.034	1026	1028	1033	rBV5	2089	3012	0.10%	0.010%
14	9.222	1056	1060	1063	rVB3	3701	3359	0.12%	0.011%
15	9.369	1077	1085	1099	rBV	391982	662964	22.84%	2.095%
16	9.728	1143	1146	1150	rBV6	2411	3321	0.11%	0.010%
17	9.904	1168	1176	1193	rBV	599593	1091096	37.59%	3.448%
18	10.269	1231	1238	1246	rBV	647451	1045423	36.02%	3.304%
19	10.416	1254	1263	1285	rBV	474819	1007830	34.72%	3.185%
20	10.669	1302	1306	1309	rVB5	2894	4488	0.15%	0.014%
21	11.163	1388	1390	1393	rBV3	2470	2908	0.10%	0.009%
22	11.645	1470	1472	1477	rBV3	2980	4012	0.14%	0.013%
23	11.886	1508	1513	1521	rBV7	5732	14197	0.49%	0.045%
24	12.633	1636	1640	1643	rBV5	1747	3219	0.11%	0.010%
25	12.951	1692	1694	1699	rVB6	2278	4100	0.14%	0.013%
26	13.016	1699	1705	1706	rBV5	2636	4414	0.15%	0.014%
27	13.110	1717	1721	1724	rBV4	2249	3389	0.12%	0.011%
28	13.575	1793	1800	1813	rBV	963287	1425877	49.13%	4.506%
29	13.663	1813	1815	1820	rVB6	3029	4480	0.15%	0.014%
30	13.839	1838	1845	1856	rBV	1255844	1793495	61.79%	5.668%
31	14.151	1891	1898	1910	rBV	897873	1323146	45.59%	4.182%
32	14.392	1932	1939	1963	rBV	147685	471988	16.26%	1.492%
33	15.151	2061	2068	2081	rBV	1582610	2222382	76.57%	7.024%
34	15.280	2083	2090	2100	rBV	328609	469623	16.18%	1.484%
35	15.392	2106	2109	2116	rVB7	8656	14771	0.51%	0.047%
36	16.433	2282	2286	2287	rBV4	2531	3108	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049500.D
Acq On : 29 Jan 2025 12:22
Operator : RC/JU
Sample : PB166286BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK286

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Title : SVOA CALIBRATION

37	16.692	2326	2330	2333	rVB3	3463	3536	0.12%	0.011%
38	16.904	2360	2366	2376	rBV	1136438	1538553	53.01%	4.862%
39	17.004	2376	2383	2396	rVV	1710952	2362660	81.40%	7.467%
40	17.827	2519	2523	2527	rBV4	2839	5245	0.18%	0.017%
41	18.315	2602	2606	2608	rBV5	2586	3600	0.12%	0.011%
42	18.645	2659	2662	2664	rBV4	2547	2933	0.10%	0.009%
43	18.874	2697	2701	2705	rVB2	14702	19717	0.68%	0.062%
44	18.945	2710	2713	2717	rBV2	14734	19847	0.68%	0.063%
45	19.309	2769	2775	2789	rBV	2185960	2902517	100.00%	9.173%
46	21.133	3080	3085	3096	rBV	1184043	1707936	58.84%	5.398%
47	23.727	3518	3526	3541	rVB	1274884	2880989	99.26%	9.105%
48	23.915	3550	3558	3573	rVB	798308	1906936	65.70%	6.027%




Sum of corrected areas: 31641378

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049500.D
Acq On : 29 Jan 2025 12:22
Operator : RC/JU
Sample : PB166286BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK286

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

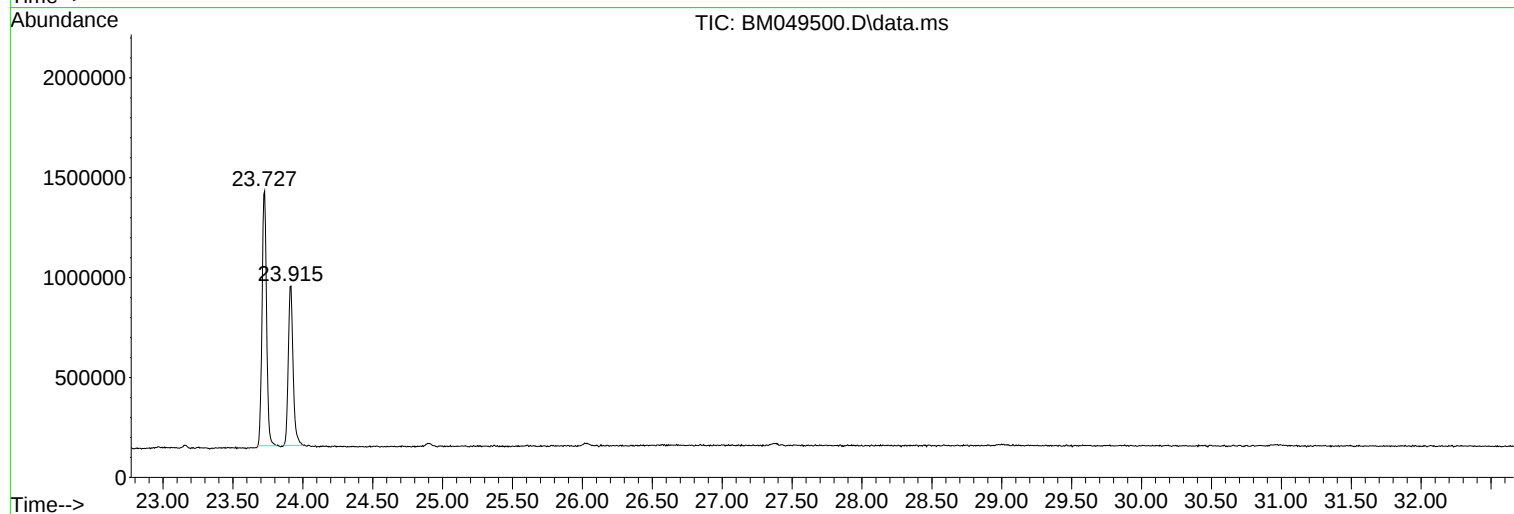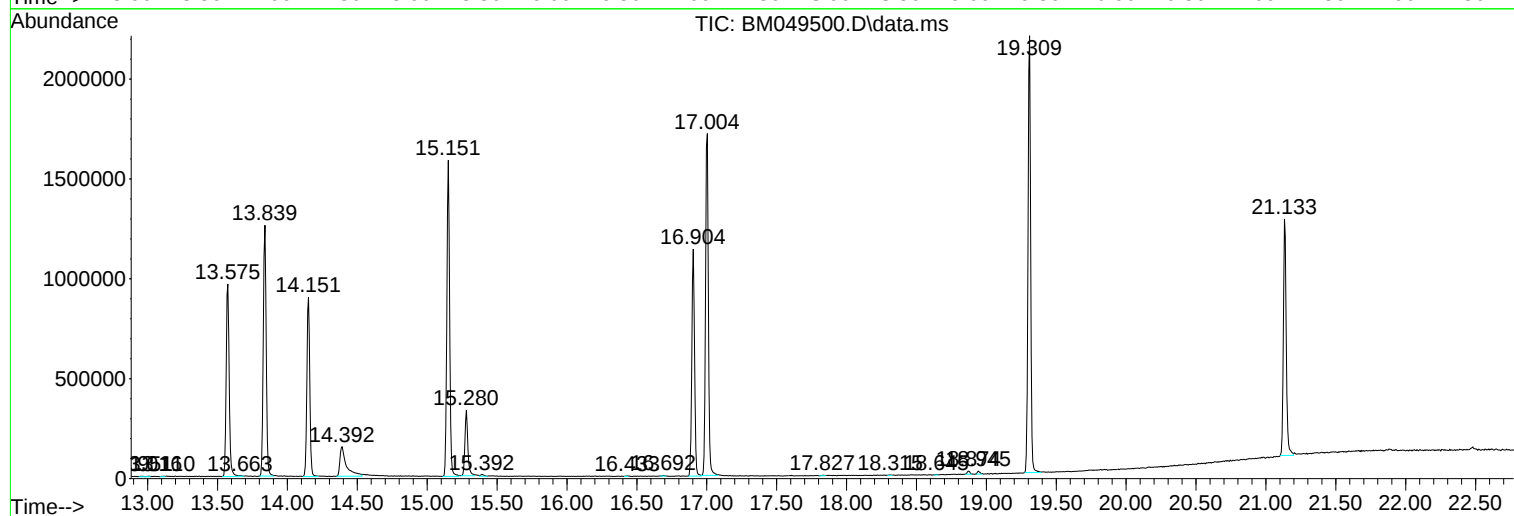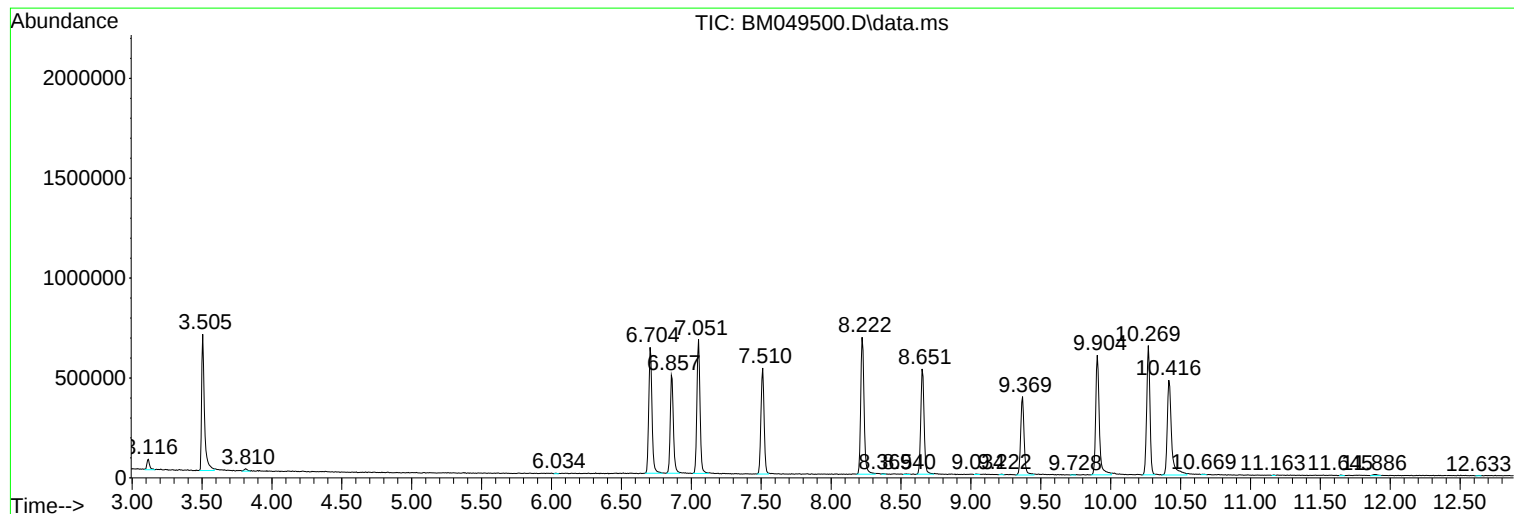

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049500.D
Acq On : 29 Jan 2025 12:22
Operator : RC/JU
Sample : PB166286BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK286

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049500.D
Acq On : 29 Jan 2025 12:22
Operator : RC/JU
Sample : PB166286BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK286

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc