

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
 Data File : BM049503.D
 Acq On : 29 Jan 2025 14:20
 Operator : RC/JU
 Sample : PB166307BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK307

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	30	rVB	52465	73405	2.30%	0.223%
2	3.504	84	88	104	rBV	718237	1033668	32.40%	3.139%
3	3.810	137	140	146	rVB5	8629	14201	0.45%	0.043%
4	4.222	208	210	214	rVB5	5274	4372	0.14%	0.013%
5	6.198	544	546	550	rBV5	2830	3832	0.12%	0.012%
6	6.704	626	632	642	rBV	682729	1065952	33.42%	3.237%
7	6.857	652	658	668	rBV	514406	821796	25.76%	2.495%
8	7.051	685	691	703	rBV	699540	1056260	33.11%	3.207%
9	7.510	763	769	779	rBV	491792	766339	24.02%	2.327%
10	8.051	857	861	865	rBV5	2089	3556	0.11%	0.011%
11	8.222	883	890	907	rBV	750859	1203852	37.74%	3.655%
12	8.651	956	963	978	rBV	537567	913640	28.64%	2.774%
13	9.369	1078	1085	1095	rBV	415672	688911	21.60%	2.092%
14	9.904	1166	1176	1195	rBV	636999	1168660	36.64%	3.548%
15	10.169	1219	1221	1228	rVB7	2802	3997	0.13%	0.012%
16	10.269	1231	1238	1247	rBV	598986	980790	30.75%	2.978%
17	10.416	1256	1263	1279	rBV	524942	1048308	32.86%	3.183%
18	11.151	1383	1388	1390	rBV3	2153	3255	0.10%	0.010%
19	11.892	1508	1514	1519	rBV6	7102	15067	0.47%	0.046%
20	13.216	1738	1739	1744	rBV3	2751	3192	0.10%	0.010%
21	13.574	1794	1800	1815	rBV	1030880	1535286	48.13%	4.662%
22	13.839	1838	1845	1857	rBV	1369935	1929825	60.50%	5.860%
23	14.151	1891	1898	1910	rBV	826826	1223769	38.36%	3.716%
24	14.386	1932	1938	1956	rBV2	177244	504461	15.81%	1.532%
25	14.568	1967	1969	1974	rVB5	4038	4938	0.15%	0.015%
26	15.068	2052	2054	2058	rBV4	2633	3446	0.11%	0.010%
27	15.151	2061	2068	2084	rVV	1729054	2397425	75.16%	7.279%
28	15.280	2084	2090	2105	rVV	364522	552287	17.31%	1.677%
29	15.392	2105	2109	2114	rVV5	9138	19329	0.61%	0.059%
30	15.445	2116	2118	2125	rVB6	2977	4460	0.14%	0.014%
31	15.615	2143	2147	2150	rBV6	2058	3393	0.11%	0.010%
32	15.739	2165	2168	2171	rVB6	2340	3199	0.10%	0.010%
33	16.692	2324	2330	2334	rBV5	3689	6714	0.21%	0.020%
34	16.904	2359	2366	2375	rBV	1047591	1429969	44.83%	4.342%
35	17.004	2375	2383	2400	rVV	1835839	2584709	81.03%	7.848%
36	17.698	2498	2501	2504	rBV5	2355	3628	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049503.D
Acq On : 29 Jan 2025 14:20
Operator : RC/JU
Sample : PB166307BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Title : SVOA CALIBRATION

37	17.839	2521	2525	2526	rBV3	2858	4333	0.14%	0.013%
38	18.274	2594	2599	2602	rBV7	2188	3620	0.11%	0.011%
39	18.874	2696	2701	2705	rBV3	17858	24131	0.76%	0.073%
40	18.945	2709	2713	2719	rVV	16359	22883	0.72%	0.069%
41	19.309	2769	2775	2790	rBV	2540207	3179159	99.66%	9.653%
42	19.715	2842	2844	2845	rBV2	5370	4351	0.14%	0.013%
43	21.139	3080	3086	3098	rBV	1091192	1637648	51.34%	4.972%
44	23.727	3518	3526	3540	rVB	1413890	3189878	100.00%	9.685%
45	23.915	3550	3558	3572	rBV	748561	1788898	56.08%	5.432%




Sum of corrected areas: 32934792

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049503.D
Acq On : 29 Jan 2025 14:20
Operator : RC/JU
Sample : PB166307BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

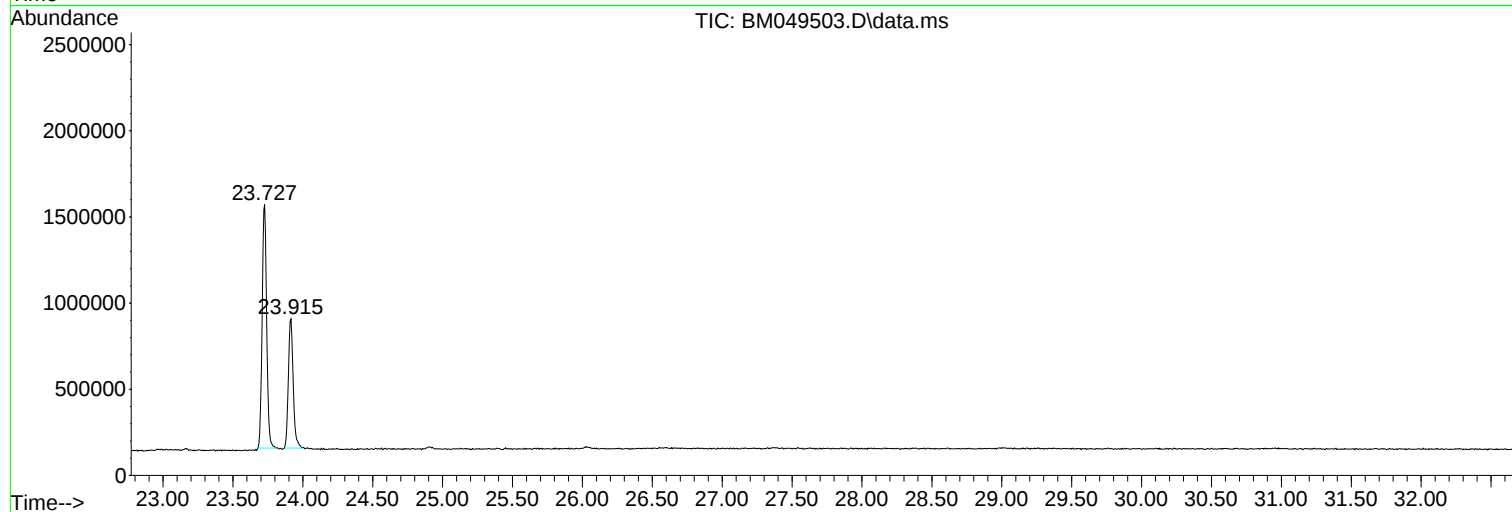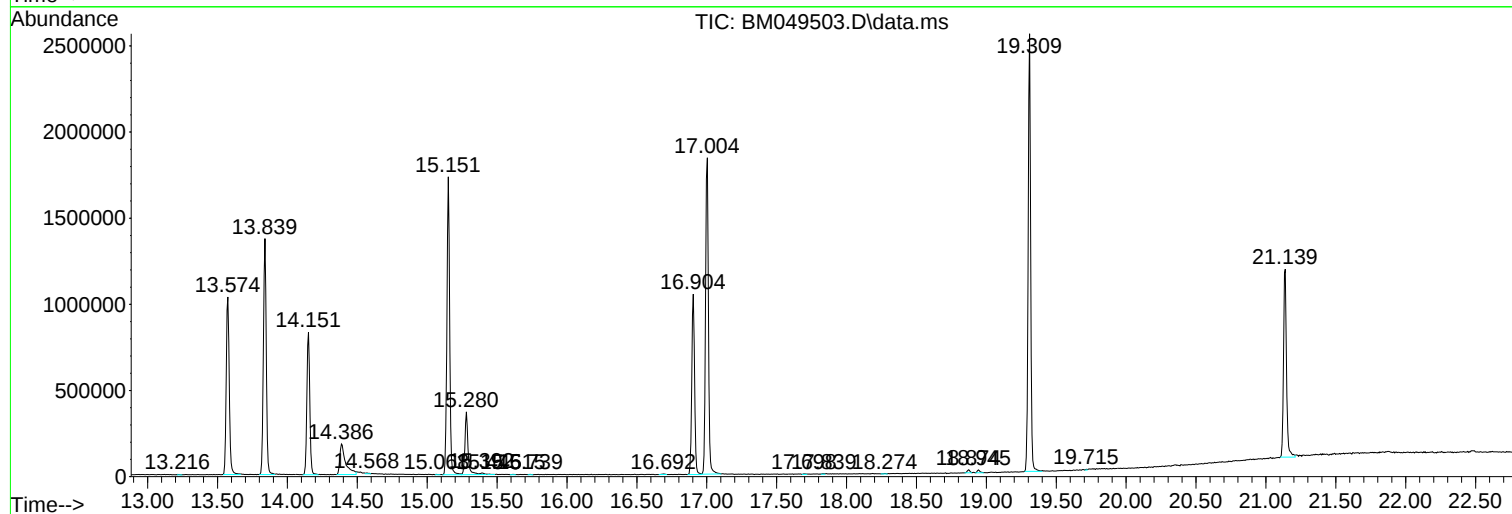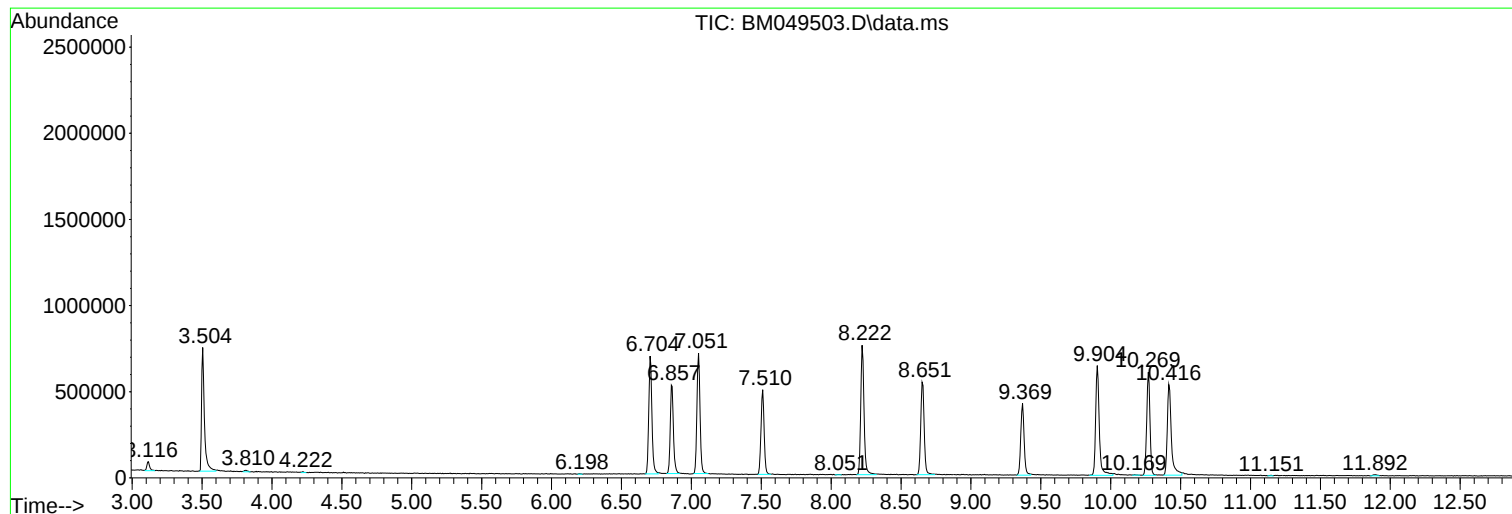

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049503.D
Acq On : 29 Jan 2025 14:20
Operator : RC/JU
Sample : PB166307BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012825\
Data File : BM049503.D
Acq On : 29 Jan 2025 14:20
Operator : RC/JU
Sample : PB166307BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------