
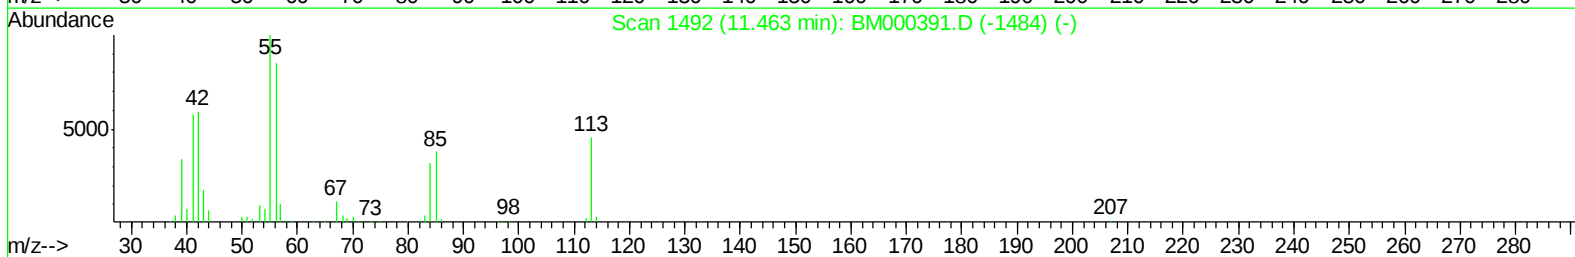
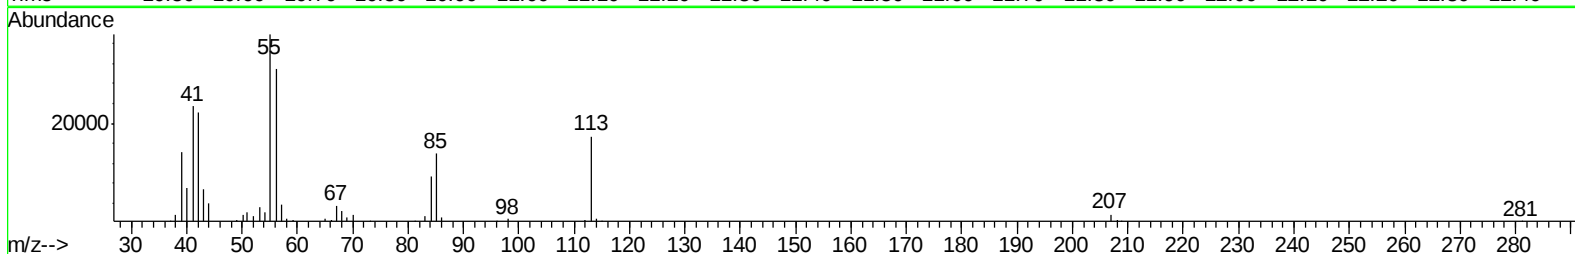


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
Data File : BM000402.D
Acq On : 30 Jan 2015 00:53
Operator : TP/IZ
Sample : SSTD02062
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jan 30 05:57:15 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 30 04:22:48 2015
Response via : Initial Calibration

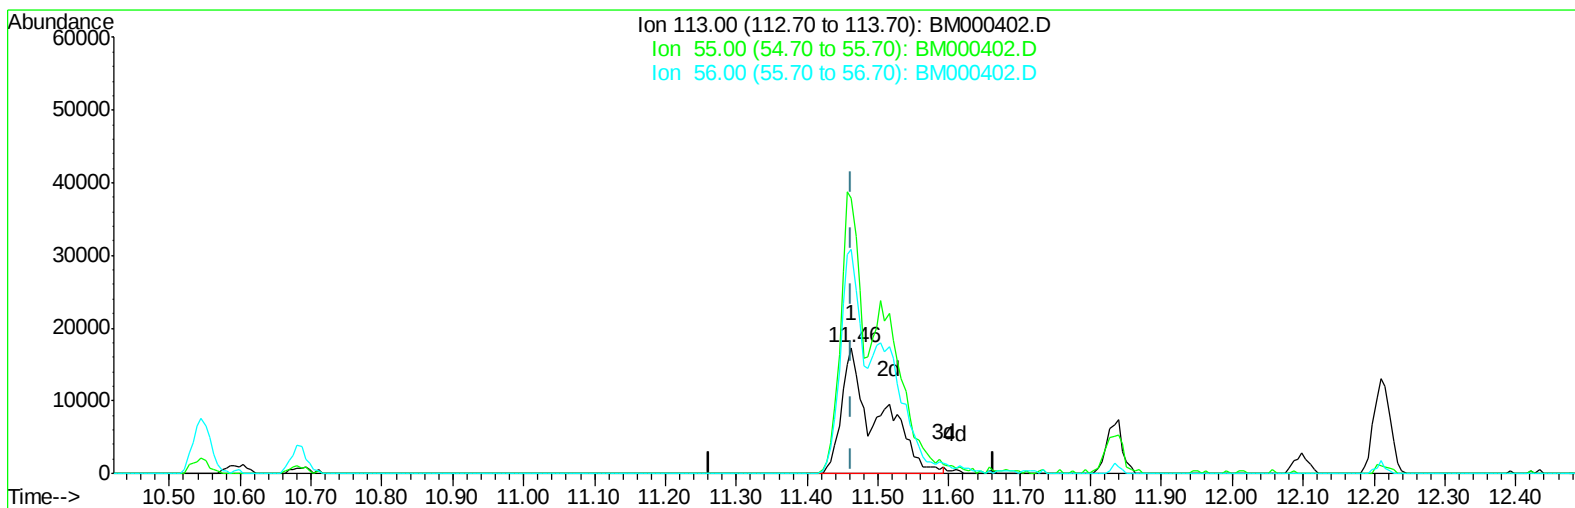

TIC: BM000402.D

(32) Caprolactam

11.463min (-0.000) 19.71ng/ul m

response 62285

Ion	Exp%	Act%
113.00	100	100
55.00	218.60	218.85
56.00	186.50	178.15
0.00	0.00	0.00