


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
 Data File : BM000388.D
 Acq On : 29 Jan 2015 15:25
 Operator : TP/IZ
 Sample : DFTPP13
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP13

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Title : SVOA CALIBRATION
 Last Update : Fri Jan 30 04:22:48 2015

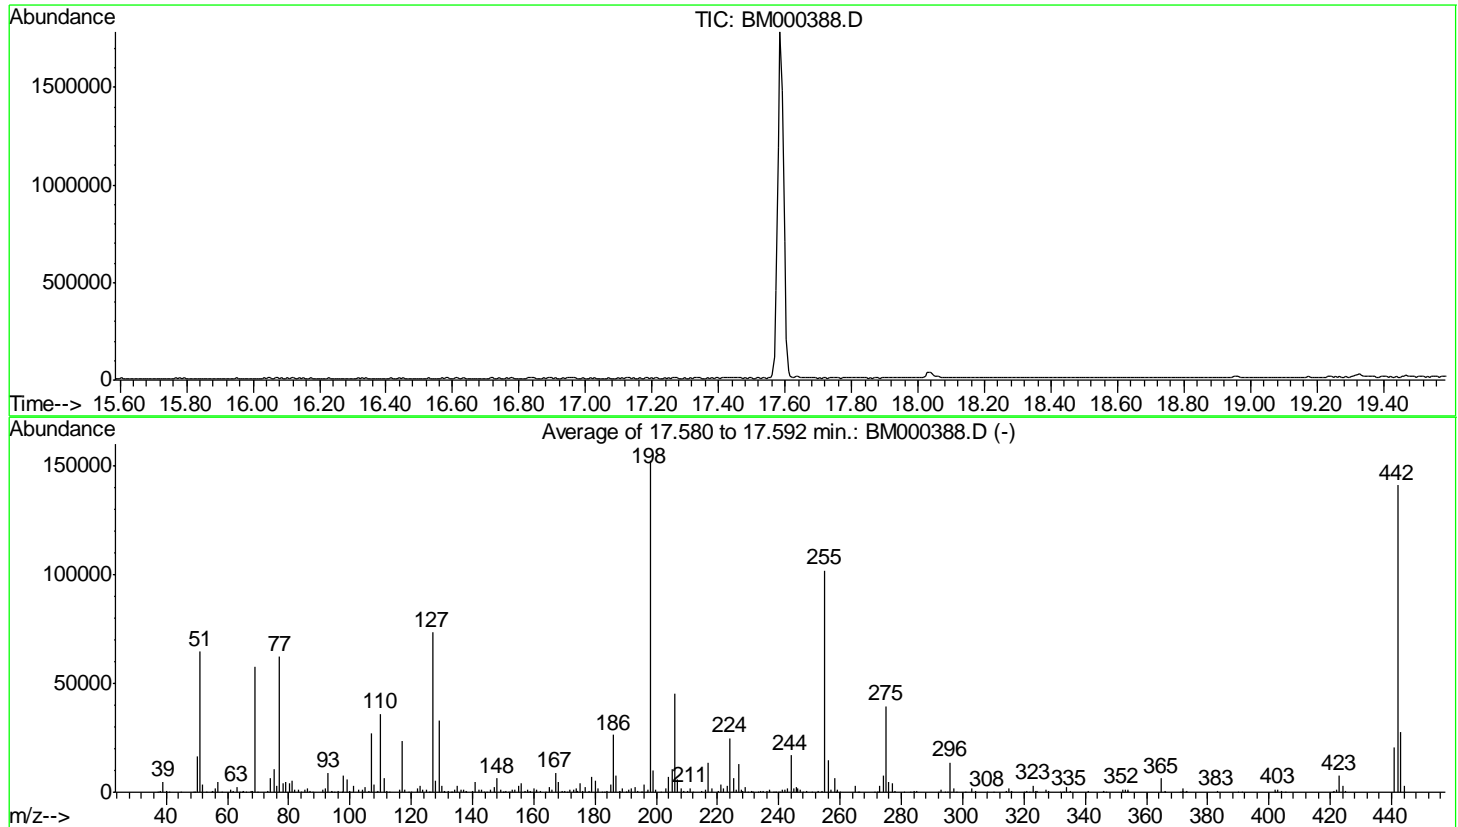

AutoFind: Scans 2532, 2533, 2534; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	64645	PASS
68	69	0.00	2	1.3	743	PASS
69	198	0.00	100	37.8	57480	PASS
70	69	0.00	2	0.3	184	PASS
127	198	10	80	48.1	73237	PASS
197	198	0.00	2	0.7	1088	PASS
198	198	100	100	100.0	152229	PASS
199	198	5	9	6.4	9762	PASS
275	198	10	60	25.9	39445	PASS
365	198	1	100	4.2	6347	PASS
441	443	0.01	100	74.7	20508	PASS
442	198	50	100	92.6	140952	PASS
443	442	15	24	19.5	27469	PASS