

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
 Data File : BM000394.D
 Acq On : 29 Jan 2015 20:10
 Operator : TP/IZ
 Sample : G1134-20RX
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB7RX

Manual Integrations
 APPROVED

apatel
 1/30/2015 5:53:16 PM

Quant Time: Jan 30 16:14:34 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 30 16:03:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	143645	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	622083	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	473427	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1037538	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	1111669	20.00	ng/ul	0.00
83) Perylene-d12	23.60	264	747041	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	5011m	2.59	ng/uL	0.00
5) Phenol-d5	6.92	99	62166	6.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	196002	30.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	207156	24.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	128828	14.75	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	128601	30.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	144379	32.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	280220	28.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	239	0.02	ng/ul	-0.12
43) Dimethylphthalate-d6	13.81	166	1167810	32.91	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	1334302	31.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.59	143	25720	4.76	ng/ul	-0.01
57) Fluorene-d10	15.39	176	1017397	32.76	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.51	200	164437	28.98	ng/ul	0.00
70) Anthracene-d10	17.24	188	1611326	33.50	ng/ul	0.00
76) Pyrene-d10	19.54	212	1816748	31.66	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.45	264	1099499	30.90	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.25	88	85806	31.59	ng/uL#	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
Data File : BM000394.D
Acq On : 29 Jan 2015 20:10
Operator : TP/IZ
Sample : G1134-20RX
Misc :
ALS Vial : 31 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AB7RX

Manual Integrations
APPROVED

apatel
1/30/2015 5:53:16 PM

Quant Time: Jan 30 16:14:34 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 30 16:03:45 2015
Response via : Initial Calibration

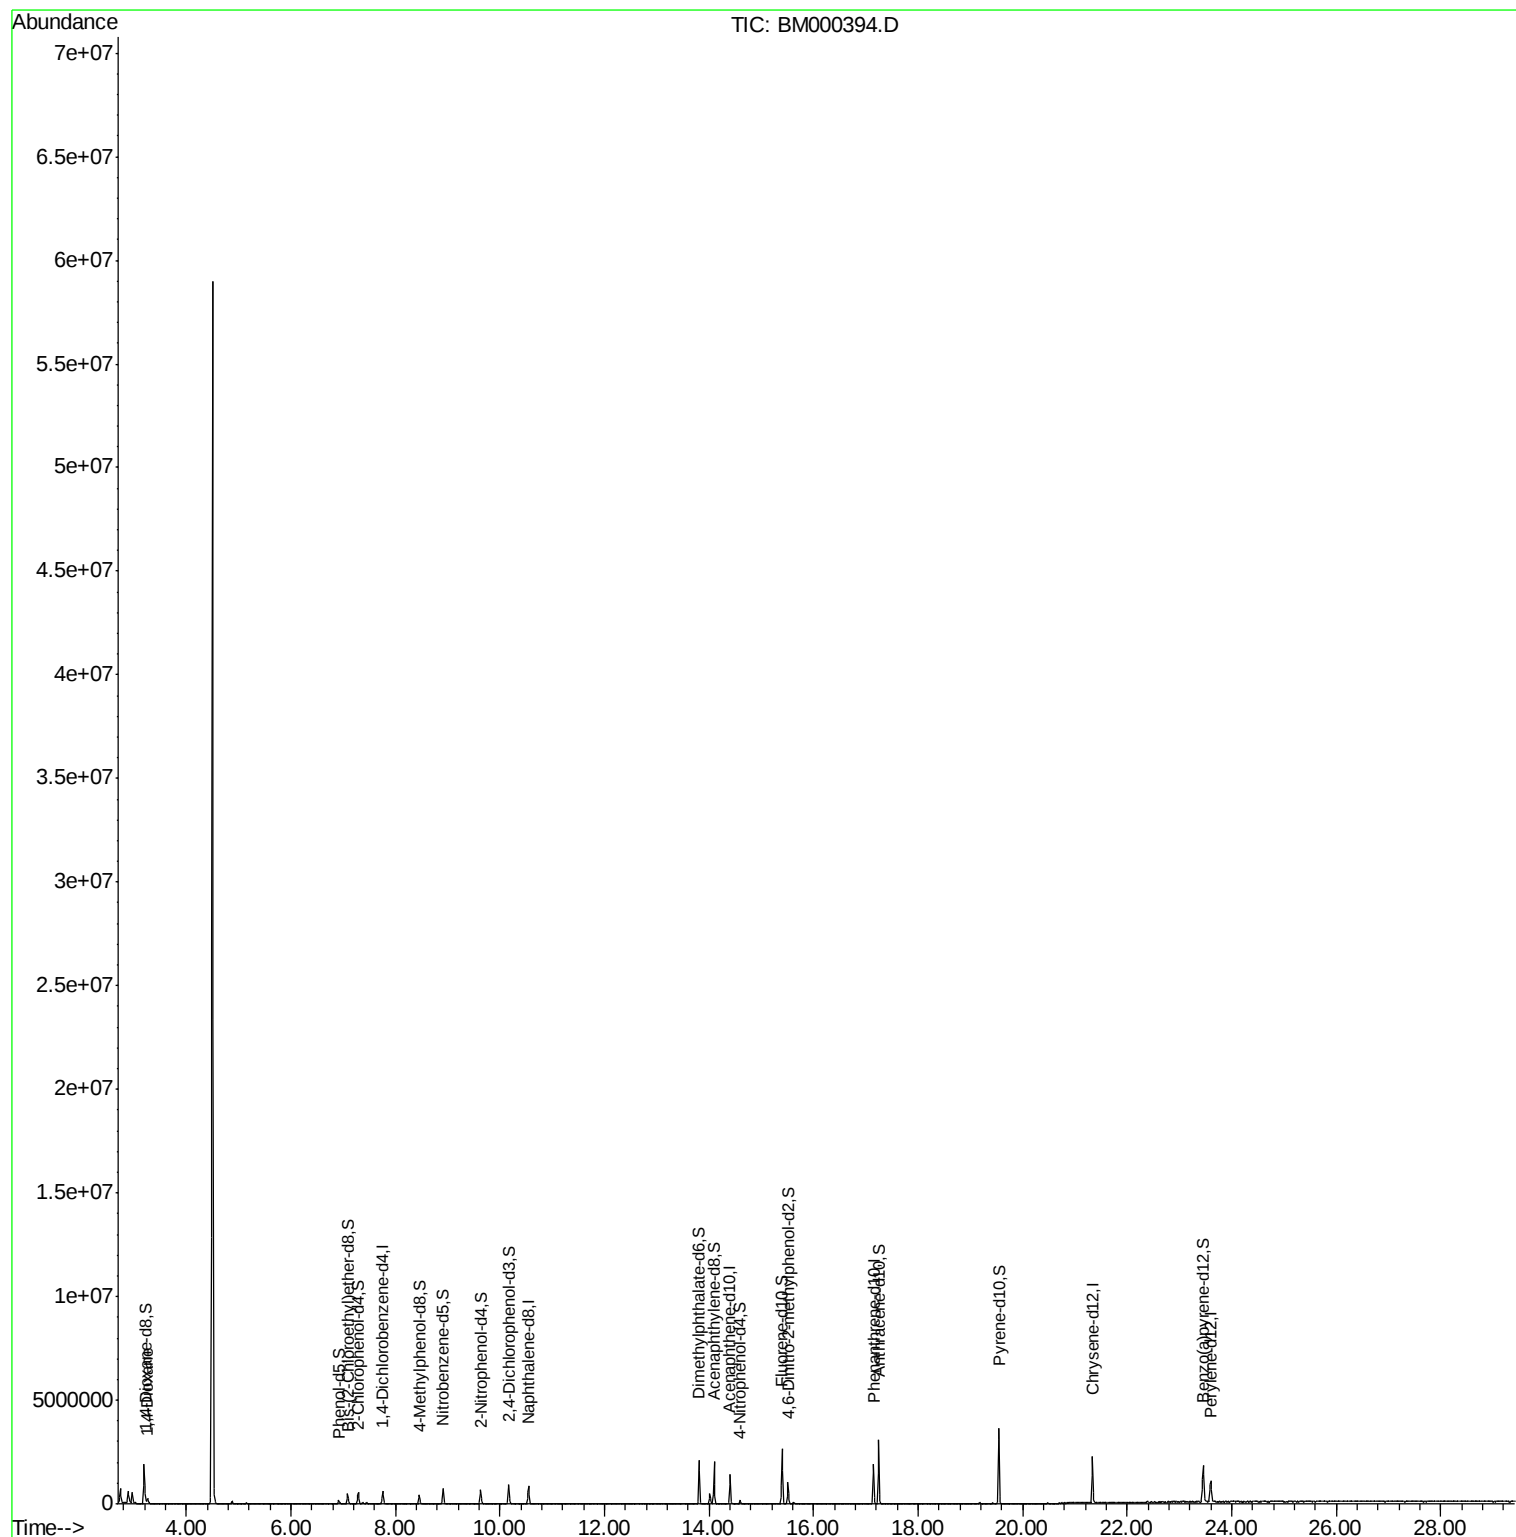

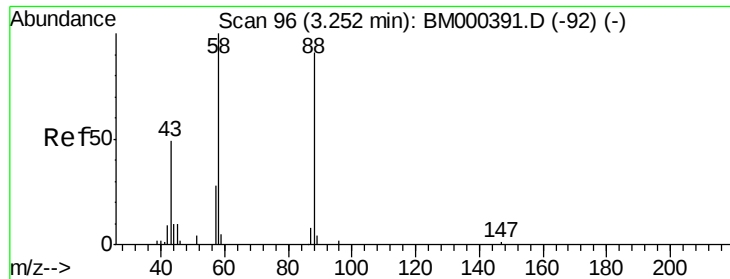

#2

1,4-Dioxane

Concen: 31.59 ng/uL

RT: 3.25 min Scan# 96

Delta R.T. 0.00 min

Lab File: BM000394.D

Acq: 29 Jan 2015 20:10

Instrument :

BNA_M

ClientSampleId :

C0AB7RX

Tgt Ion:	88	Resp:	85806
Ion Ratio	Lower	Upper	
88	100		
43	51.0	40.0	60.0
58	101.3	40.0	60.0

Manual Integrations
APPROVED

apatel
1/30/2015 5:53:16 PM

