

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
 Data File : BM000401.D
 Acq On : 30 Jan 2015 00:18
 Operator : TP/IZ
 Sample : G1115-02RXDL 25X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK4RXDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.881	29	33	44	rBV	90293	161638	5.57%	1.095%
2	2.957	44	46	51	rVB2	23202	29753	1.03%	0.202%
3	3.146	76	78	81	rBV4	3287	3324	0.11%	0.023%
4	3.193	81	86	93	rVV	441518	680300	23.46%	4.611%
5	3.251	93	96	103	rVB	55763	83447	2.88%	0.566%
6	3.357	113	114	120	rVB5	5147	6635	0.23%	0.045%
7	3.763	180	183	186	rBV4	4827	7185	0.25%	0.049%
8	3.828	193	194	196	rVV2	4490	3202	0.11%	0.022%
9	3.881	199	203	208	rBV6	3254	6486	0.22%	0.044%
10	4.028	226	228	230	rVB2	4745	3187	0.11%	0.022%
11	4.228	260	262	266	rVV3	3519	4131	0.14%	0.028%
12	4.381	286	288	291	rVB2	3062	3067	0.11%	0.021%
13	4.487	299	306	316	rVB	512551	805626	27.78%	5.460%
14	4.751	347	351	353	rVB3	3435	4326	0.15%	0.029%
15	4.851	365	368	373	rVB6	3843	6660	0.23%	0.045%
16	5.657	501	505	508	rBV4	3497	4845	0.17%	0.033%
17	5.916	547	549	554	rVB3	3472	5347	0.18%	0.036%
18	6.163	587	591	594	rBV5	2881	4341	0.15%	0.029%
19	6.381	626	628	631	rVB3	3376	3674	0.13%	0.025%
20	6.698	678	682	684	rBV2	3337	3609	0.12%	0.024%
21	6.916	716	719	723	rVB5	4312	4133	0.14%	0.028%
22	7.087	744	748	752	rBV4	7721	12395	0.43%	0.084%
23	7.245	771	775	778	rVB3	2430	3616	0.12%	0.025%
24	7.287	778	782	788	rBV4	10517	18366	0.63%	0.124%
25	7.357	791	794	800	rVV2	2267	4746	0.16%	0.032%
26	7.463	810	812	817	rVB3	2891	4451	0.15%	0.030%
27	7.692	848	851	854	rBV3	3398	4727	0.16%	0.032%
28	7.751	854	861	869	rVV	545970	886427	30.57%	6.008%
29	7.839	873	876	879	rVB3	2649	3023	0.10%	0.020%
30	8.451	977	980	987	rBV6	7212	12433	0.43%	0.084%
31	8.857	1044	1049	1052	rBV3	1935	3496	0.12%	0.024%
32	8.910	1052	1058	1063	rVV4	12411	18910	0.65%	0.128%
33	9.557	1167	1168	1172	rBV3	3276	3678	0.13%	0.025%
34	9.633	1176	1181	1187	rBV5	8928	16083	0.55%	0.109%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
 Data File : BM000401.D
 Acq On : 30 Jan 2015 00:18
 Operator : TP/IZ
 Sample : G1115-02RXDL 25X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK4RXDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Title : SVOA CALIBRATION

35	10.169	1266	1272	1276	rBV4	14942	23519	0.81%	0.159%
36	10.545	1326	1336	1344	rBV	760099	1242770	42.86%	8.423%
37	11.092	1426	1429	1431	rBV2	2772	3016	0.10%	0.020%
38	11.733	1533	1538	1540	rBV3	2050	3171	0.11%	0.021%
39	13.145	1775	1778	1783	rBV3	2342	3860	0.13%	0.026%
40	13.457	1829	1831	1833	rBV2	3250	3147	0.11%	0.021%
41	13.515	1838	1841	1847	rVB4	1905	3309	0.11%	0.022%
42	13.804	1887	1890	1896	rVV2	48078	66209	2.28%	0.449%
43	13.857	1896	1899	1902	rVB	5206	4963	0.17%	0.034%
44	14.010	1919	1925	1934	rBV4	34203	62742	2.16%	0.425%
45	14.092	1934	1939	1944	rVB2	38676	58749	2.03%	0.398%
46	14.398	1985	1991	1998	rBV	1235796	1810081	62.43%	12.268%
47	14.633	2028	2031	2034	rBV3	3066	3974	0.14%	0.027%
48	15.215	2127	2130	2132	rBV3	2563	3190	0.11%	0.022%
49	15.392	2155	2160	2165	rBV	74703	111271	3.84%	0.754%
50	15.515	2176	2181	2183	rBV5	9193	11680	0.40%	0.079%
51	16.174	2289	2293	2297	rVB2	2389	4166	0.14%	0.028%
52	16.351	2321	2323	2325	rVB3	4514	4457	0.15%	0.030%
53	16.392	2328	2330	2332	rBV2	3660	3770	0.13%	0.026%
54	16.680	2378	2379	2383	rBV2	2853	3375	0.12%	0.023%
55	16.856	2404	2409	2410	rVV2	2506	3281	0.11%	0.022%
56	16.933	2414	2422	2427	rVB5	8660	16229	0.56%	0.110%
57	17.145	2451	2458	2467	rVV2	1700410	2404161	82.92%	16.294%
58	17.245	2470	2475	2481	rVB2	85386	120266	4.15%	0.815%
59	17.692	2548	2551	2553	rBV3	3183	4106	0.14%	0.028%
60	17.815	2570	2572	2575	rBV4	3307	3671	0.13%	0.025%
61	17.880	2580	2583	2586	rVV3	2453	3190	0.11%	0.022%
62	18.039	2608	2610	2612	rBV	4379	3874	0.13%	0.026%
63	18.062	2612	2614	2617	rVB3	4122	4214	0.15%	0.029%
64	18.098	2617	2620	2623	rBV3	4157	5840	0.20%	0.040%
65	18.333	2657	2660	2663	rVB2	2612	2992	0.10%	0.020%
66	18.450	2677	2680	2682	rBV3	3110	3595	0.12%	0.024%
67	18.492	2685	2687	2690	rVB3	2678	3162	0.11%	0.021%
68	18.539	2693	2695	2697	rVB3	3815	3378	0.12%	0.023%
69	18.862	2748	2750	2754	rVB3	2931	3247	0.11%	0.022%
70	18.974	2766	2769	2772	rBV	5284	5474	0.19%	0.037%
71	19.003	2772	2774	2777	rVV4	4205	4018	0.14%	0.027%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
 Data File : BM000401.D
 Acq On : 30 Jan 2015 00:18
 Operator : TP/IZ
 Sample : G1115-02RXDL 25X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK4RXDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Title : SVOA CALIBRATION

72	19.274	2819	2820	2824	rBV4	3175	3579	0.12%	0.024%
73	19.339	2828	2831	2832	rVB3	5600	5099	0.18%	0.035%
74	19.368	2832	2836	2838	rBV3	6237	7318	0.25%	0.050%
75	19.474	2849	2854	2856	rVB4	4532	7712	0.27%	0.052%
76	19.539	2858	2865	2872	rVV2	93263	142011	4.90%	0.962%
77	19.650	2882	2884	2887	rVB3	3241	4248	0.15%	0.029%
78	19.686	2887	2890	2892	rVB3	5061	4377	0.15%	0.030%
79	19.715	2892	2895	2897	rBV3	4807	6120	0.21%	0.041%
80	19.803	2908	2910	2912	rBV2	2819	3196	0.11%	0.022%
81	19.939	2932	2933	2936	rVB3	4999	3921	0.14%	0.027%
82	19.968	2936	2938	2940	rBV4	4782	4887	0.17%	0.033%
83	20.033	2947	2949	2954	rBV5	3062	5823	0.20%	0.039%
84	20.174	2971	2973	2975	rBV3	3890	3411	0.12%	0.023%
85	20.209	2977	2979	2980	rBV2	4034	3824	0.13%	0.026%
86	20.333	2999	3000	3002	rBV2	3713	3287	0.11%	0.022%
87	20.515	3027	3031	3036	rBV8	8509	14892	0.51%	0.101%
88	20.574	3039	3041	3044	rVV3	5276	6225	0.21%	0.042%
89	20.603	3044	3046	3048	rVB3	4357	3078	0.11%	0.021%
90	21.003	3112	3114	3116	rBV2	5084	3941	0.14%	0.027%
91	21.044	3118	3121	3124	rVV6	8572	11788	0.41%	0.080%
92	21.127	3132	3135	3143	rBV7	20446	27790	0.96%	0.188%
93	21.286	3161	3162	3165	rBV3	6673	5188	0.18%	0.035%
94	21.333	3165	3170	3180	rBV	2248319	2899510	100.00%	19.651%
95	21.580	3210	3212	3213	rBV2	8426	5620	0.19%	0.038%
96	22.885	3431	3434	3440	rBV6	23155	36115	1.25%	0.245%
97	23.450	3523	3530	3539	rBV5	83765	202474	6.98%	1.372%
98	23.591	3547	3554	3566	rVB	1297359	2416649	83.35%	16.379%
99	23.703	3571	3573	3574	rBV2	13627	9055	0.31%	0.061%
100	24.103	3639	3641	3647	rVB7	30301	50443	1.74%	0.342%


Sum of corrected areas: 14754965

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
Data File : BM000401.D
Acq On : 30 Jan 2015 00:18
Operator : TP/IZ
Sample : G1115-02RXDL 25X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK4RXDL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

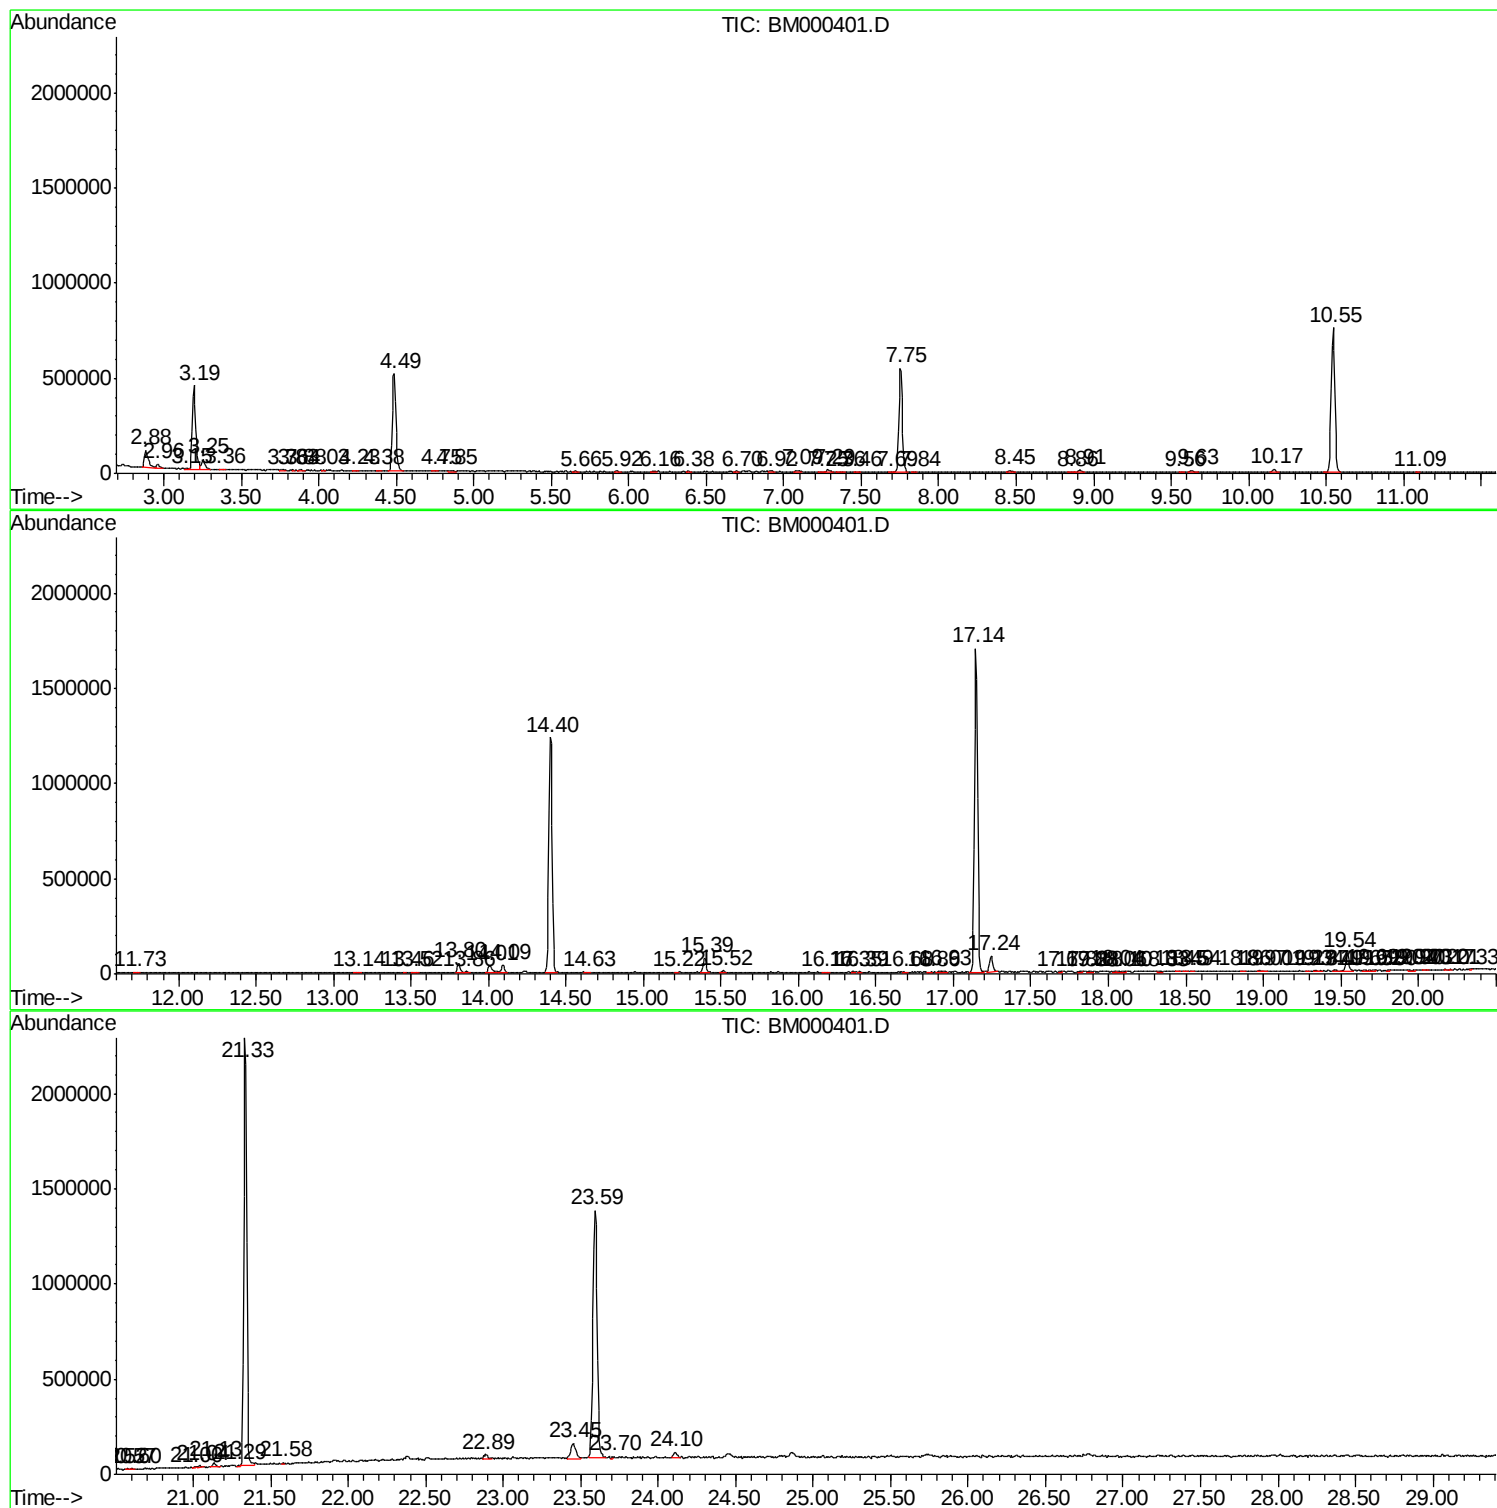

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
Data File : BM000401.D
Acq On : 30 Jan 2015 00:18
Operator : TP/IZ
Sample : G1115-02RXDL 25X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK4RXDL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012915\
Data File : BM000401.D
Acq On : 30 Jan 2015 00:18
Operator : TP/IZ
Sample : G1115-02RXDL 25X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK4RXDL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc