


Data Path : Z:\HPCHEM1\BNA_M\Data\BM012916\
Data File : BM004139.D
Acq On : 29 Jan 2016 09:58
Operator : SJ/IZ
Sample : DFTPP45
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP45

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM012916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 29 14:08:14 2016

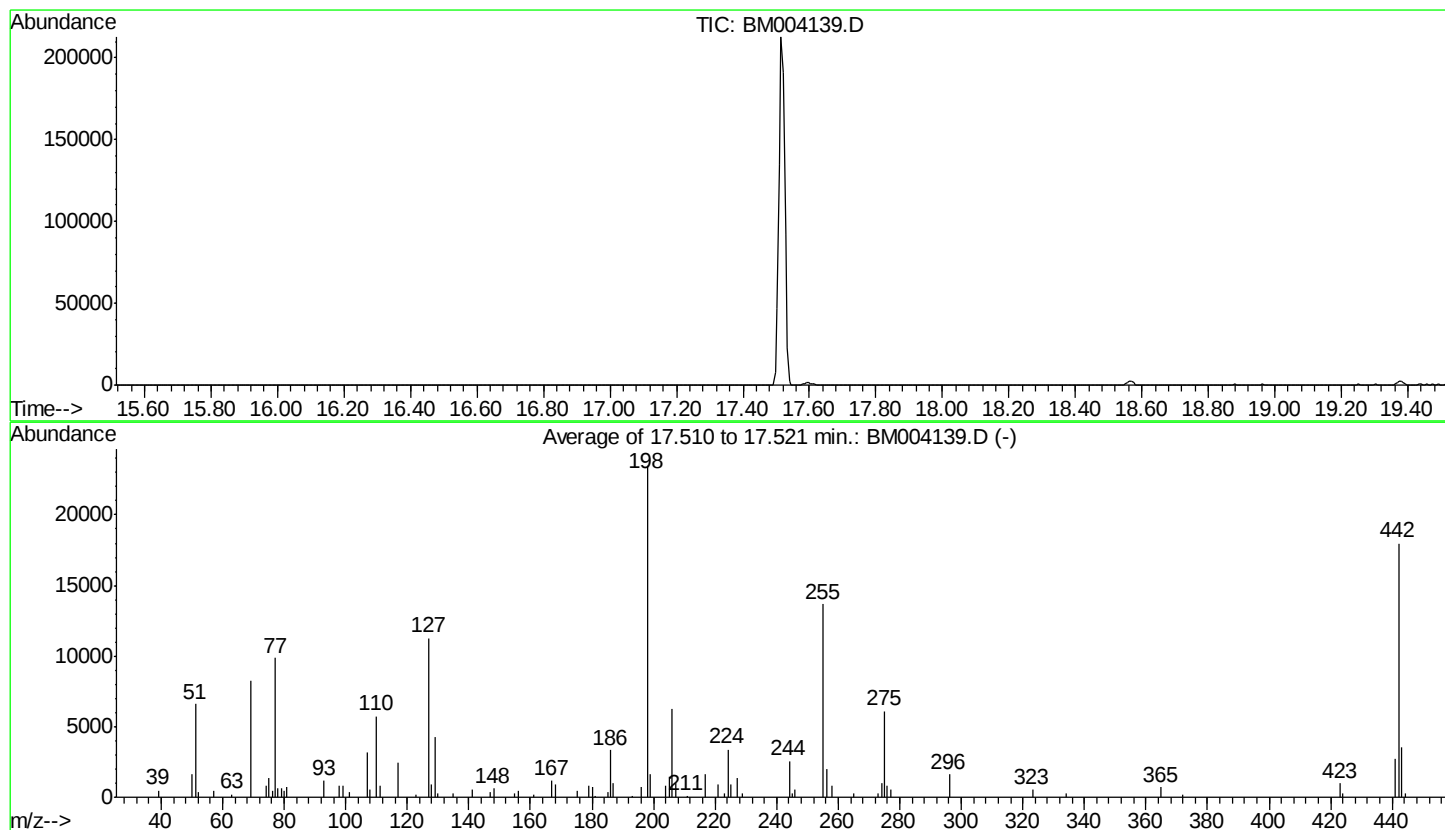

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	6588	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.1	8246	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	11284	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	23488	PASS
199	198	5	9	6.9	1624	PASS
275	198	10	60	26.0	6113	PASS
365	198	1	100	2.9	691	PASS
441	443	0.01	100	76.8	2719	PASS
442	198	50	100	76.4	17956	PASS
443	442	15	24	19.7	3541	PASS

m/z	Abundance
39.00	466.0
50.00	1466.0
51.10	5921.0
52.00	319.0
57.00	380.0
69.00	7271.0
74.00	723.0
75.00	1242.0
76.10	383.0
77.10	8660.0
78.10	619.0
79.00	575.0
80.00	413.0
81.00	647.0
93.00	1025.0
98.00	745.0
99.00	803.0
101.00	326.0
107.00	2652.0
108.00	466.0
110.00	4861.0
111.00	694.0
117.00	2073.0
127.00	9470.0
128.00	747.0
129.00	3524.0
141.00	466.0
147.00	321.0
148.00	563.0
156.10	376.0
167.00	960.0
168.00	831.0
175.00	358.0
179.00	626.0
180.00	617.0
185.00	310.0
186.10	2627.0
187.00	791.0
196.00	583.0
198.00	18448.0
199.00	1213.0
204.00	700.0
205.00	1077.0
206.10	4538.0
207.10	770.0
217.00	1176.0
221.00	688.0
224.10	2476.0
225.00	659.0
227.00	1094.0
244.10	1974.0
246.00	363.0
255.10	9788.0
256.10	1446.0
258.00	574.0
274.10	686.0
275.10	4290.0
276.00	615.0
277.00	398.0
296.00	1040.0
323.10	349.0
365.00	453.0
423.10	562.0
441.10	1608.0
442.20	9997.0
443.10	2063.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

m/z	Abundance
39.00	564.0
50.10	2006.0
51.10	7876.0
52.00	358.0
57.00	607.0
63.00	366.0
69.00	9891.0
74.00	1089.0
75.00	1573.0
76.10	569.0
77.10	11641.0
78.10	831.0
79.00	703.0
80.00	650.0
81.00	766.0
93.00	1456.0
98.00	1033.0
99.00	907.0
101.00	468.0
107.00	3687.0
108.00	618.0
110.00	6936.0
111.00	1006.0
117.00	2901.0
123.00	323.0
127.00	13398.0
128.00	1033.0
129.00	5091.0
130.00	465.0
135.00	416.0
141.00	627.0
147.00	403.0
148.00	685.0
155.00	389.0
156.00	532.0
161.00	334.0
167.00	1336.0
168.00	993.0
175.00	523.0
179.00	1021.0
180.00	890.0
181.00	343.0
185.00	459.0
186.10	4108.0
187.10	1201.0
193.00	352.0
196.00	754.0
198.00	27488.0
199.00	1899.0
204.00	981.0
205.10	1762.0
206.10	7581.0
207.10	1079.0
217.00	1798.0
221.10	970.0
223.10	412.0
224.10	3939.0
225.10	1040.0
227.00	1642.0
229.00	364.0
244.10	3105.0
245.10	360.0
246.00	659.0
255.10	15966.0
256.10	2446.0
258.10	847.0
265.00	320.0
273.00	442.0
274.00	1213.0
275.10	7222.0
276.10	974.0
277.00	622.0
296.10	1828.0
323.10	611.0
334.10	364.0
365.10	786.0
372.10	327.0
423.10	1091.0
424.10	473.0
441.10	2931.0
442.10	20640.0
443.10	4038.0
444.10	386.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

m/z	Abundance
39.10	428.0
50.00	1520.0
51.10	5968.0
52.00	315.0
57.00	430.0
63.00	301.0
69.00	7577.0
74.00	703.0
75.00	1247.0
76.10	450.0
77.10	9283.0
78.00	594.0
79.00	599.0
80.00	415.0
81.00	670.0
93.00	1044.0
98.00	807.0
99.00	704.0
101.00	376.0
107.00	3163.0
108.00	435.0
110.00	5477.0
111.00	866.0
117.00	2253.0
123.00	357.0
127.10	10984.0
128.00	839.0
129.00	4190.0
130.00	348.0
135.00	387.0
141.00	552.0
147.00	313.0
148.00	643.0
155.00	339.0
156.00	478.0
161.00	321.0
167.00	1170.0
168.00	842.0
175.00	448.0
179.00	885.0
180.00	708.0
185.10	460.0
186.10	3314.0
187.00	968.0
196.00	794.0
198.00	24528.0
199.00	1761.0
204.10	907.0
205.10	1529.0
206.10	6594.0
207.10	1059.0
210.90	300.0
217.00	1840.0
221.10	990.0
223.10	364.0
224.10	3759.0
225.00	950.0
227.00	1464.0
229.00	337.0
244.10	2651.0
245.10	353.0
246.00	504.0
255.10	15220.0
256.10	2040.0
258.00	956.0
265.10	374.0
273.10	472.0
274.00	1116.0
275.10	6827.0
276.00	907.0
277.00	545.0
296.00	1955.0
323.10	567.0
334.00	449.0
365.00	835.0
372.10	313.0
423.10	1258.0
424.10	419.0
441.10	3618.0
442.10	23232.0
443.20	4524.0
444.10	461.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

Scan 2450 (17.498 min): BM004139.D
DFTPP45

m/z	Abundance
51.00	643.0
69.00	900.0
77.10	914.0
107.00	340.0
110.00	462.0
127.00	882.0
129.00	395.0
198.00	1558.0
206.00	418.0
255.00	810.0
275.10	341.0
442.10	574.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

m/z Abundance

Instrument :
BNA_M
ClientSampleId :
DFTPP45