


Data Path : Z:\HPCHEM1\BNA\_M\Data\BM012916\  
Data File : BM004139.D  
Acq On : 29 Jan 2016 09:58  
Operator : SJ/IZ  
Sample : DFTPP45  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM012916.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Jan 29 14:08:14 2016

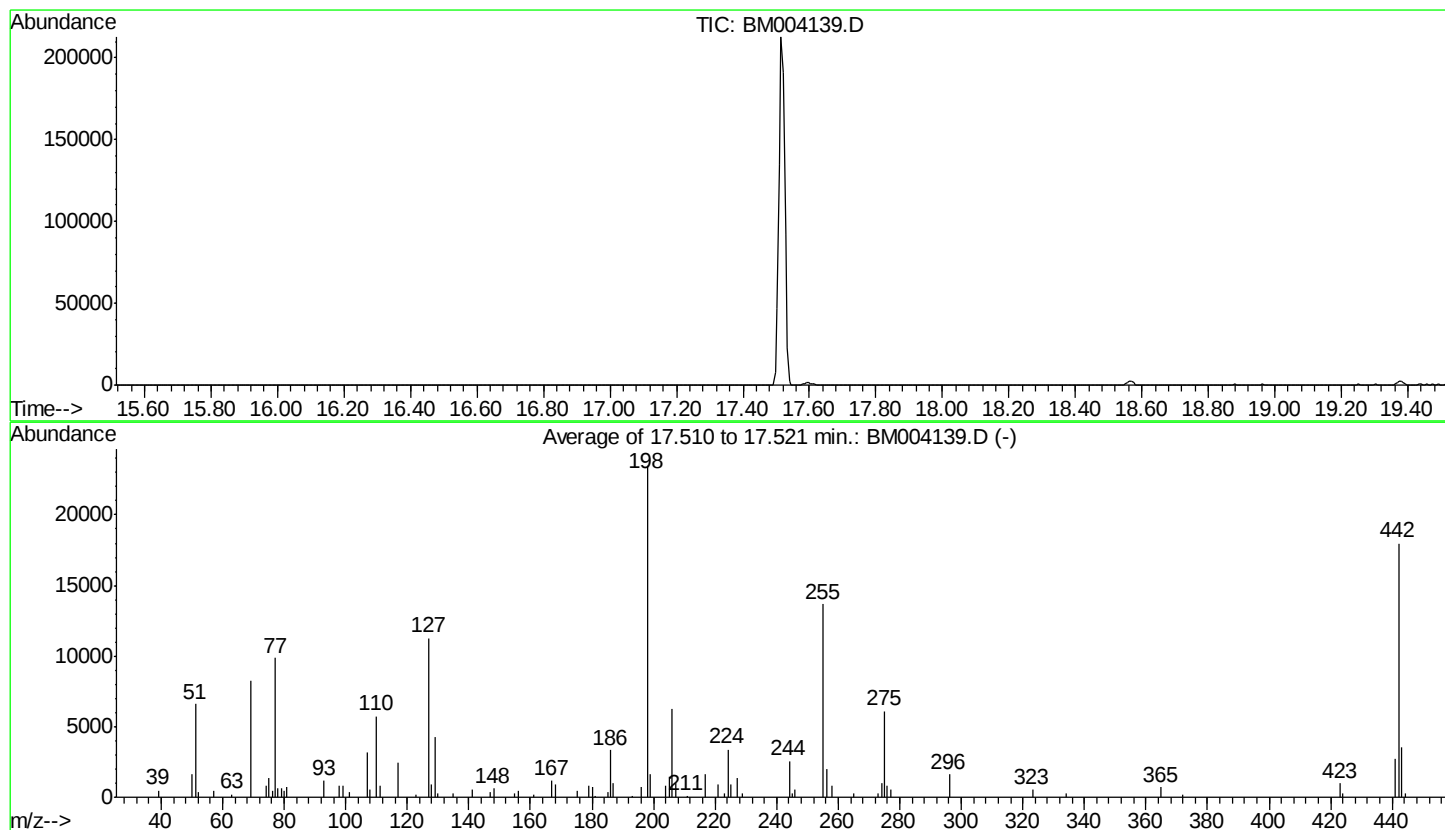

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 28.0      | 6588    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 35.1      | 8246    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 48.0      | 11284   | PASS             |
| 197         | 198          | 0.00         | 1            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 23488   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 1624    | PASS             |
| 275         | 198          | 10           | 60           | 26.0      | 6113    | PASS             |
| 365         | 198          | 1            | 100          | 2.9       | 691     | PASS             |
| 441         | 443          | 0.01         | 100          | 76.8      | 2719    | PASS             |
| 442         | 198          | 50           | 100          | 76.4      | 17956   | PASS             |
| 443         | 442          | 15           | 24           | 19.7      | 3541    | PASS             |

| m/z    | Abundance |
|--------|-----------|
| 39.00  | 466.0     |
| 50.00  | 1466.0    |
| 51.10  | 5921.0    |
| 52.00  | 319.0     |
| 57.00  | 380.0     |
| 69.00  | 7271.0    |
| 74.00  | 723.0     |
| 75.00  | 1242.0    |
| 76.10  | 383.0     |
| 77.10  | 8660.0    |
| 78.10  | 619.0     |
| 79.00  | 575.0     |
| 80.00  | 413.0     |
| 81.00  | 647.0     |
| 93.00  | 1025.0    |
| 98.00  | 745.0     |
| 99.00  | 803.0     |
| 101.00 | 326.0     |
| 107.00 | 2652.0    |
| 108.00 | 466.0     |
| 110.00 | 4861.0    |
| 111.00 | 694.0     |
| 117.00 | 2073.0    |
| 127.00 | 9470.0    |
| 128.00 | 747.0     |
| 129.00 | 3524.0    |
| 141.00 | 466.0     |
| 147.00 | 321.0     |
| 148.00 | 563.0     |
| 156.10 | 376.0     |
| 167.00 | 960.0     |
| 168.00 | 831.0     |
| 175.00 | 358.0     |
| 179.00 | 626.0     |
| 180.00 | 617.0     |
| 185.00 | 310.0     |
| 186.10 | 2627.0    |
| 187.00 | 791.0     |
| 196.00 | 583.0     |
| 198.00 | 18448.0   |
| 199.00 | 1213.0    |
| 204.00 | 700.0     |
| 205.00 | 1077.0    |
| 206.10 | 4538.0    |
| 207.10 | 770.0     |
| 217.00 | 1176.0    |
| 221.00 | 688.0     |
| 224.10 | 2476.0    |
| 225.00 | 659.0     |
| 227.00 | 1094.0    |
| 244.10 | 1974.0    |
| 246.00 | 363.0     |
| 255.10 | 9788.0    |
| 256.10 | 1446.0    |
| 258.00 | 574.0     |
| 274.10 | 686.0     |
| 275.10 | 4290.0    |
| 276.00 | 615.0     |
| 277.00 | 398.0     |
| 296.00 | 1040.0    |
| 323.10 | 349.0     |
| 365.00 | 453.0     |
| 423.10 | 562.0     |
| 441.10 | 1608.0    |
| 442.20 | 9997.0    |
| 443.10 | 2063.0    |

Instrument :  
BNA\_M  
ClientSampleId :

| m/z    | Abundance |
|--------|-----------|
| 39.00  | 564.0     |
| 50.10  | 2006.0    |
| 51.10  | 7876.0    |
| 52.00  | 358.0     |
| 57.00  | 607.0     |
| 63.00  | 366.0     |
| 69.00  | 9891.0    |
| 74.00  | 1089.0    |
| 75.00  | 1573.0    |
| 76.10  | 569.0     |
| 77.10  | 11641.0   |
| 78.10  | 831.0     |
| 79.00  | 703.0     |
| 80.00  | 650.0     |
| 81.00  | 766.0     |
| 93.00  | 1456.0    |
| 98.00  | 1033.0    |
| 99.00  | 907.0     |
| 101.00 | 468.0     |
| 107.00 | 3687.0    |
| 108.00 | 618.0     |
| 110.00 | 6936.0    |
| 111.00 | 1006.0    |
| 117.00 | 2901.0    |
| 123.00 | 323.0     |
| 127.00 | 13398.0   |
| 128.00 | 1033.0    |
| 129.00 | 5091.0    |
| 130.00 | 465.0     |
| 135.00 | 416.0     |
| 141.00 | 627.0     |
| 147.00 | 403.0     |
| 148.00 | 685.0     |
| 155.00 | 389.0     |
| 156.00 | 532.0     |
| 161.00 | 334.0     |
| 167.00 | 1336.0    |
| 168.00 | 993.0     |
| 175.00 | 523.0     |
| 179.00 | 1021.0    |
| 180.00 | 890.0     |
| 181.00 | 343.0     |
| 185.00 | 459.0     |
| 186.10 | 4108.0    |
| 187.10 | 1201.0    |
| 193.00 | 352.0     |
| 196.00 | 754.0     |
| 198.00 | 27488.0   |
| 199.00 | 1899.0    |
| 204.00 | 981.0     |
| 205.10 | 1762.0    |
| 206.10 | 7581.0    |
| 207.10 | 1079.0    |
| 217.00 | 1798.0    |
| 221.10 | 970.0     |
| 223.10 | 412.0     |
| 224.10 | 3939.0    |
| 225.10 | 1040.0    |
| 227.00 | 1642.0    |
| 229.00 | 364.0     |
| 244.10 | 3105.0    |
| 245.10 | 360.0     |
| 246.00 | 659.0     |
| 255.10 | 15966.0   |
| 256.10 | 2446.0    |
| 258.10 | 847.0     |
| 265.00 | 320.0     |
| 273.00 | 442.0     |
| 274.00 | 1213.0    |
| 275.10 | 7222.0    |
| 276.10 | 974.0     |
| 277.00 | 622.0     |
| 296.10 | 1828.0    |
| 323.10 | 611.0     |
| 334.10 | 364.0     |
| 365.10 | 786.0     |
| 372.10 | 327.0     |
| 423.10 | 1091.0    |
| 424.10 | 473.0     |
| 441.10 | 2931.0    |
| 442.10 | 20640.0   |
| 443.10 | 4038.0    |
| 444.10 | 386.0     |

Instrument :  
BNA\_M  
ClientSampleId :

| m/z    | Abundance |
|--------|-----------|
| 39.10  | 428.0     |
| 50.00  | 1520.0    |
| 51.10  | 5968.0    |
| 52.00  | 315.0     |
| 57.00  | 430.0     |
| 63.00  | 301.0     |
| 69.00  | 7577.0    |
| 74.00  | 703.0     |
| 75.00  | 1247.0    |
| 76.10  | 450.0     |
| 77.10  | 9283.0    |
| 78.00  | 594.0     |
| 79.00  | 599.0     |
| 80.00  | 415.0     |
| 81.00  | 670.0     |
| 93.00  | 1044.0    |
| 98.00  | 807.0     |
| 99.00  | 704.0     |
| 101.00 | 376.0     |
| 107.00 | 3163.0    |
| 108.00 | 435.0     |
| 110.00 | 5477.0    |
| 111.00 | 866.0     |
| 117.00 | 2253.0    |
| 123.00 | 357.0     |
| 127.10 | 10984.0   |
| 128.00 | 839.0     |
| 129.00 | 4190.0    |
| 130.00 | 348.0     |
| 135.00 | 387.0     |
| 141.00 | 552.0     |
| 147.00 | 313.0     |
| 148.00 | 643.0     |
| 155.00 | 339.0     |
| 156.00 | 478.0     |
| 161.00 | 321.0     |
| 167.00 | 1170.0    |
| 168.00 | 842.0     |
| 175.00 | 448.0     |
| 179.00 | 885.0     |
| 180.00 | 708.0     |
| 185.10 | 460.0     |
| 186.10 | 3314.0    |
| 187.00 | 968.0     |
| 196.00 | 794.0     |
| 198.00 | 24528.0   |
| 199.00 | 1761.0    |
| 204.10 | 907.0     |
| 205.10 | 1529.0    |
| 206.10 | 6594.0    |
| 207.10 | 1059.0    |
| 210.90 | 300.0     |
| 217.00 | 1840.0    |
| 221.10 | 990.0     |
| 223.10 | 364.0     |
| 224.10 | 3759.0    |
| 225.00 | 950.0     |
| 227.00 | 1464.0    |
| 229.00 | 337.0     |
| 244.10 | 2651.0    |
| 245.10 | 353.0     |
| 246.00 | 504.0     |
| 255.10 | 15220.0   |
| 256.10 | 2040.0    |
| 258.00 | 956.0     |
| 265.10 | 374.0     |
| 273.10 | 472.0     |
| 274.00 | 1116.0    |
| 275.10 | 6827.0    |
| 276.00 | 907.0     |
| 277.00 | 545.0     |
| 296.00 | 1955.0    |
| 323.10 | 567.0     |
| 334.00 | 449.0     |
| 365.00 | 835.0     |
| 372.10 | 313.0     |
| 423.10 | 1258.0    |
| 424.10 | 419.0     |
| 441.10 | 3618.0    |
| 442.10 | 23232.0   |
| 443.20 | 4524.0    |
| 444.10 | 461.0     |

Instrument :  
BNA\_M  
ClientSampleId :

| m/z    | Abundance |
|--------|-----------|
| 51.00  | 643.0     |
| 69.00  | 900.0     |
| 77.10  | 914.0     |
| 107.00 | 340.0     |
| 110.00 | 462.0     |
| 127.00 | 882.0     |
| 129.00 | 395.0     |
| 198.00 | 1558.0    |
| 206.00 | 418.0     |
| 255.00 | 810.0     |
| 275.10 | 341.0     |
| 442.10 | 574.0     |

Instrument :

BNA\_M

ClientSampleId :