

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012918\
 Data File : BM013994.D
 Acq On : 30 Jan 2018 13:10
 Operator : SJ/JU
 Sample : PB106171BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 30 13:49:44 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 30 07:49:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	76218	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	297249	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	185832	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	434141	20.00	ng/ul	0.00
75) Chrysene-d12	21.18	240	500533	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	522841	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	11757	6.10	ng/uL	0.00
5) Phenol-d5	6.76	99	172725	29.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	106007	29.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	148816	31.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	146649	32.60	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	78016	33.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	77972	31.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	138114	29.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	182173	44.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	517957	33.82	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	641763	32.86	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	42302	17.00	ng/ul	0.01
57) Fluorene-d10	15.22	176	449768	33.39	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	60740	23.24	ng/ul	0.00
70) Anthracene-d10	16.97	188	434141	20.53	ng/ul	-0.10
76) Pyrene-d10	19.38	212	823008	35.32	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.22	264	846253	35.21	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.29	70	4621	1.272	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012918\
Data File : BM013994.D
Acq On : 30 Jan 2018 13:10
Operator : SJ/JU
Sample : PB106171BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 30 13:49:44 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 30 07:49:34 2018
Response via : Initial Calibration

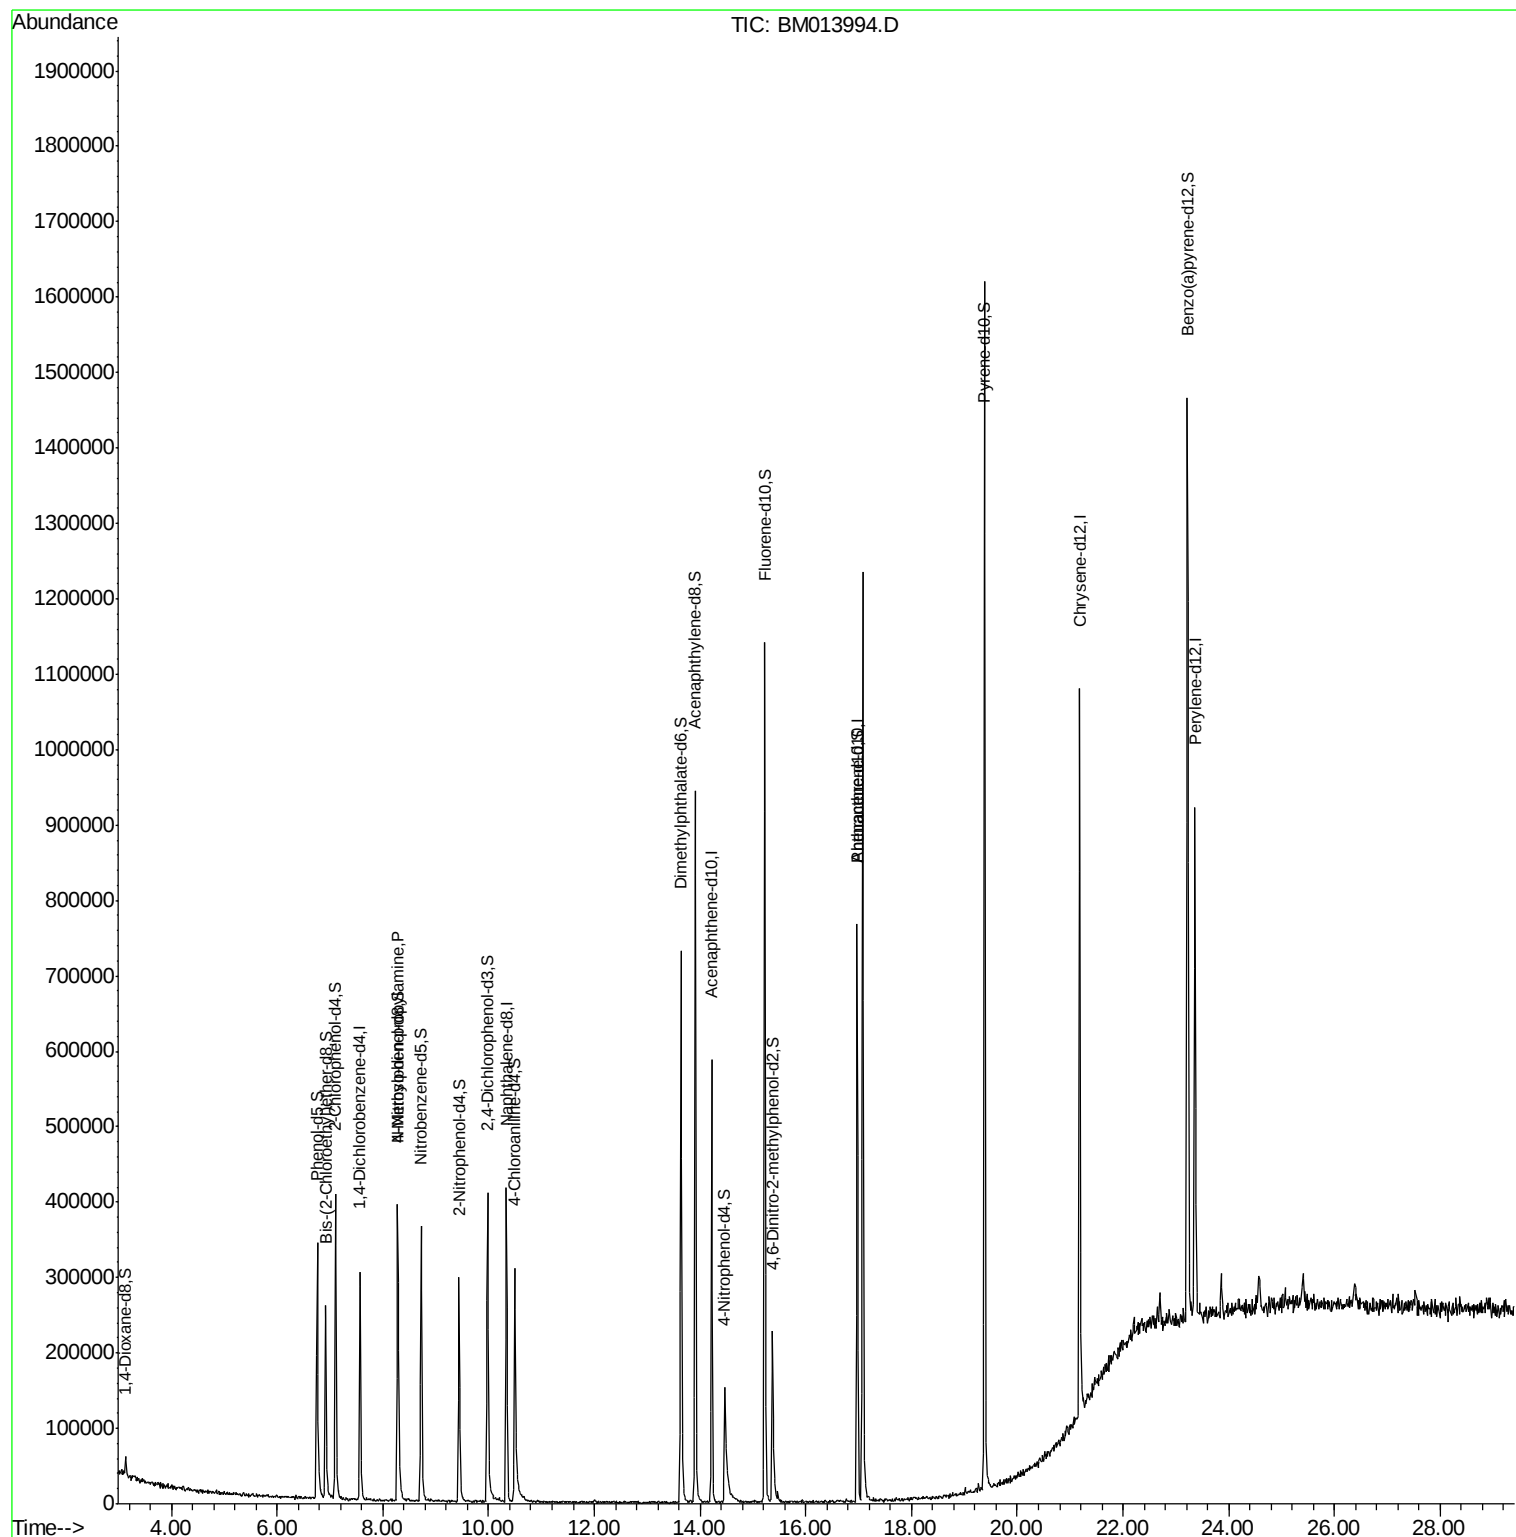

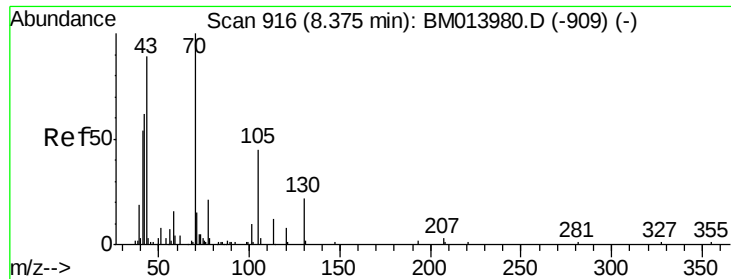

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.272 ng/ul
 RT: 8.29 min Scan# 901
 Delta R.T. -0.09 min
 Lab File: BM013994.D
 Acq: 30 Jan 2018 13:10

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 4621
 Ion Ratio Lower Upper
 70 100
 42 340.8 76.0 114.0#
 101 0.0 6.7 10.1#
 130 0.0 14.6 22.0#

