
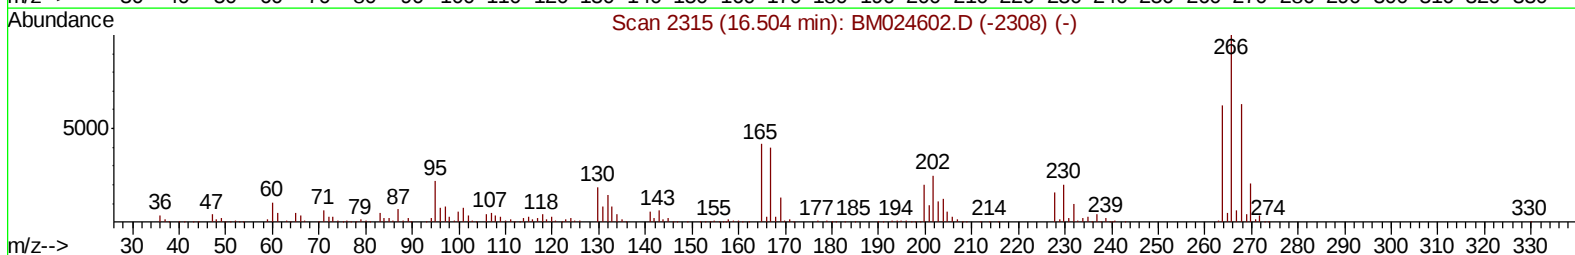
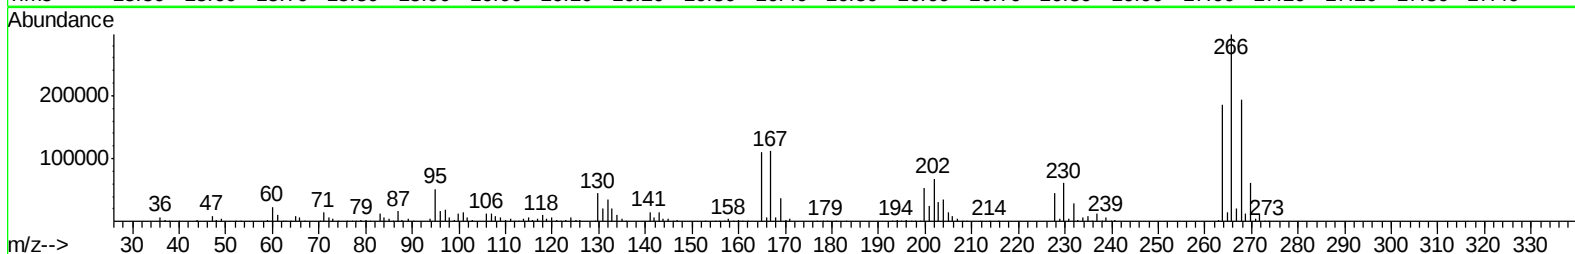


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012920\
Data File : BM024640.D
Acq On : 29 Jan 2020 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:36:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 23 14:57:07 2020
Response via : Initial Calibration

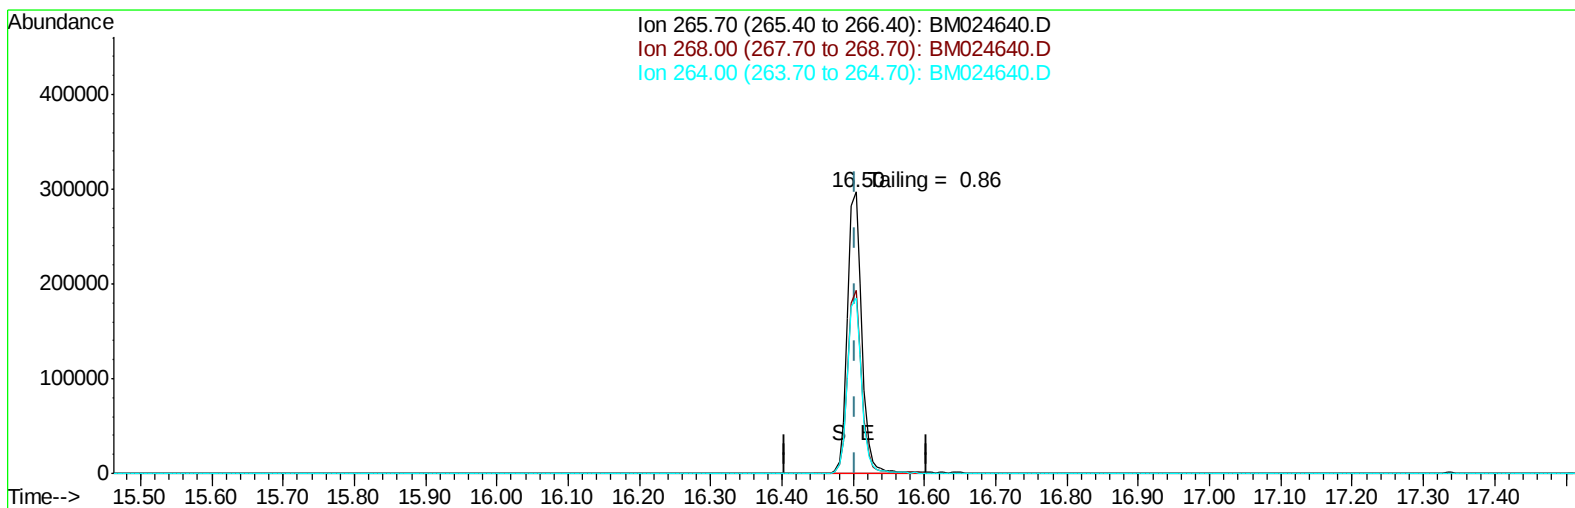

TIC: BM024640.D

(70) Pentachlorophenol (C)




16.504min (-0.000) 410179.74ng

response 388640

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	65.08
264.00	62.40	62.15
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012920\
 Data File : BM024640.D
 Acq On : 29 Jan 2020 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:36:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 23 14:57:07 2020
 Response via : Initial Calibration

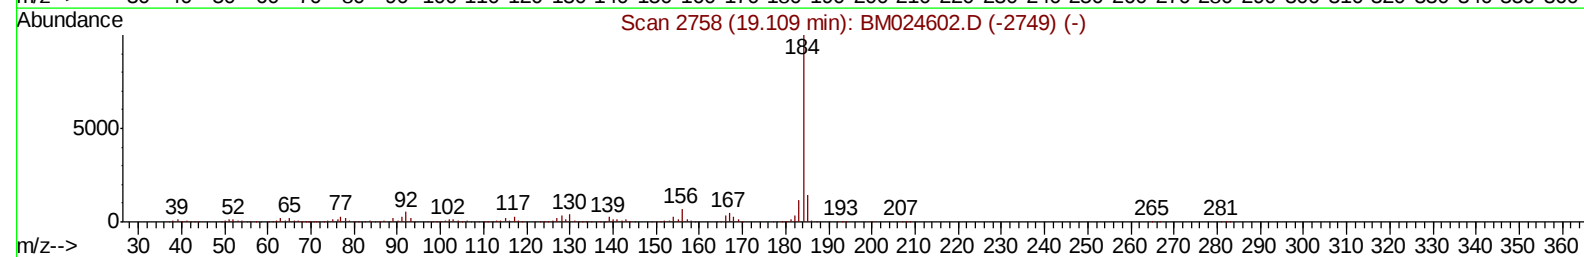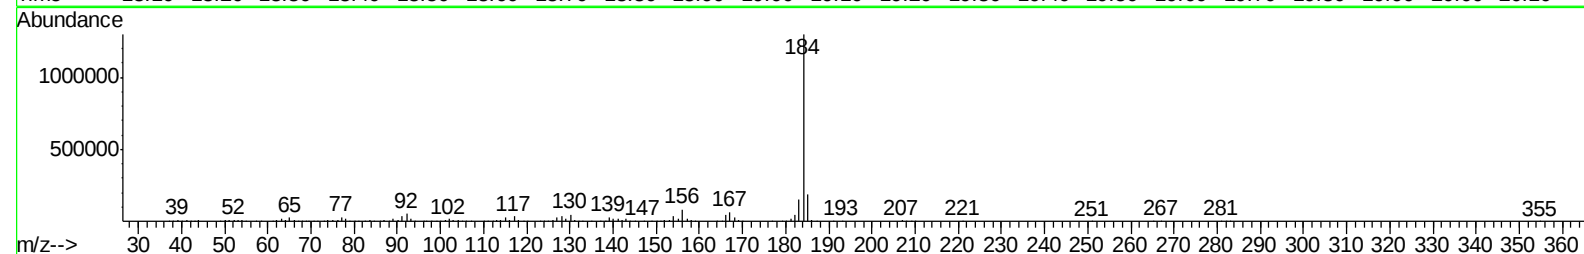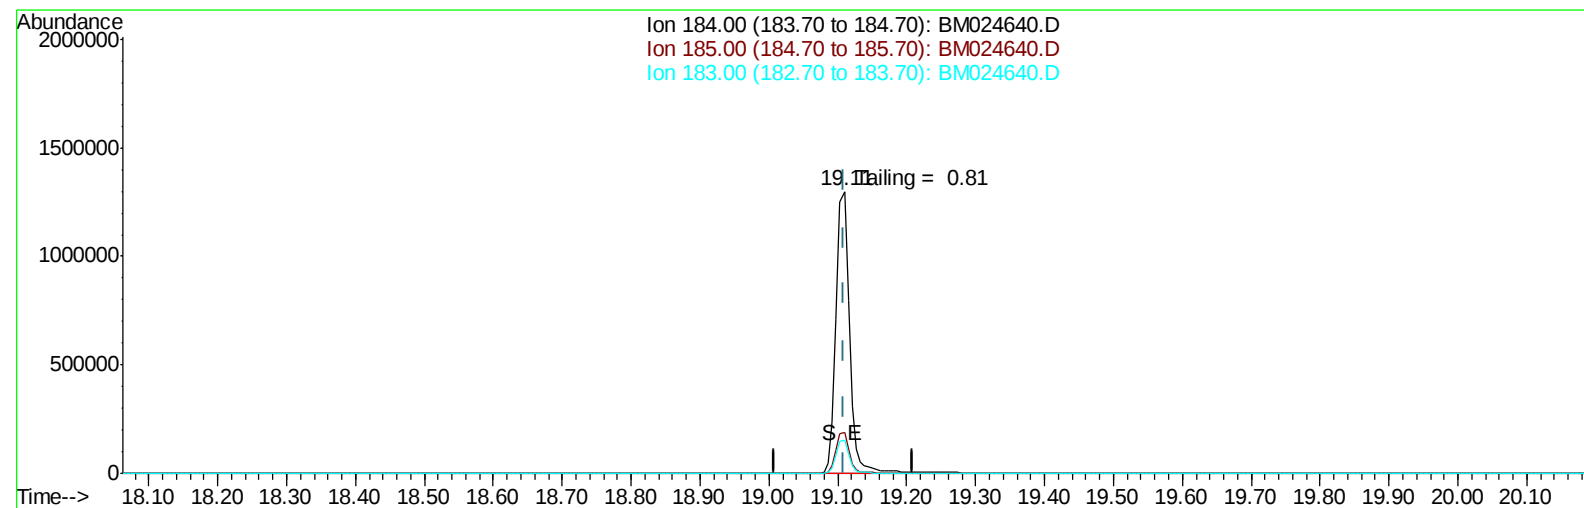

TIC: BM024640.D

(77) Benzidine

19.109min (-0.000) 0.00ng

response 1757337

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.54
183.00	12.00	11.72
0.00	0.00	0.00