
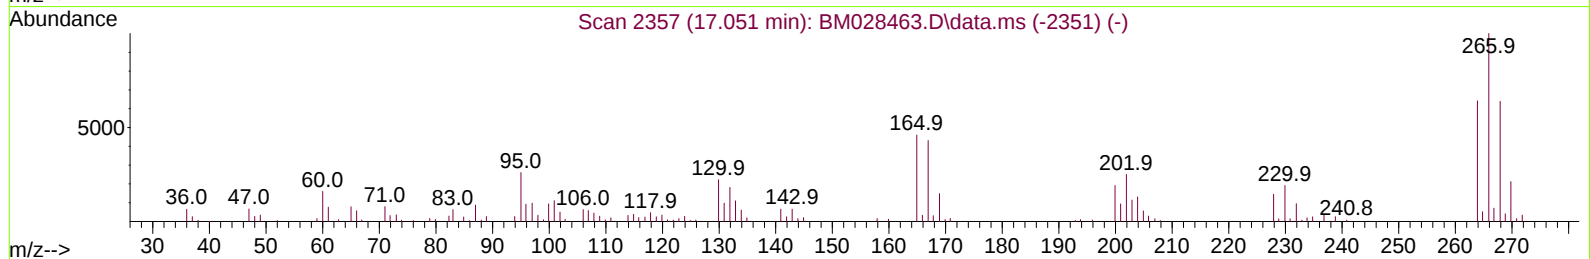
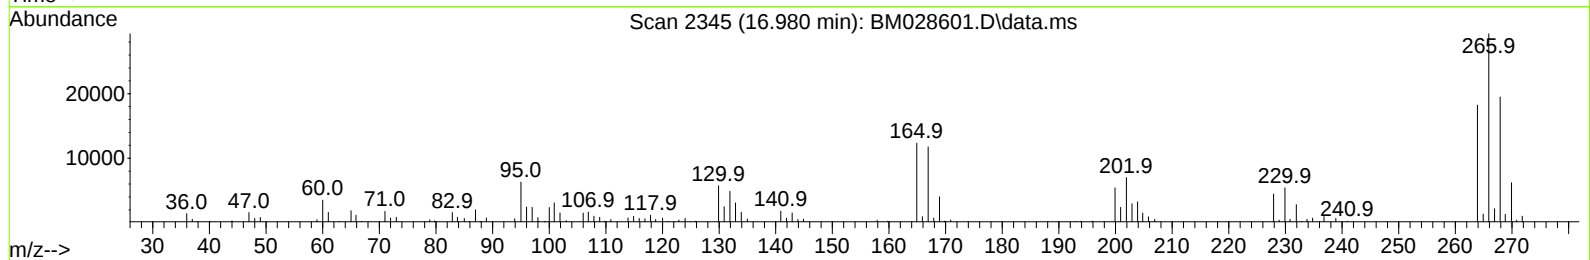


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012921\
Data File : BM028601.D
Acq On : 29 Jan 2021 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 01:36:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

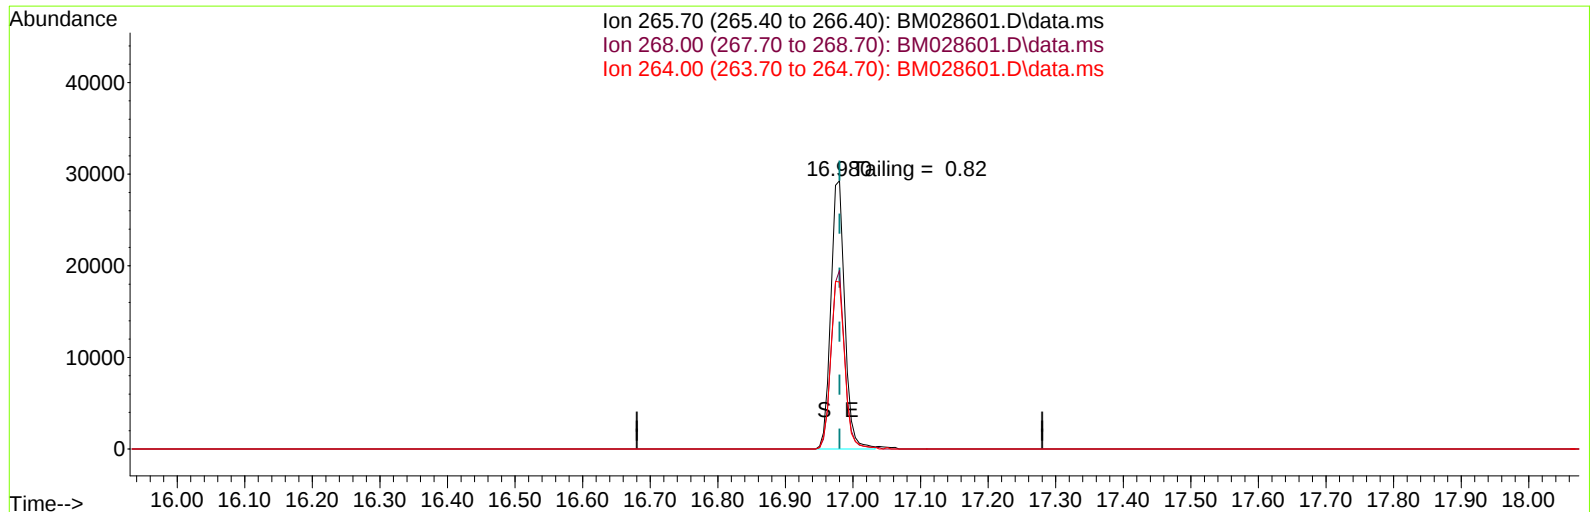

TIC: BM028601.D\data.ms

(70) Pentachlorophenol (C)




16.980min (-0.000) 0.00 ng

response 42290

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	66.58
264.00	63.30	62.26
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012921\  
Data File : BM028601.D  
Acq On    : 29 Jan 2021  12:08  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jan 30 01:36:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

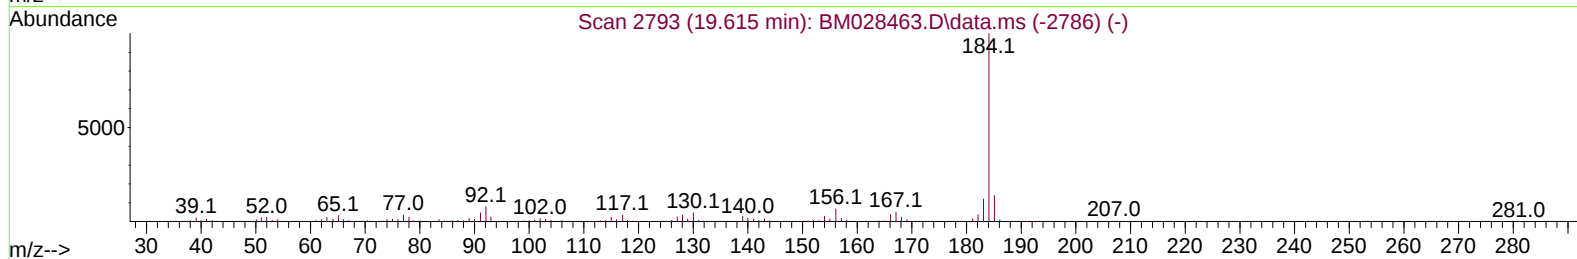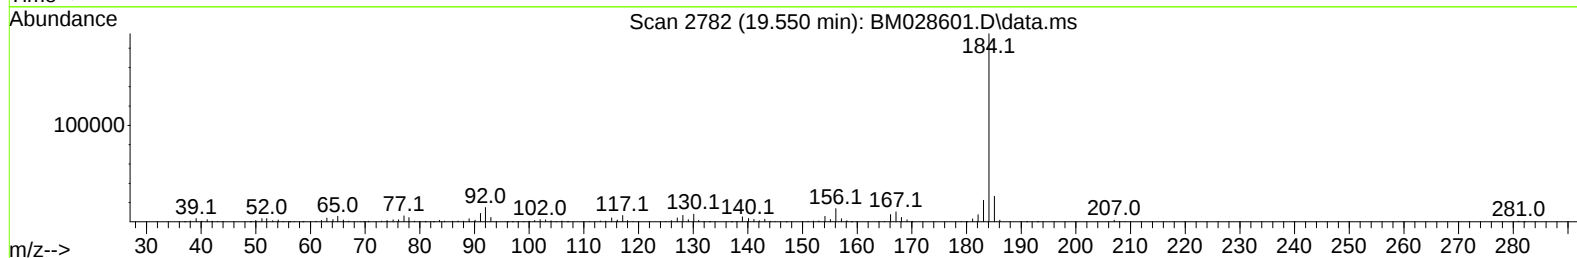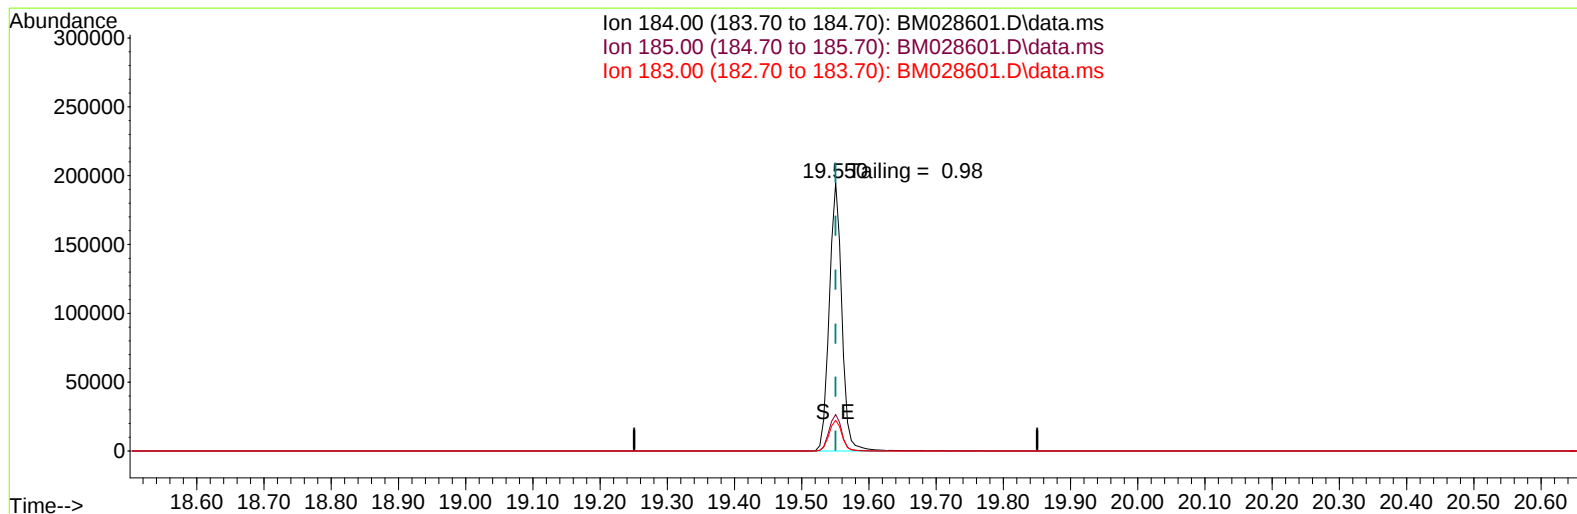

TIC: BM028601.D\data.ms

(77) Benzidine

19.550min (-0.000) 0.00 ng

response **252991**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.61
183.00	12.10	11.47
0.00	0.00	0.00