

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM012921\  
 Data File : BM028603.D  
 Acq On : 29 Jan 2021 13:20  
 Operator : CG/JU  
 Sample : PB134387BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB134387BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012021.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028603.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.005       | 135           | 139         | 146          | rVB      | 15536          | 20032         | 1.36%           | 0.297%        |
| 2         | 5.481       | 383           | 390         | 400          | rBV      | 480862         | 705114        | 47.92%          | 10.454%       |
| 3         | 7.116       | 661           | 668         | 684          | rBB      | 463462         | 716830        | 48.71%          | 10.627%       |
| 4         | 7.934       | 801           | 807         | 814          | rBB      | 99134          | 148853        | 10.12%          | 2.207%        |
| 5         | 9.110       | 998           | 1007        | 1015         | rBV      | 284307         | 464029        | 31.53%          | 6.879%        |
| 6         | 10.745      | 1278          | 1285        | 1293         | rBV      | 125373         | 202258        | 13.74%          | 2.999%        |
| 7         | 13.210      | 1697          | 1704        | 1710         | rBV      | 704719         | 1005679       | 68.34%          | 14.910%       |
| 8         | 14.586      | 1932          | 1938        | 1944         | rBV      | 184710         | 255306        | 17.35%          | 3.785%        |
| 9         | 16.074      | 2185          | 2191        | 2200         | rVB      | 561112         | 771881        | 52.45%          | 11.444%       |
| 10        | 17.321      | 2397          | 2403        | 2410         | rBV      | 217447         | 296603        | 20.16%          | 4.397%        |
| 11        | 19.921      | 2840          | 2845        | 2850         | rBV      | 1185113        | 1471579       | 100.00%         | 21.817%       |
| 12        | 21.239      | 3066          | 3069        | 3073         | rBV      | 17497          | 21552         | 1.46%           | 0.320%        |
| 13        | 21.462      | 3102          | 3107        | 3112         | rBV      | 277742         | 331986        | 22.56%          | 4.922%        |
| 14        | 23.721      | 3485          | 3491        | 3502         | rVB2     | 180833         | 333444        | 22.66%          | 4.943%        |




Sum of corrected areas: 6745146

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM012921\  
Data File : BM028603.D  
Acq On : 29 Jan 2021 13:20  
Operator : CG/JU  
Sample : PB134387BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB134387BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

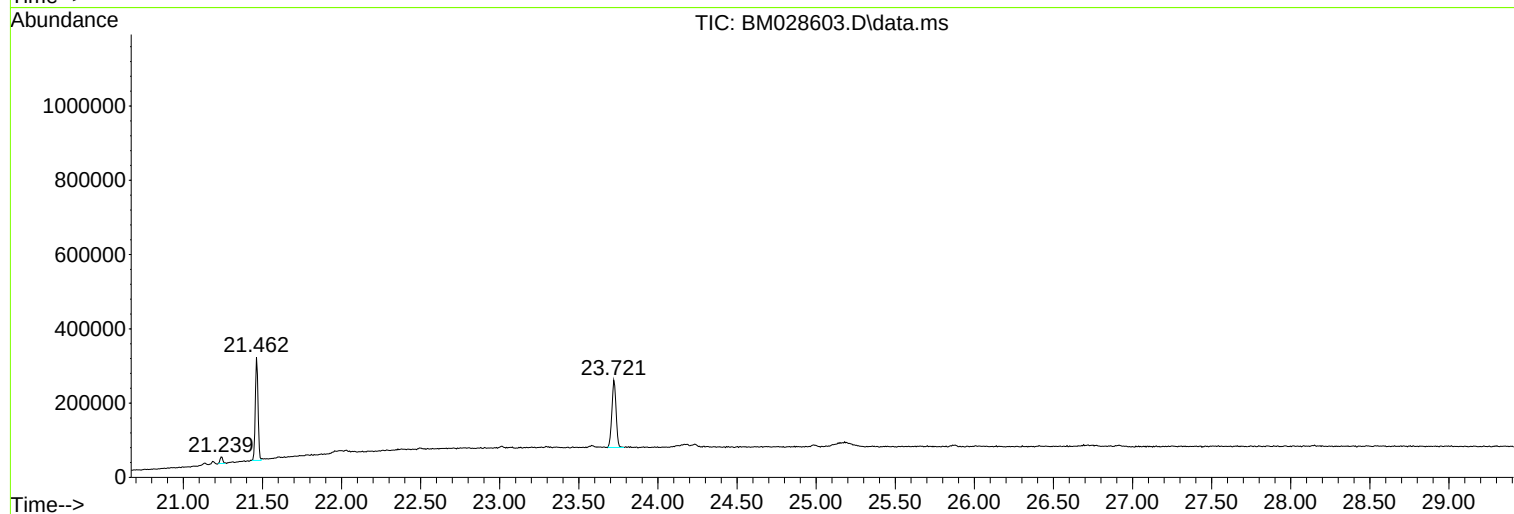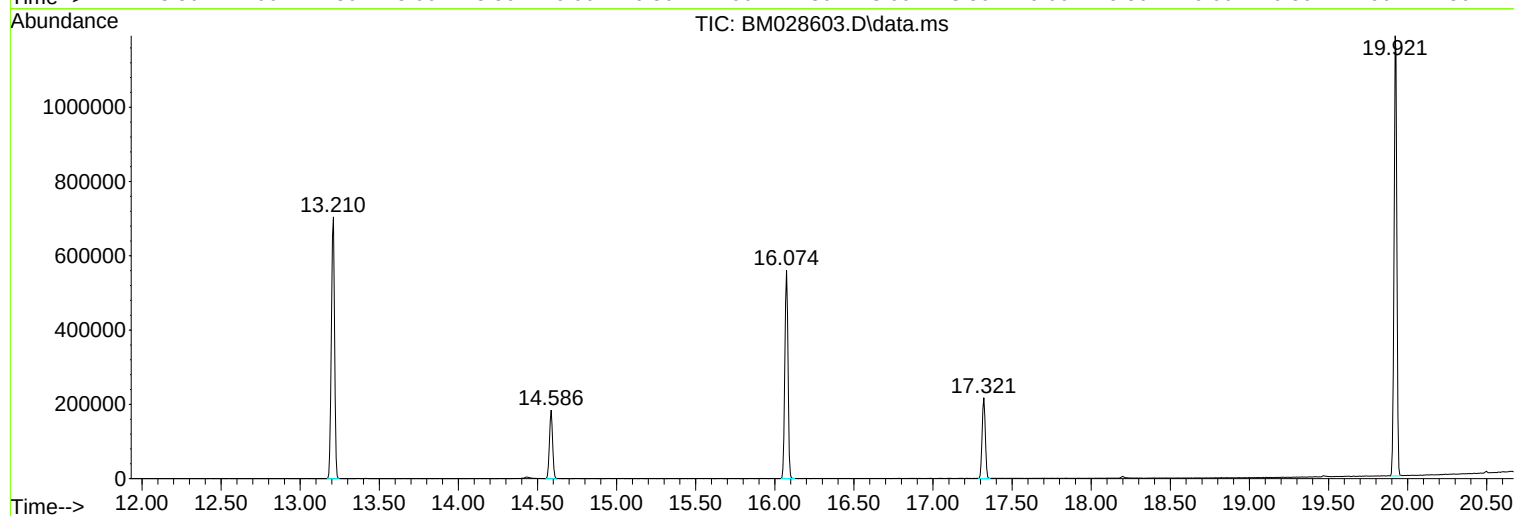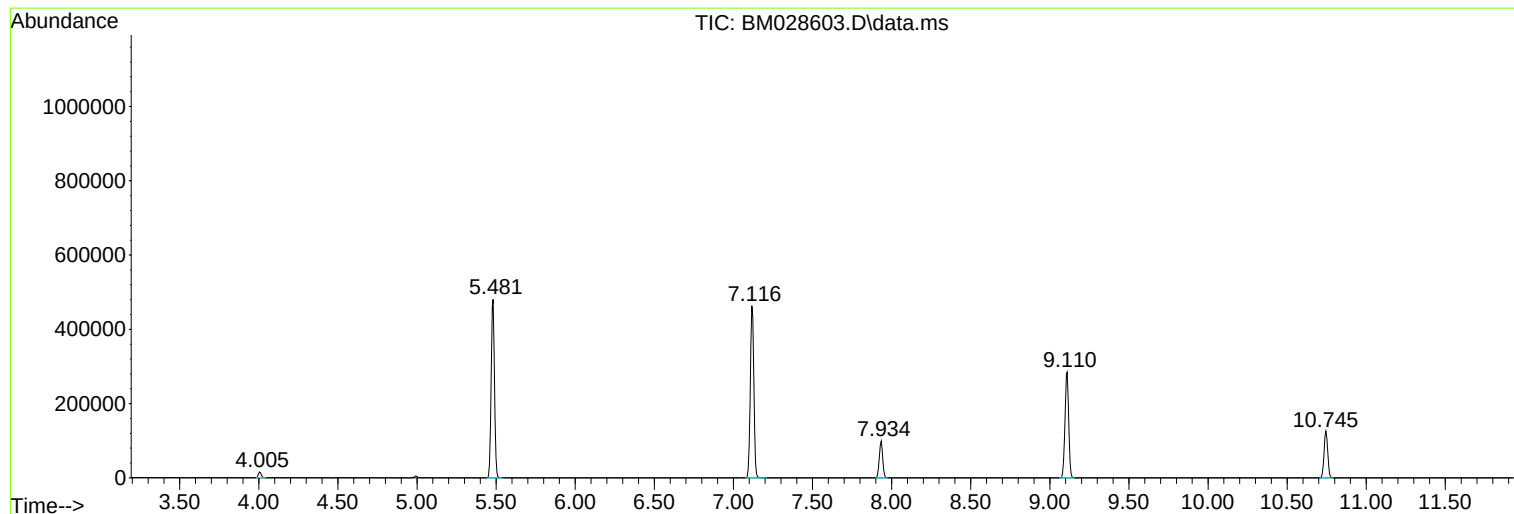

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM012921\  
Data File : BM028603.D  
Acq On : 29 Jan 2021 13:20  
Operator : CG/JU  
Sample : PB134387BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB134387BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM012921\  
Data File : BM028603.D  
Acq On : 29 Jan 2021 13:20  
Operator : CG/JU  
Sample : PB134387BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB134387BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|