
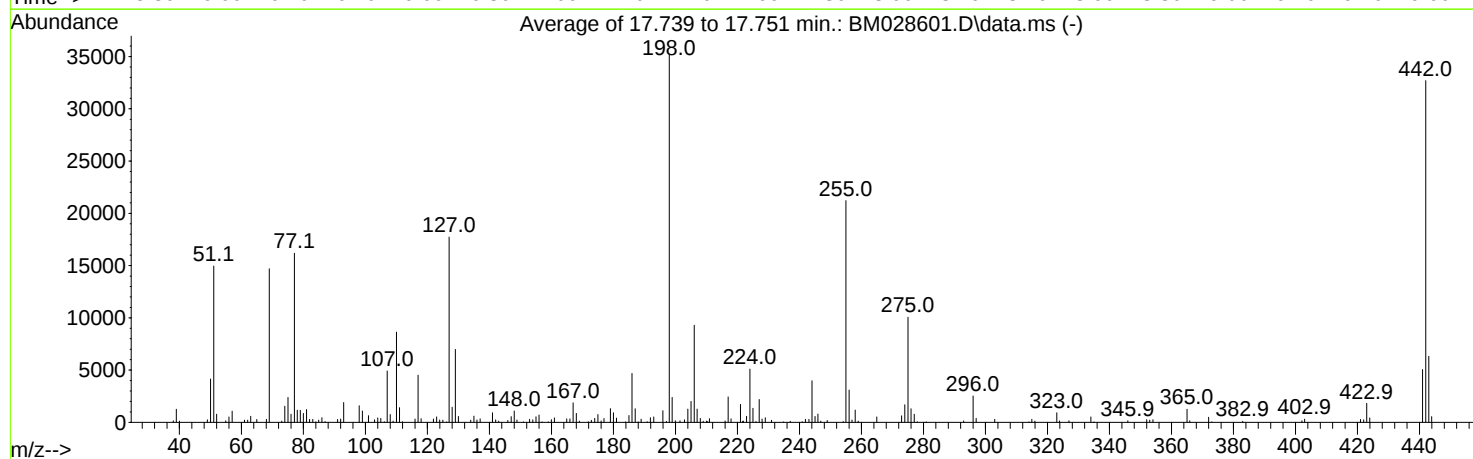


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012921\
 Data File : BM028601.D
 Acq On : 29 Jan 2021 12:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 16:19:07 2021

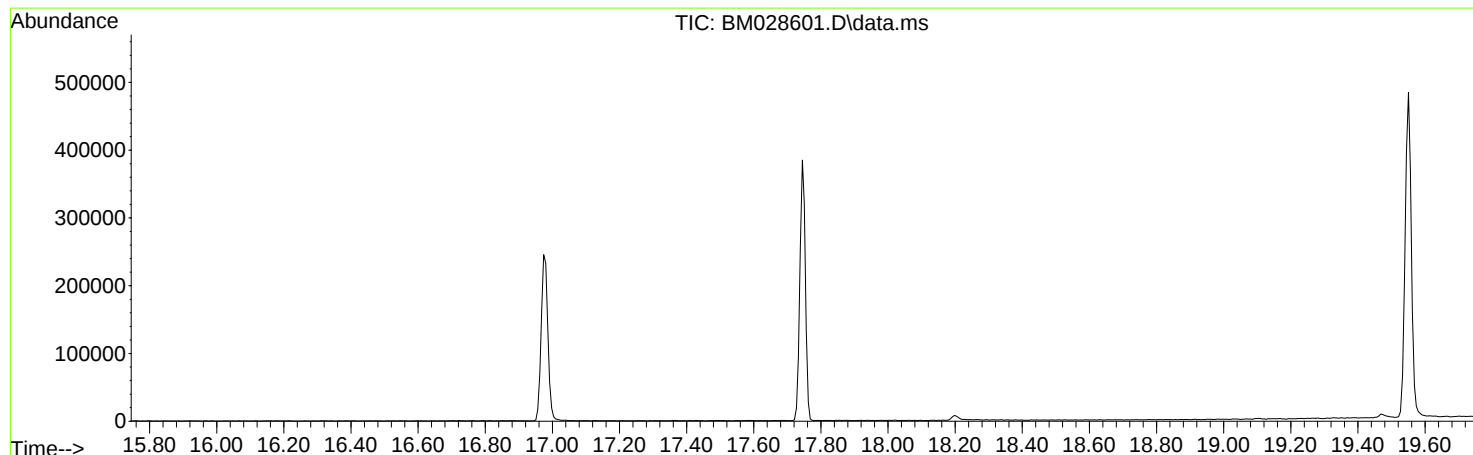

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	14954	PASS
68	69	0.00	2	2.0	289	PASS
69	198	0.00	100	41.8	14704	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	17728	PASS
197	198	0.00	2	0.3	99	PASS
198	198	100	100	100.0	35197	PASS
199	198	5	9	6.8	2387	PASS
275	198	10	60	28.6	10065	PASS
365	198	1	100	3.6	1254	PASS
441	198	0.01	100	14.3	5049	PASS
442	442	50	100	100.0	32709	PASS
443	442	15	24	19.3	6328	PASS