
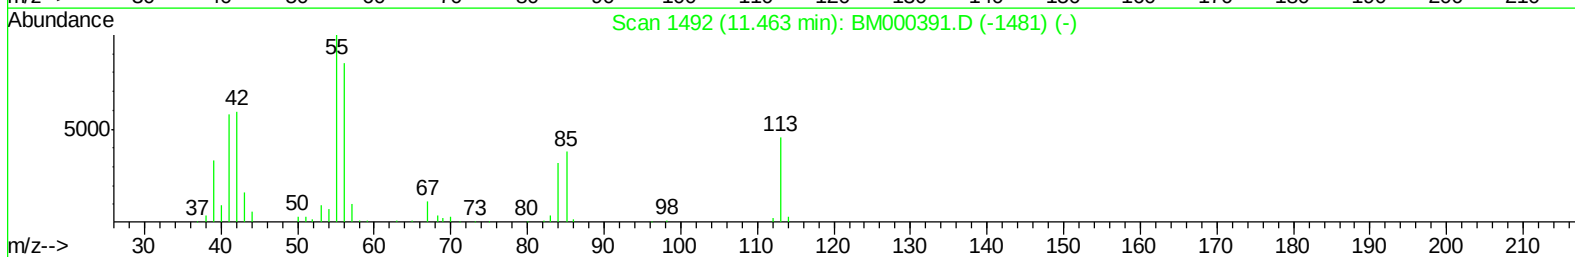
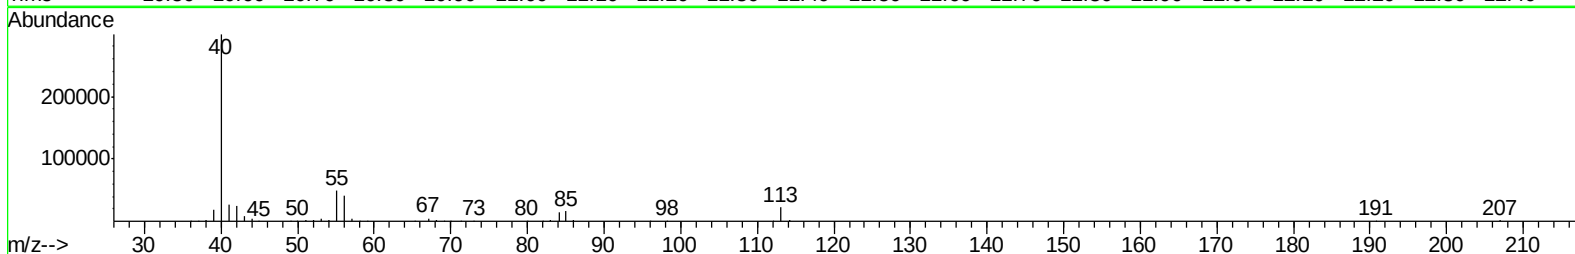


Data Path : Z:\HPCHEM1\BNA_M\Data\BM013015\
Data File : BM000407.D
Acq On : 30 Jan 2015 19:20
Operator : TP/IZ
Sample : SSTD02064
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jan 30 23:07:07 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 30 16:03:45 2015
Response via : Initial Calibration

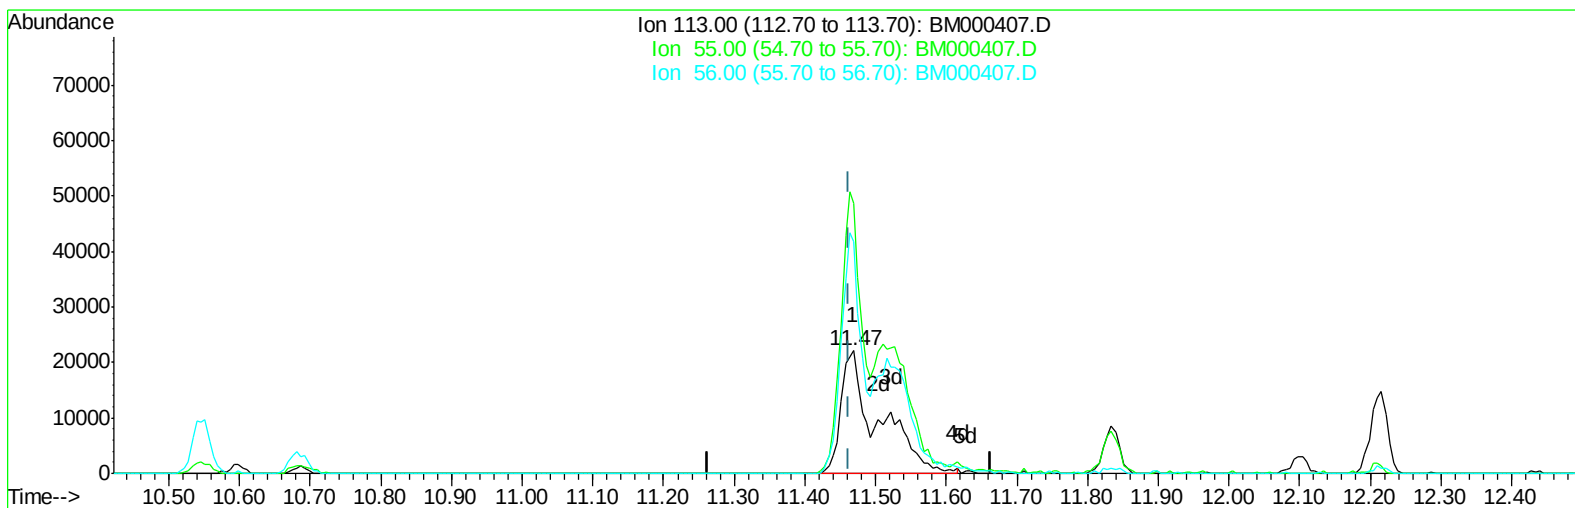

TIC: BM000407.D

(32) Caprolactam

11.469min (+0.006) 20.79ng/ul m

response 81277

Ion	Exp%	Act%
113.00	100	100
55.00	218.60	219.97
56.00	186.50	188.62
0.00	0.00	0.00