

Data Path : Z:\HPCHEM1\BNA_M\Data\BM013015\
 Data File : BM000406.D
 Acq On : 30 Jan 2015 18:45
 Operator : TP/IZ
 Sample : G1134-15RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB2RE

Quant Time: Jan 30 22:47:04 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 30 16:03:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	142246	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	621288	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	427005	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	1030917	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	987805	20.00	ng/ul	0.00
83) Perylene-d12	23.60	264	742503	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	2740	1.43	ng/uL	0.00
5) Phenol-d5	6.92	99	56357	5.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	169283	26.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	176191	21.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	127148	14.71	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	120036	28.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	133603	30.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	267099	27.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	3199	0.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	1302365	40.70	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	1401916	37.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.60	143	30126	6.18	ng/ul	0.00
57) Fluorene-d10	15.40	176	1099807	39.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	192984	34.23	ng/ul	0.00
70) Anthracene-d10	17.25	188	1771605	37.07	ng/ul	0.00
76) Pyrene-d10	19.54	212	1994367	39.11	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.45	264	1186152	33.54	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.25	88	3075	1.14 ng/uL#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM013015\
Data File : BM000406.D
Acq On : 30 Jan 2015 18:45
Operator : TP/IZ
Sample : G1134-15RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB2RE

Quant Time: Jan 30 22:47:04 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 30 16:03:45 2015
Response via : Initial Calibration

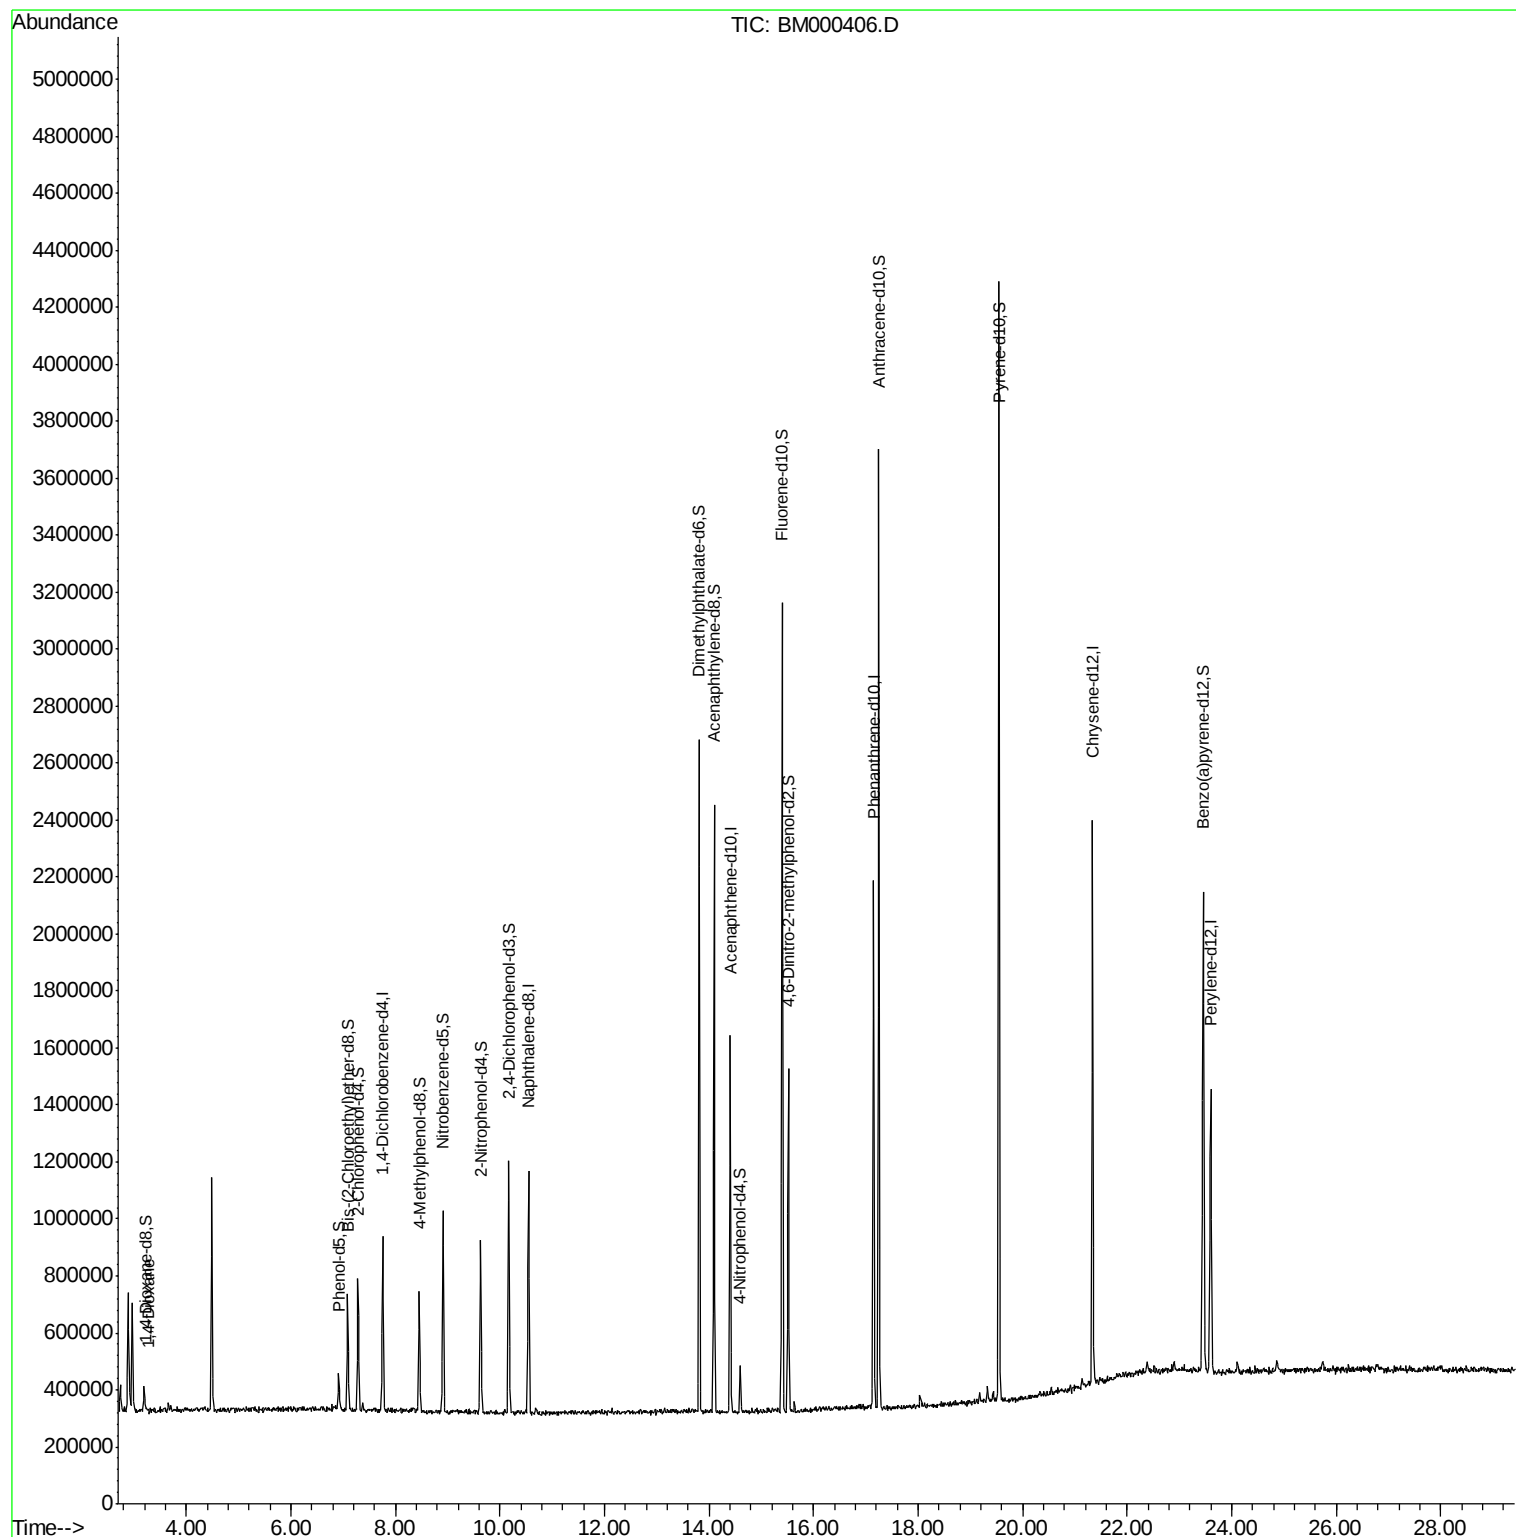

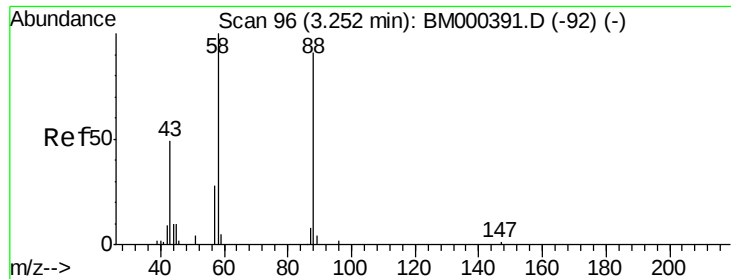

#2

1,4-Dioxane

Concen: 1.14 ng/uL

RT: 3.25 min Scan# 96

Delta R.T. 0.00 min

Lab File: BM000406.D


Acq: 30 Jan 2015 18:45

Instrument :

BNA_M

ClientSampleId :

C0AB2RE

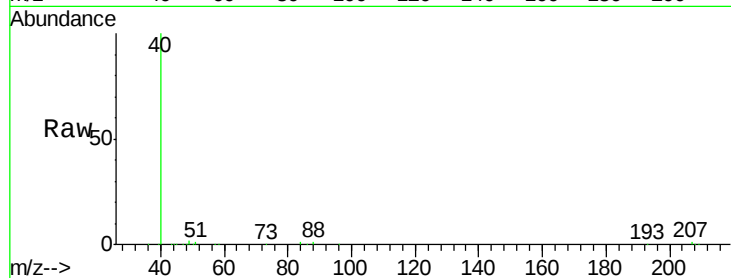

Tgt Ion:	88	Resp:	3075
Ion	Ratio	Lower	Upper
88	100		
43	37.8	40.0	60.0#
58	57.2	40.0	60.0

