


Data Path : Z:\HPCHEM1\BNA_M\Data\BM013015\
 Data File : BM000403.D
 Acq On : 30 Jan 2015 15:54
 Operator : TP/IZ
 Sample : DFTPP14
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP14

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Title : SVOA CALIBRATION
 Last Update : Fri Jan 30 16:03:45 2015

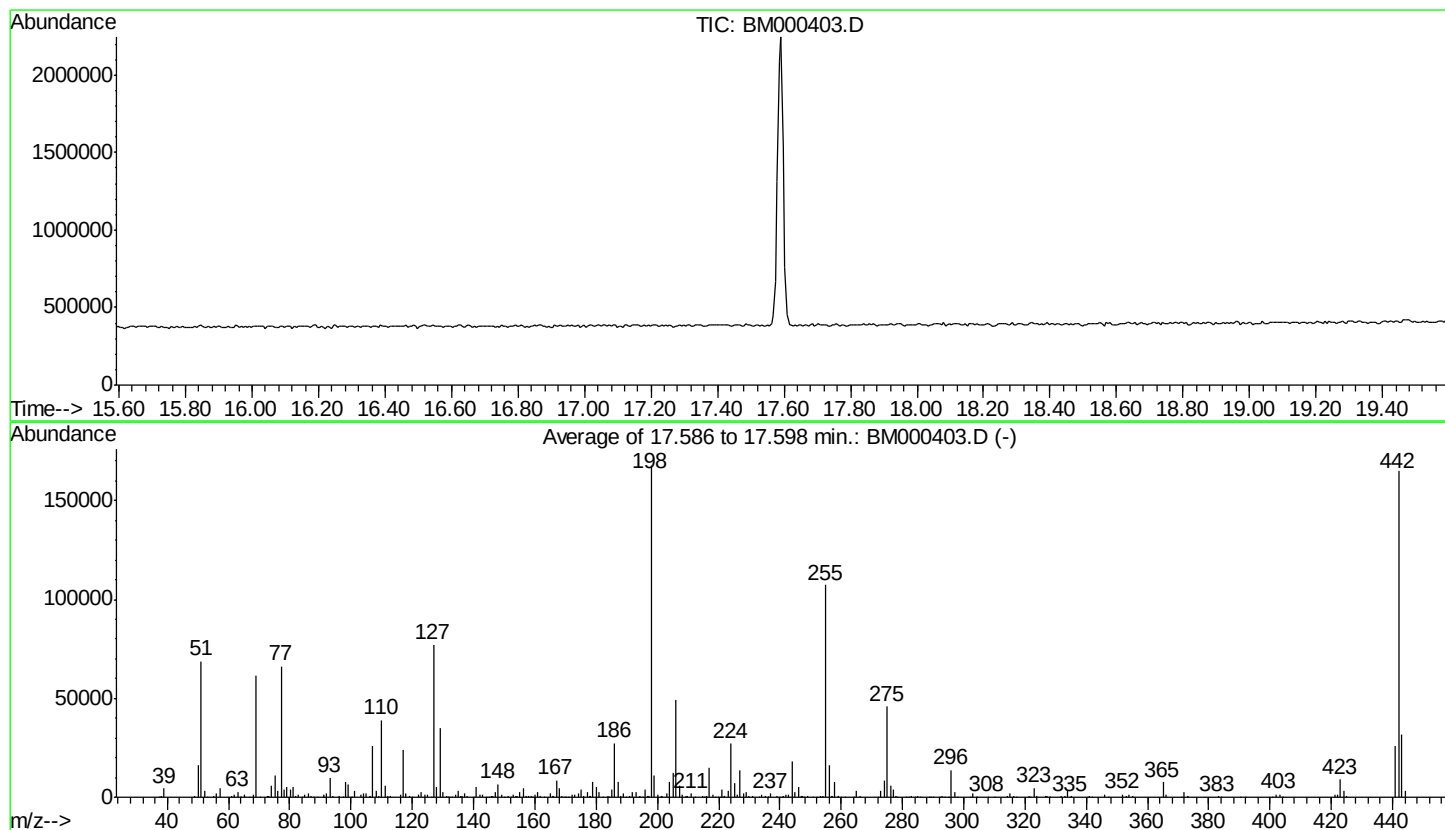

AutoFind: Scans 2533, 2534, 2535; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	68928	PASS
68	69	0.00	2	1.8	1109	PASS
69	198	0.00	100	36.5	61245	PASS
70	69	0.00	2	0.3	184	PASS
127	198	10	80	46.1	77325	PASS
197	198	0.00	2	0.4	635	PASS
198	198	100	100	100.0	167672	PASS
199	198	5	9	6.4	10814	PASS
275	198	10	60	27.2	45658	PASS
365	198	1	100	4.5	7484	PASS
441	443	0.01	100	81.6	26010	PASS
442	198	50	100	98.5	165226	PASS
443	442	15	24	19.3	31861	PASS