

Quantitation Report (LSC Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM013015\
 Data File : BM000406.D
 Acq On : 30 Jan 2015 18:45
 Operator : TP/IZ
 Sample : G1134-15RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB2RE

Manual Integrations
 APPROVED

apatel
 2/2/2015 12:49:55 PM

Quant Time: Feb 02 09:16:47 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 30 16:03:45 2015
 Response via : Initial Calibration

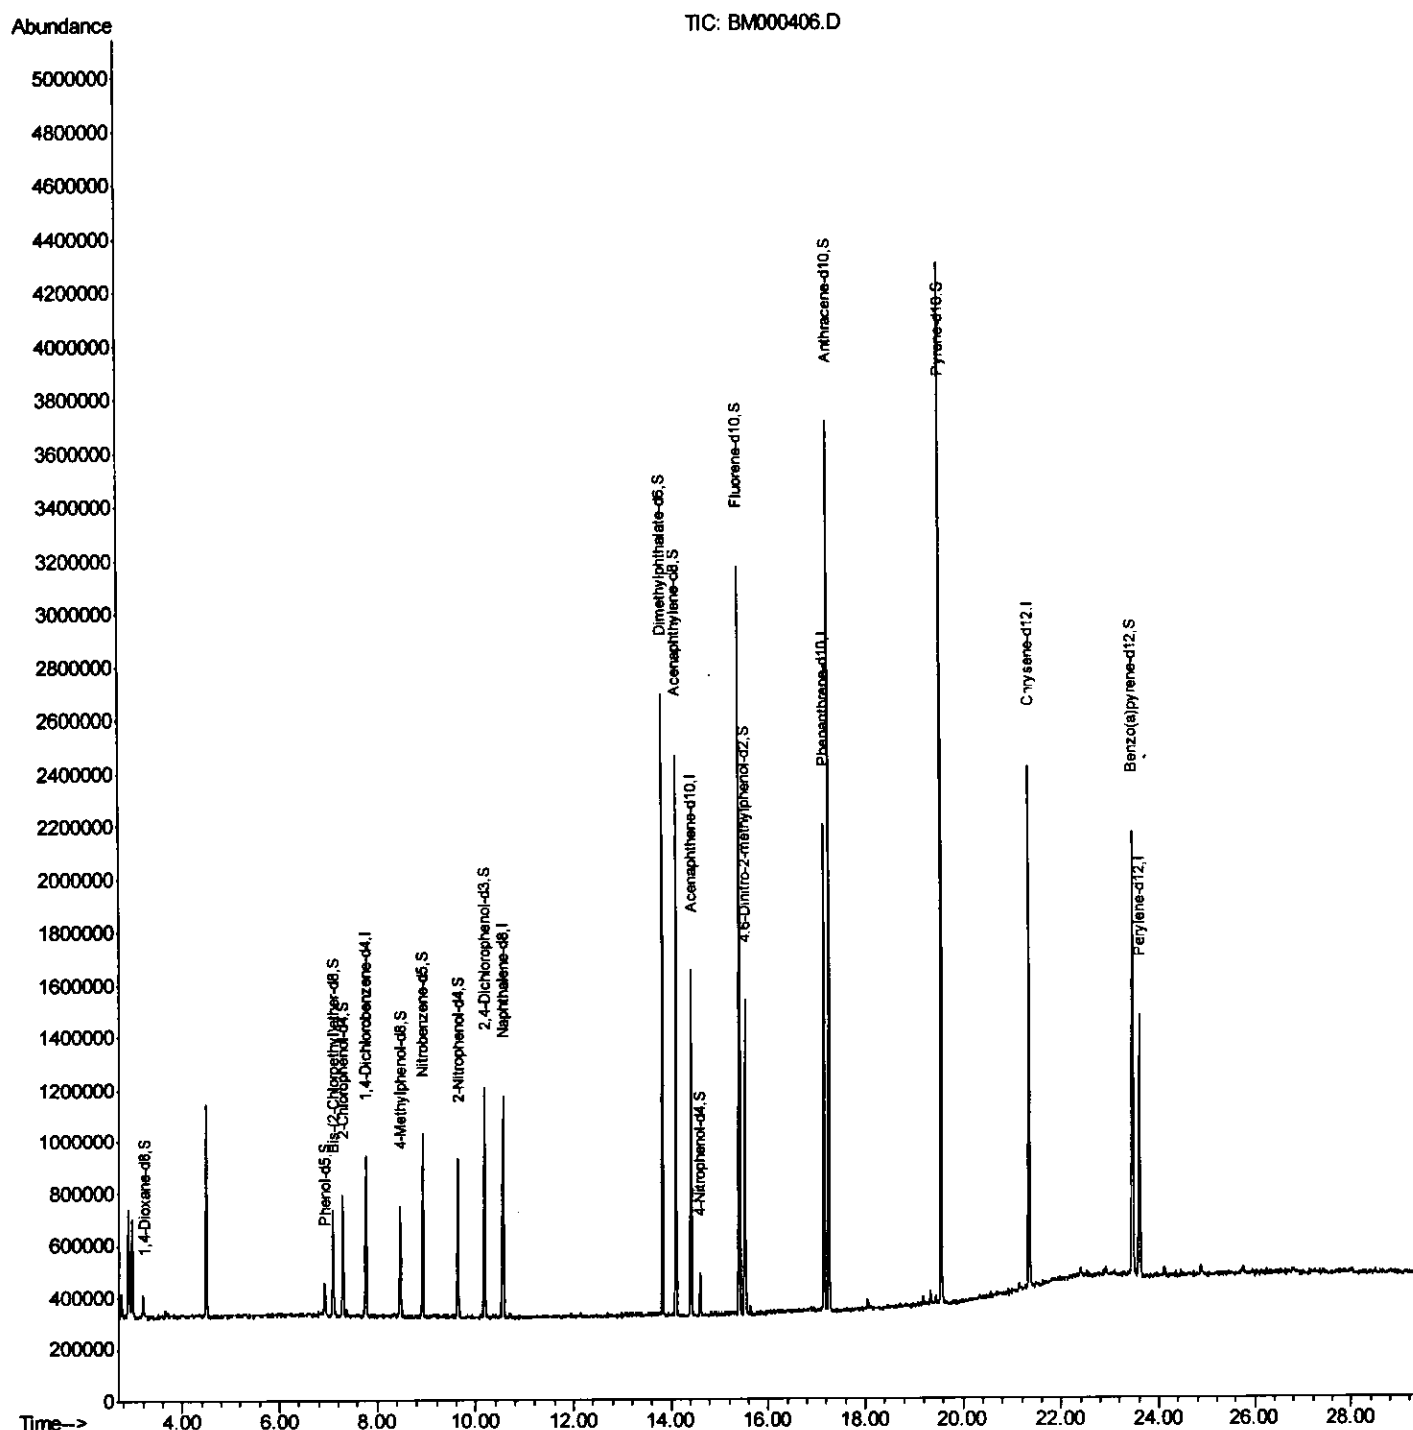

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM013015\
 Data File : BM000406.D
 Acq On : 30 Jan 2015 18:45
 Operator : TP/IZ
 Sample : G1134-15RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB2RE

Quant Time: Jan 30 23:06:52 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 30 16:03:45 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 2/2/2015 12:49:55 PM

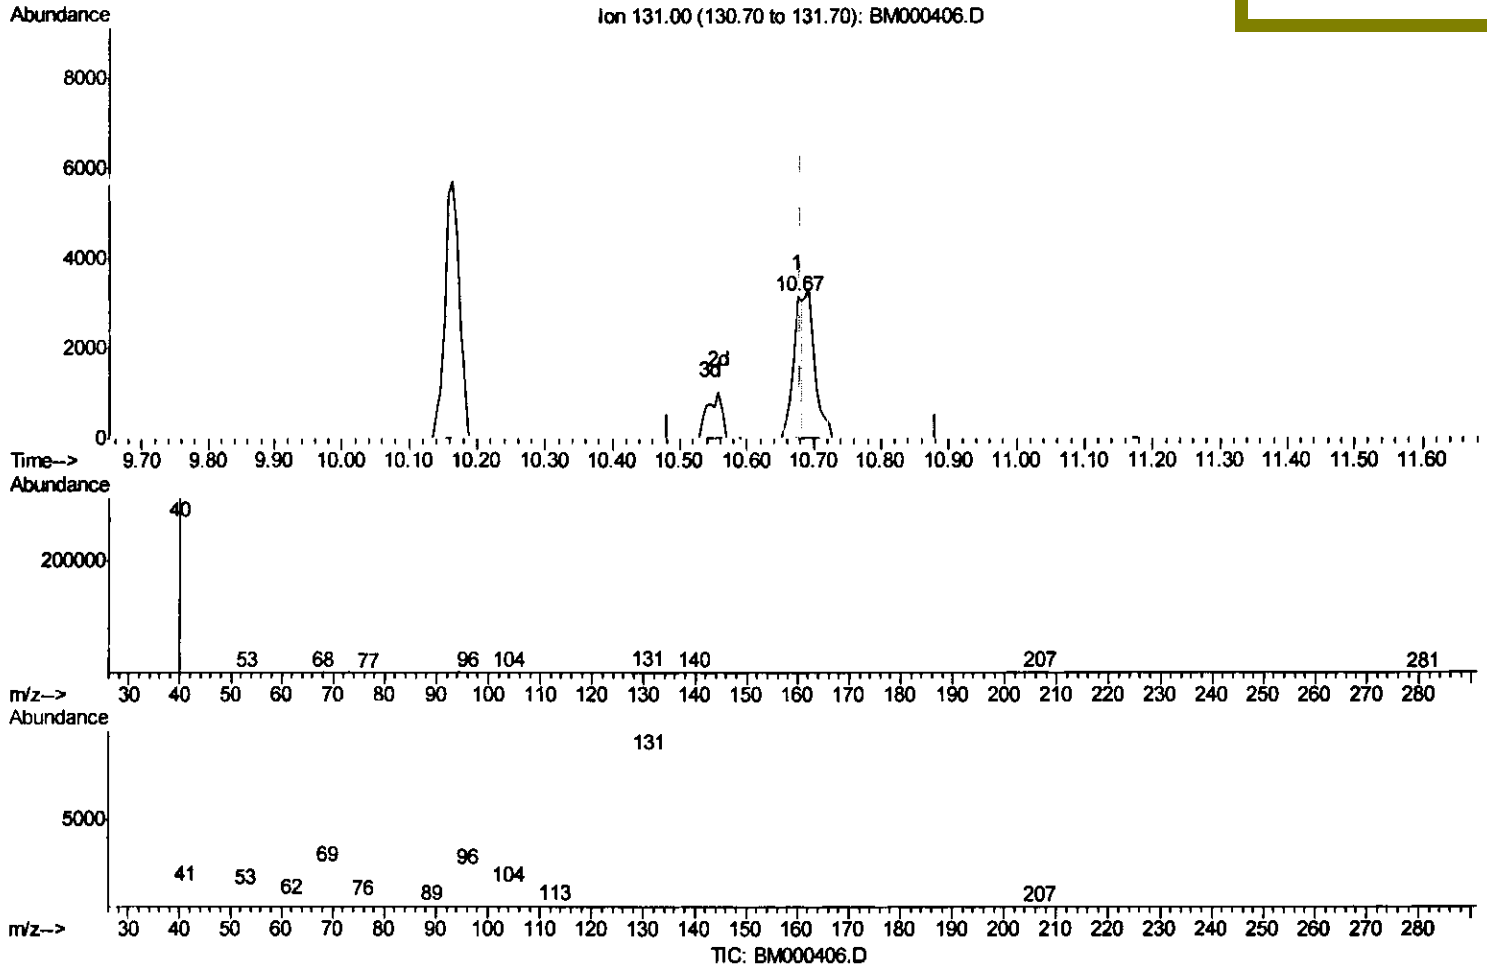

(29) 4-Chloroaniline-d4 (S)

10.675min (-0.006) 0.28ng/ul

response 3199

Ion	Exp%	Act%
131.00	100	100
133.00	31.30	23.54#
69.00	22.80	15.66#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM013015\
 Data File : BM000406.D
 Acq On : 30 Jan 2015 18:45
 Operator : TP/IZ
 Sample : G1134-15RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB2RE

Manual Integrations
 APPROVED

apatel
 2/2/2015 12:49:55 PM

Quant Time: Jan 30 23:06:52 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 30 16:03:45 2015
 Response via : Initial Calibration

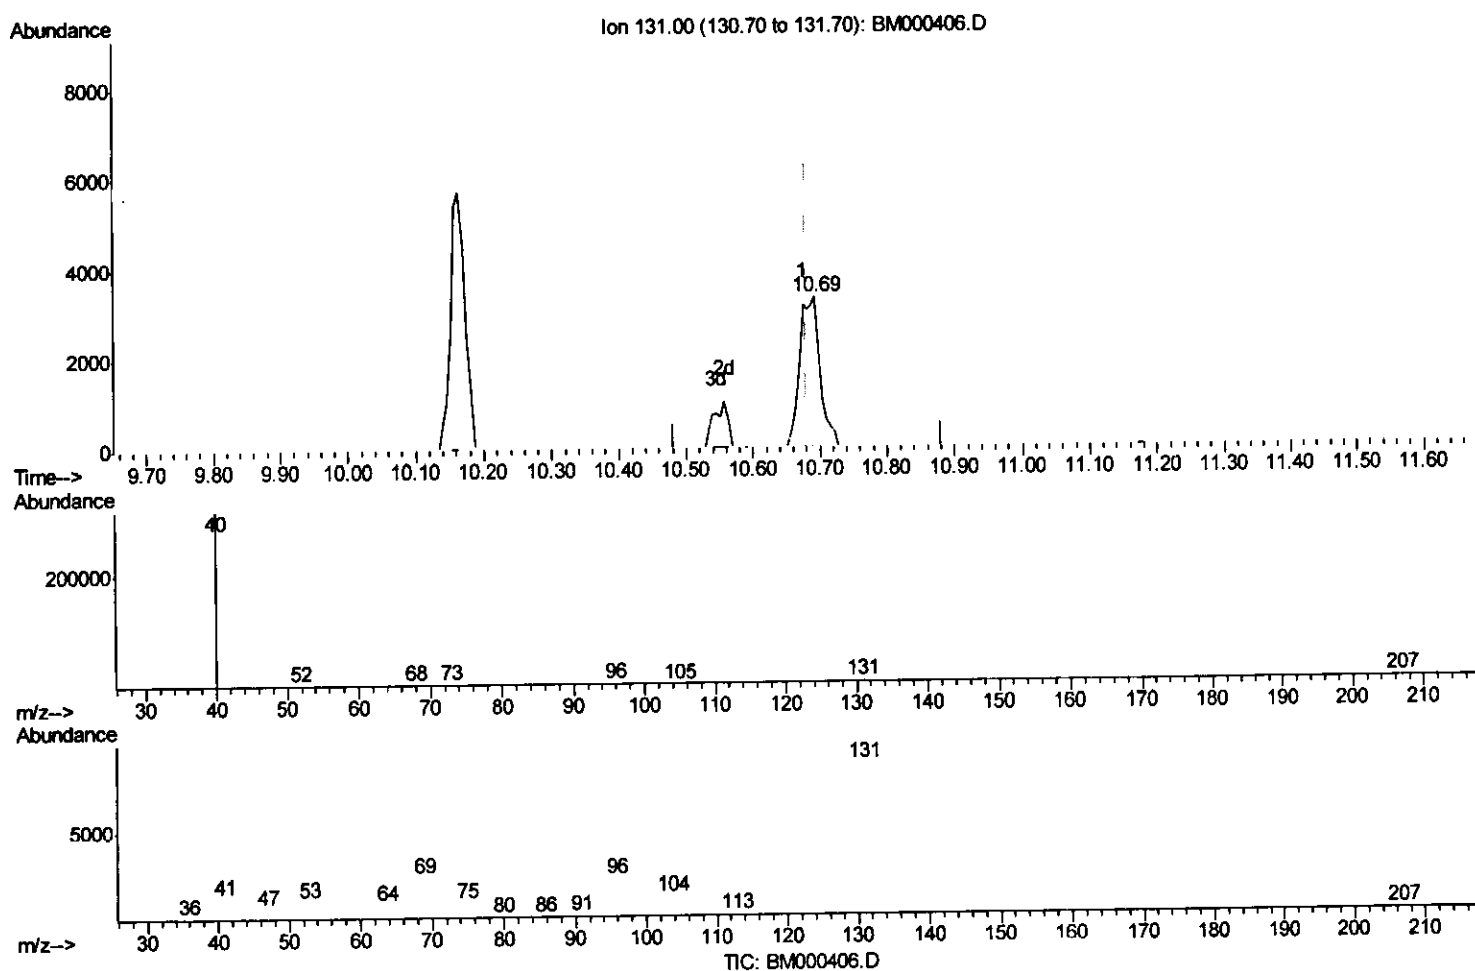

(29) 4-Chloroaniline-d4 (S)

10.693min (+0.012) 0.60ng/ul m

response 6987

Ion	Exp%	Act%
131.00	100	100
133.00	31.30	32.23
69.00	22.80	16.72#
0.00	0.00	0.00

T.P.
 2/5/15

Data Path : Z:\HPCHEM1\BNA_M\Data\BM013015\
 Data File : BM000406.D
 Acq On : 30 Jan 2015 18:45
 Operator : TP/IZ
 Sample : G1134-15RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAB2RE

Quant Time: Feb 02 09:16:47 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 30 16:03:45 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 2/2/2015 12:49:55 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	142246	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	621288	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	427005	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	1030917	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	987805	20.00	ng/ul	0.00
83) Perylene-d12	23.60	264	742503	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	2740	1.43	ng/uL	0.00
5) Phenol-d5	6.92	99	56357	5.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	169283	26.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	176191	21.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	127148	14.71	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	120036	28.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	133603	30.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	267099	27.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	6987m	0.60	ng/ul	0.01
43) Dimethylphthalate-d6	13.81	166	1302365	40.70	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	1401916	37.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.60	143	30126	6.18	ng/ul	0.00
57) Fluorene-d10	15.40	176	1099807	39.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	192984	34.23	ng/ul	0.00
70) Anthracene-d10	17.25	188	1771605	37.07	ng/ul	0.00
76) Pyrene-d10	19.54	212	1994367	39.11	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.45	264	1186152	33.54	ng/ul	0.00

T.P.
 2/5/15

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed