


Data Path : Z:\HPCHEM1\BNA M\DATA\BM013016\
 Data File : BM004146.D
 Acq On : 29 Jan 2016 15:01
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM012216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 22 14:46:41 2016

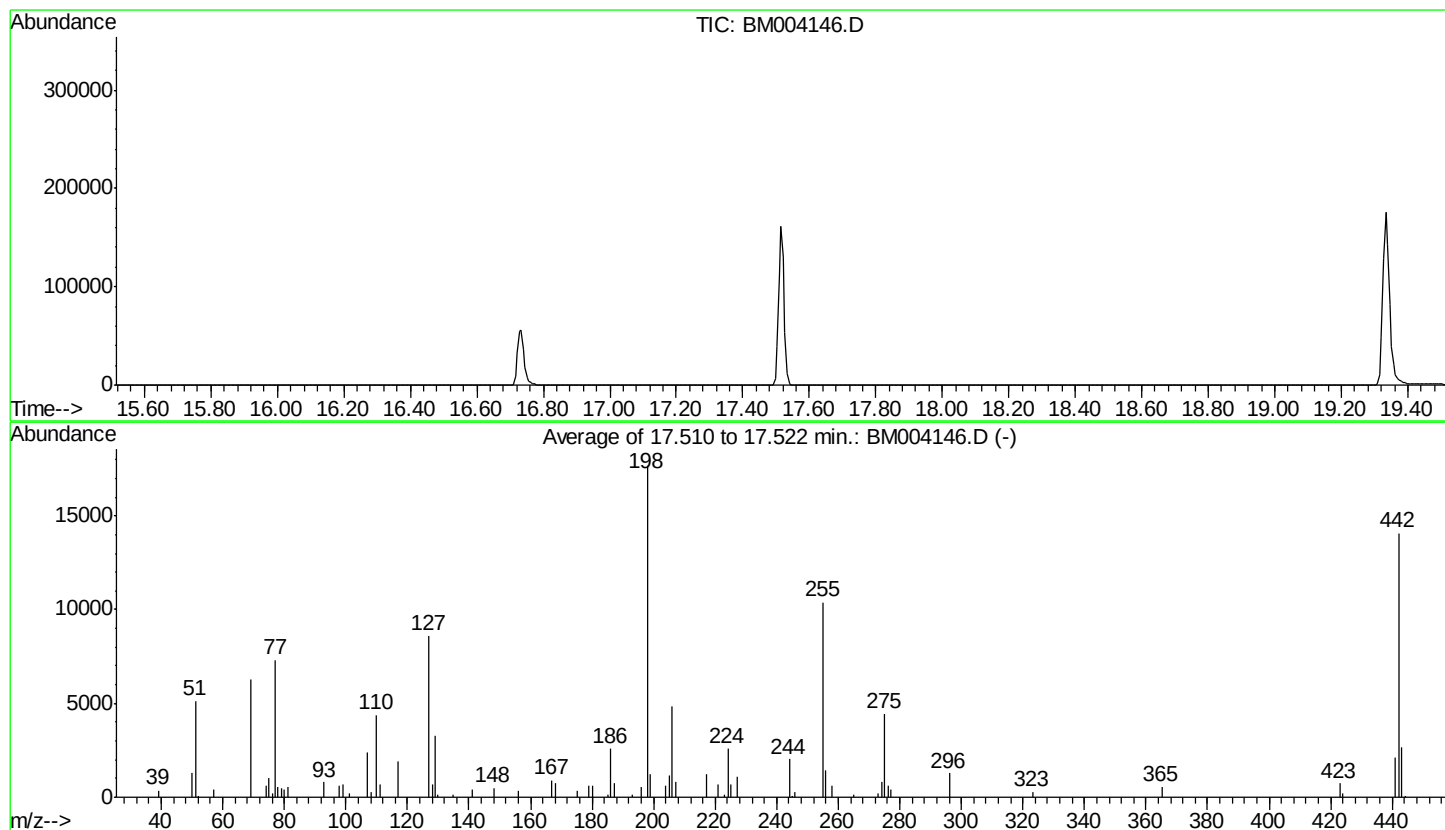

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	5146	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.4	6258	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	8621	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17675	PASS
199	198	5	9	6.8	1199	PASS
275	198	10	60	25.2	4455	PASS
365	198	1	100	3.1	552	PASS
441	442	0.01	24	15.2	2136	PASS
442	198	50	100	79.7	14085	PASS
443	442	15	24	18.9	2663	PASS