

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM013017\
 Data File : BM008919.D
 Acq On : 30 Jan 2017 19:31
 Operator : SJ/MA
 Sample : PB96398BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK98

Quant Time: Jan 31 02:58:01 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 31 02:42:41 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	41840	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	159127	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	118358	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	258481	20.00	ng/ul	0.00
75) Chrysene-d12	21.47	240	326142	20.00	ng/ul	0.00
83) Perylene-d12	23.83	264	321894	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.38	96	7260	6.94	ng/uL	0.00
5) Phenol-d5	7.07	99	127492	32.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.25	67	110435	34.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.45	132	84940	35.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.61	113	94234	31.90	ng/ul	0.00
19) Nitrobenzene-d5	9.09	128	40480	35.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.80	143	43561	34.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.33	165	93383	34.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	103343	41.92	ng/ul	0.00
43) Dimethylphthalate-d6	13.96	166	321007	37.00	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	354649	36.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.74	143	46975	33.17	ng/ul	0.00
57) Fluorene-d10	15.54	176	269715	33.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	49581	29.63	ng/ul	0.00
70) Anthracene-d10	17.40	188	458029	37.09	ng/ul	0.00
76) Pyrene-d10	19.69	212	541912	37.69	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.68	264	522991	35.78	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.61	70	5540	1.52	ng/ul#	1
21) Isophorone	9.80	82	14385	1.84	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM013017\
Data File : BM008919.D
Acq On : 30 Jan 2017 19:31
Operator : SJ/MA
Sample : PB96398BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK98

Quant Time: Jan 31 02:58:01 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 31 02:42:41 2017
Response via : Initial Calibration




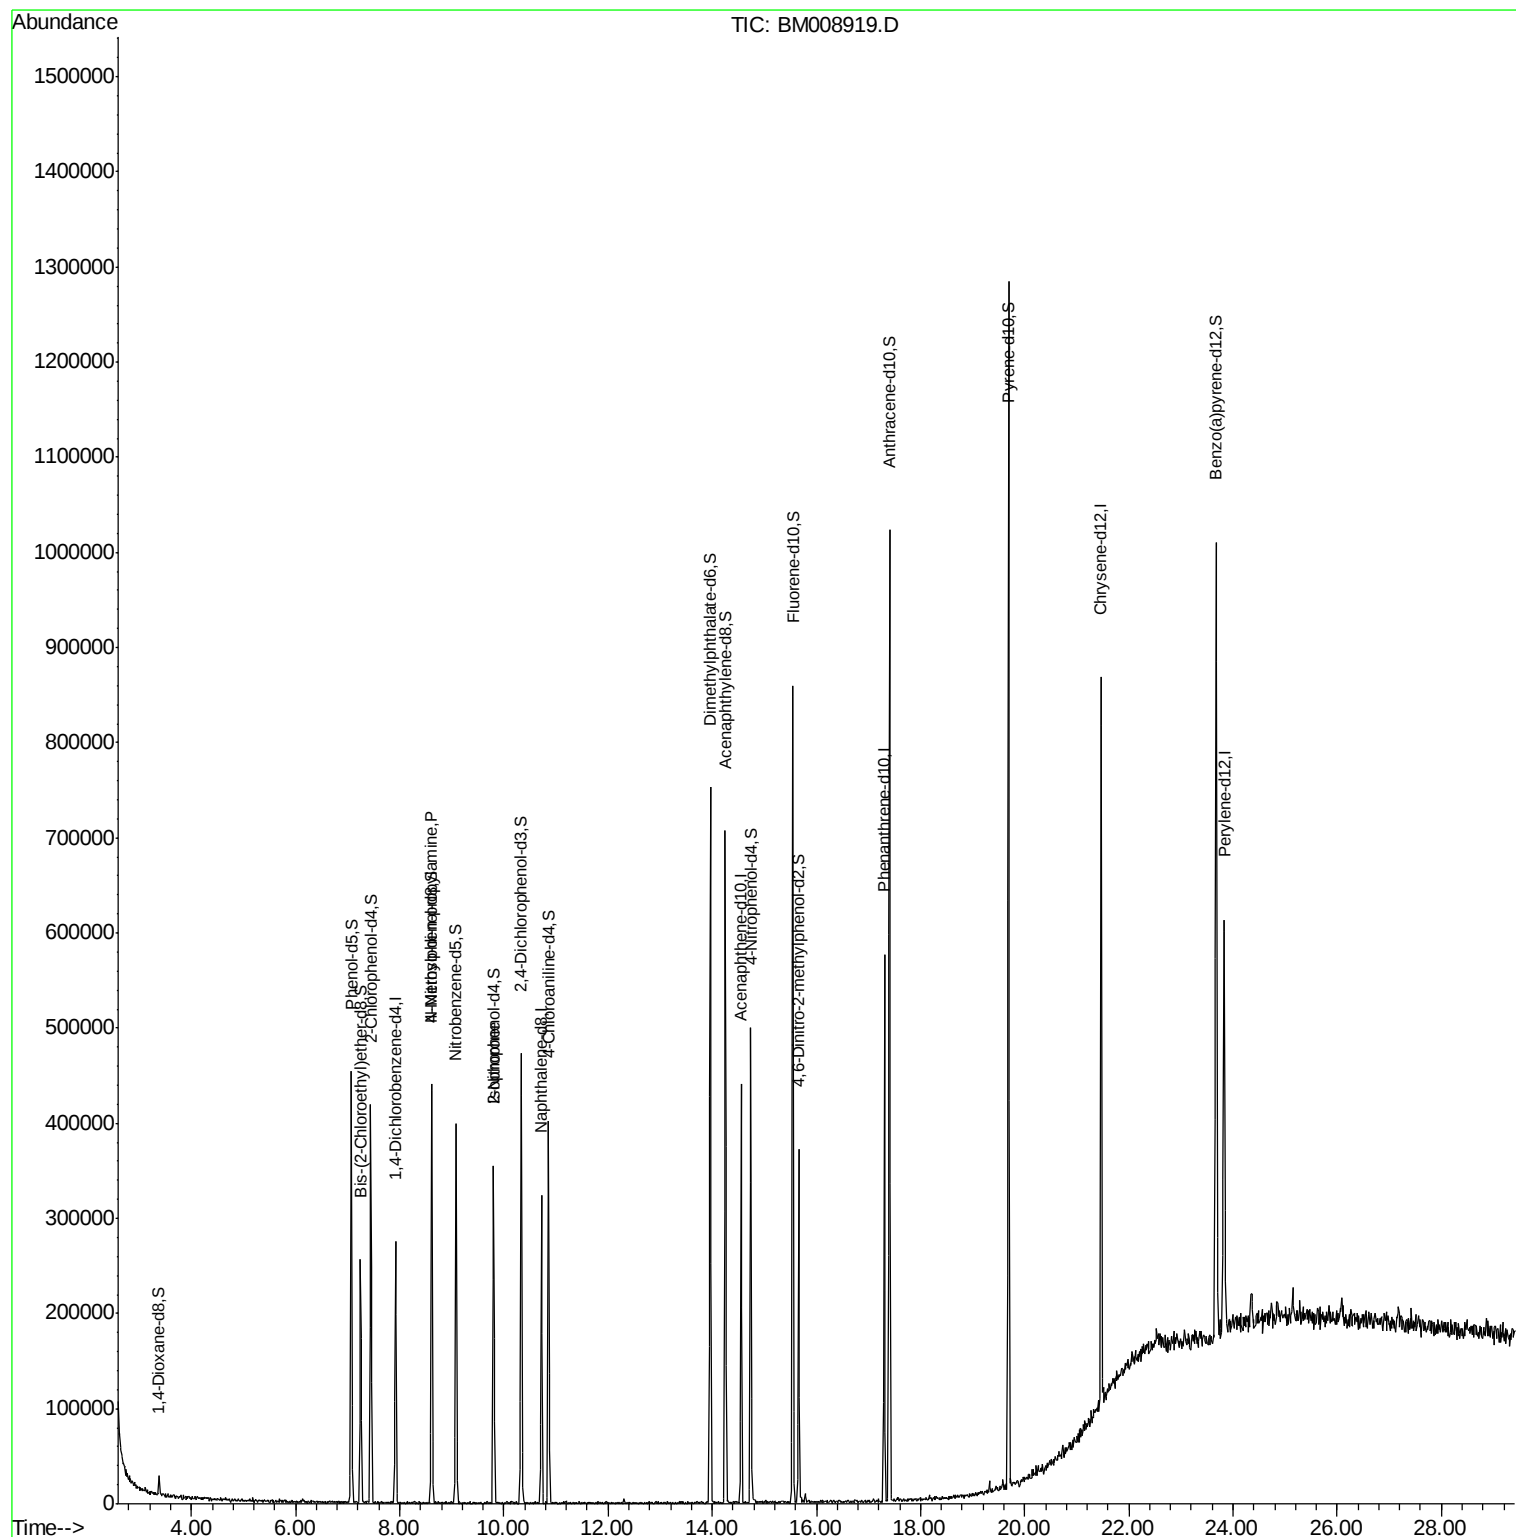


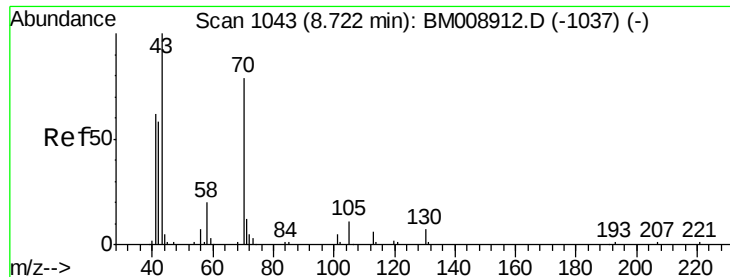

#15
N-Nitroso-di-n-propylamine
Concen: 1.52 ng/ul
RT: 8.61 min Scan# 1024
Delta R.T. -0.11 min
Lab File: BM008919.D
Acq: 30 Jan 2017 19:31

Instrument :
BNA_M
ClientSampleId :
SBLK98

Tgt Ion:	70	Resp:	5540
Ion	Ratio	Lower	Upper
70	100		
42	499.4	64.2	96.2#
101	0.0	5.1	7.7#
130	0.0	8.3	12.5#

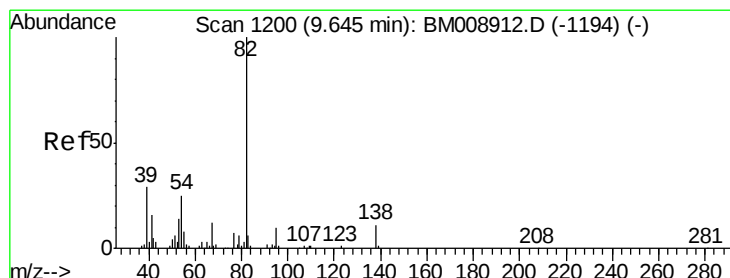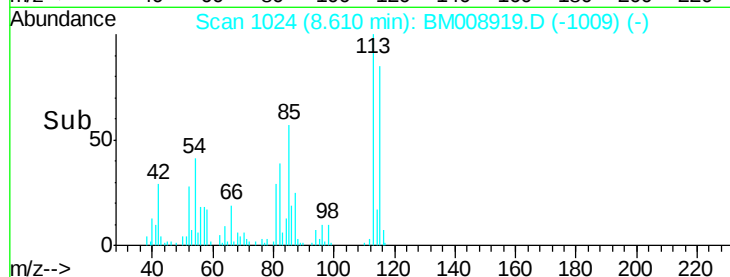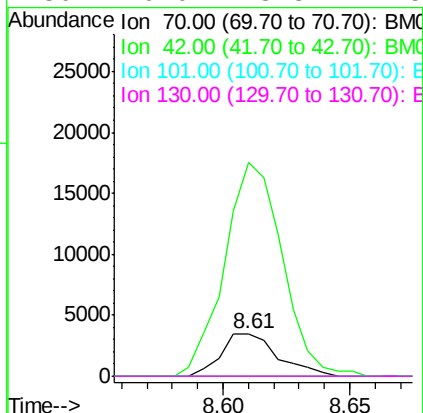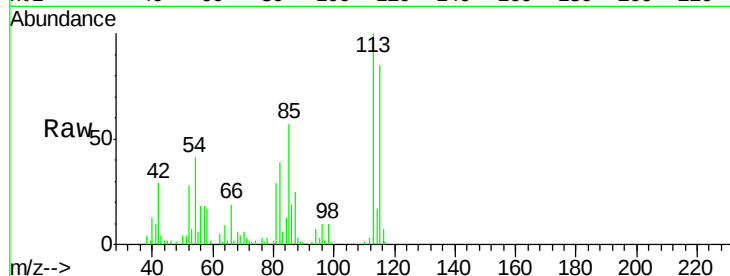

#21
Isophorone
Concen: 1.84 ng/ul
RT: 9.80 min Scan# 1227
Delta R.T. 0.16 min
Lab File: BM008919.D
Acq: 30 Jan 2017 19:31

Tgt Ion:	82	Resp:	14385
Ion	Ratio	Lower	Upper
82	100		
95	4.9	7.7	11.5#
138	0.0	9.4	14.0#

