

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013017\
 Data File : BM008917.D
 Acq On : 30 Jan 2017 18:19
 Operator : SJ/MA
 Sample : I1506-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9RA9

Quant Time: Jan 31 03:15:33 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM013017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 31 02:42:41 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	43982	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	173812	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	121234	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	264971	20.00	ng/ul	0.00
75) Chrysene-d12	21.47	240	357962	20.00	ng/ul	0.00
83) Perylene-d12	23.83	264	353155	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.38	96	4709	4.28	ng/uL	0.00
5) Phenol-d5	7.07	99	22459	5.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.25	67	85028	25.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.45	132	51481	20.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.61	113	34504	11.11	ng/ul	0.00
19) Nitrobenzene-d5	9.09	128	29299	23.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.80	143	32977	23.64	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.33	165	66628	22.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	4908	1.82	ng/ul	0.00
43) Dimethylphthalate-d6	13.96	166	251659	28.32	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	272459	27.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.74	143	5982	4.12	ng/ul	0.00
57) Fluorene-d10	15.55	176	218219	26.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	39622	23.10	ng/ul	0.00
70) Anthracene-d10	17.40	188	354421	28.00	ng/ul	0.00
76) Pyrene-d10	19.69	212	447698	28.37	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.68	264	453136	28.26	ng/ul	0.00


Target Compounds						Ovalue
6) Phenol	7.10	94	5993	1.38	ng/ul	85
44) Dimethylphthalate	14.01	163	13424	1.55	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013017\
Data File : BM008917.D
Acq On : 30 Jan 2017 18:19
Operator : SJ/MA
Sample : I1506-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9RA9

Quant Time: Jan 31 03:15:33 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM013017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 31 02:42:41 2017
Response via : Initial Calibration

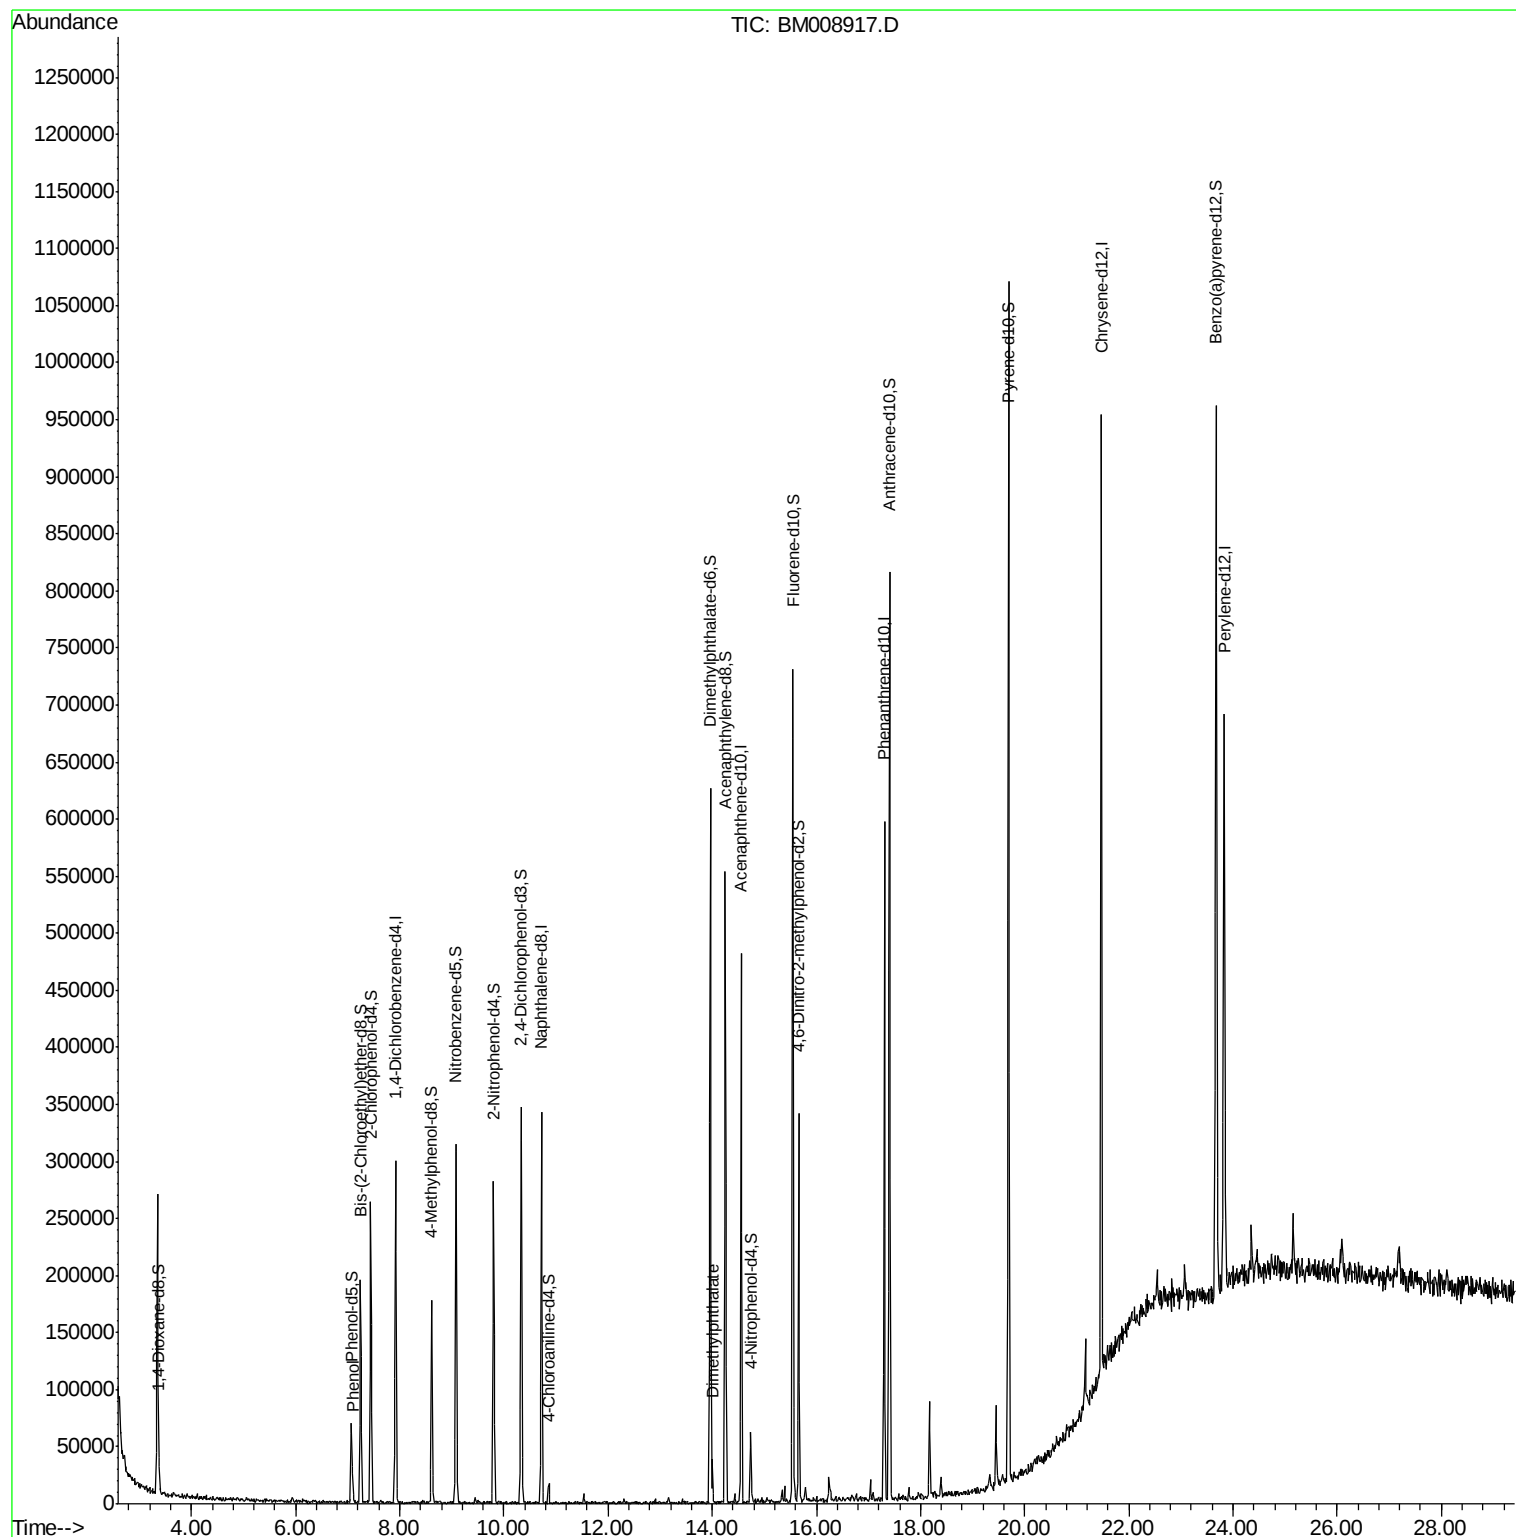

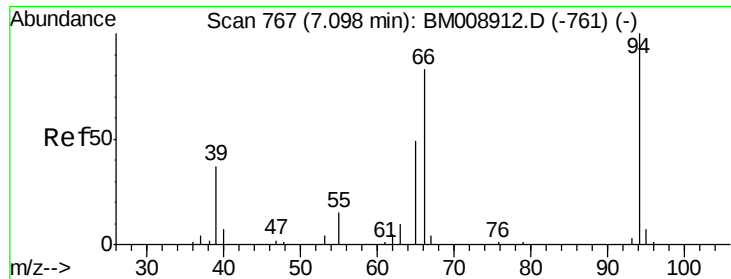

#6

Phenol

Concen: 1.38 ng/ul

RT: 7.10 min Scan# 767

Delta R.T. -0.00 min

Lab File: BM008917.D

Acq: 30 Jan 2017 18:19

Instrument :

BNA_M

ClientSampleId :

G9RA9





Tot Ion: 94 Resp: 5993

Ion Ratio Lower Upper

94 100

65 44.4 39.8 59.6

66 70.3 69.9 104.9

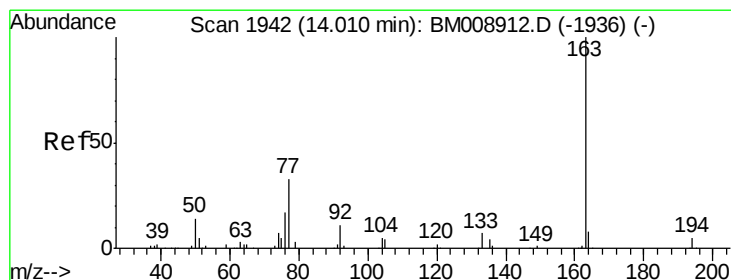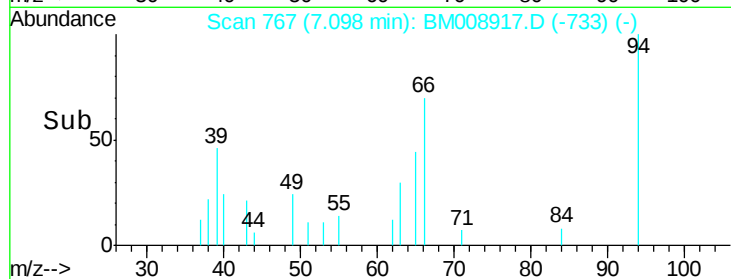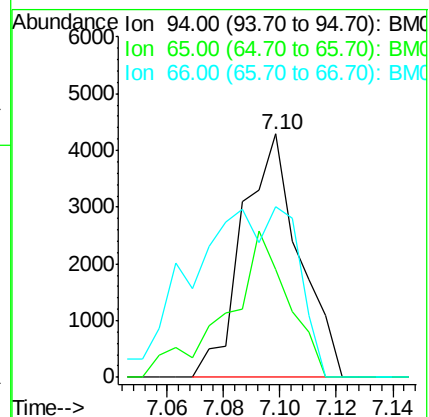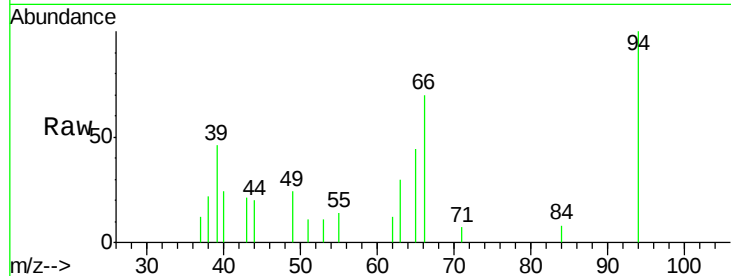

#44

Dimethylphthalate

Concen: 1.55 ng/ul

RT: 14.01 min Scan# 1942

Delta R.T. -0.00 min

Lab File: BM008917.D

Acq: 30 Jan 2017 18:19

Tgt Ion: 163 Resp: 13424

Ion Ratio Lower Upper

163 100

194 7.8 3.0 4.6#

164 11.4 8.6 12.8

