

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013017\
 Data File : BM008922.D
 Acq On : 30 Jan 2017 21:19
 Operator : SJ/MA
 Sample : I1467-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDMX4

Quant Time: Jan 31 03:27:50 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM013017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 31 02:42:41 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	46843	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	187894	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	148207	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	327700	20.00	ng/ul	0.00
75) Chrysene-d12	21.47	240	403808	20.00	ng/ul	0.00
83) Perylene-d12	23.83	264	390209	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.38	96	5825	4.97	ng/uL	0.00
5) Phenol-d5	7.07	99	40117	9.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.25	67	139173	38.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.45	132	83107	30.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.61	113	71701	21.68	ng/ul	0.00
19) Nitrobenzene-d5	9.09	128	54193	39.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.80	143	60945	40.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.33	165	114966	36.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	5568	1.91	ng/ul	0.00
43) Dimethylphthalate-d6	13.96	166	432147	39.78	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	496758	40.33	ng/ul	0.00
51) 4-Nitrophenol-d4	14.74	143	13808	7.79	ng/ul	0.00
57) Fluorene-d10	15.55	176	388793	38.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	69661	32.83	ng/ul	0.00
70) Anthracene-d10	17.40	188	645865	41.25	ng/ul	0.00
76) Pyrene-d10	19.69	212	754472	42.38	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.68	264	690042	38.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
33) 4-Chloro-3-methylphenol	11.99	107	9664	2.28	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013017\
Data File : BM008922.D
Acq On : 30 Jan 2017 21:19
Operator : SJ/MA
Sample : I1467-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDMX4

Quant Time: Jan 31 03:27:50 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM013017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 31 02:42:41 2017
Response via : Initial Calibration

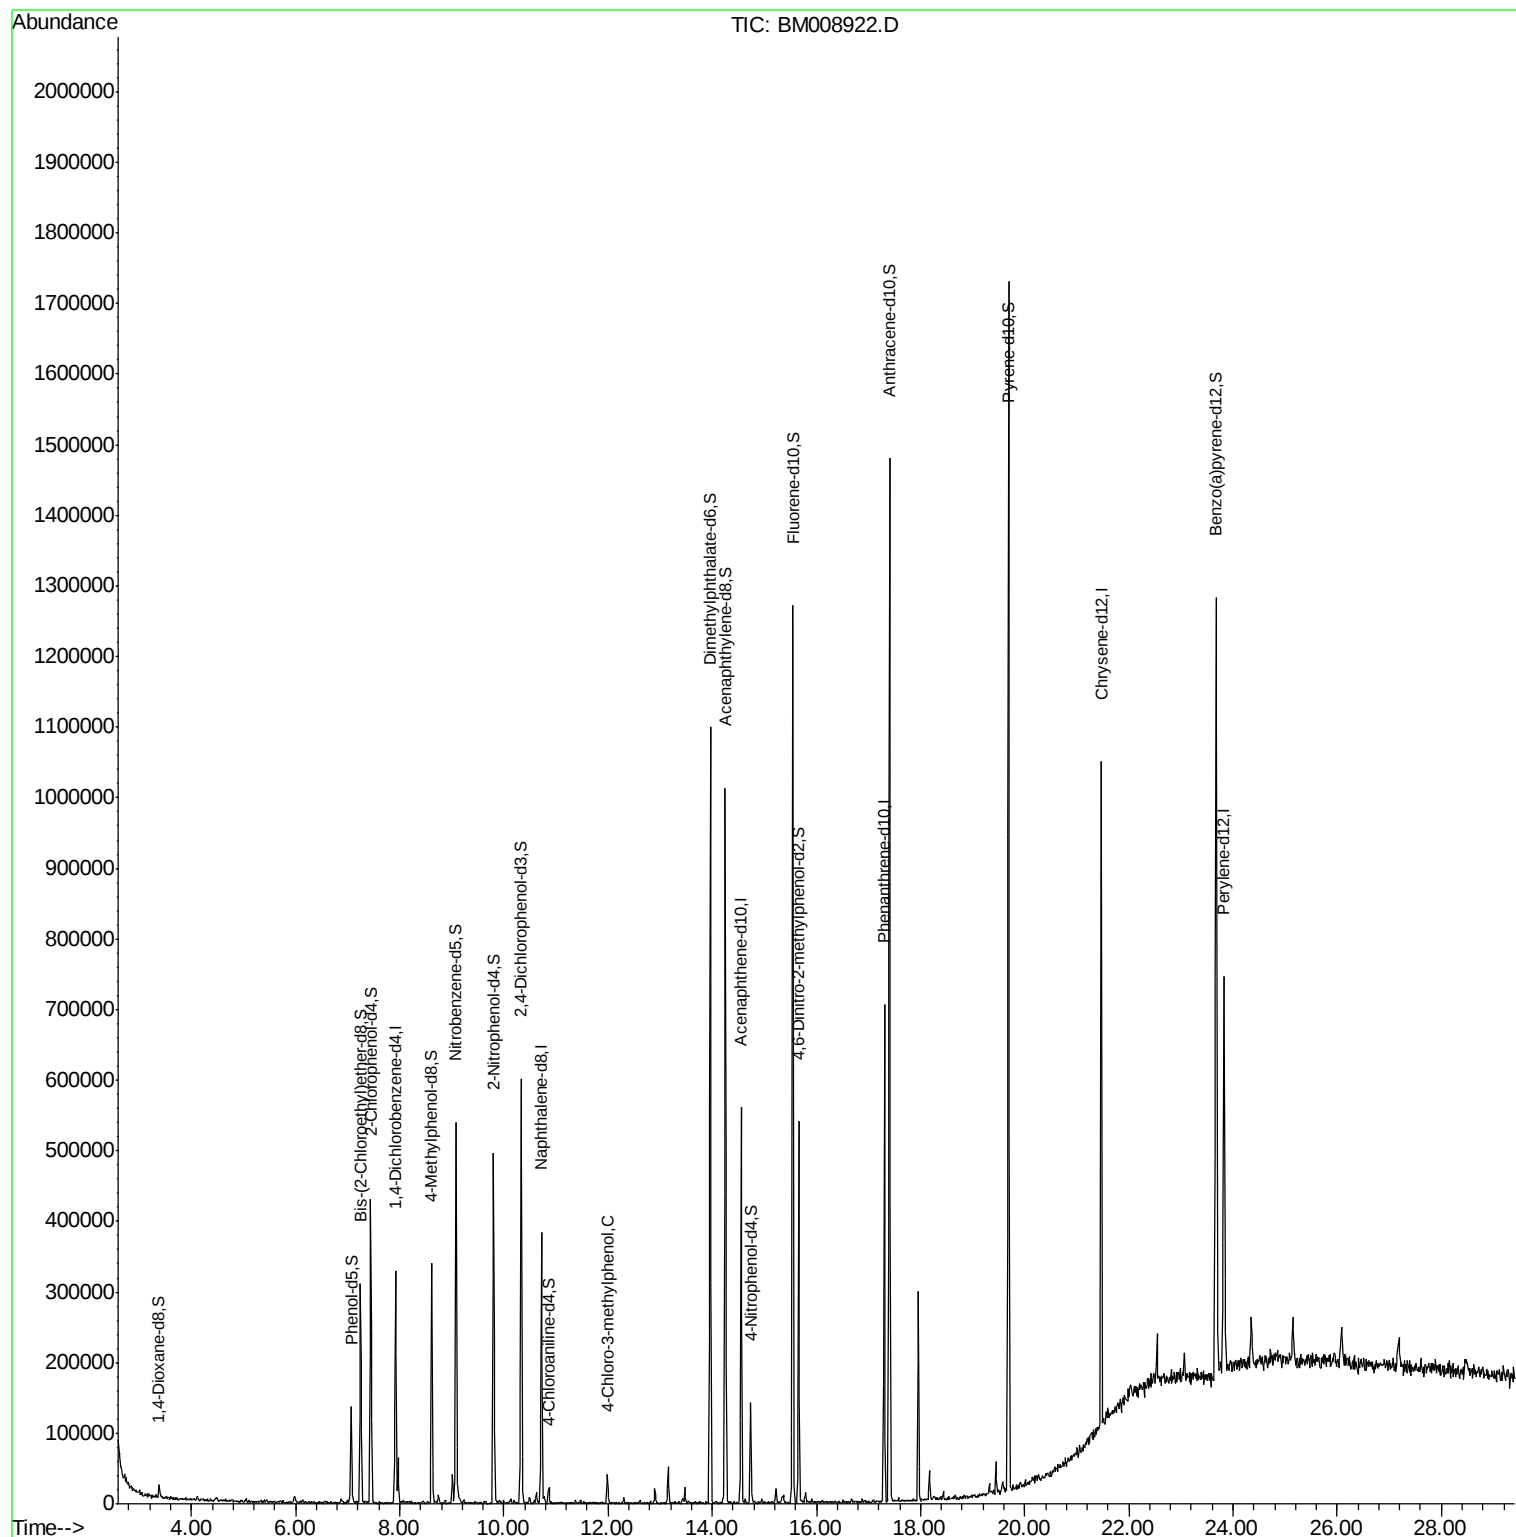

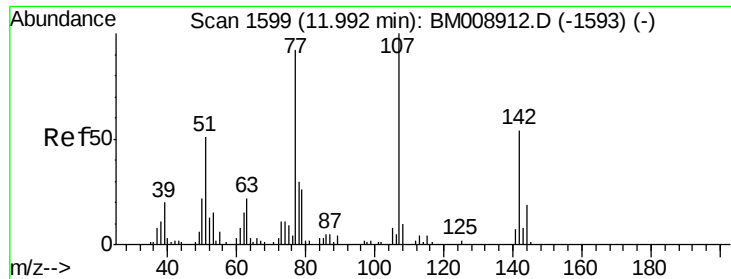

#33
 4-Chloro-3-methylphenol
 Concen: 2.28 ng/ul
 RT: 11.99 min Scan# 1599
 Delta R.T. -0.00 min
 Lab File: BM008922.D
 Acq: 30 Jan 2017 21:19

Instrument :
 BNA_M
 ClientSampleId :
 BDMX4

Tot Ion:107 Resp: 9664
 Ion Ratio Lower Upper
 107 100
 144 24.2 14.4 21.6#
 142 69.9 50.7 76.1

