

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013017\
 Data File : BM008924.D
 Acq On : 30 Jan 2017 22:31
 Operator : SJ/MA
 Sample : PB96373BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013017.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	129	134	142	rVB3	25555	41959	1.99%	0.183%
2	7.069	755	762	771	rVB2	482068	754593	35.76%	3.298%
3	7.245	785	792	799	rBV	283914	430270	20.39%	1.881%
4	7.445	820	826	833	rVB2	461110	719356	34.09%	3.144%
5	7.916	900	906	914	rVB2	312998	505428	23.95%	2.209%
6	8.610	1016	1024	1032	rBV	524627	820885	38.90%	3.588%
7	9.086	1098	1105	1113	rVB	458969	757038	35.87%	3.309%
8	9.804	1220	1227	1235	rBV2	417587	678692	32.16%	2.966%
9	10.333	1309	1317	1325	rBV2	551706	892977	42.31%	3.903%
10	10.722	1376	1383	1390	rVB	385258	636059	30.14%	2.780%
11	10.857	1399	1406	1413	rBV	502842	850559	40.30%	3.718%
12	13.963	1928	1934	1943	rVB	926233	1247352	59.10%	5.452%
13	14.251	1977	1983	1992	rVB	862441	1223680	57.98%	5.348%
14	14.557	2028	2035	2041	rBV	542935	798094	37.82%	3.488%
15	14.739	2060	2066	2075	rBV	606379	863752	40.93%	3.775%
16	15.551	2197	2204	2210	rVB	1096270	1533464	72.66%	6.702%
17	15.662	2216	2223	2232	rBV	470984	661662	31.35%	2.892%
18	17.303	2496	2502	2509	rVB2	717264	1010192	47.87%	4.415%
19	17.403	2512	2519	2527	rVB	1223254	1755630	83.19%	7.673%
20	19.692	2902	2908	2917	rVB	1547264	2046190	96.96%	8.943%
21	21.474	3205	3211	3217	rBV	982455	1307377	61.95%	5.714%
22	22.038	3305	3307	3311	rBV5	23577	33944	1.61%	0.148%
23	23.680	3578	3586	3595	rBV2	1018508	2110409	100.00%	9.224%
24	23.827	3605	3611	3621	rBV	645951	1200171	56.87%	5.246%


Sum of corrected areas: 22879733

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013017\
Data File : BM008924.D
Acq On : 30 Jan 2017 22:31
Operator : SJ/MA
Sample : PB96373BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM013017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

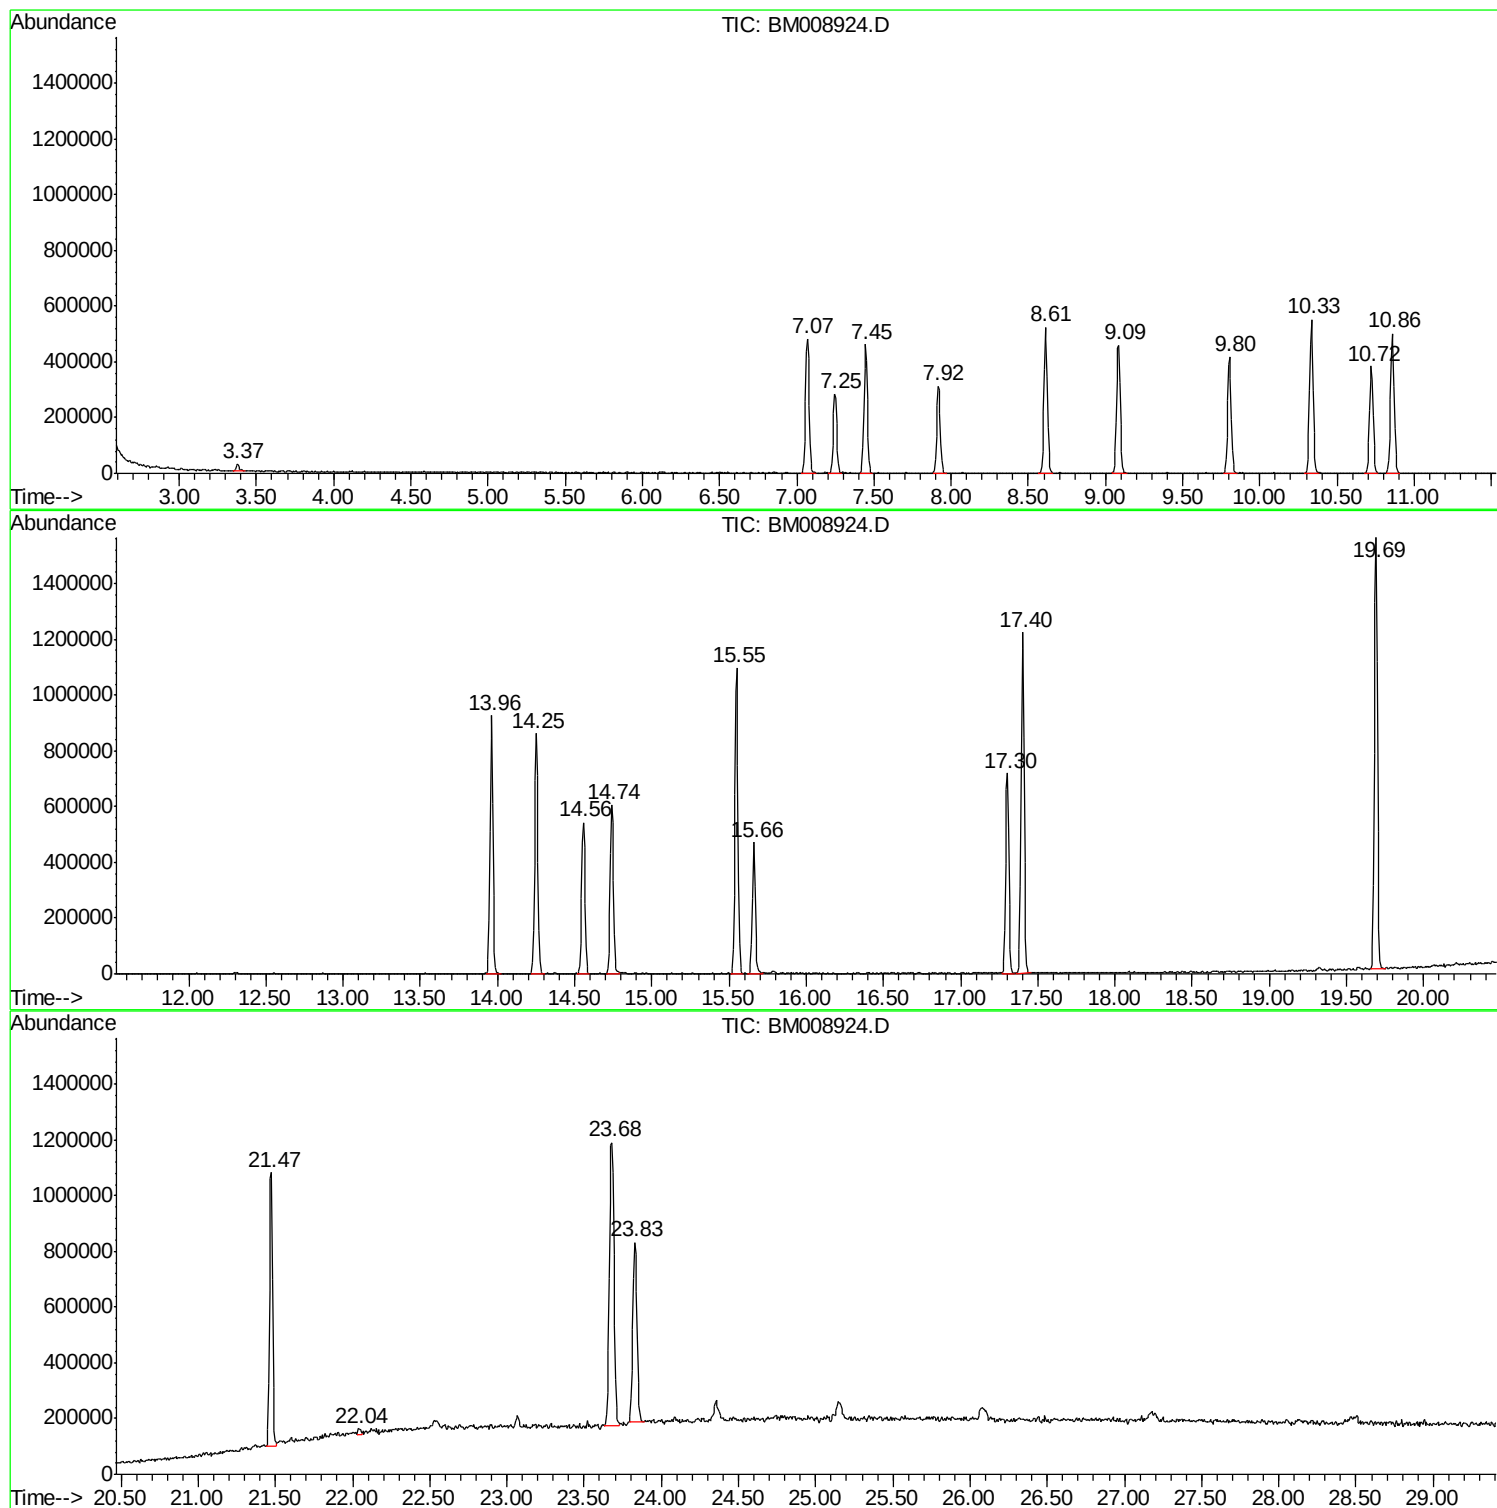

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM013017\
Data File : BM008924.D
Acq On : 30 Jan 2017 22:31
Operator : SJ/MA
Sample : PB96373BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM013017\
Data File : BM008924.D
Acq On : 30 Jan 2017 22:31
Operator : SJ/MA
Sample : PB96373BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc