

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013018\
 Data File : BM014004.D
 Acq On : 30 Jan 2018 19:11
 Operator : SJ/JU
 Sample : J1314-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 31 05:07:22 2018
 Quant Method : Z:\HPCHEM1\BNA M\Methods\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 30 07:49:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	77103	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	303514	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	187852	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	471753	20.00	ng/ul	0.00
75) Chrysene-d12	21.18	240	596370	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	619264	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	8483	4.35	ng/uL	0.00
5) Phenol-d5	6.76	99	142361	24.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	86614	24.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	111622	23.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	116672	25.64	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	58363	24.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	69277	27.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	119077	24.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	147401	35.34	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	462134	29.85	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	557912	28.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.48	143	28971	11.51	ng/ul	0.02
57) Fluorene-d10	15.22	176	406768	29.88	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	46374	16.33	ng/ul	0.00
70) Anthracene-d10	17.07	188	660520	28.75	ng/ul	0.00
76) Pyrene-d10	19.38	212	799504	28.79	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.22	264	866659	30.45	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	166167	10.916	ng/ul#	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013018\
Data File : BM014004.D
Acq On : 30 Jan 2018 19:11
Operator : SJ/JU
Sample : J1314-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 31 05:07:22 2018
Quant Method : Z:\HPCHEM1\BNA M\Methods\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 30 07:49:34 2018
Response via : Initial Calibration

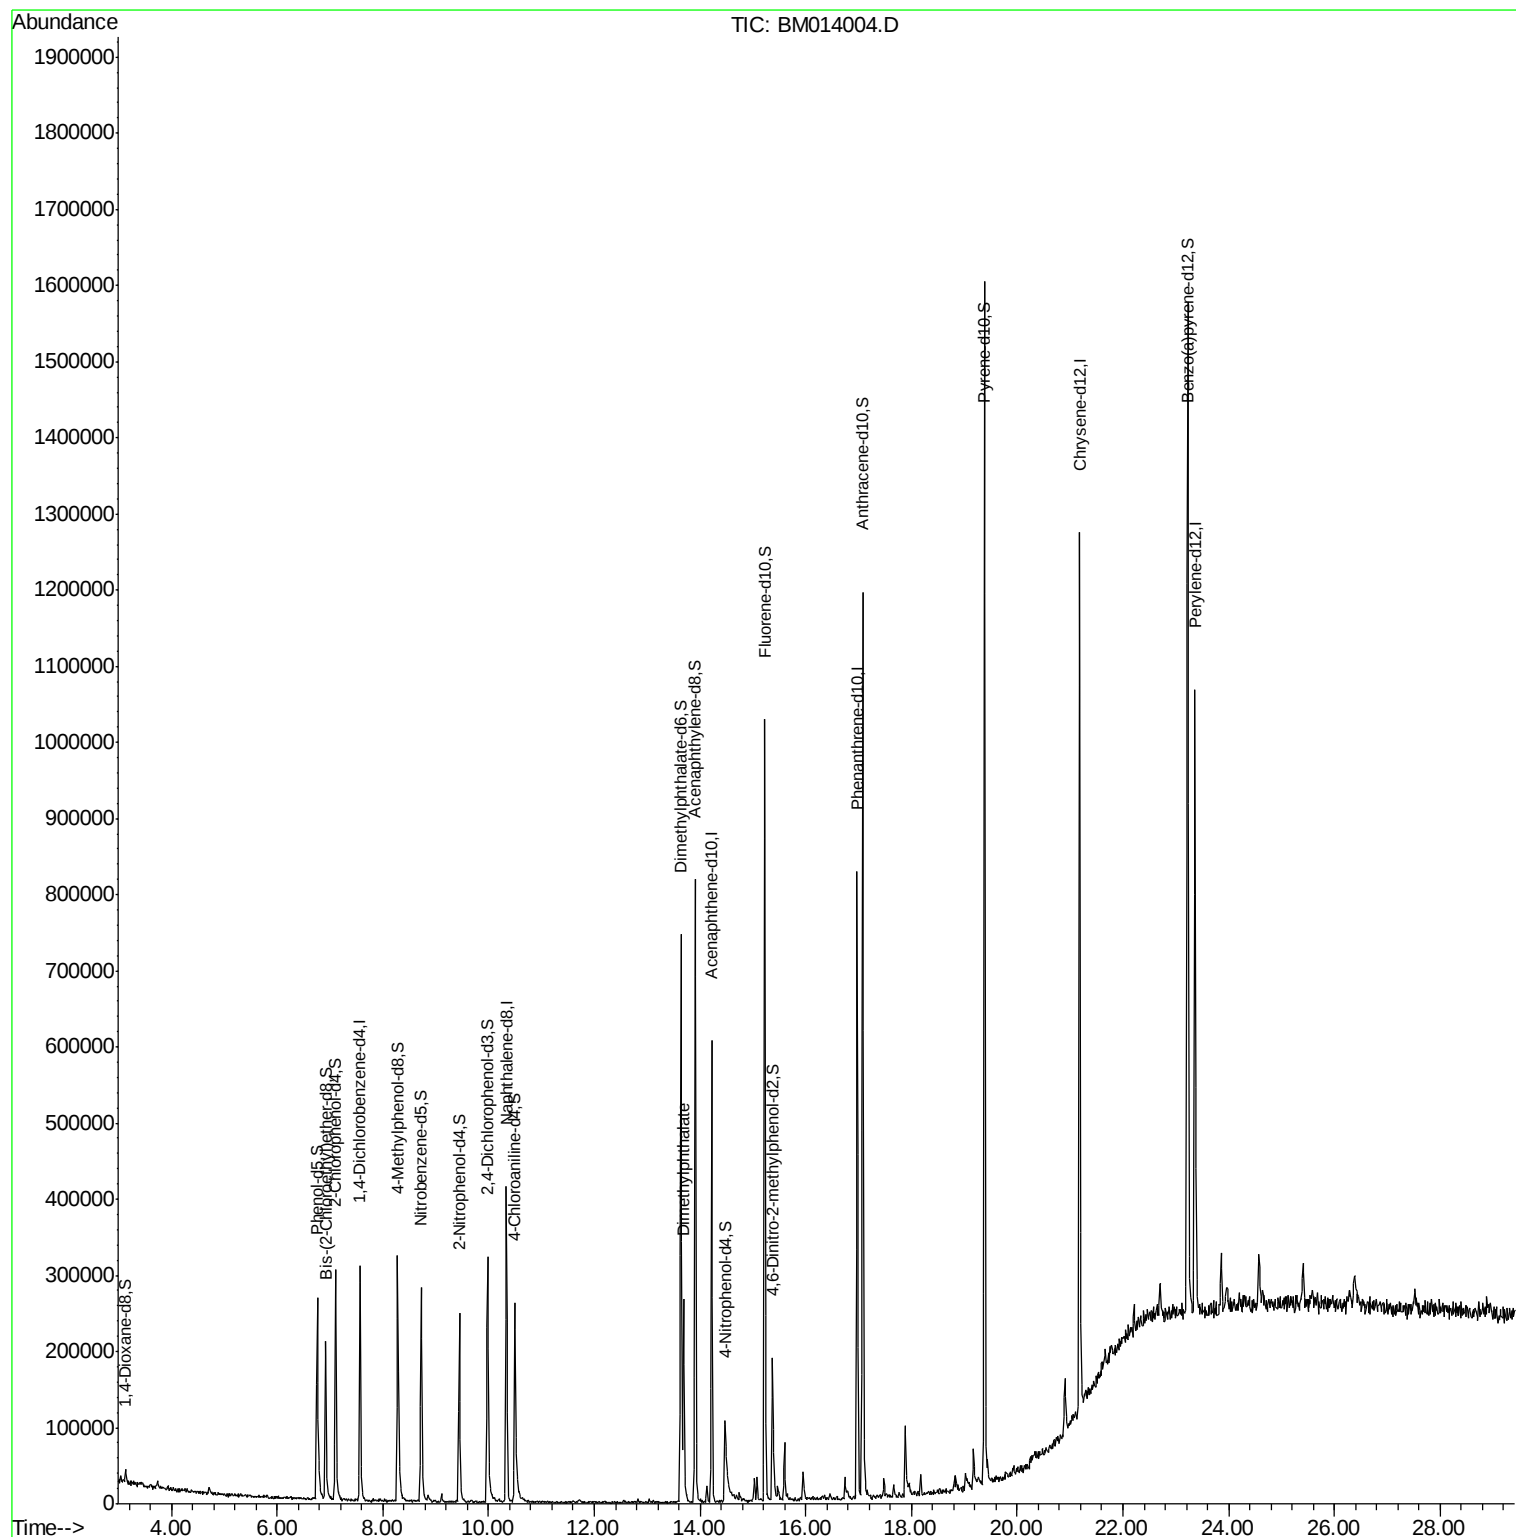

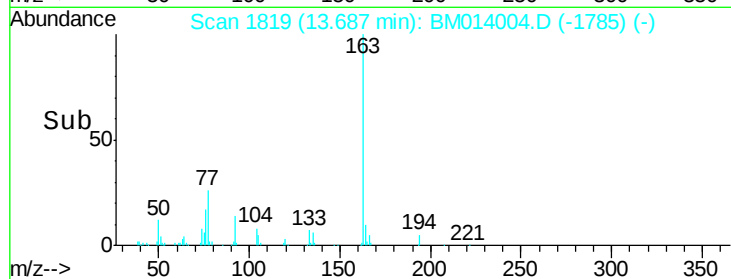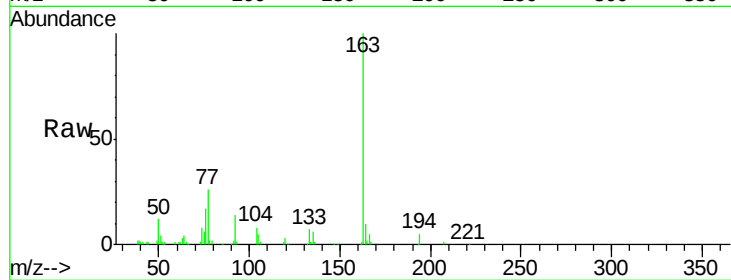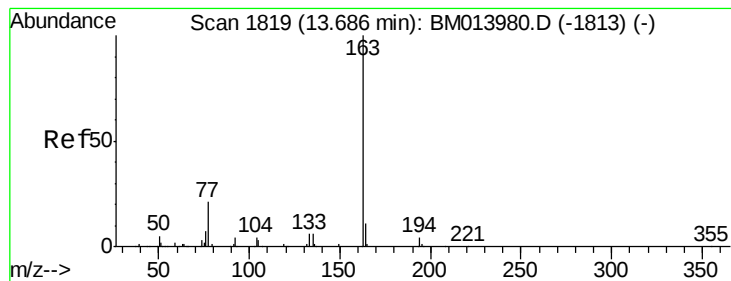

#44

Dimethylphthalate

Concen: 10.916 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. 0.00 min

Lab File: BM014004.D

Acq: 30 Jan 2018 19:11

Instrument :

BNA_M

ClientSampleId :

Tot Ion:163 Resp: 166167

Ion Ratio Lower Upper

163 100

194 5.4 3.5 5.3#

164 10.5 8.2 12.4

