

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_M\DATA\BM013018\
 Data File : BM014018.D
 Acq On : 31 Jan 2018 03:58
 Operator : SJ/JU
 Sample : J1315-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6C67

Manual Integrations
 APPROVED

Sohil
 1/31/2018 8:36:29 PM

Quant Time: Jan 31 07:17:45 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 31 07:06:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	99019	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	398814	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	247960	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	589658	20.00	ng/ul	0.00
75) Chrysene-d12	21.18	240	688490	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	694585	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	10804m	4.31	ng/uL	0.00
5) Phenol-d5	6.75	99	207186	27.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	126246	27.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	175955	28.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	176496	30.20	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	89028	28.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	98442	30.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	176296	27.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	228230	41.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	640787	31.36	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	797692	30.61	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	67468m	20.31	ng/ul	0.01
57) Fluorene-d10	15.22	176	571293	31.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	67241	18.95	ng/ul	0.00
70) Anthracene-d10	17.07	188	905094m	31.51	ng/ul	0.00
76) Pyrene-d10	19.38	212	1052123	32.82	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.22	264	1062999	33.30	ng/ul	0.00

Target Compounds						Qvalue
6) Phenol	6.78	94	30633	4.018	ng/ul	97
44) Dimethylphthalate	13.69	163	136877	6.812	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_M\DATA\BM013018\
Data File : BM014018.D
Acq On : 31 Jan 2018 03:58
Operator : SJ/JU
Sample : J1315-10
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6C67

Manual Integrations
APPROVED

Sohil
1/31/2018 8:36:29 PM

Quant Time: Jan 31 07:17:45 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 31 07:06:39 2018
Response via : Initial Calibration

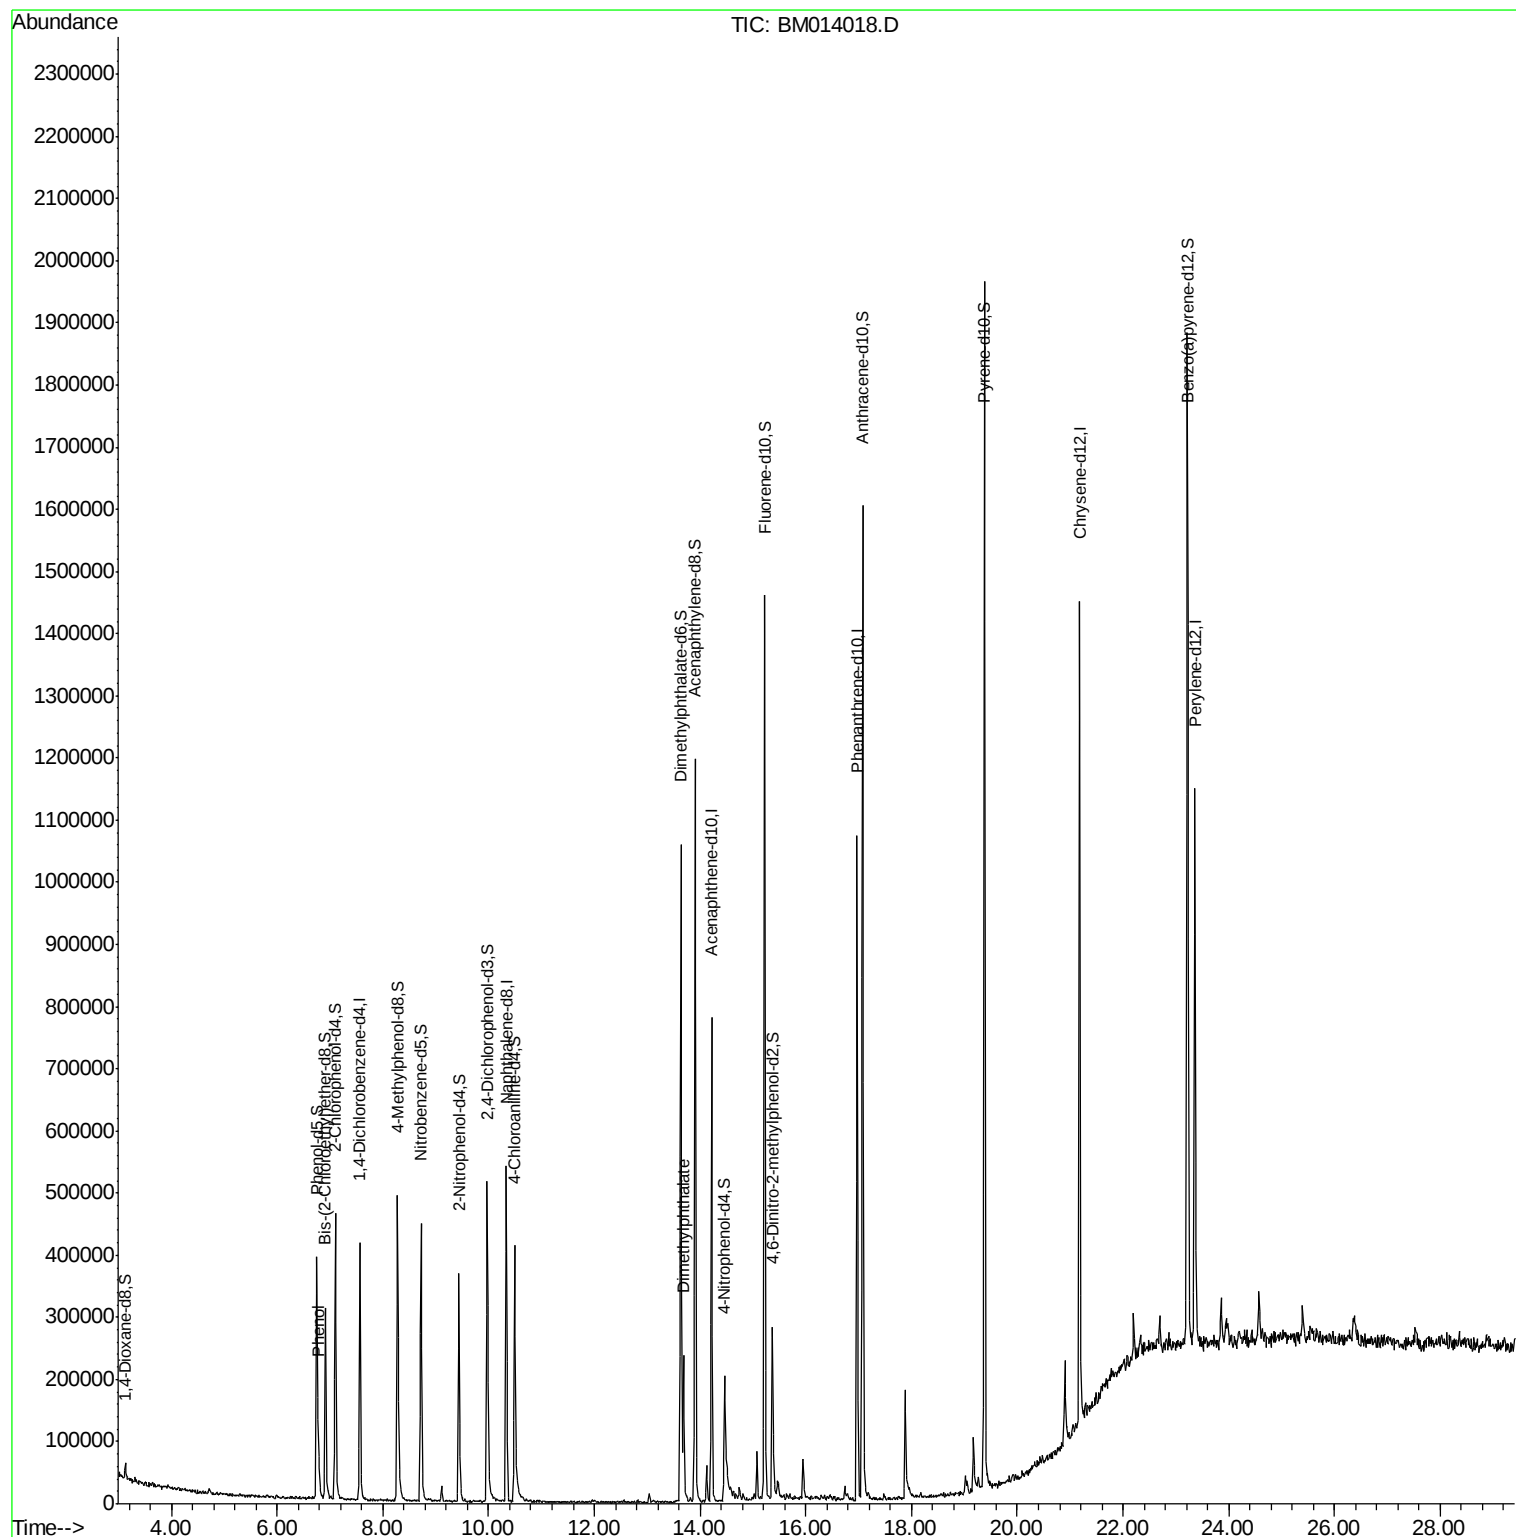

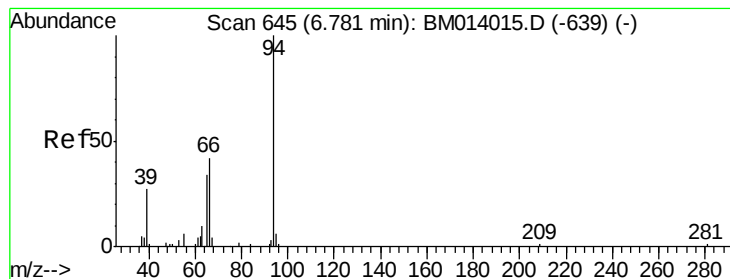

#6

Phenol

Concen: 4.018 ng/ul

RT: 6.78 min Scan# 645

Delta R.T. -0.00 min

Lab File: BM014018.D

Acq: 31 Jan 2018 03:58

Instrument :

BNA_M





ClientSampled :

F6C67

Tgt Ion:	94	Resp:	30633
Ion	Ratio	Lower	Upper
94	100		
65	34.4	28.2	42.4
66	61.7	47.2	70.8

Manual Integrations
APPROVED

Sohil
1/31/2018 8:36:29 PM

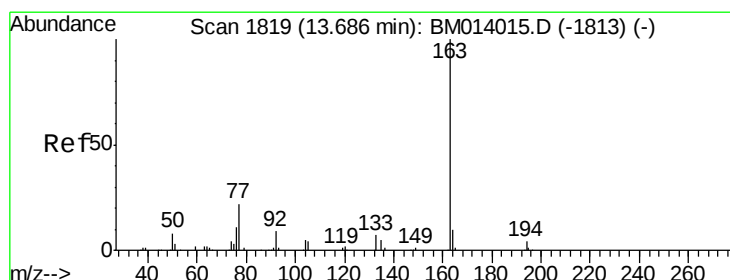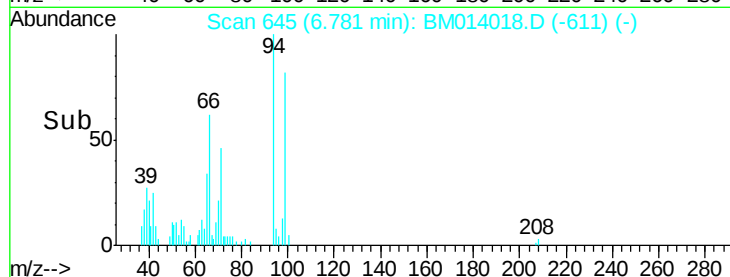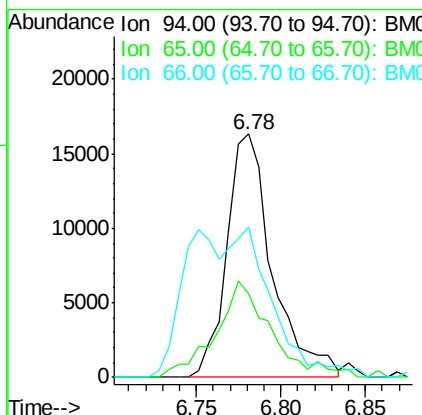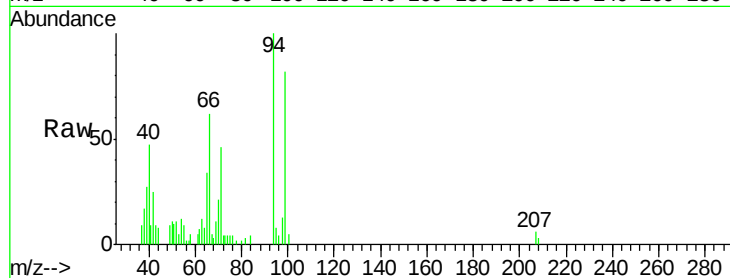

#44

Dimethylphthalate

Concen: 6.812 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. -0.00 min

Lab File: BM014018.D

Acq: 31 Jan 2018 03:58

Tgt Ion:	163	Resp:	136877
Ion	Ratio	Lower	Upper
163	100		
194	4.7	3.5	5.3
164	8.4	8.2	12.4

