
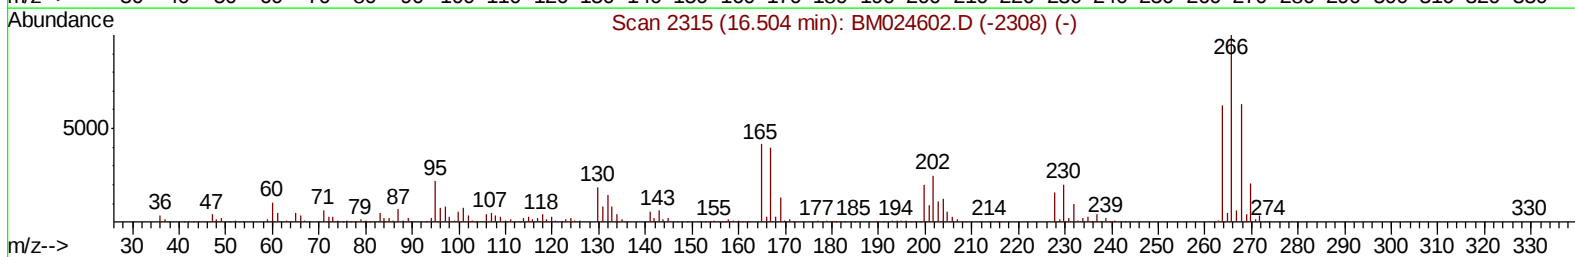
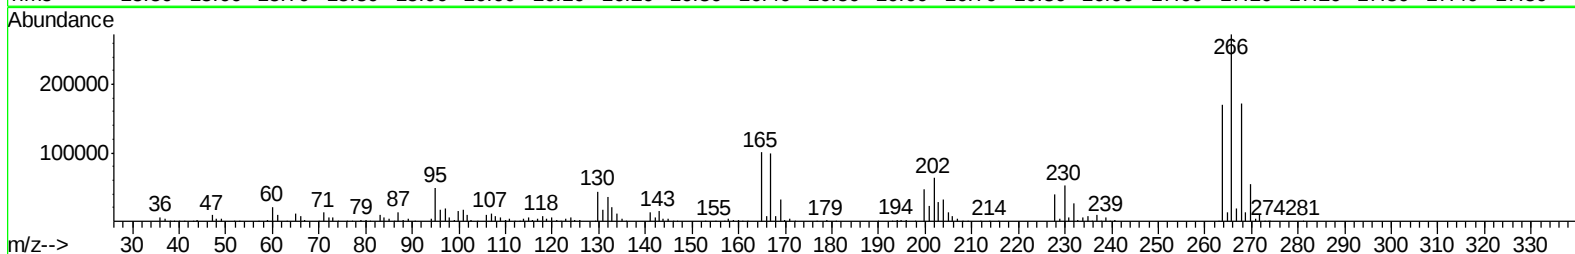


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013020\
 Data File : BM024658.D
 Acq On : 30 Jan 2020 14:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 03:16:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 23 14:57:07 2020
 Response via : Initial Calibration

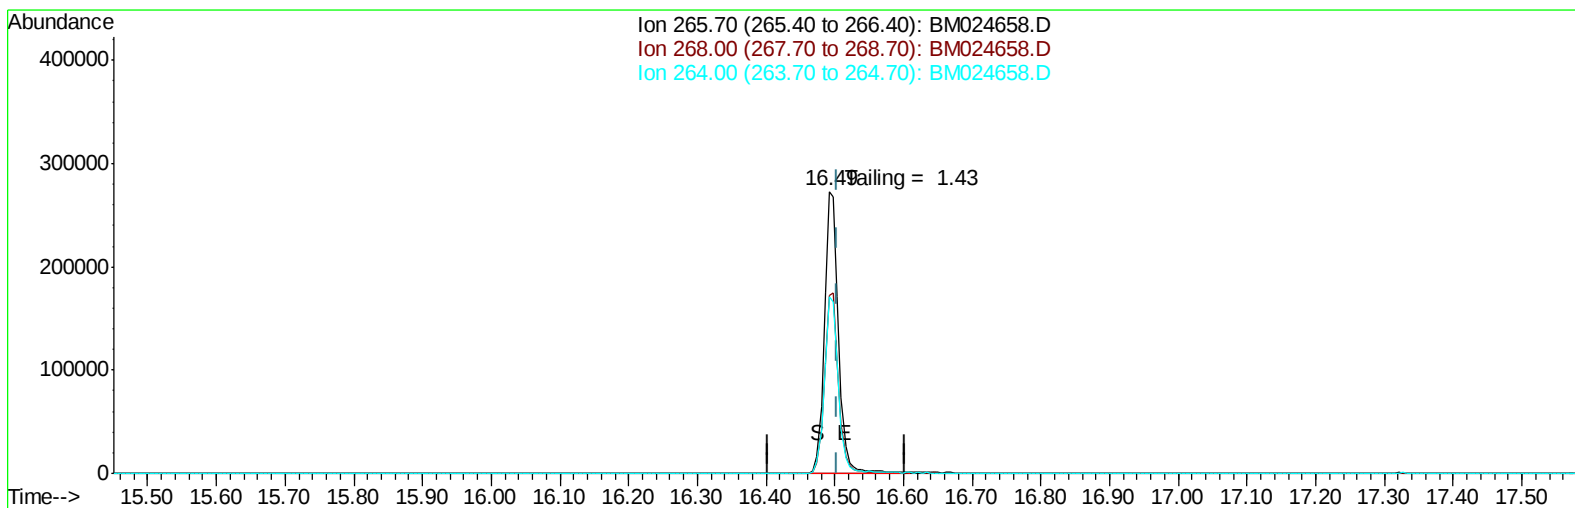

TIC: BM024658.D

(70) Pentachlorophenol (C)




16.492min (-0.012) 0.00ng

response 391838

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	63.22
264.00	62.40	62.54
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013020\
 Data File : BM024658.D
 Acq On : 30 Jan 2020 14:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 03:16:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 23 14:57:07 2020
 Response via : Initial Calibration

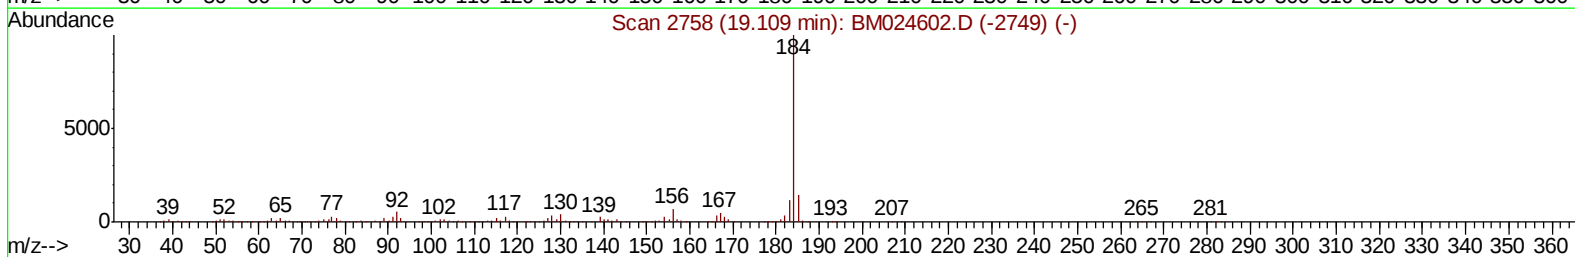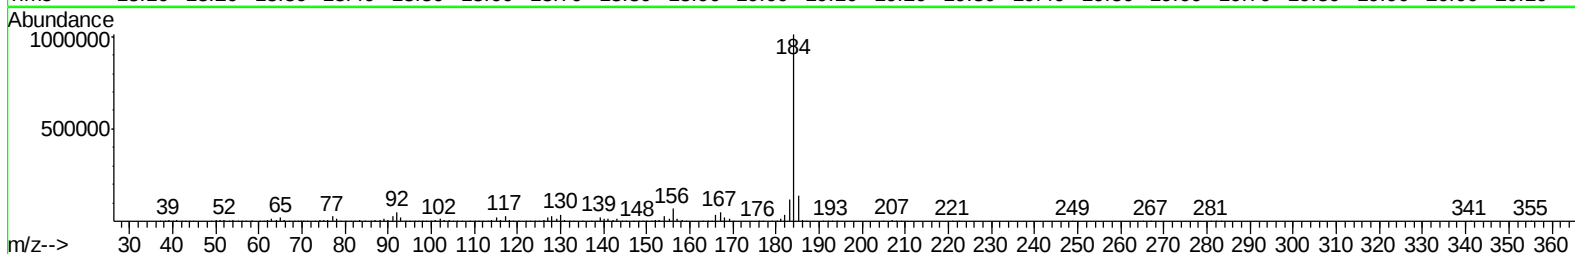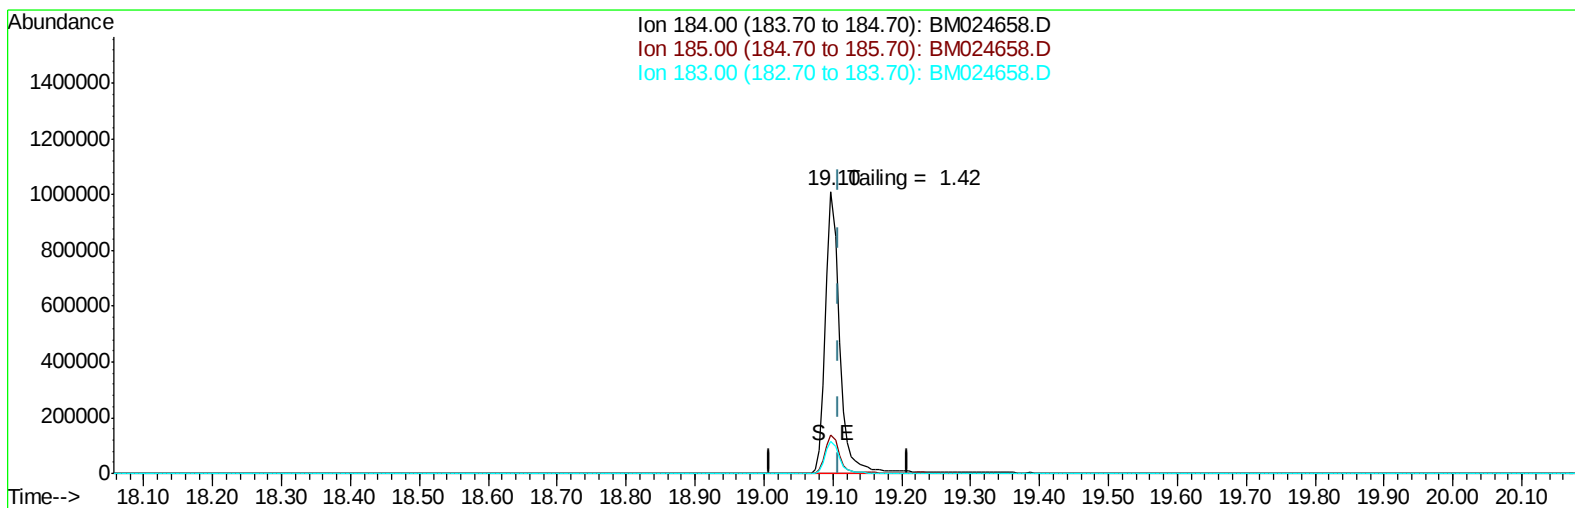

TIC: BM024658.D

(77) Benzidine

19.098min (-0.012) 92797.10ng

response 1428501

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.83
183.00	12.00	11.55
0.00	0.00	0.00