

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013020\
 Data File : BM024675.D
 Acq On : 31 Jan 2020 01:06
 Operator : CG/JU
 Sample : L1287-03DL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 AOC-3-EXC-PIT-(0-5)-BDL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	366	371	378	rBV	402748	575446	8.32%	0.449%
2	6.628	626	636	650	rBV	386436	672466	9.72%	0.525%
3	7.428	765	772	784	rVB	734536	1168265	16.89%	0.911%
4	7.745	819	826	831	rBV	370693	598264	8.65%	0.467%
5	7.798	831	835	840	rVB	126787	184272	2.66%	0.144%
6	7.963	853	863	873	rBV3	73829	214179	3.10%	0.167%
7	8.563	961	965	971	rVB	218336	347850	5.03%	0.271%
8	9.604	1135	1142	1153	rBV5	78372	235567	3.41%	0.184%
9	10.186	1233	1241	1246	rBV	948567	1651762	23.89%	1.289%
10	10.233	1246	1249	1257	rVB	283294	470742	6.81%	0.367%
11	11.257	1415	1423	1427	rBV	215199	422108	6.10%	0.329%
12	11.857	1518	1525	1536	rVB	860487	1622379	23.46%	1.266%
13	11.975	1538	1545	1551	rBV7	60570	185514	2.68%	0.145%
14	12.086	1551	1564	1569	rBV	1763476	3002282	43.41%	2.342%
15	12.645	1655	1659	1662	rVV	307211	427657	6.18%	0.334%
16	12.692	1662	1667	1672	rVB	690333	1053410	15.23%	0.822%
17	12.904	1699	1703	1707	rVB2	169238	232332	3.36%	0.181%
18	12.957	1708	1712	1718	rBV5	102566	204678	2.96%	0.160%
19	13.098	1731	1736	1749	rVB	374342	793971	11.48%	0.619%
20	13.239	1754	1760	1761	rBV	705371	1009537	14.60%	0.788%
21	13.398	1778	1787	1792	rVV	1295941	2371502	34.29%	1.850%
22	13.451	1792	1796	1802	rVV	757704	1144361	16.55%	0.893%
23	13.510	1802	1806	1816	rVV3	327097	896517	12.96%	0.699%
24	13.610	1816	1823	1824	rVV2	471263	680306	9.84%	0.531%
25	13.633	1824	1827	1831	rVV	754603	1197678	17.32%	0.934%
26	13.669	1831	1833	1838	rVB2	288890	342237	4.95%	0.267%
27	13.798	1849	1855	1865	rBV2	808818	1510009	21.84%	1.178%
28	13.921	1872	1876	1881	rVB	236768	297818	4.31%	0.232%
29	14.080	1896	1903	1909	rBV2	1566088	2742038	39.65%	2.139%
30	14.145	1909	1914	1918	rBV	1983368	2816496	40.73%	2.197%
31	14.304	1935	1941	1950	rBV2	329700	772311	11.17%	0.603%
32	14.386	1951	1955	1959	rVV3	166240	220821	3.19%	0.172%
33	14.492	1966	1973	1979	rVB2	522578	1044356	15.10%	0.815%
34	14.568	1979	1986	1990	rBV	595650	880639	12.73%	0.687%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013020\
 Data File : BM024675.D
 Acq On : 31 Jan 2020 01:06
 Operator : CG/JU
 Sample : L1287-03DL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 AOC-3-EXC-PIT-(0-5)-BDL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.657	1998	2001	2004	rVB4	149297	187435	2.71%	0.146%
36	14.716	2005	2011	2015	rVV3	377325	768541	11.11%	0.600%
37	14.763	2016	2019	2024	rVB	467829	640666	9.26%	0.500%
38	14.886	2033	2040	2043	rBV3	431576	751989	10.87%	0.587%
39	14.957	2049	2052	2056	rVB	209960	273938	3.96%	0.214%
40	15.080	2070	2073	2077	rVB2	263685	356289	5.15%	0.278%
41	15.133	2077	2082	2088	rBV	1707493	2438789	35.27%	1.903%
42	15.186	2088	2091	2096	rVV2	191762	360403	5.21%	0.281%
43	15.233	2096	2099	2101	rVV	298627	363147	5.25%	0.283%
44	15.263	2101	2104	2107	rVV	396044	495685	7.17%	0.387%
45	15.298	2107	2110	2113	rVB2	192257	218575	3.16%	0.171%
46	15.398	2123	2127	2131	rVV2	340682	514361	7.44%	0.401%
47	15.433	2131	2133	2136	rVB2	165534	185753	2.69%	0.145%
48	15.574	2149	2157	2167	rVB6	814029	1936752	28.01%	1.511%
49	15.668	2168	2173	2179	rBV4	187677	405879	5.87%	0.317%
50	15.827	2197	2200	2205	rVB3	241571	330287	4.78%	0.258%
51	15.880	2205	2209	2214	rVB	738364	1016647	14.70%	0.793%
52	15.963	2220	2223	2227	rBV3	187348	251092	3.63%	0.196%
53	16.151	2247	2255	2259	rBV2	844241	1647973	23.83%	1.286%
54	16.198	2259	2263	2269	rVB2	485631	683783	9.89%	0.533%
55	16.292	2276	2279	2286	rVB2	388682	624306	9.03%	0.487%
56	16.415	2297	2300	2304	rVB5	218530	293351	4.24%	0.229%
57	16.504	2311	2315	2320	rVB4	267580	463727	6.71%	0.362%
58	16.651	2336	2340	2344	rVV	554608	746886	10.80%	0.583%
59	16.704	2345	2349	2357	rVB3	463376	731446	10.58%	0.571%
60	16.833	2366	2371	2374	rBV	1900262	2725579	39.41%	2.127%
61	16.874	2374	2378	2383	rVB	4976174	6714968	97.10%	5.239%
62	16.962	2389	2393	2398	rVB	1751735	2284962	33.04%	1.783%
63	17.039	2401	2406	2411	rBV2	462761	887236	12.83%	0.692%
64	17.415	2466	2470	2475	rVB2	447454	626846	9.06%	0.489%
65	17.562	2490	2495	2502	rVB	314055	558178	8.07%	0.435%
66	17.709	2515	2520	2524	rBV	1531390	2246647	32.49%	1.753%
67	17.756	2524	2528	2536	rVB	1686252	2512595	36.33%	1.960%
68	17.839	2537	2542	2547	rVV2	774483	1220861	17.65%	0.953%
69	17.898	2547	2552	2556	rVV2	2168175	3754494	54.29%	2.929%
70	17.939	2556	2559	2569	rVB	1173795	1825208	26.39%	1.424%
71	18.115	2585	2589	2591	rBV2	302608	460637	6.66%	0.359%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013020\
 Data File : BM024675.D
 Acq On : 31 Jan 2020 01:06
 Operator : CG/JU
 Sample : L1287-03DL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 AOC-3-EXC-PIT-(0-5)-BDL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	18.215	2603	2606	2611	rVB	556622	664766	9.61%	0.519%
73	18.327	2623	2625	2630	rVB4	204253	256011	3.70%	0.200%
74	18.474	2647	2650	2654	rVB2	547080	708921	10.25%	0.553%
75	18.521	2655	2658	2661	rBV	333104	447522	6.47%	0.349%
76	18.615	2670	2674	2675	rBV	324614	410180	5.93%	0.320%
77	18.645	2675	2679	2684	rVB	1036765	1485241	21.48%	1.159%
78	18.703	2684	2689	2692	rBV3	501105	865355	12.51%	0.675%
79	18.780	2699	2702	2704	rBV3	296422	414561	5.99%	0.323%
80	18.903	2718	2723	2728	rBV	3493269	4721092	68.27%	3.683%
81	18.980	2732	2736	2739	rBV	1162828	1425525	20.61%	1.112%
82	19.056	2745	2749	2754	rVB	928663	1285894	18.59%	1.003%
83	19.262	2780	2784	2789	rVB	3976151	5253403	75.97%	4.099%
84	19.486	2818	2822	2826	rBV	1551990	1951929	28.23%	1.523%
85	19.603	2838	2842	2852	rBV	520464	1118429	16.17%	0.873%
86	19.703	2855	2859	2862	rBV	755846	957047	13.84%	0.747%
87	19.768	2867	2870	2875	rVB	1265767	1802256	26.06%	1.406%
88	19.874	2884	2888	2891	rVB	1056401	1211434	17.52%	0.945%
89	19.927	2894	2897	2902	rVB	746128	926192	13.39%	0.723%
90	20.068	2918	2921	2925	rVB	551476	623152	9.01%	0.486%
91	20.115	2925	2929	2935	rVB	679914	930796	13.46%	0.726%
92	20.762	3036	3039	3042	rBV2	464762	568034	8.21%	0.443%
93	20.997	3075	3079	3082	rBV	4283426	5236941	75.73%	4.086%
94	21.039	3082	3086	3090	rVV2	3808574	6915442	100.00%	5.395%
95	21.074	3090	3092	3103	rVB	2069425	2818156	40.75%	2.199%
96	21.327	3131	3135	3138	rBV	1505465	1683923	24.35%	1.314%
97	22.533	3336	3340	3345	rBV2	1005979	2134659	30.87%	1.665%
98	22.974	3411	3415	3422	rVB	828280	1432924	20.72%	1.118%
99	23.062	3425	3430	3435	rVB	1258452	2079759	30.07%	1.623%
100	23.150	3440	3445	3450	rVV	2068153	3346265	48.39%	2.611%


Sum of corrected areas: 128171490

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013020\
Data File : BM024675.D
Acq On : 31 Jan 2020 01:06
Operator : CG/JU
Sample : L1287-03DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-BDL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

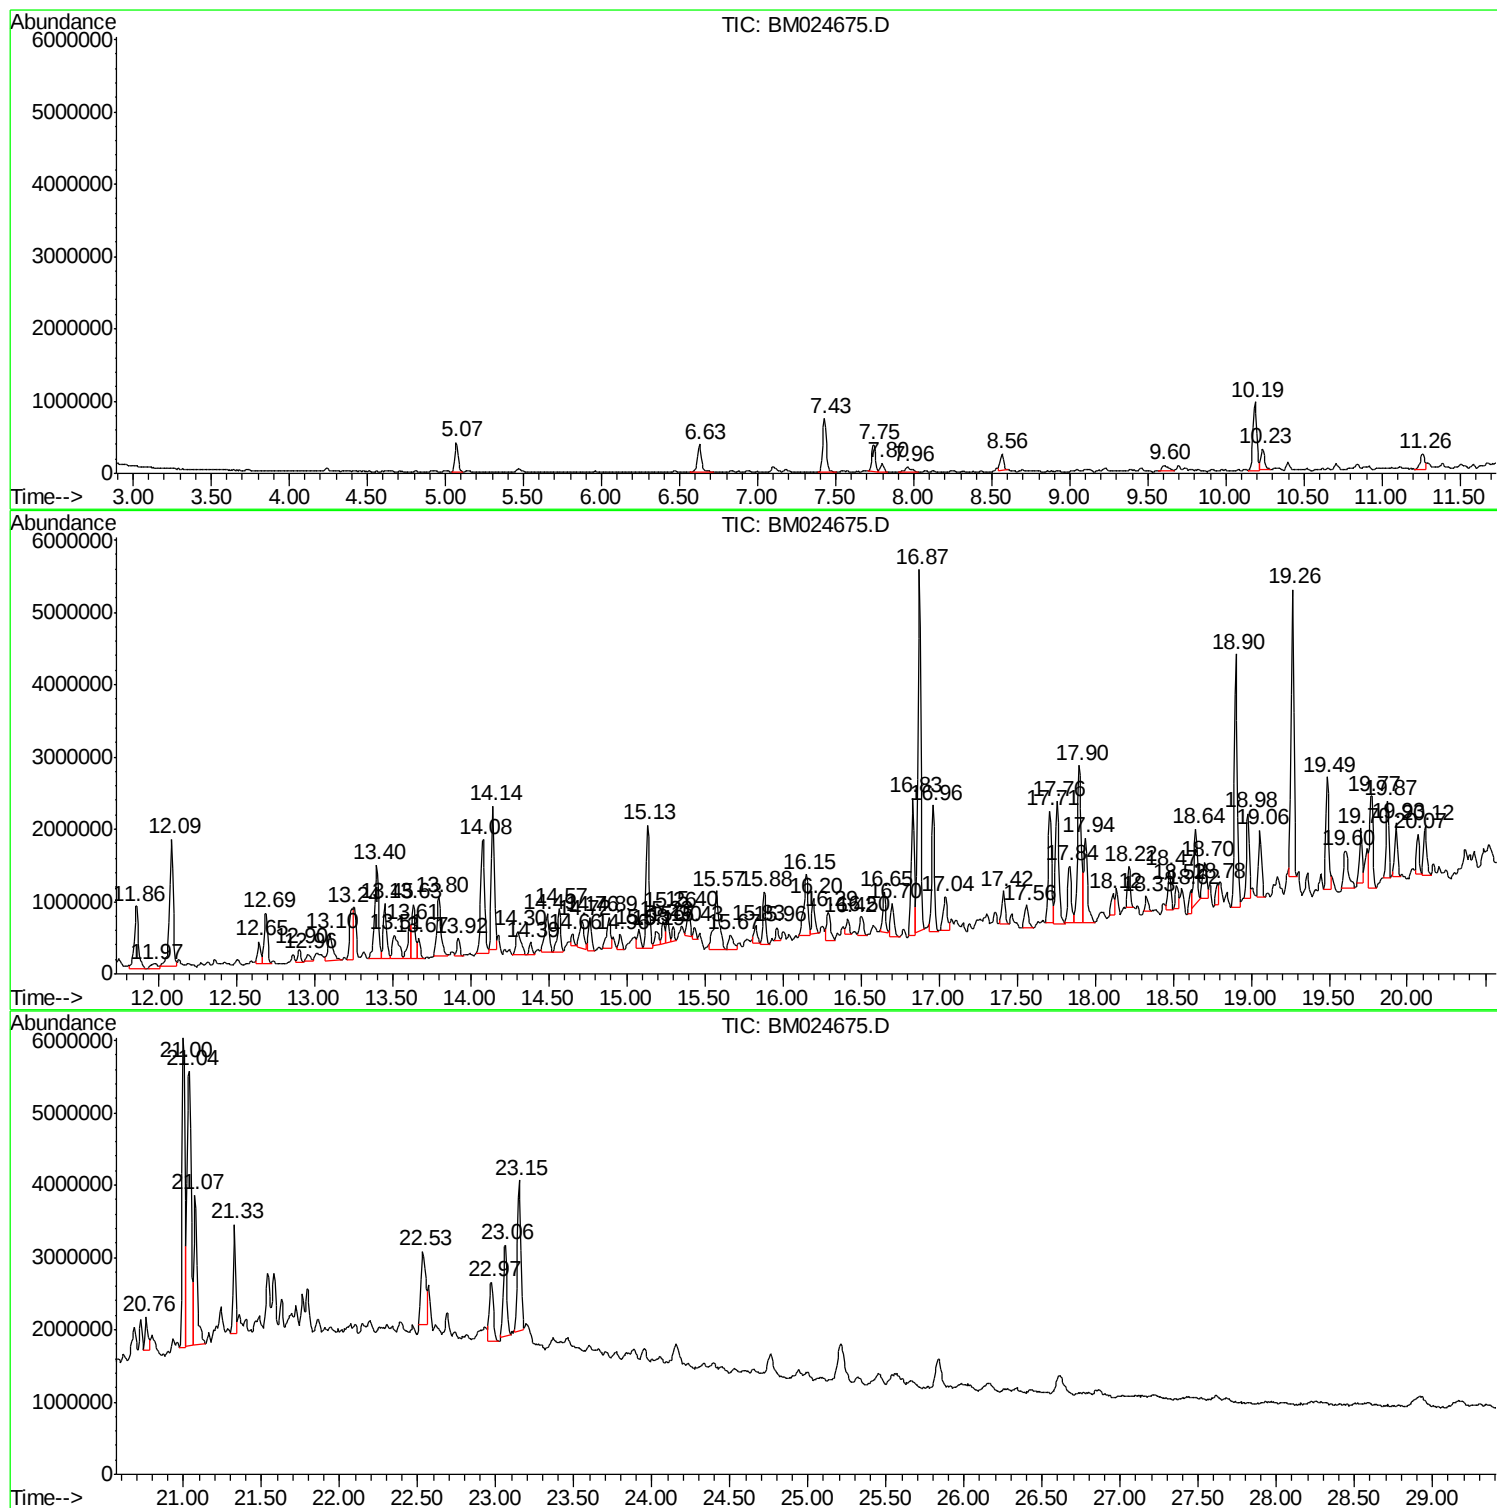

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM013020\
Data_File : BM024675.D
Acq_On : 31-Jan-2020 01:066
Operator : CG/JUU
Sample : L1287-03DL_5X
Misc :
ALS_Vial : 18 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-BDL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
