


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM013020\  
 Data File : BM024658.D  
 Acq On : 30 Jan 2020 14:16  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM012320.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jan 23 14:57:07 2020

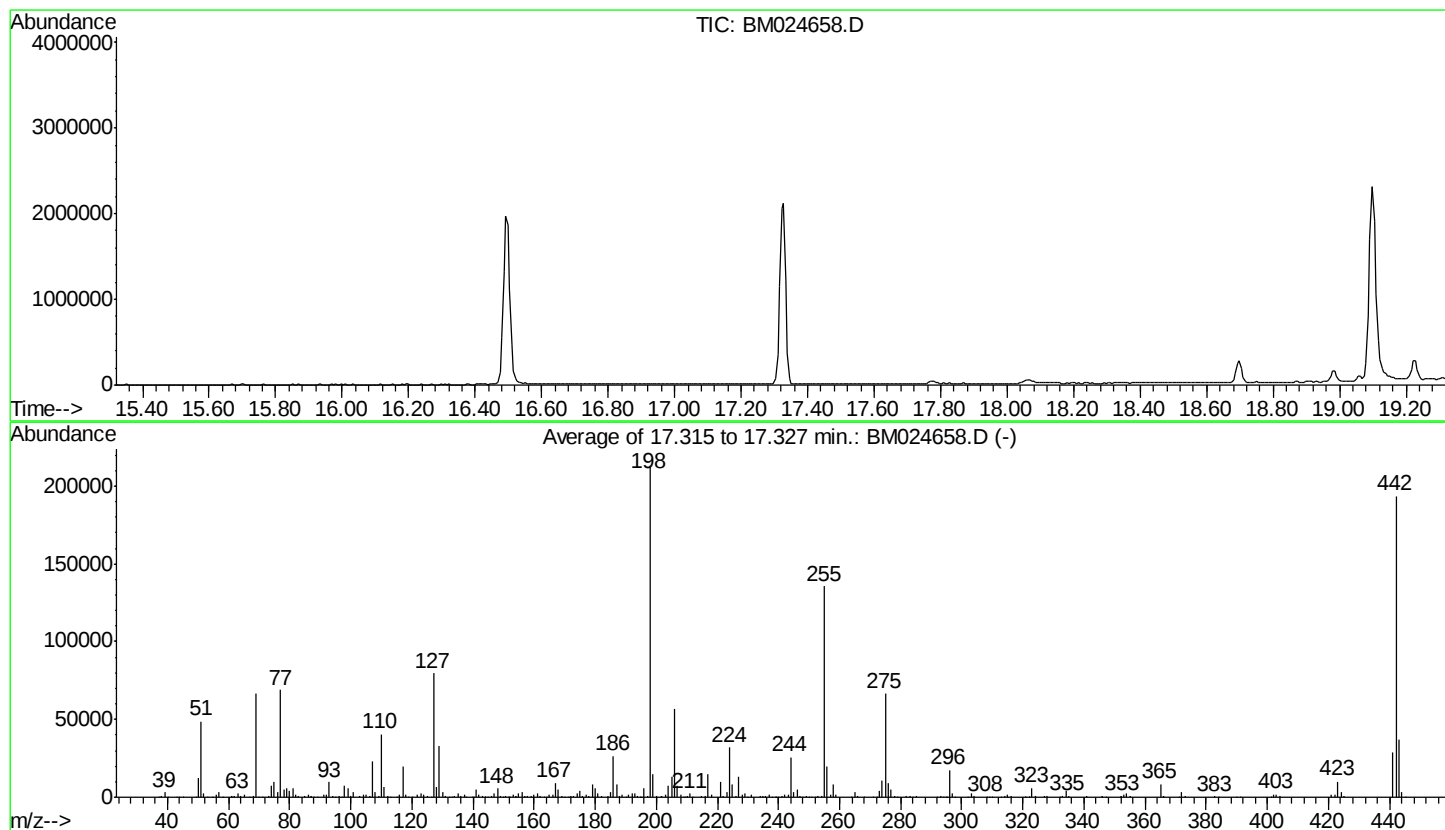

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 22.9      | 48896   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 923     | PASS             |
| 69          | 198          | 0.00         | 100          | 31.2      | 66589   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 403     | PASS             |
| 127         | 198          | 10           | 80           | 37.3      | 79557   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 761     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 213141  | PASS             |
| 199         | 198          | 5            | 9            | 7.1       | 15102   | PASS             |
| 275         | 198          | 10           | 60           | 31.2      | 66456   | PASS             |
| 365         | 198          | 1            | 100          | 3.9       | 8384    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.5      | 28847   | PASS             |
| 442         | 198          | 50           | 100          | 90.8      | 193536  | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 37266   | PASS             |