
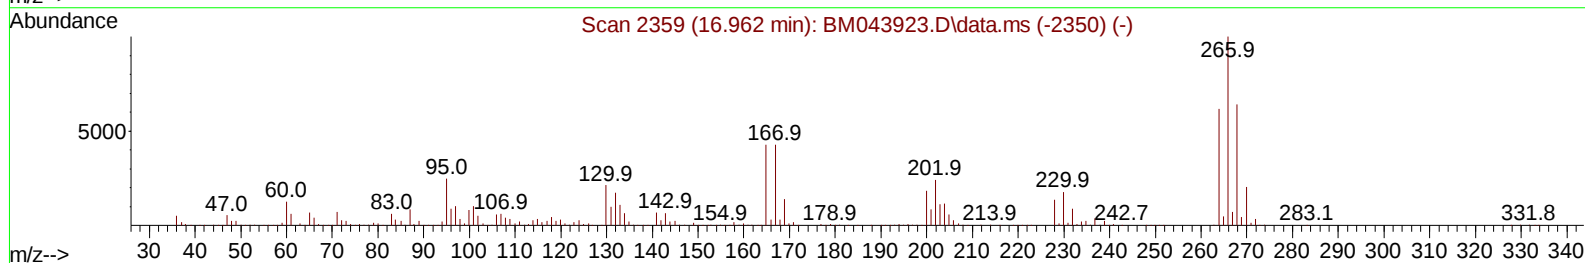
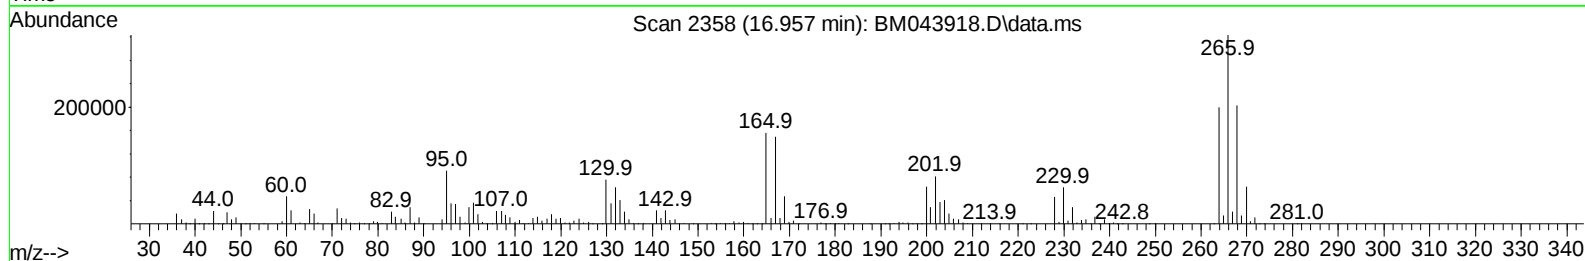


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013024\
Data File : BM043918.D
Acq On : 30 Jan 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 00:49:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 00:42:42 2024
Response via : Initial Calibration

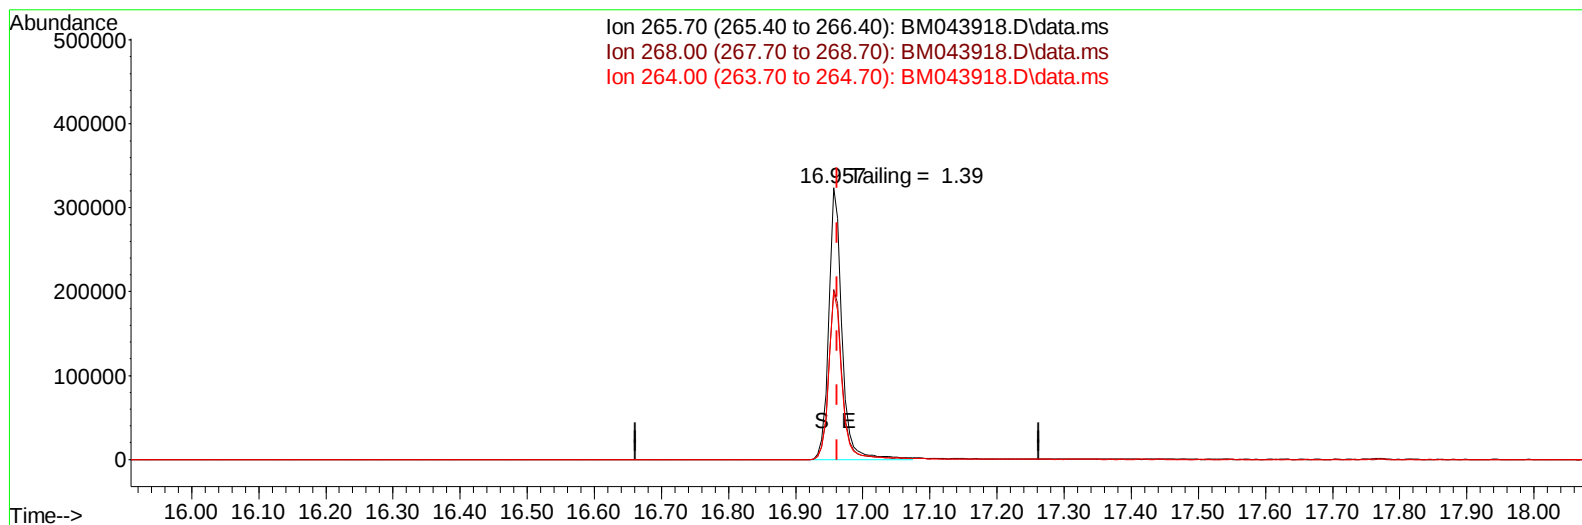

TIC: BM043918.D\data.ms

(70) Pentachloropheno1 (C)




16.957min (-0.005) 0.00 ng

response 448423

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.71
264.00	61.70	61.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013024\
Data File : BM043918.D
Acq On : 30 Jan 2024 09:53
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 00:49:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 00:42:42 2024
Response via : Initial Calibration

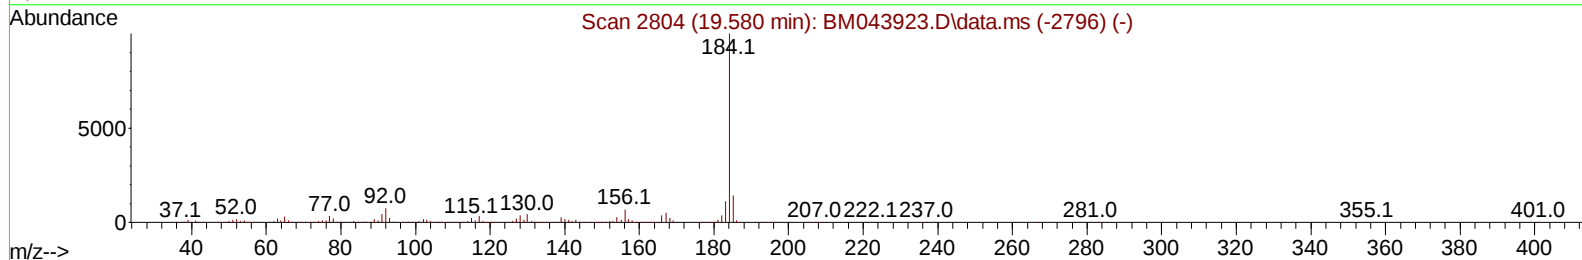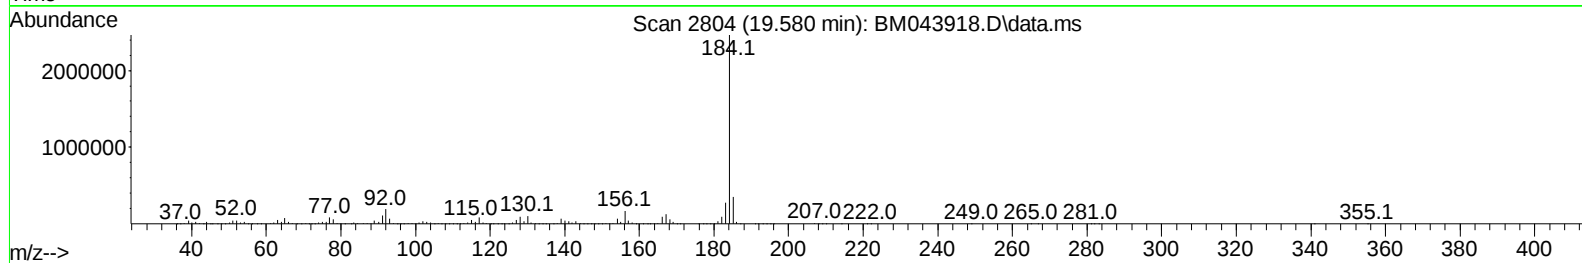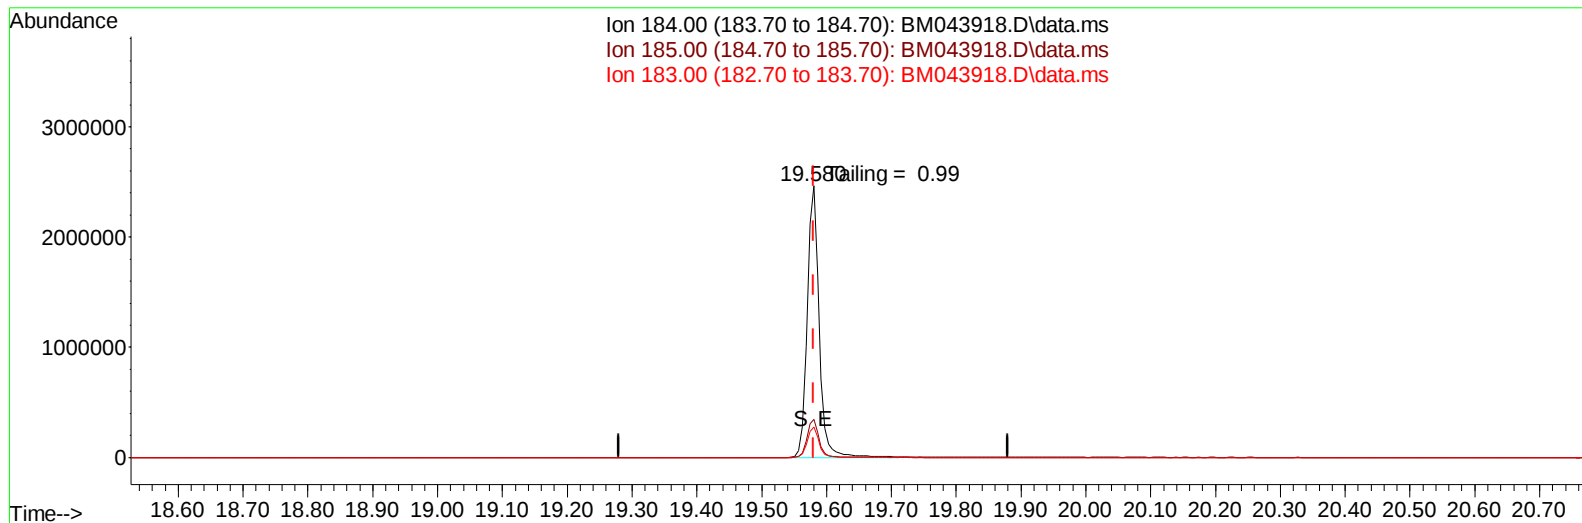

TIC: BM043918.D\data.ms

(77) Benzidine

19.580min (-0.000) 0.00 ng

response 3208557

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.10
183.00	11.30	11.20
0.00	0.00	0.00