
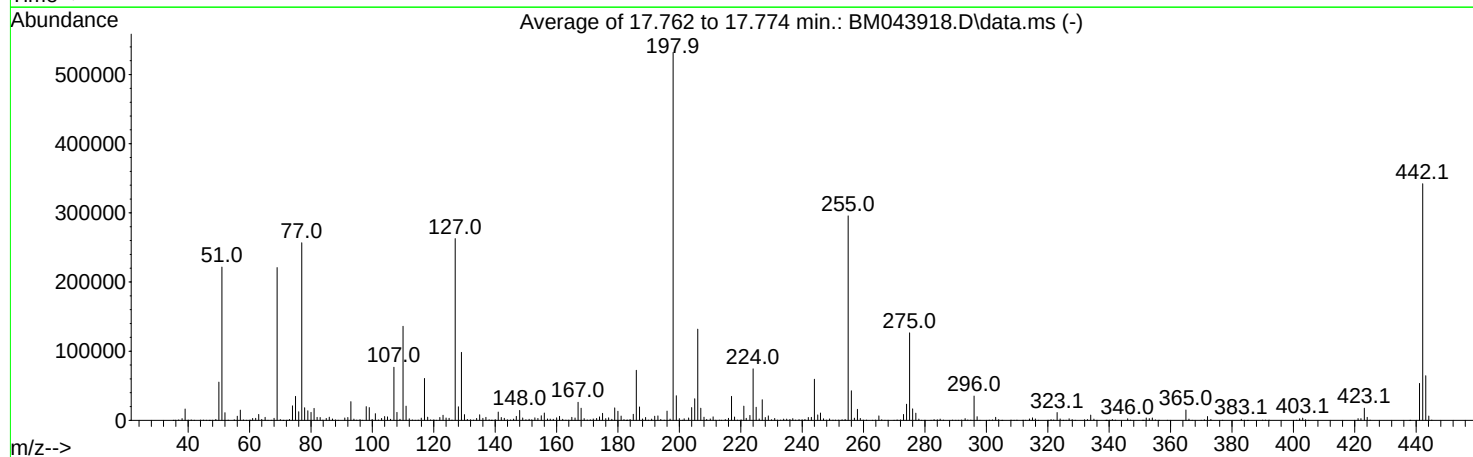


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM013024\  
Data File : BM043918.D  
Acq On : 30 Jan 2024 09:53  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM013024.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Jan 31 00:42:42 2024

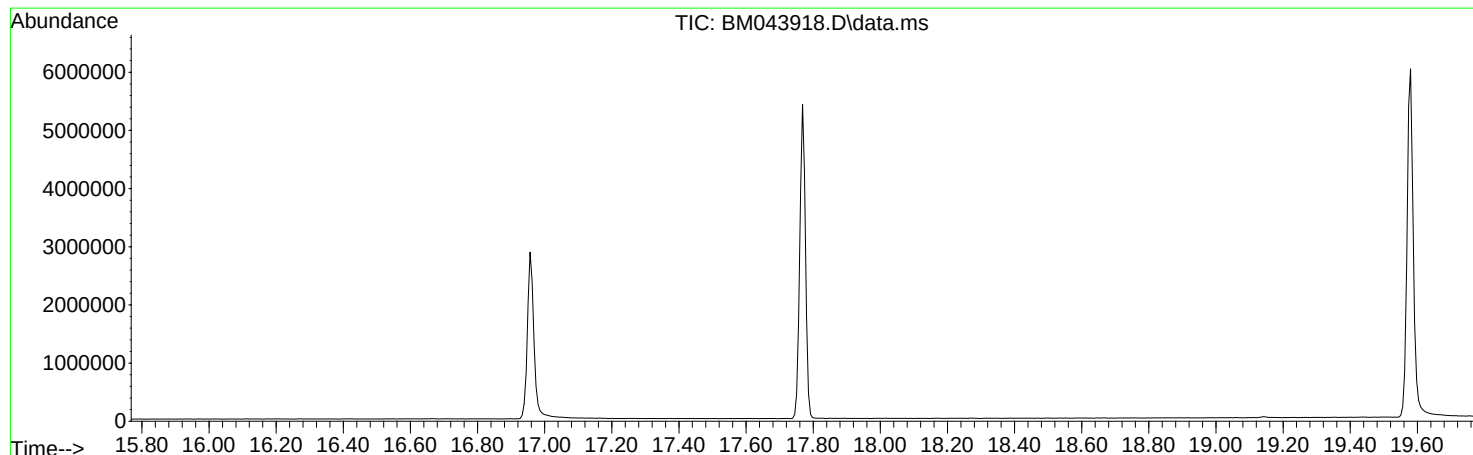




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.7         | 221539     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.4          | 3038       | PASS                |
| 69             | 198             | 0.00            | 100             | 41.5         | 220843     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 1161       | PASS                |
| 127            | 198             | 10              | 80              | 49.4         | 262891     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 1795       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 531840     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 35736      | PASS                |
| 275            | 198             | 10              | 60              | 23.8         | 126608     | PASS                |
| 365            | 198             | 1               | 100             | 2.8          | 15130      | PASS                |
| 441            | 198             | 0.01            | 100             | 10.1         | 53549      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 342101     | PASS                |
| 443            | 442             | 15              | 24              | 18.8         | 64469      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM013024\  
Data File : BM043918.D  
Acq On : 30 Jan 2024 09:53  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Jan 31 00:49:59 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM013024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 31 00:42:42 2024  
Response via : Initial Calibration

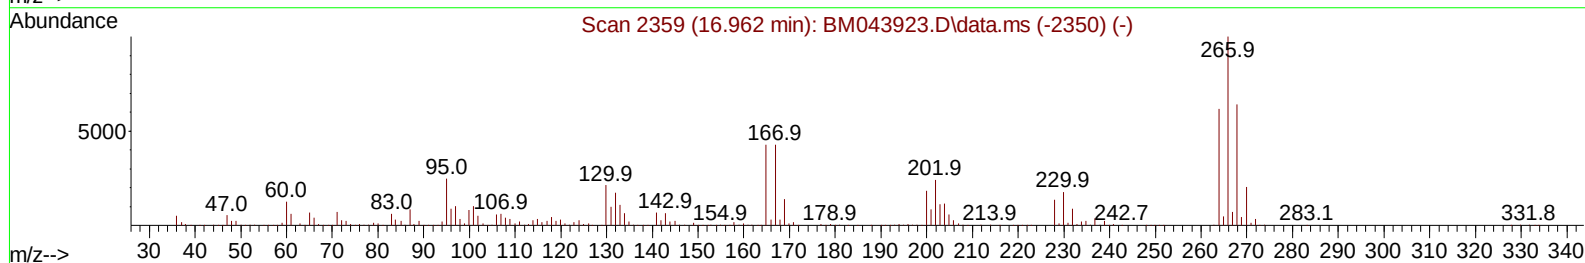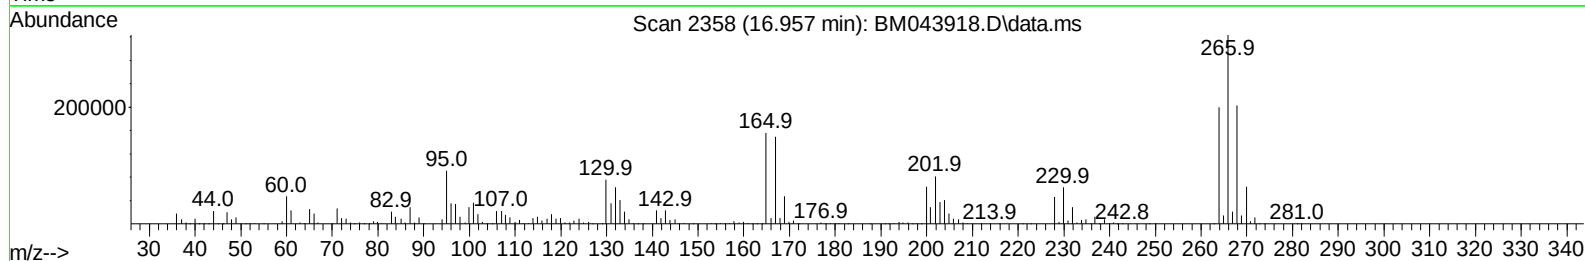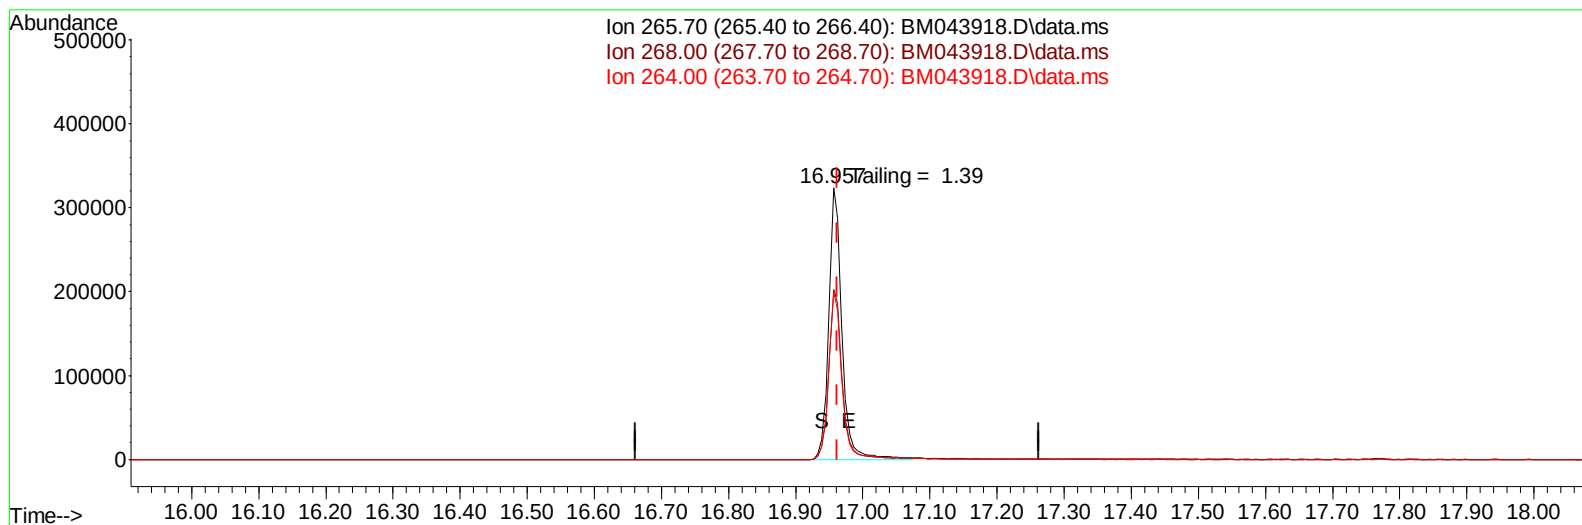

TIC: BM043918.D\data.ms

**(70) Pentachlorophenol (C)**

**16.957min (-0.005) 0.00 ng**




**response 448423**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.00  | 62.71  |
| 264.00 | 61.70  | 61.62  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM013024\  
Data File : BM043918.D  
Acq On : 30 Jan 2024 09:53  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Jan 31 00:49:59 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM013024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 31 00:42:42 2024  
Response via : Initial Calibration

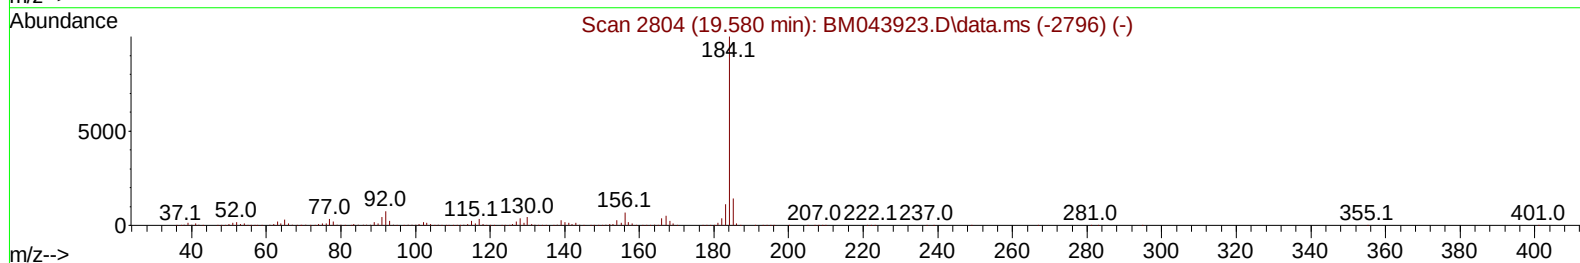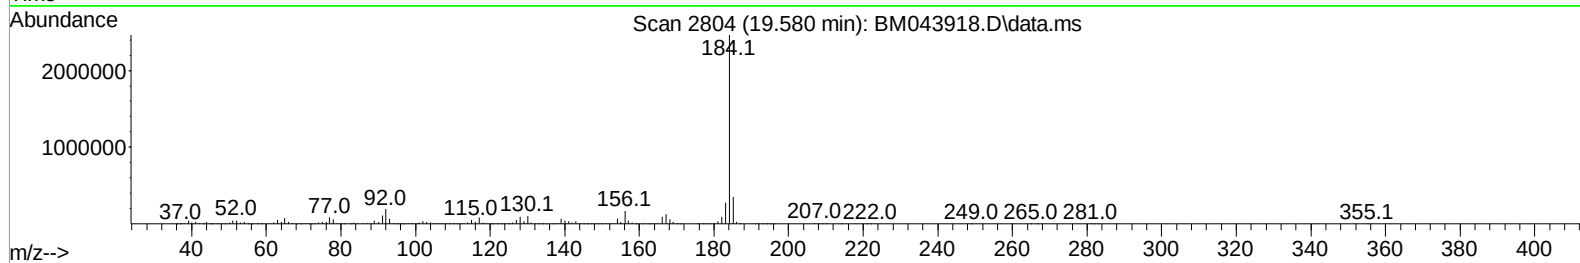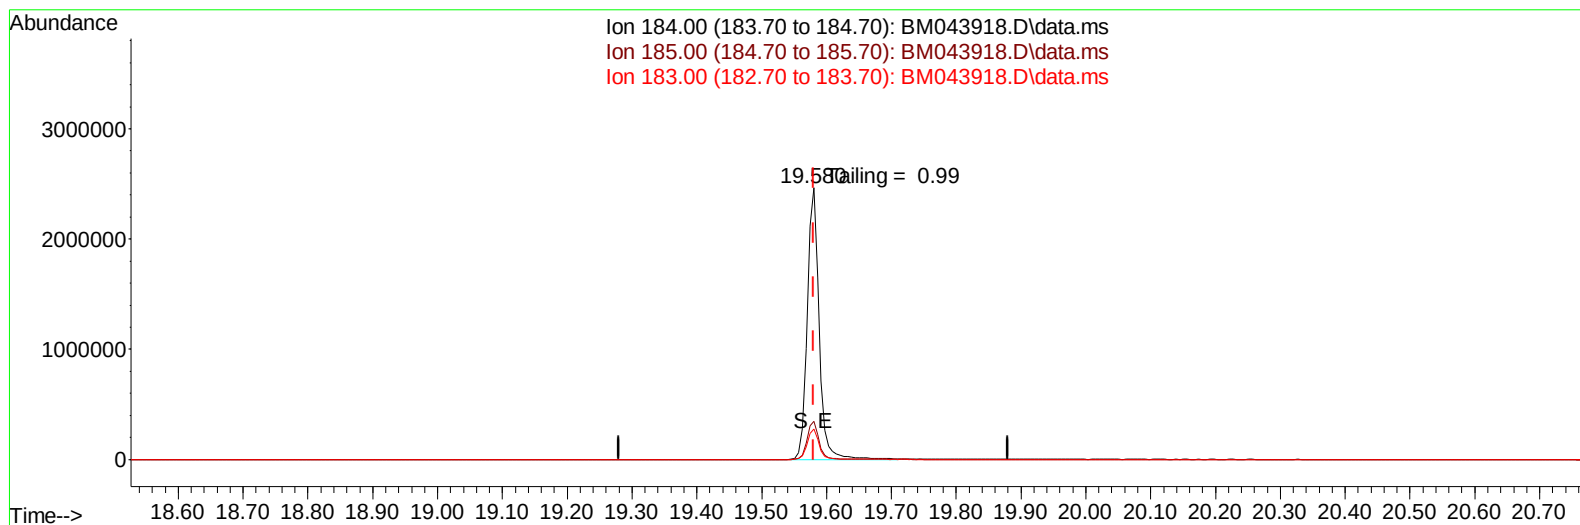

TIC: BM043918.D\data.ms

(77) Benzidine

19.580min (-0.000) 0.00 ng

response 3208557

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.10  |
| 183.00 | 11.30  | 11.20  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/30/2024     | BNA_M            | <u>BM043918.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1203761          | 20.815             |
| DDD           | 12176            | 20.427             |
| DDE           | 871              | 19.862             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 13047         | 1216808          | 1.07               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP