




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049553.D
Acq On : 31 Jan 2025 11:20
Operator : RC/JU
Sample : Q1184-14DL 100X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2965DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

Quant Time: Feb 03 07:46:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

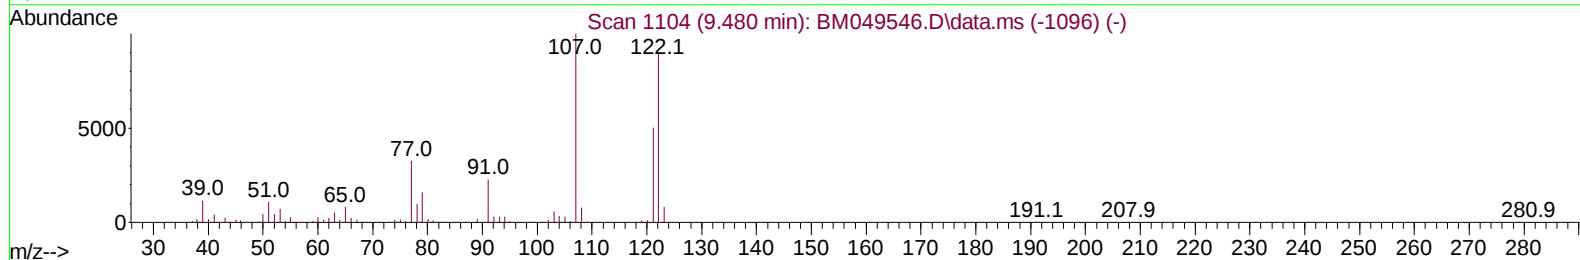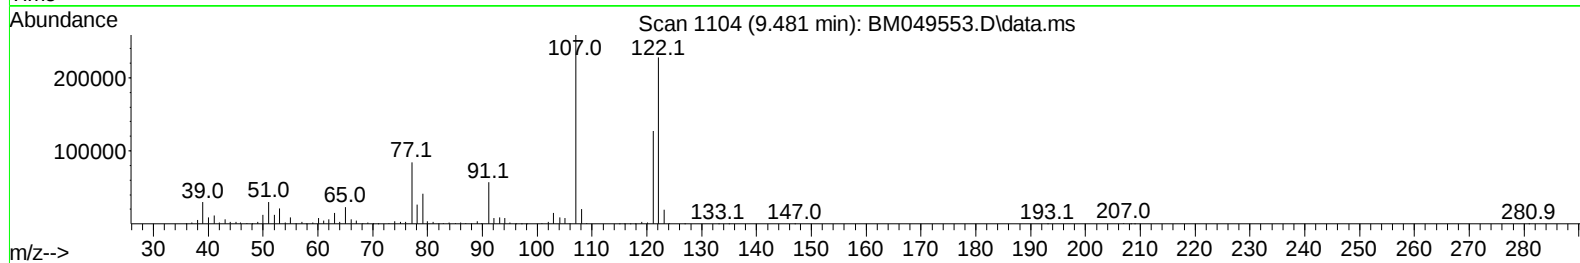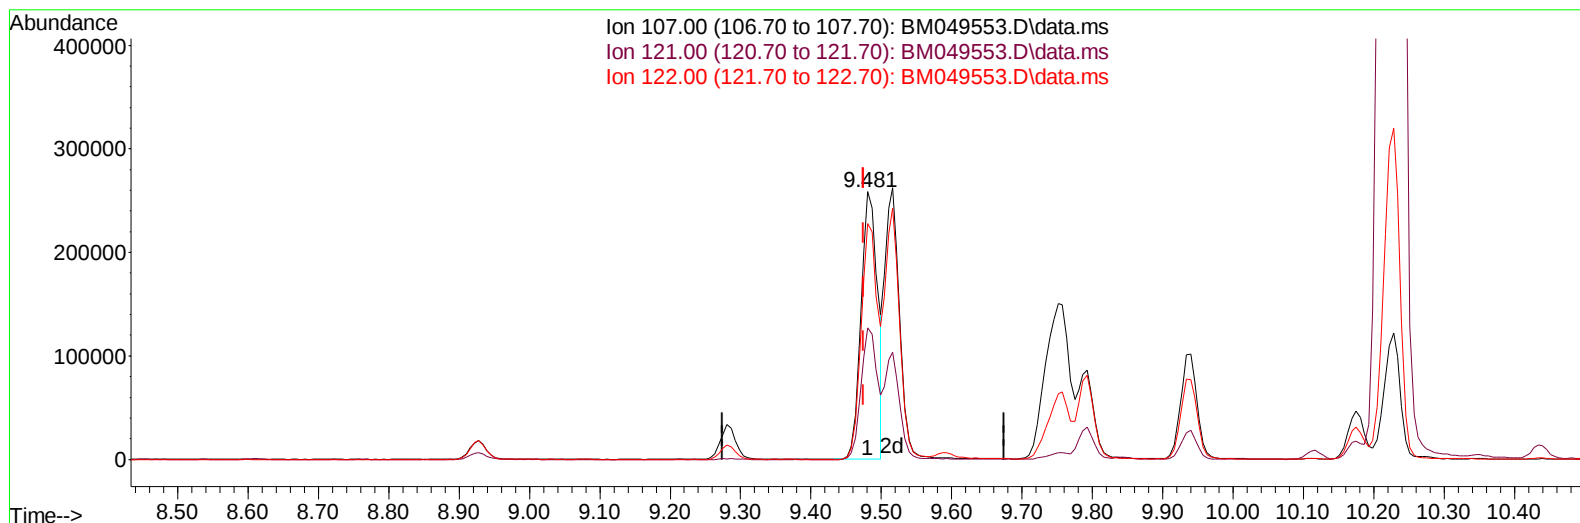

TIC: BM049553.D\data.ms

(26) 2,4-Dimethylphenol

9.481min (+ 0.006) 31.19 ng/ul

response 420011

Ion	Exp%	Act%
107.00	100.00	100.00
121.00	49.50	49.07
122.00	85.90	88.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049553.D
Acq On : 31 Jan 2025 11:20
Operator : RC/JU
Sample : Q1184-14DL 100X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2965DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 07:46:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

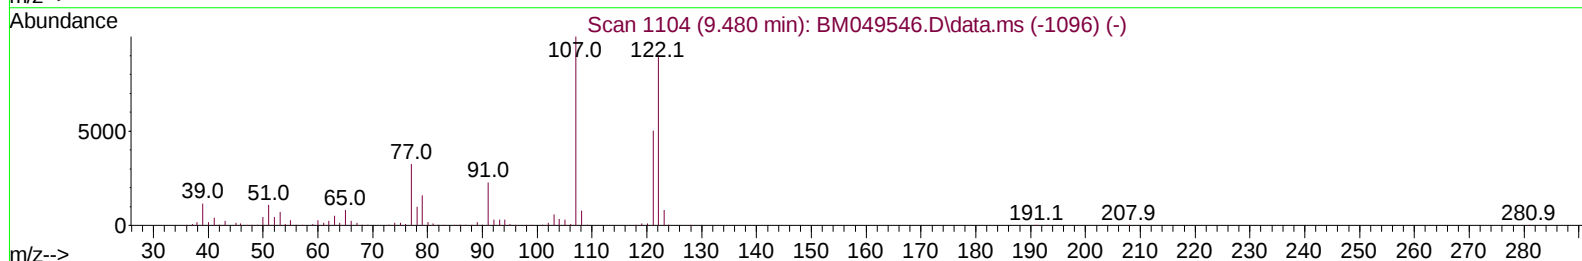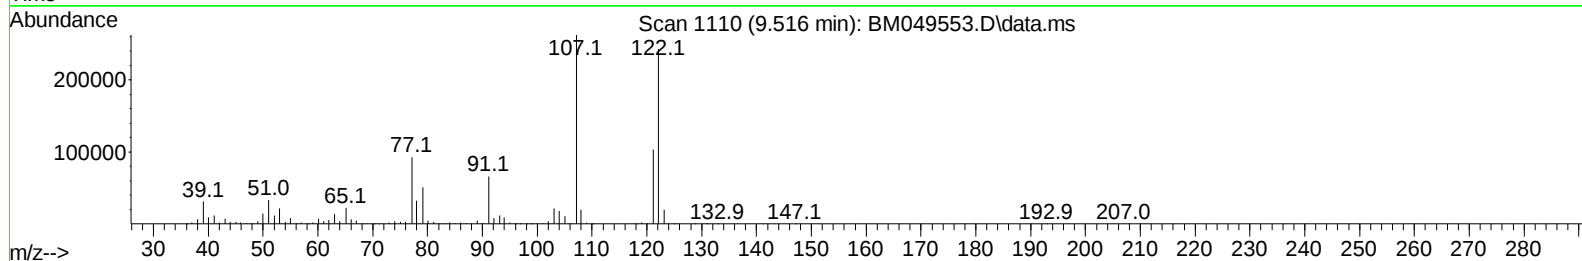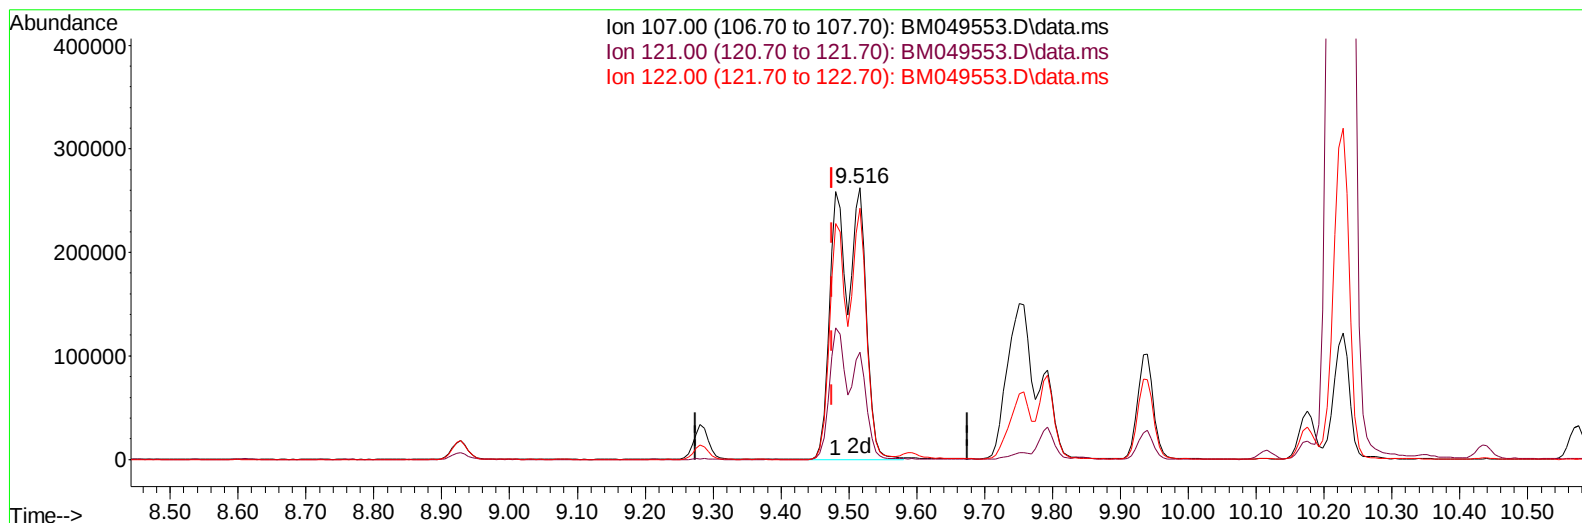

TIC: BM049553.D\data.ms

(26) 2,4-Dimethylphenol

9.516min (+ 0.041) 59.84 ng/ul m

response 805775

Ion	Exp%	Act%
107.00	100.00	100.00
121.00	49.50	39.39#
122.00	85.90	92.44
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049553.D
Acq On : 31 Jan 2025 11:20
Operator : RC/JU
Sample : Q1184-14DL 100X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2965DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 07:46:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

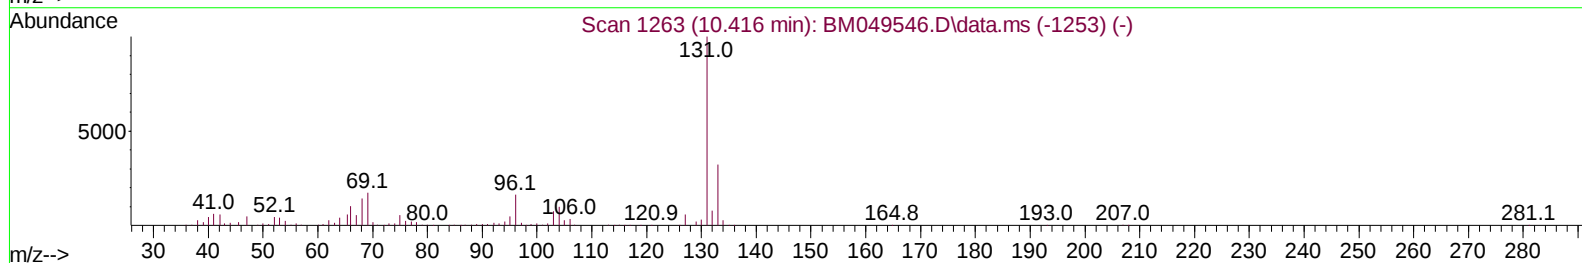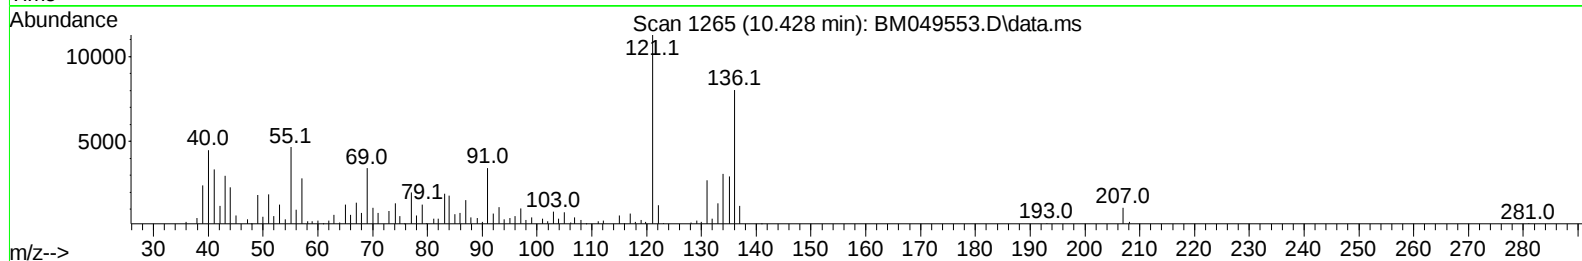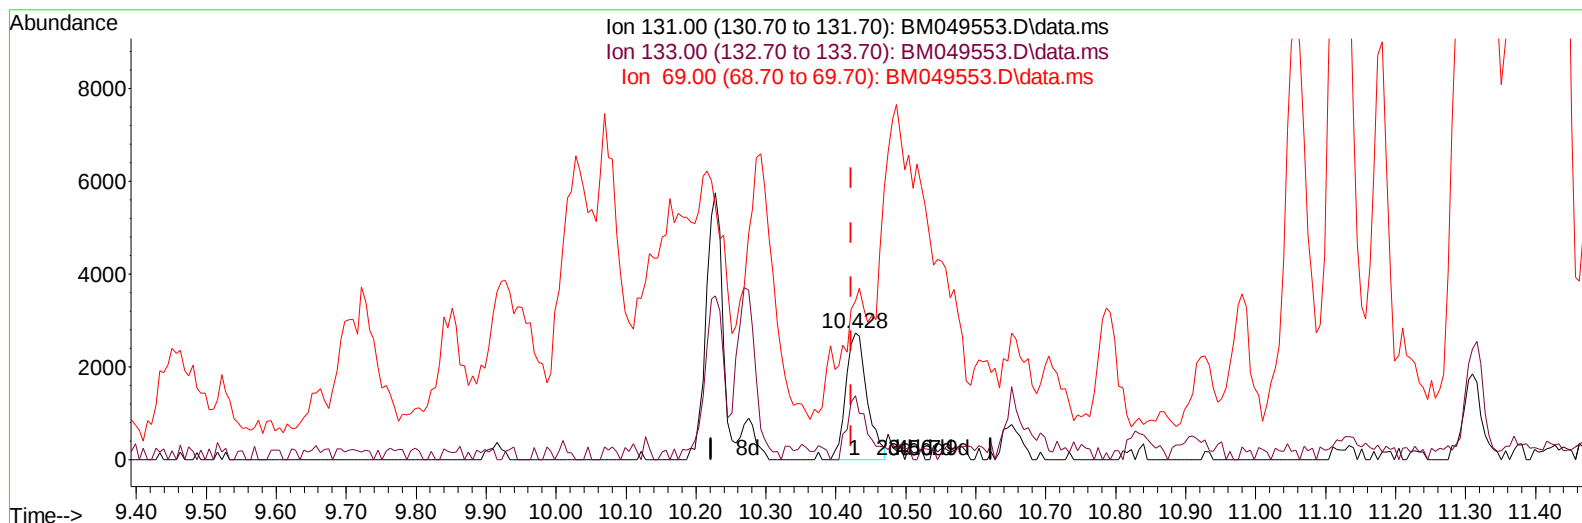

TIC: BM049553.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.428min (+ 0.006) 0.33 ng/u1

response 5716

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.80	50.31#
69.00	18.50	125.27#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049553.D
Acq On : 31 Jan 2025 11:20
Operator : RC/JU
Sample : Q1184-14DL 100X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2965DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 07:46:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

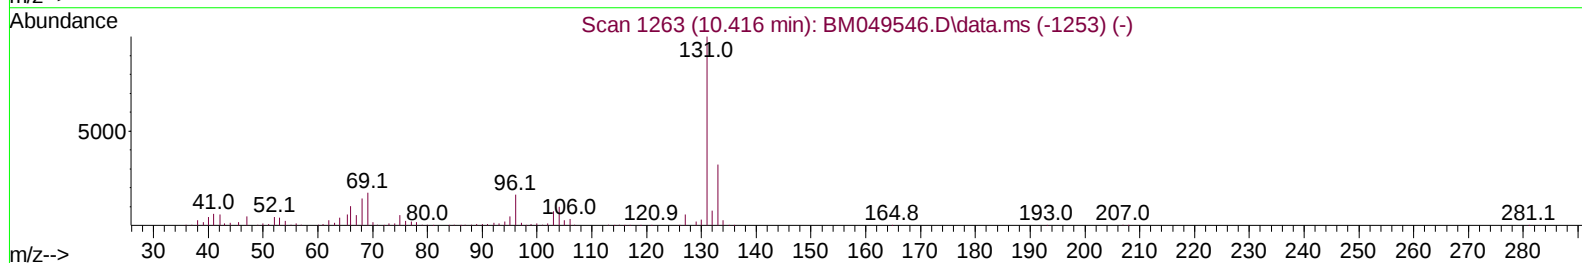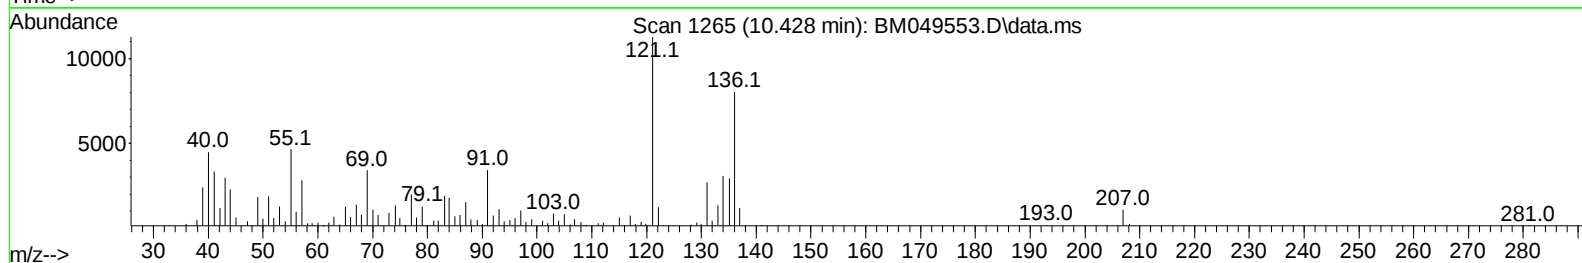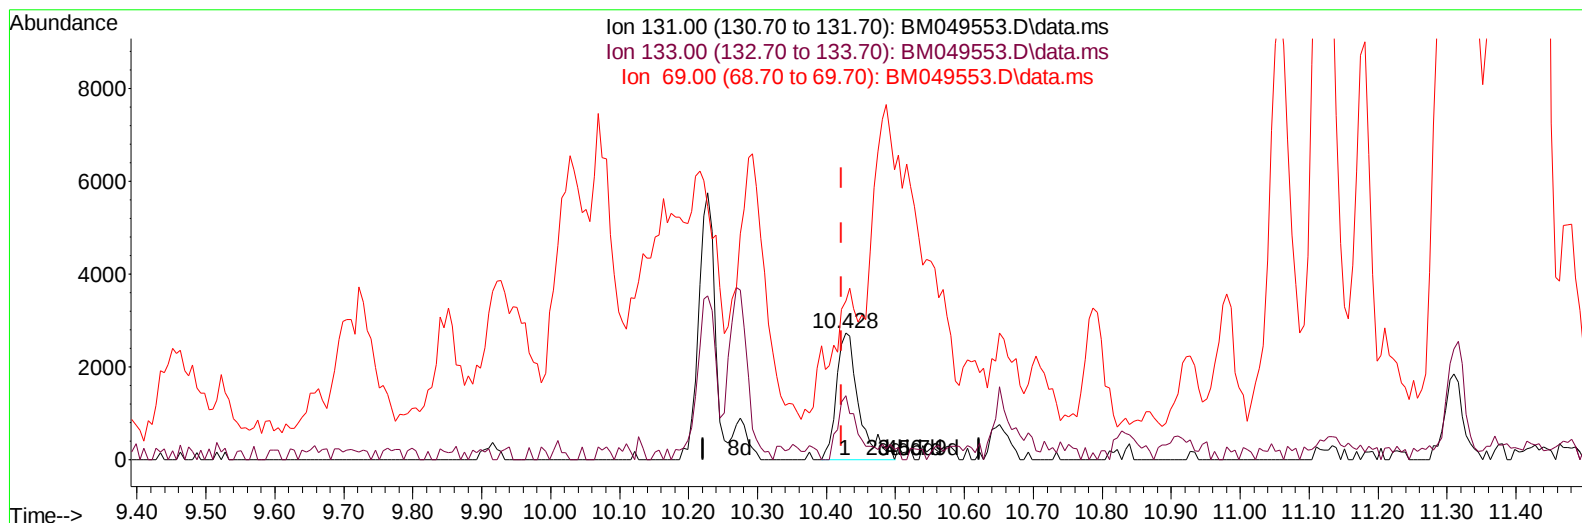

TIC: BM049553.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.428min (+ 0.006) 0.36 ng/ul m

response 6165

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.80	50.31#
69.00	18.50	125.27#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049553.D
Acq On : 31 Jan 2025 11:20
Operator : RC/JU
Sample : Q1184-14DL 100X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2965DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 07:46:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

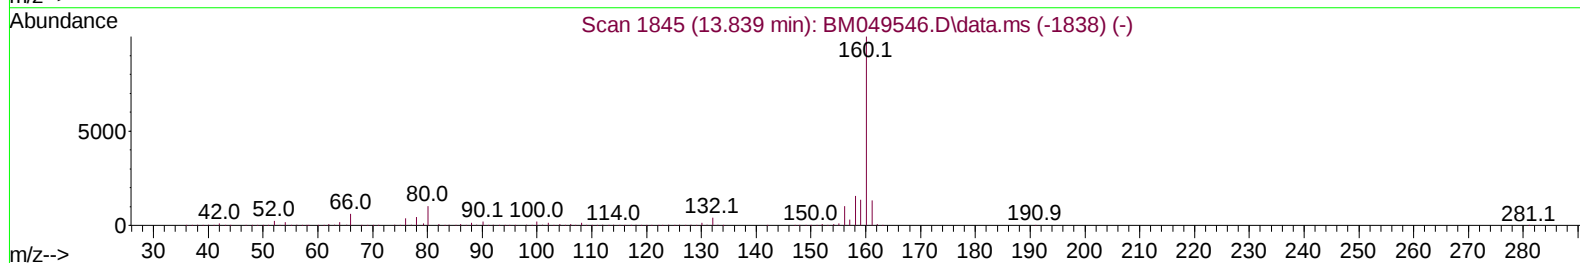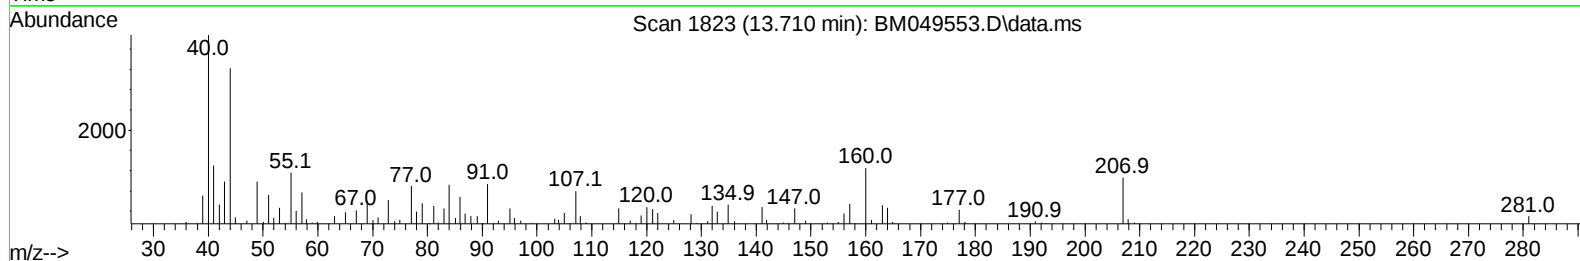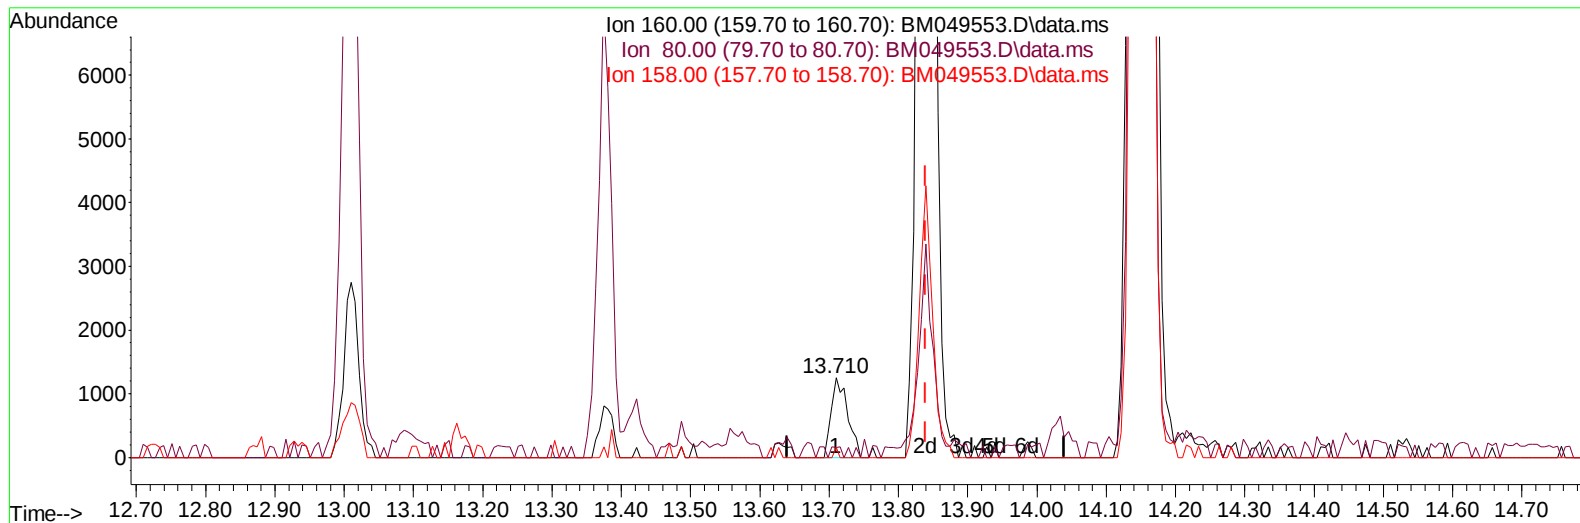

TIC: BM049553.D\data.ms

(49) Acenaphthylene-d8 (S)

13.710min (-0.129) 0.04 ng/u1

response 2062

Ion	Exp%	Act%
160.00	100.00	100.00
80.00	10.40	12.45
158.00	15.20	12.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
 Data File : BM049553.D
 Acq On : 31 Jan 2025 11:20
 Operator : RC/JU
 Sample : Q1184-14DL 100X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2965DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2025
 Supervised By :mohammad ahmed 02/04/2025

Quant Time: Feb 03 07:49:44 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 28 14:45:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	215985	20.000	ng/ul	0.00
20) Naphthalene-d8	10.269	136	789756	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.151	164	576739	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.904	188	1169977	20.000	ng/ul	0.00
79) Chrysene-d12	21.139	240	1106395	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	1211247	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.111	96	590	0.101	ng/uL	-0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.728	99	4383	0.250	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.863	67	7889	0.658	ng/ul	0.00
11) 2-Chlorophenol-d4	7.057	132	9041	0.667	ng/ul	0.00
15) 4-Methylphenol-d8	8.240	113	6470	0.504	ng/ul	0.01
21) Nitrobenzene-d5	8.657	128	4488	0.743	ng/ul	0.00
24) 2-Nitrophenol-d4	9.375	143	5017	0.761	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.922	165	11307	0.841	ng/ul	0.02
31) 4-Chloroaniline-d4	10.428	131	6165m	0.357	ng/ul	0.00
46) Dimethylphthalate-d6	13.575	166	27108	0.641	ng/ul	0.00
49) Acenaphthylene-d8	13.839	160	35552m	0.716	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.151	176	29268	0.787	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.298	200	1316	0.178	ng/ul	0.02
73) Anthracene-d10	17.004	188	50610	0.866	ng/ul	0.00
81) Pyrene-d10	19.310	212	53275	0.824	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264	50329	0.779	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.757	94	443631	24.115	ng/ul	97
18) 4-Methylphenol	8.304	108	136627	9.819	ng/ul	90
26) 2,4-Dimethylphenol	9.516	107	805775m	59.838	ng/ul	
30) Naphthalene	10.316	128	152562	3.628	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049553.D
Acq On : 31 Jan 2025 11:20
Operator : RC/JU
Sample : Q1184-14DL 100X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2965DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 07:49:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

