




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
 Data File : BM049557.D
 Acq On : 31 Jan 2025 14:38
 Operator : RC/JU
 Sample : Q1190-02 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 28 14:45:18 2025
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
 Supervised By :mohammad ahmed 02/04/2025

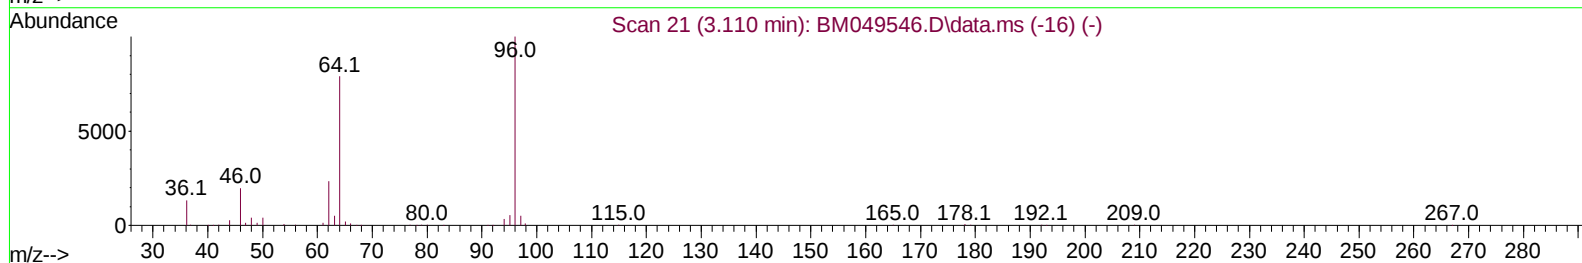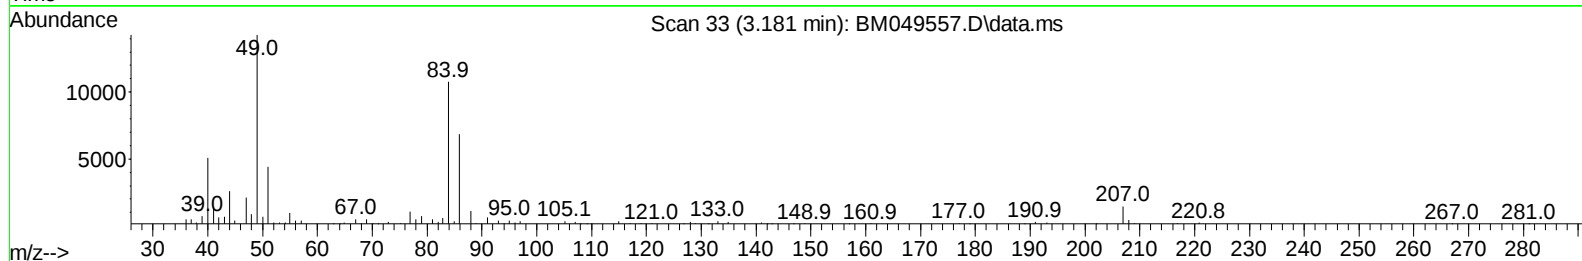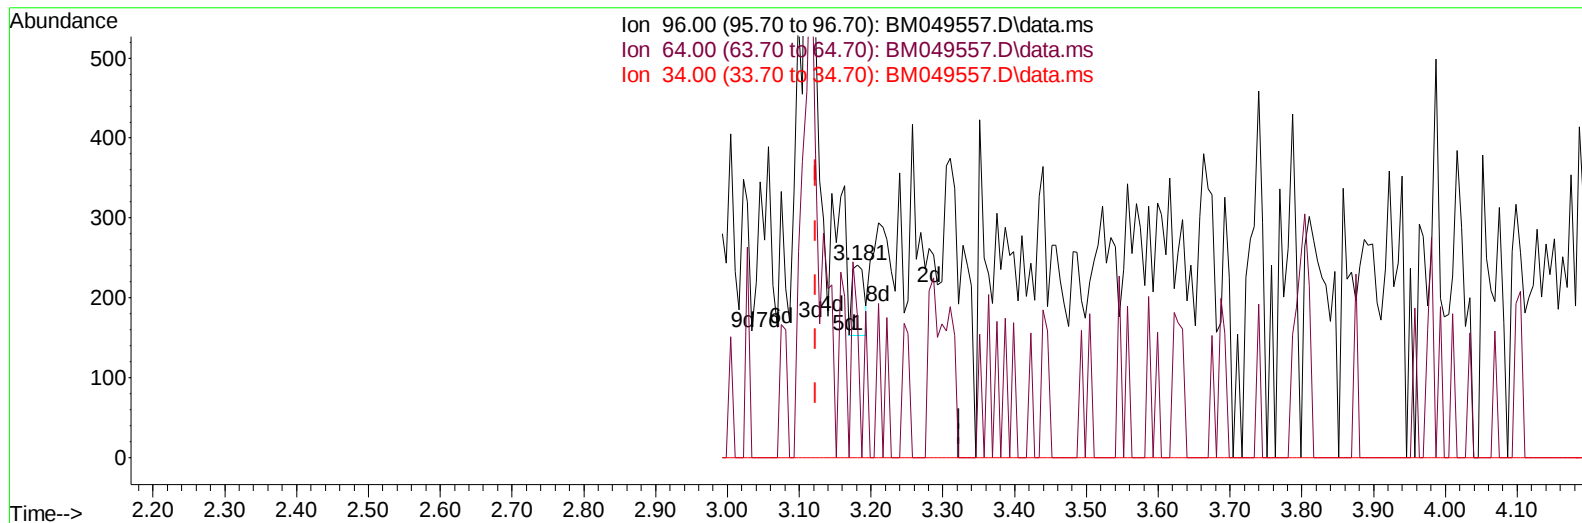

TIC: BM049557.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (+ 0.059) 0.02 ng/uL

response 102

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	82.20	73.44
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

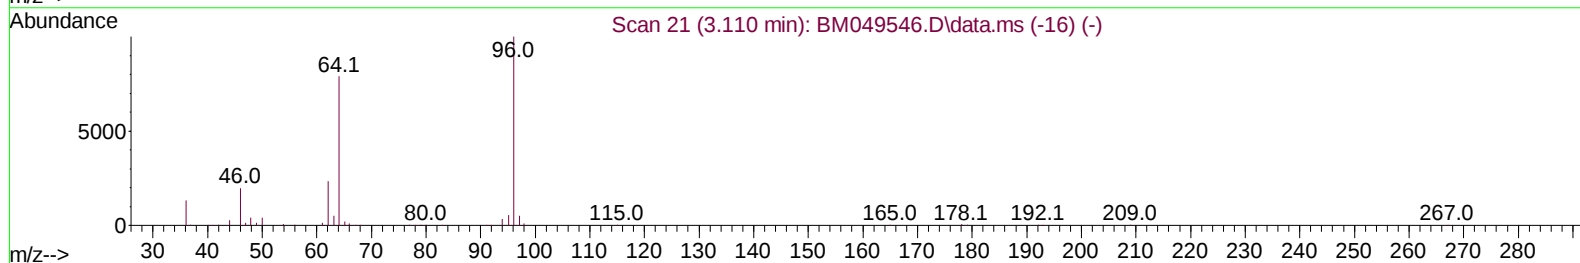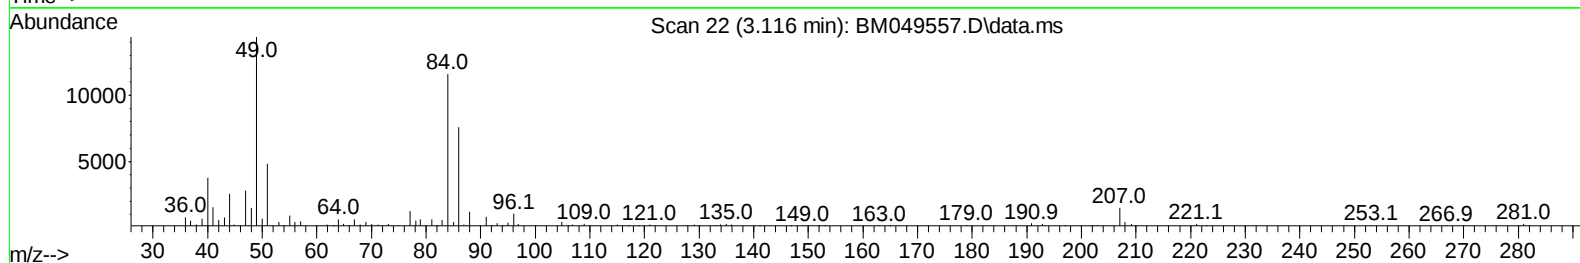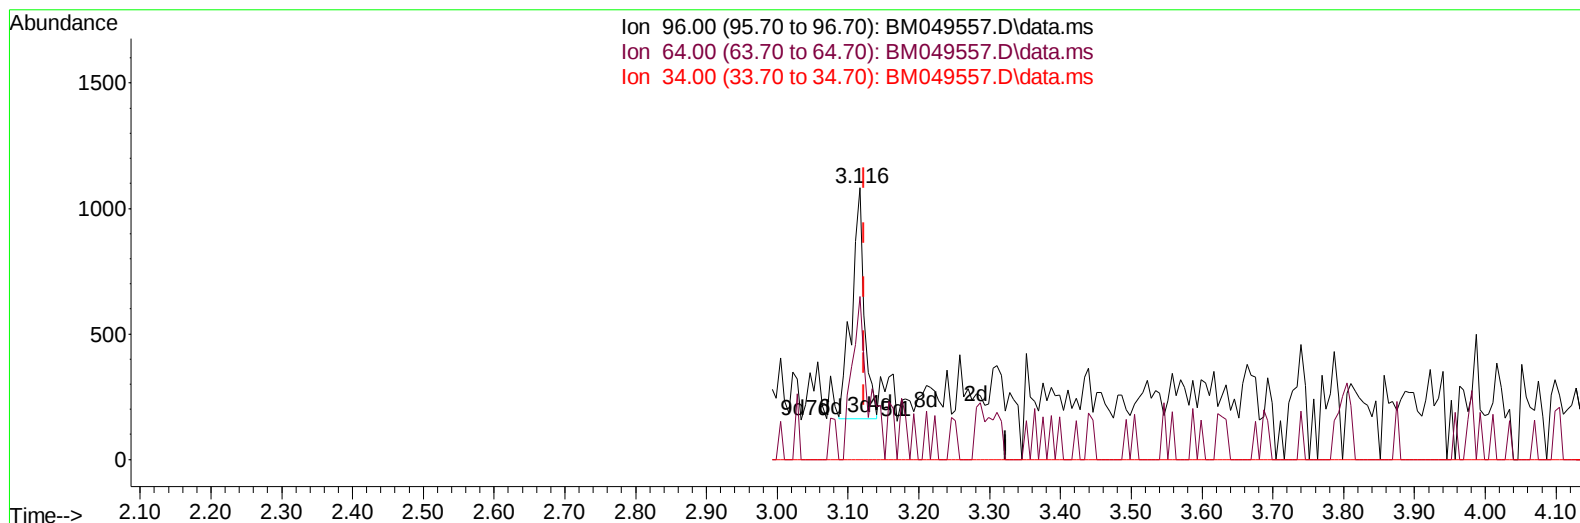

TIC: BM049557.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.116min (-0.006) 0.19 ng/uL m

response 1136

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	82.20	59.98#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

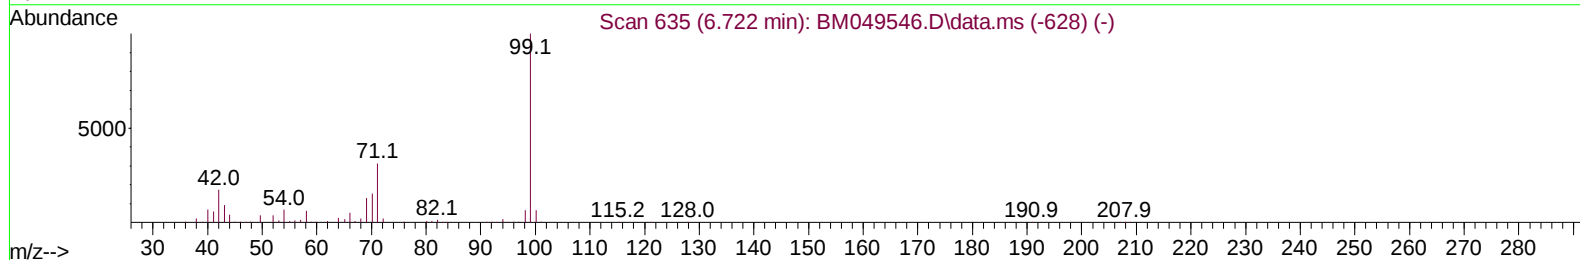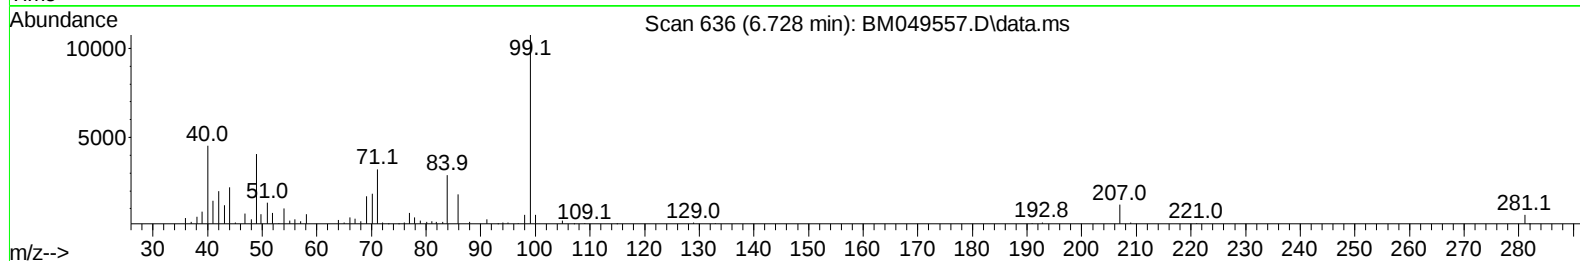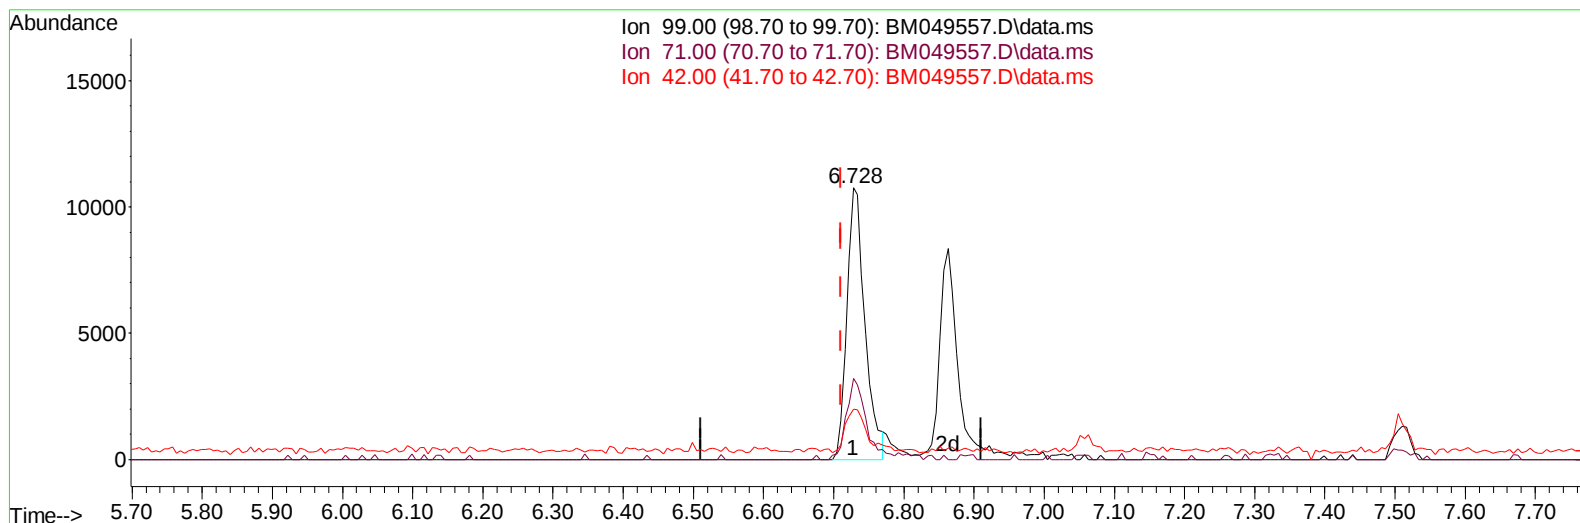

TIC: BM049557.D\data.ms

(7) Phenol-d5 (S)

6.728min (+ 0.018) 1.09 ng/u1

response 19318

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	33.10	29.84
42.00	19.20	18.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

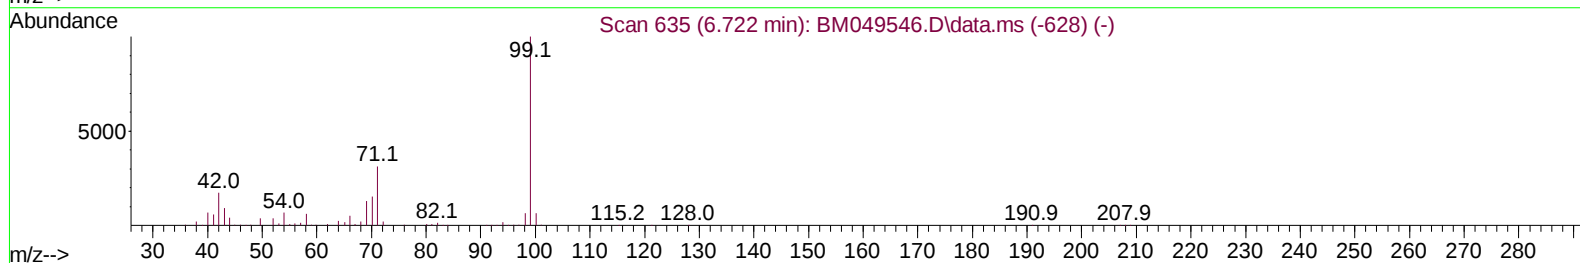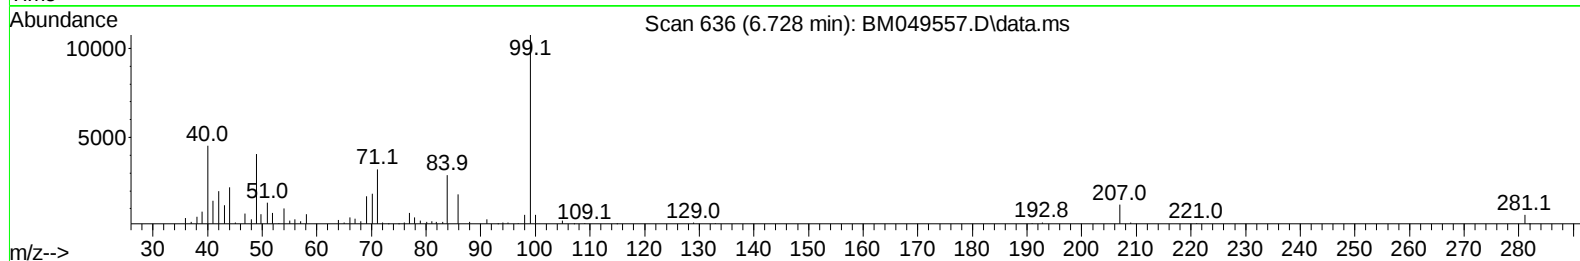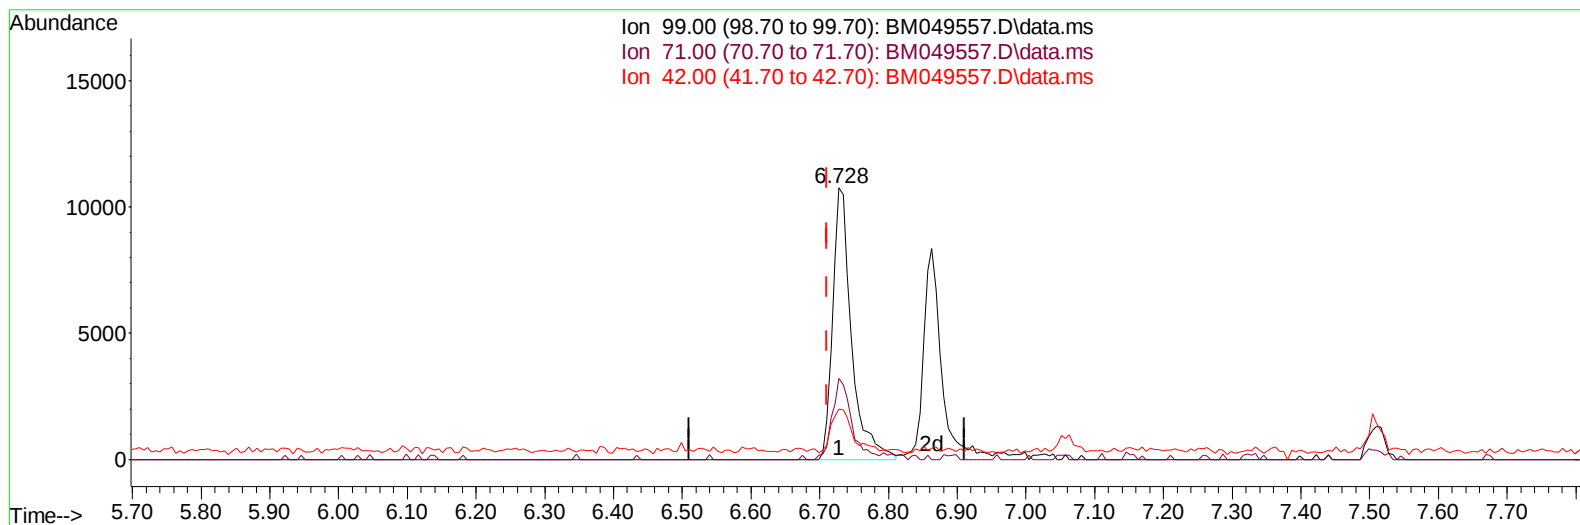

TIC: BM049557.D\data.ms

(7) Phenol-d5 (S)

6.728min (+ 0.018) 1.16 ng/ul m

response 20484

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	33.10	29.84
42.00	19.20	18.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

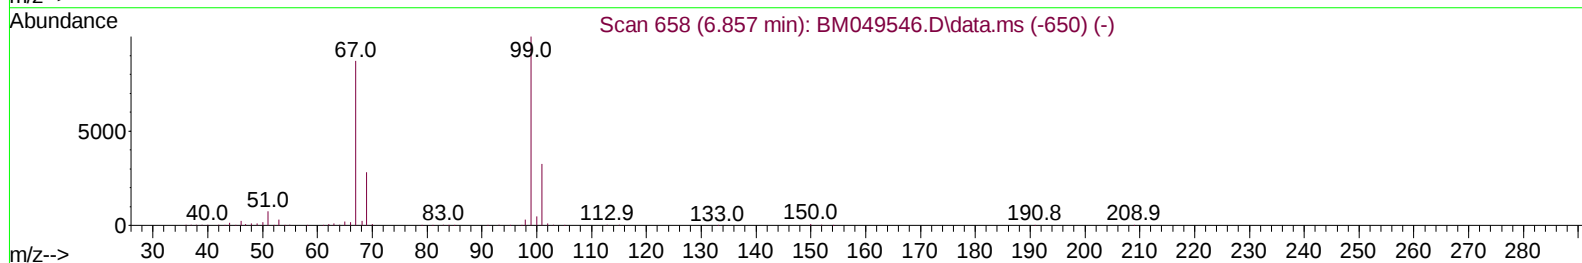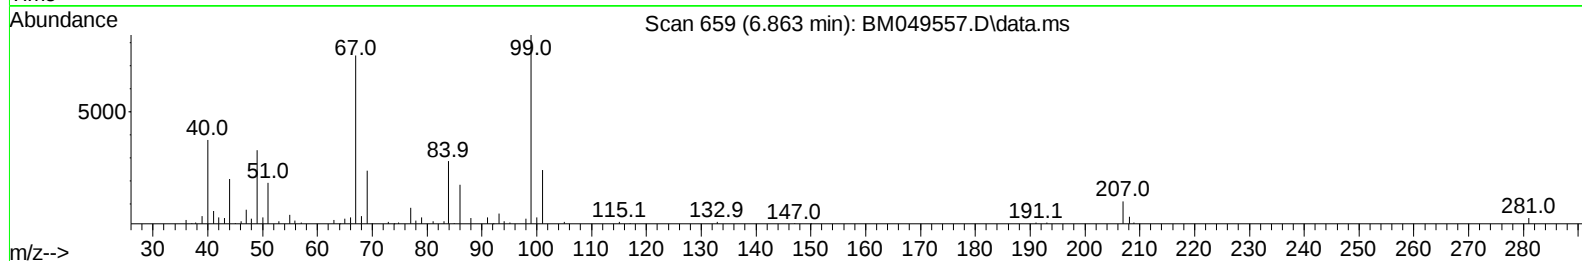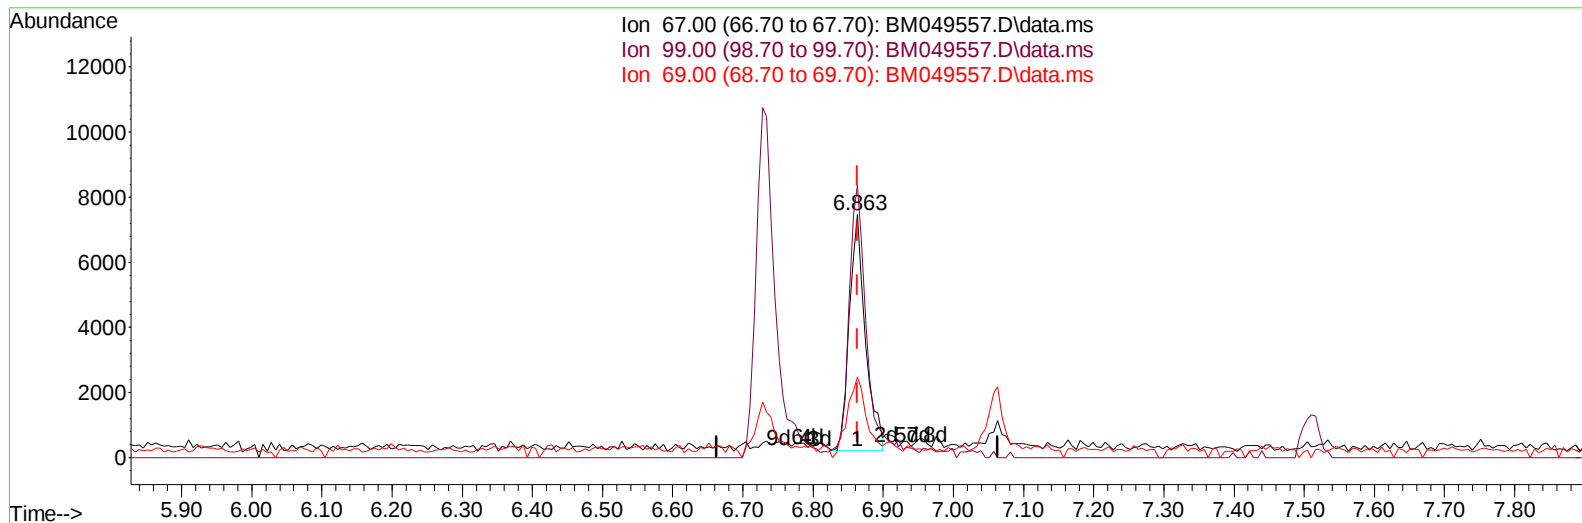

TIC: BM049557.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

6.863min (-0.000) 0.96 ng/u1

response 11636

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	113.00	111.77
69.00	31.70	33.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

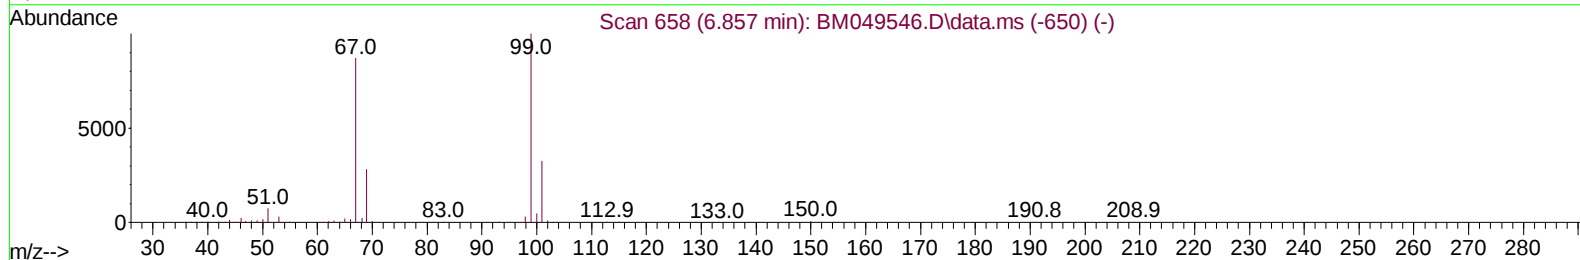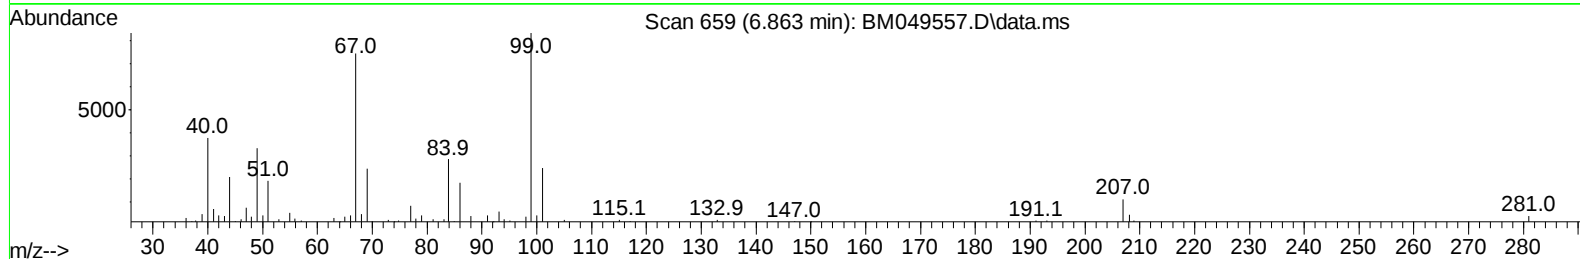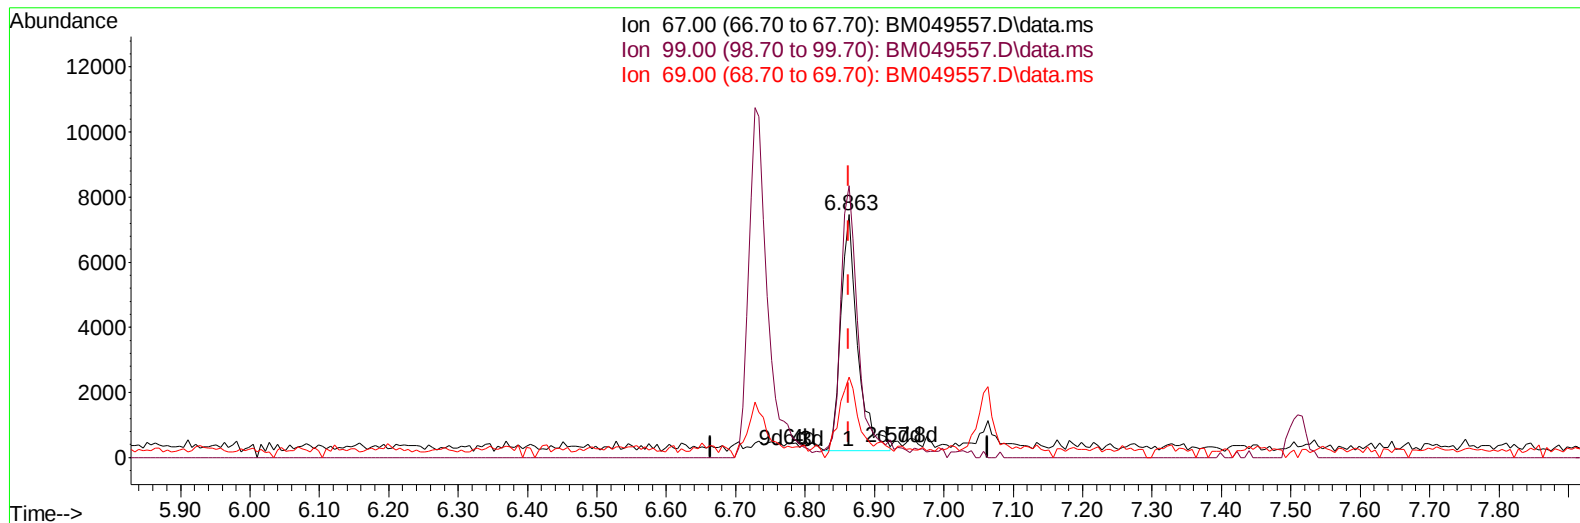

TIC: BM049557.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

6.863min (-0.000) 1.01 ng/ul m

response 12203

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	113.00	111.77
69.00	31.70	33.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

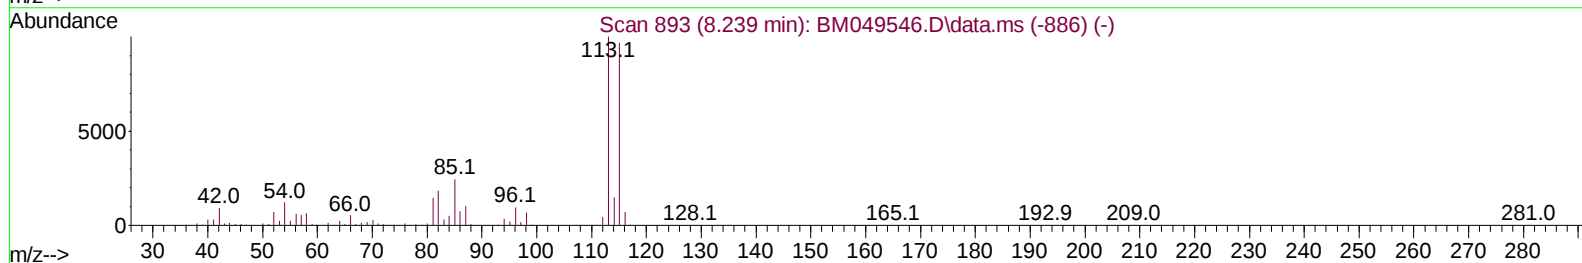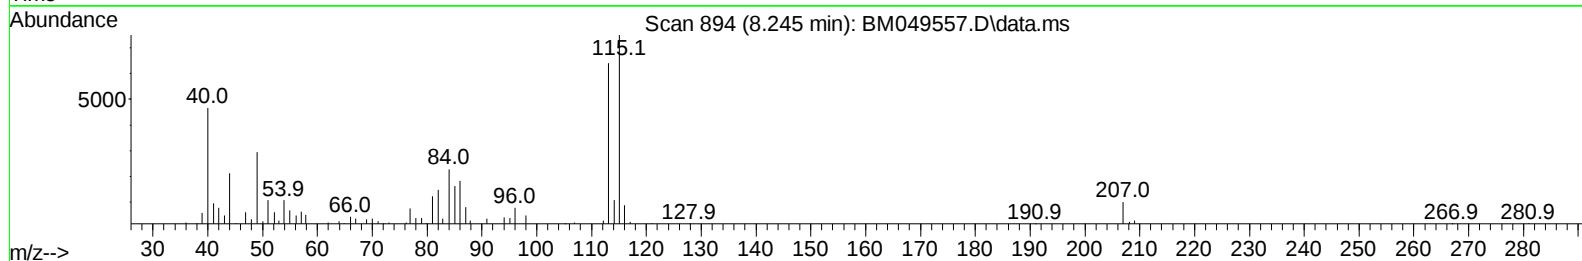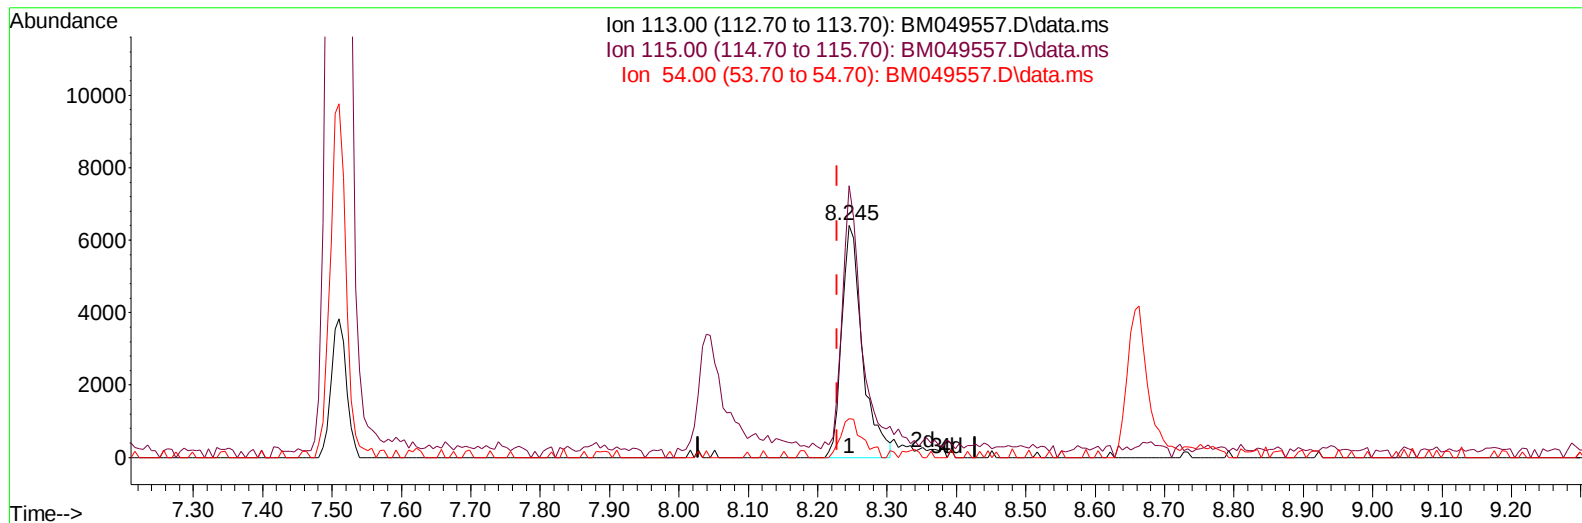

TIC: BM049557.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.245min (+ 0.018) 1.01 ng/u1

response 13133

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	95.60	116.96#
54.00	13.90	16.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

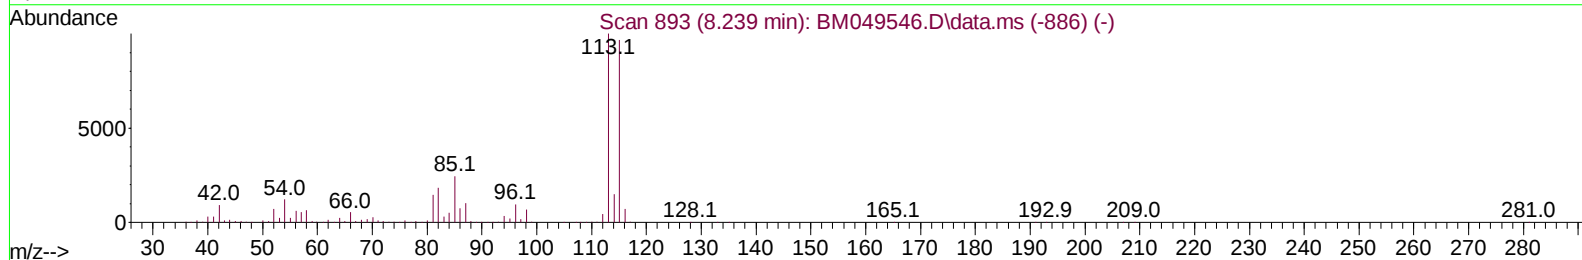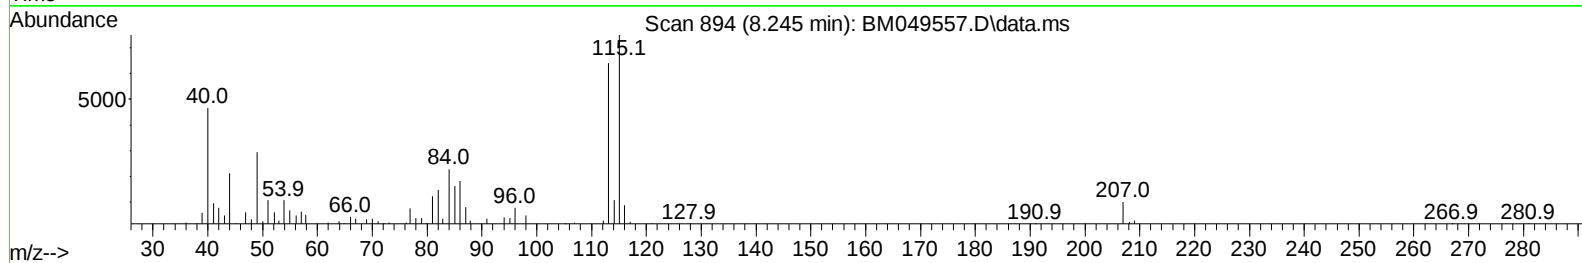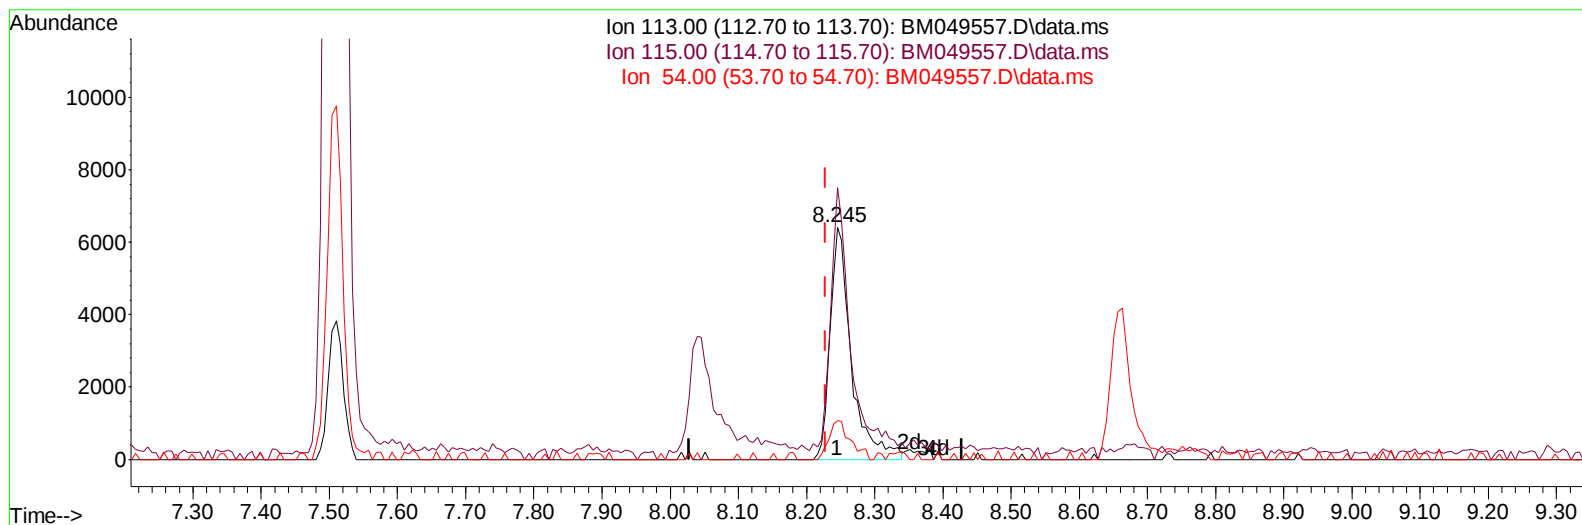

TIC: BM049557.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.245min (+ 0.018) 1.07 ng/ul m

response 13817

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	95.60	116.96#
54.00	13.90	16.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

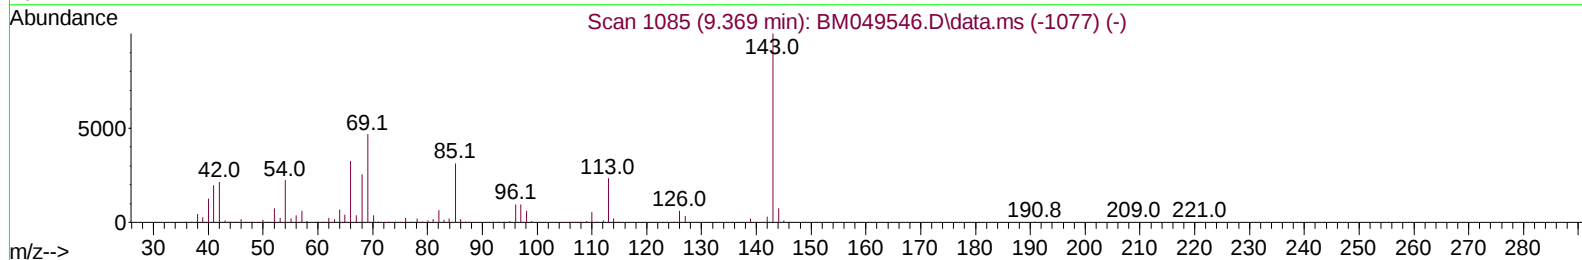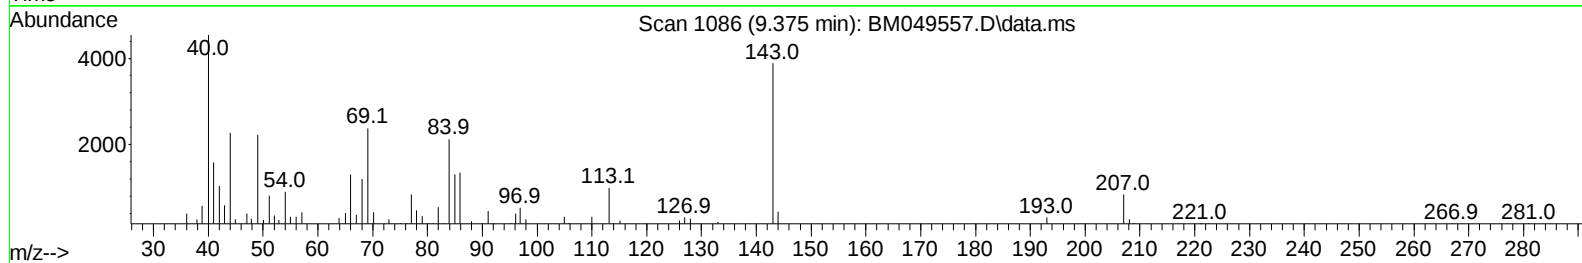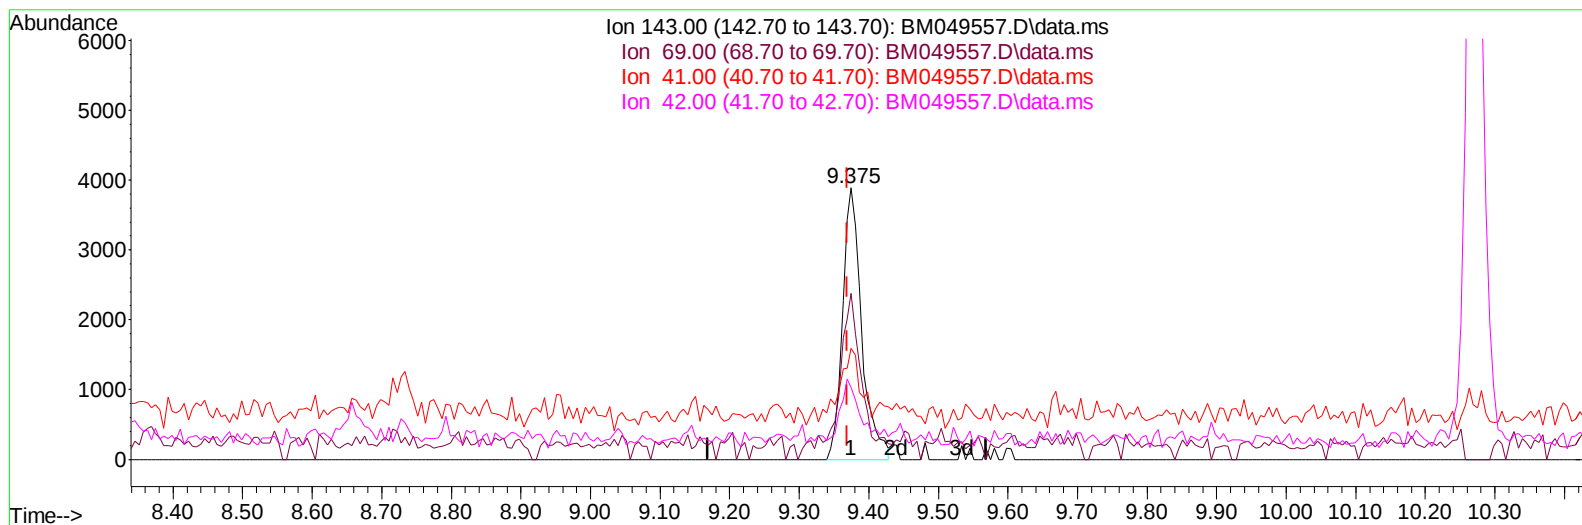

TIC: BM049557.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.375min (+ 0.006) 1.04 ng/u1

response 7403

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	54.90	61.23
41.00	24.60	40.88#
42.00	27.00	26.45




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

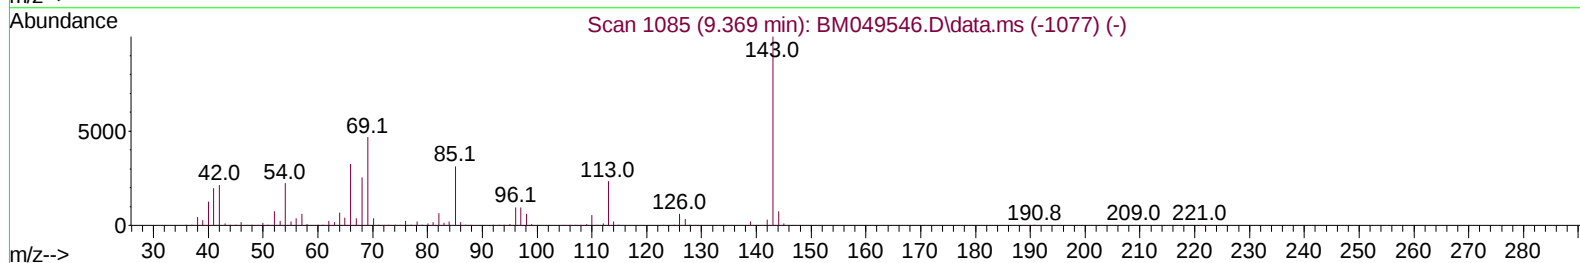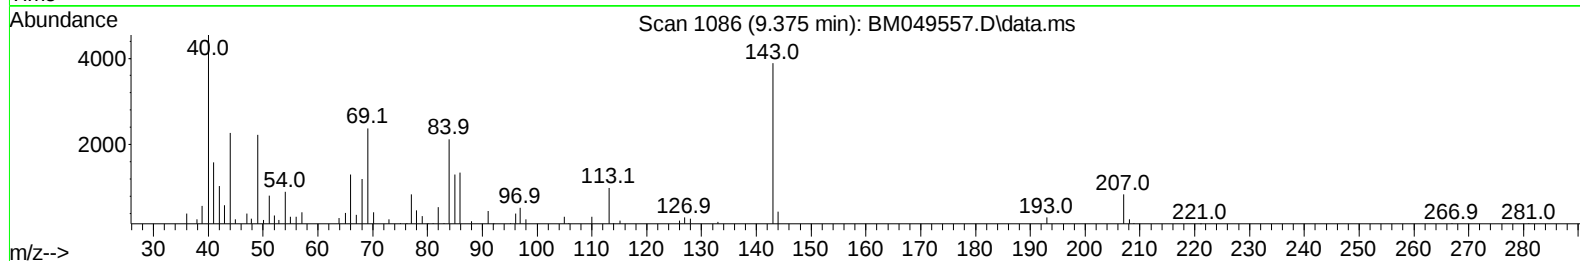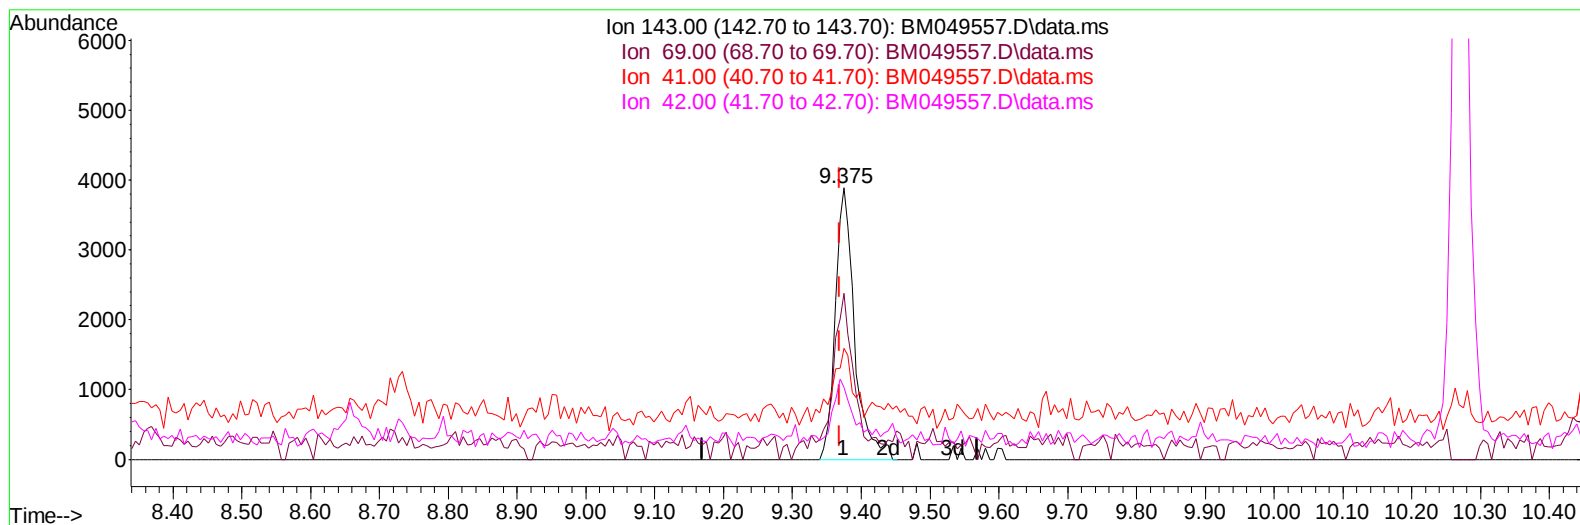

TIC: BM049557.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.375min (+ 0.006) 1.06 ng/ul m

response 7548

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	54.90	61.23
41.00	24.60	40.88#
42.00	27.00	26.45




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

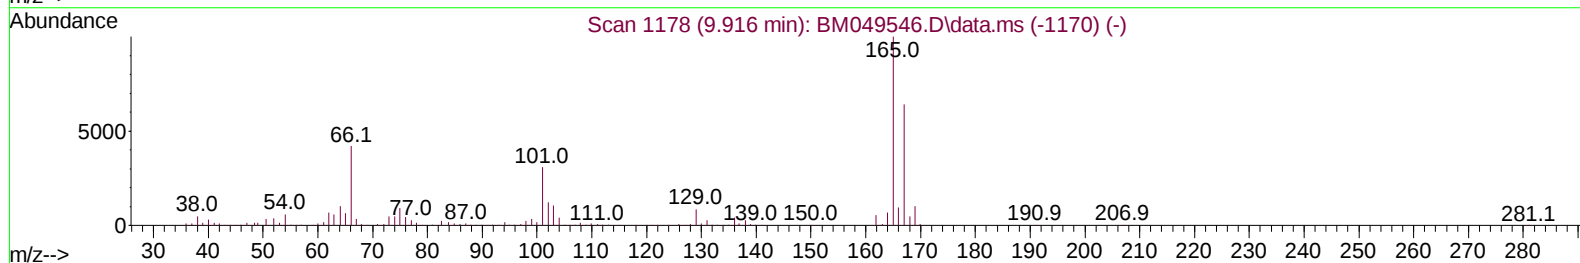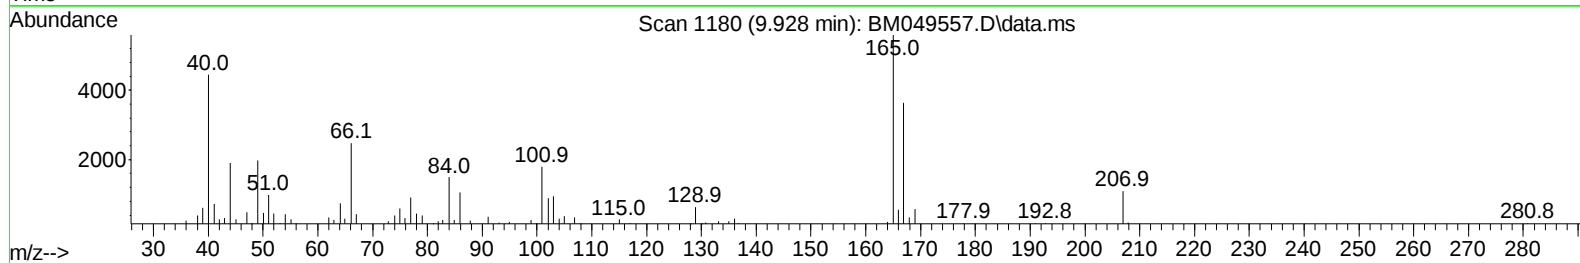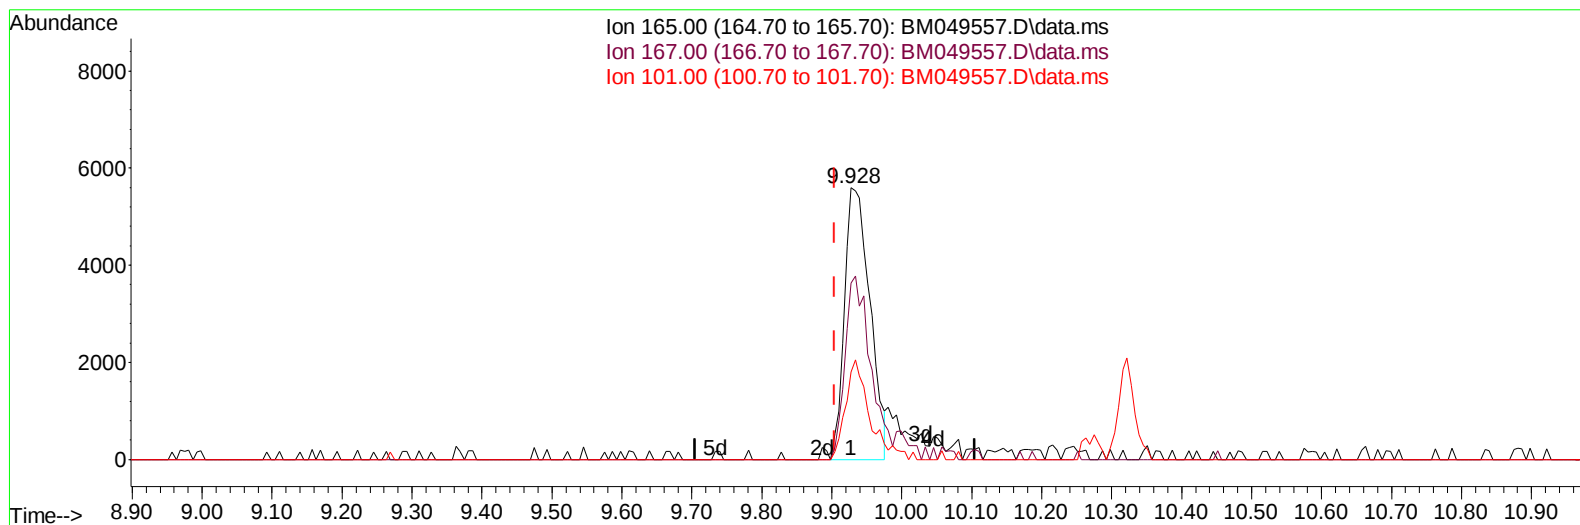

TIC: BM049557.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

9.928min (+ 0.023) 0.97 ng/u1

response 14075

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.20	65.07
101.00	31.40	32.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

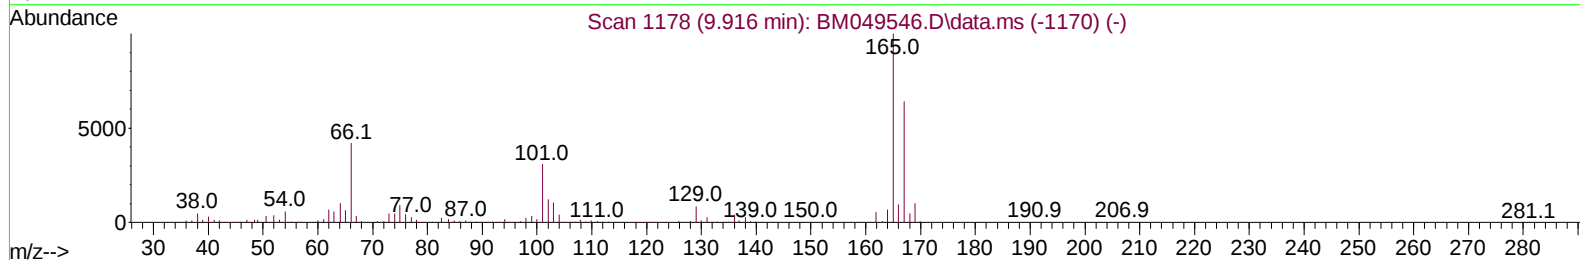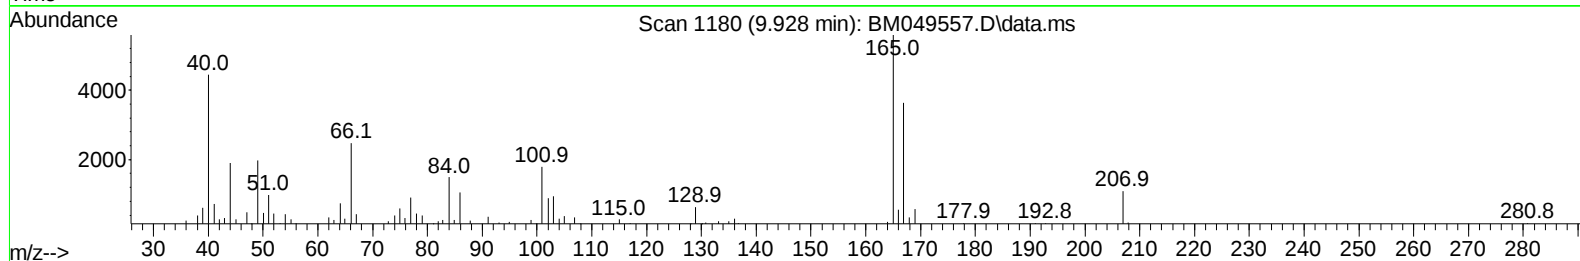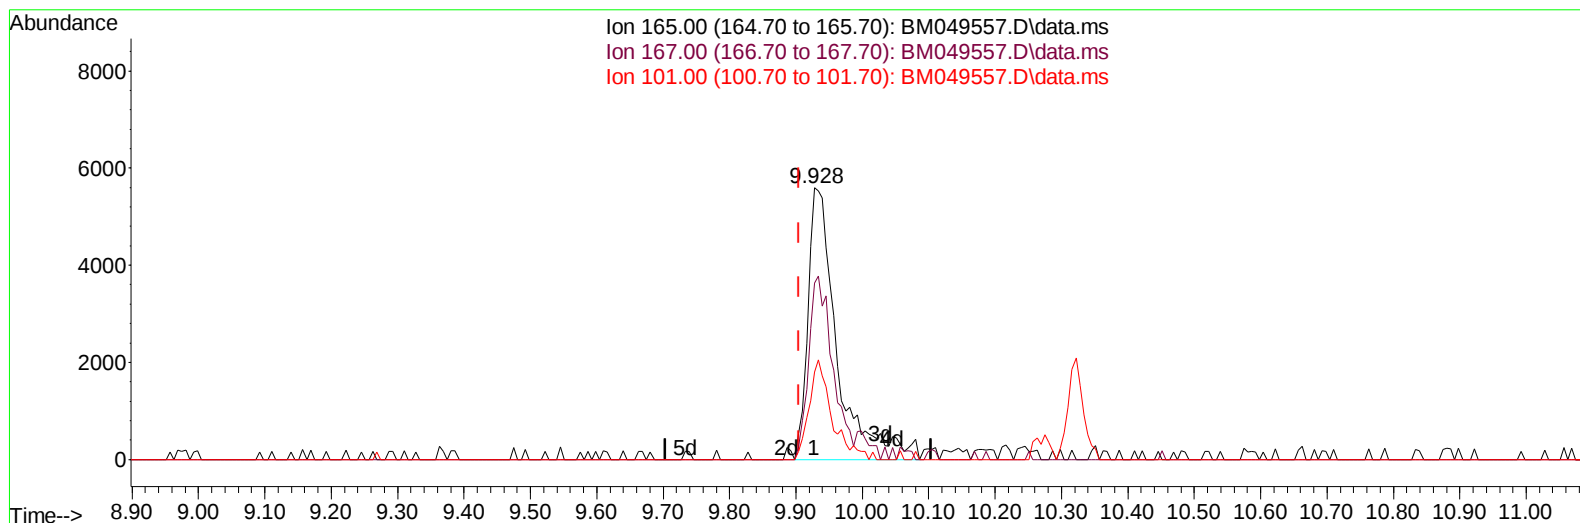

TIC: BM049557.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

9.928min (+ 0.023) 1.18 ng/ul m

response 17192

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.20	65.07
101.00	31.40	32.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

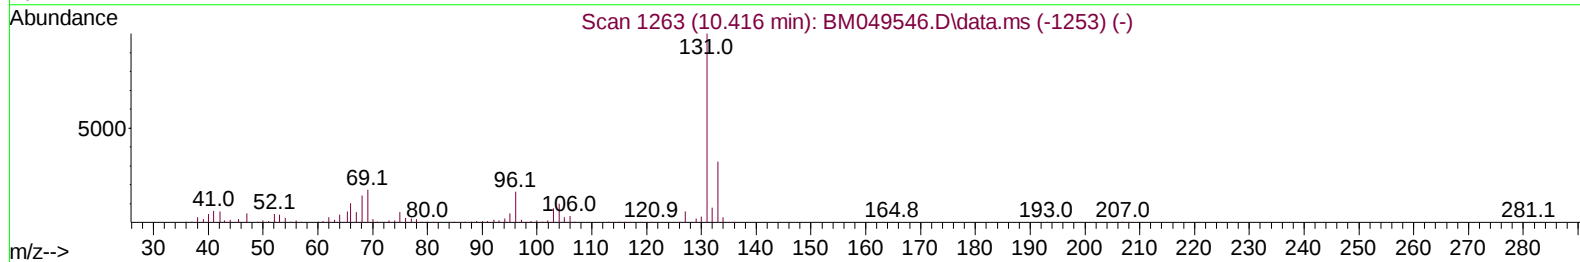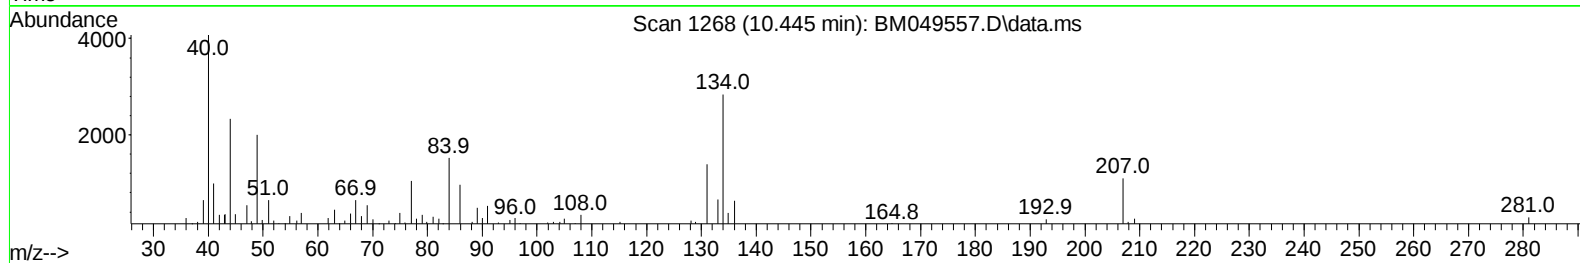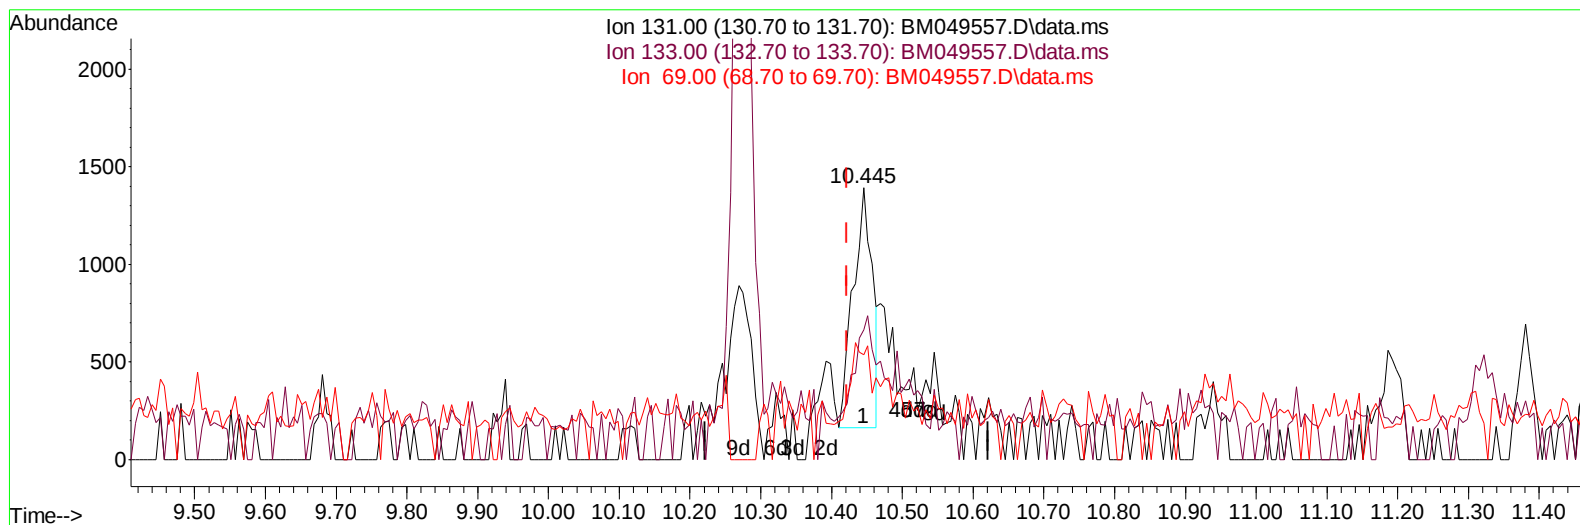

TIC: BM049557.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.445min (+ 0.023) 0.12 ng/u1

response 2333

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.80	47.66#
69.00	18.50	38.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

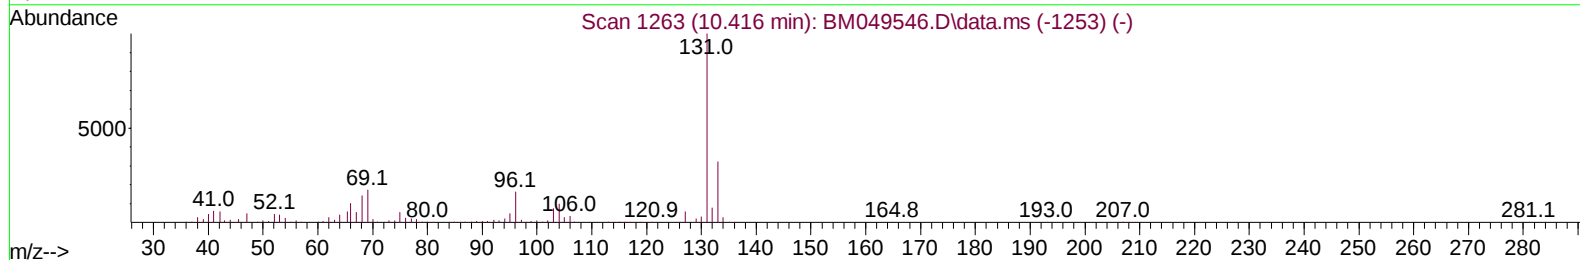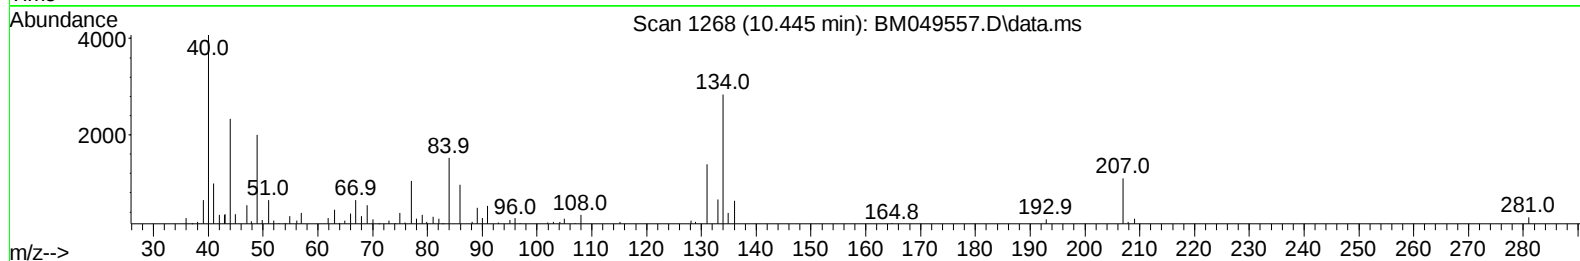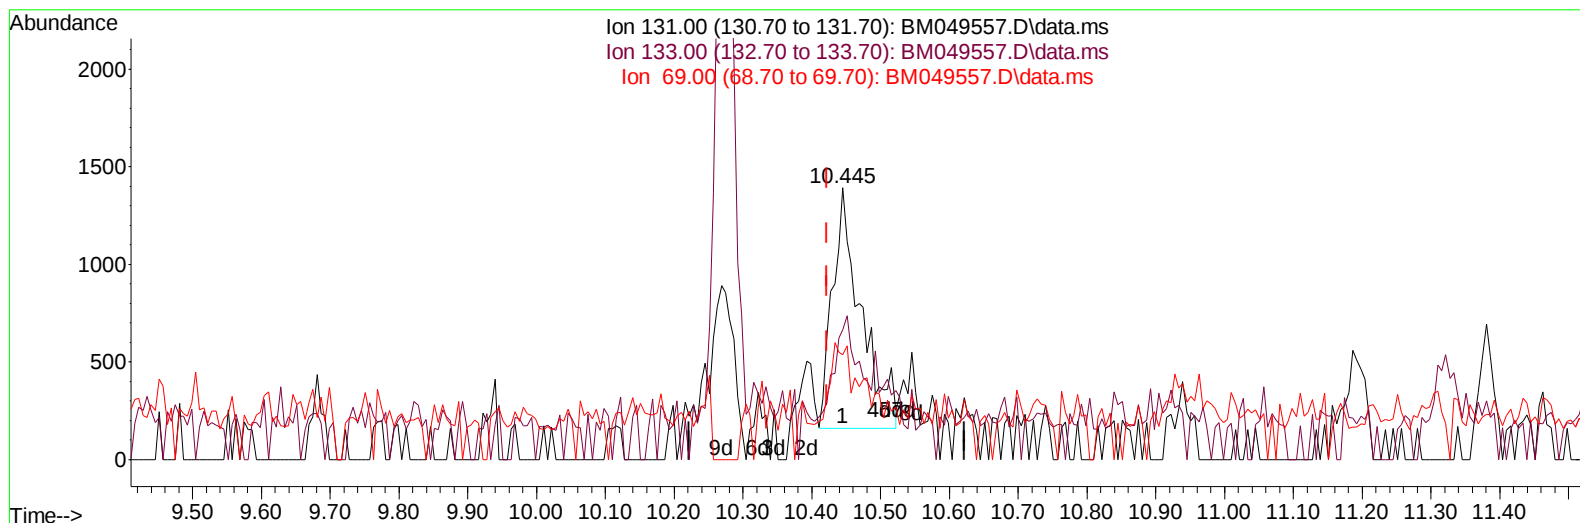

TIC: BM049557.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.445min (+ 0.023) 0.19 ng/ul m

response 3531

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.80	47.66#
69.00	18.50	38.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:12:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

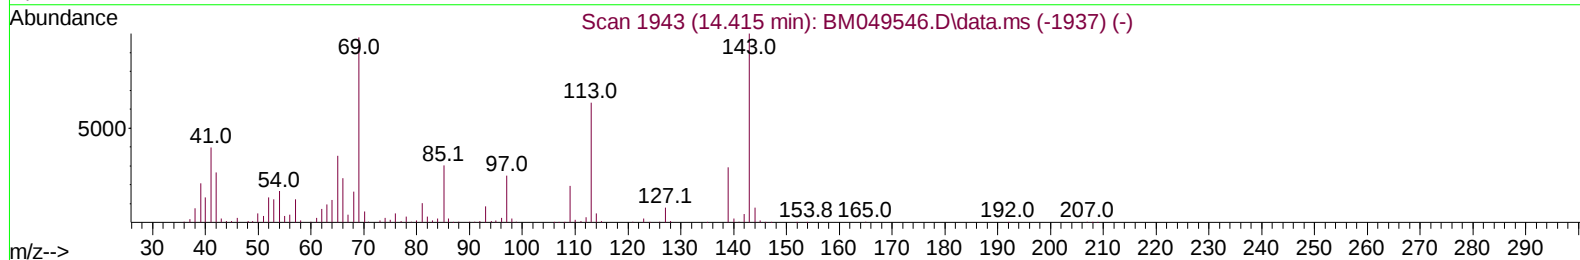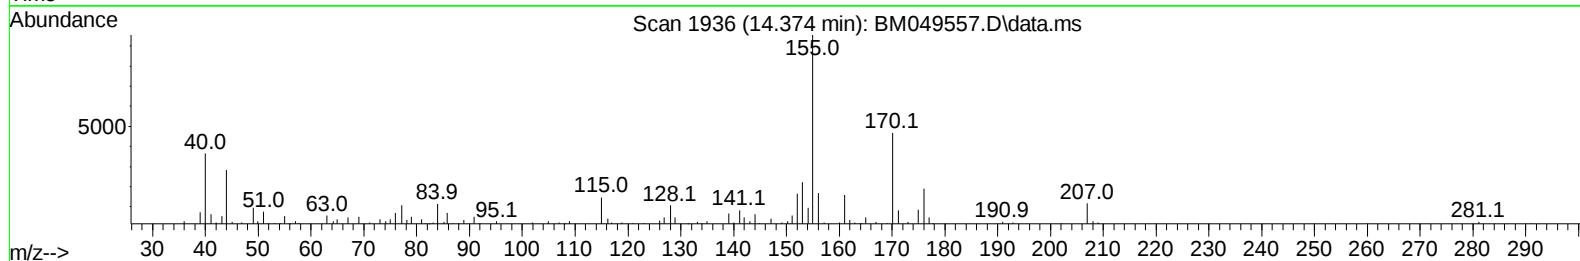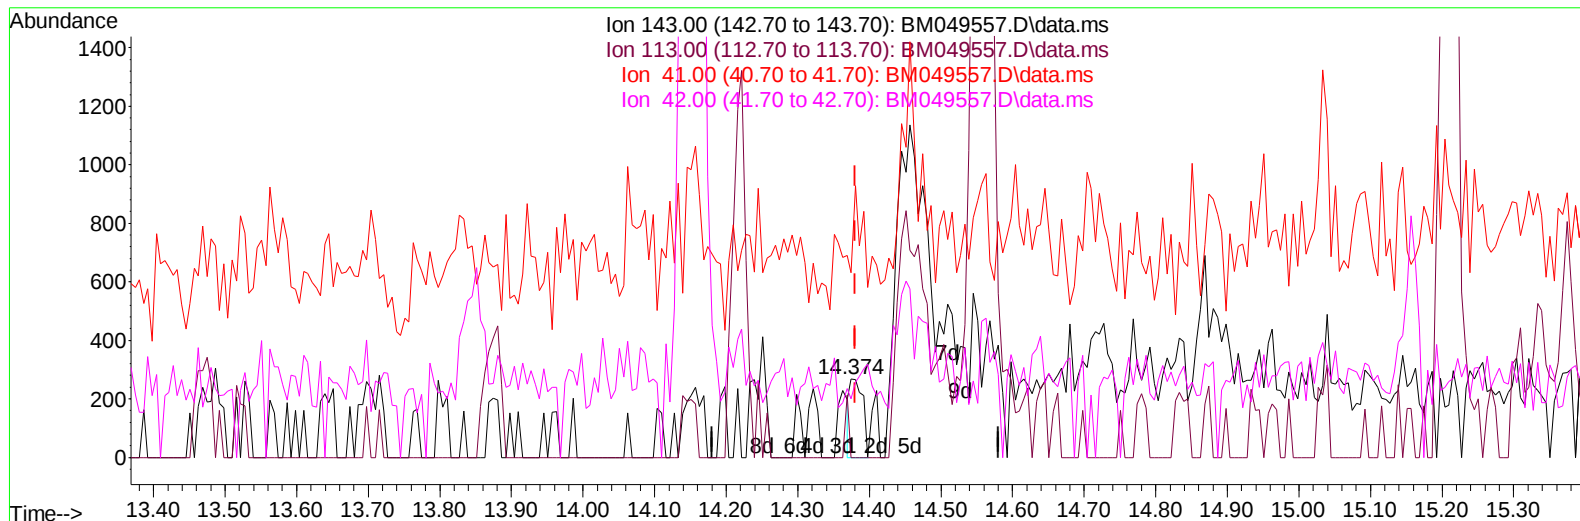

TIC: BM049557.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.374min (-0.006) 0.05 ng/u1

response 342

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	69.90	0.00#
41.00	42.70	235.45#
42.00	32.00	74.63#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:17:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

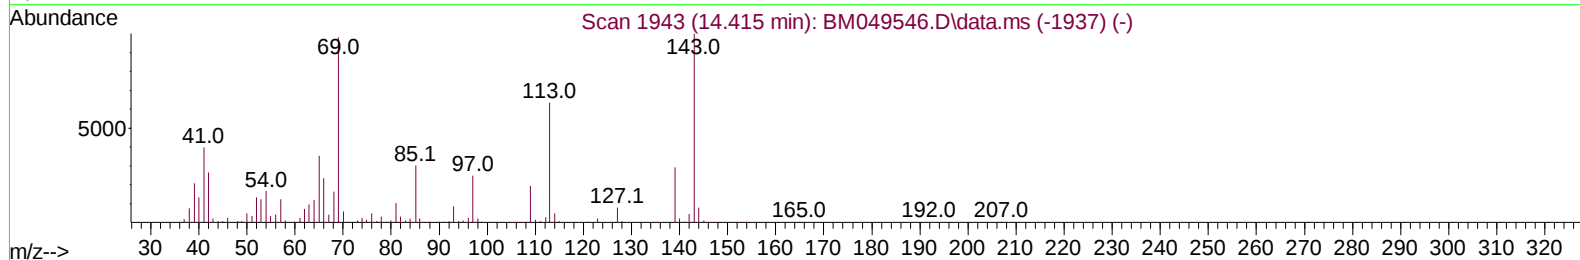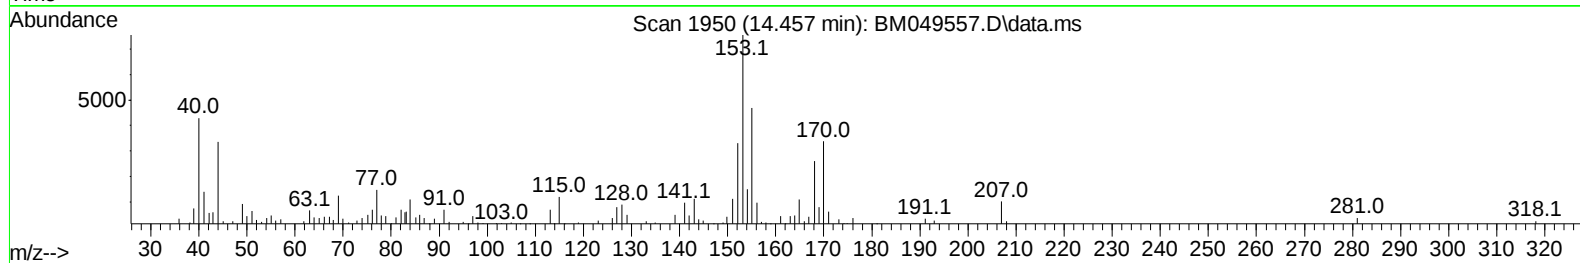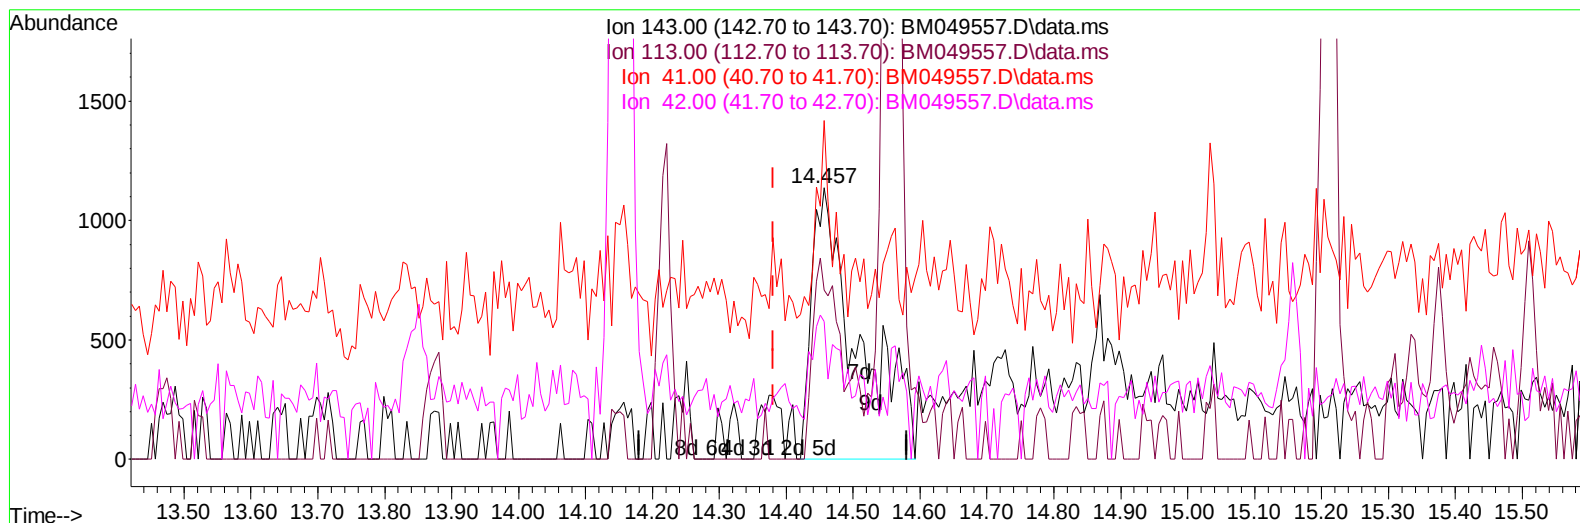

TIC: BM049557.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.457min (+ 0.076) 0.78 ng/ul m

response 5447

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	69.90	62.27
41.00	42.70	124.89#
42.00	32.00	50.75#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:17:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

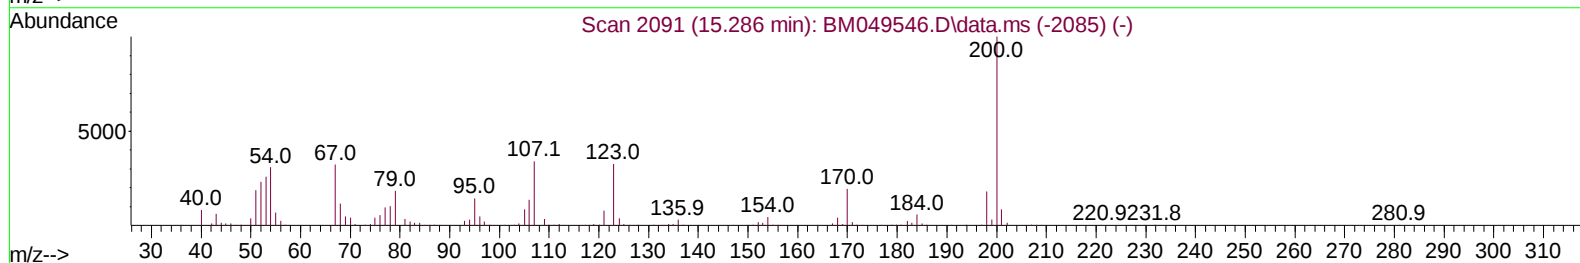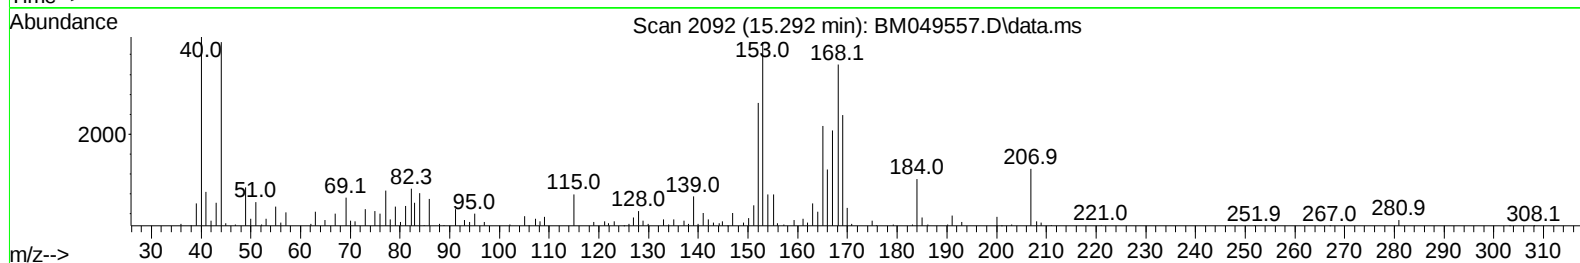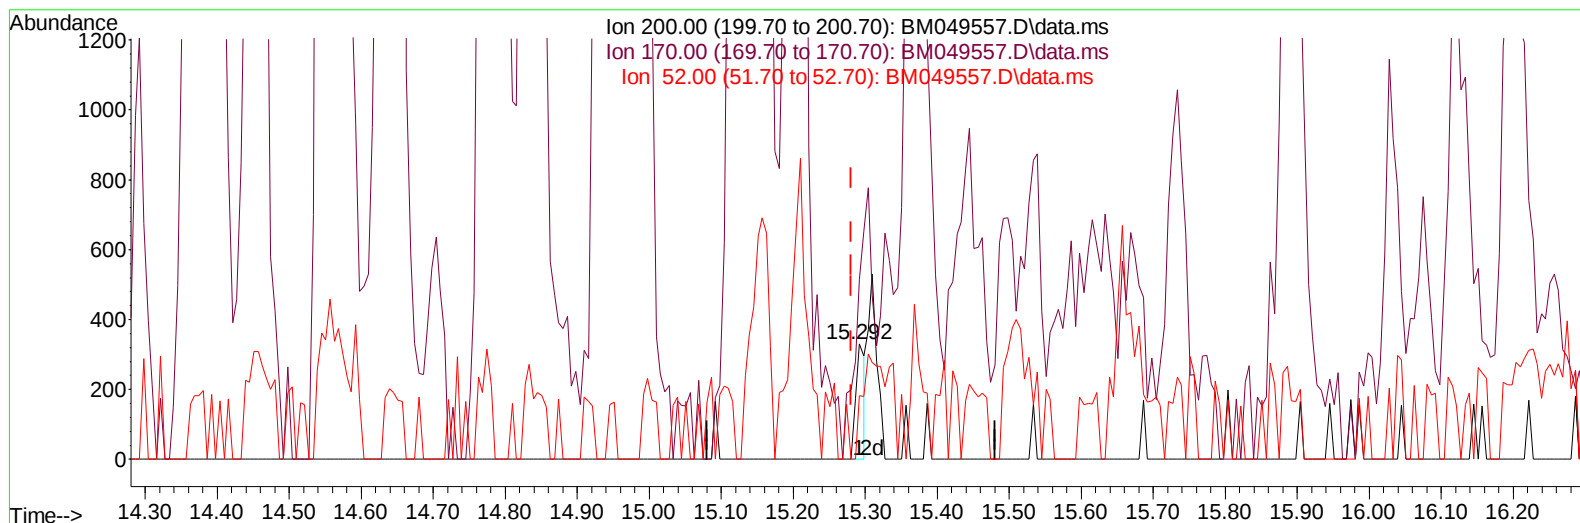

TIC: BM049557.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.292min (+ 0.012) 0.04 ng/ul

response 282

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	19.40	154.98#
52.00	38.90	54.98#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:17:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

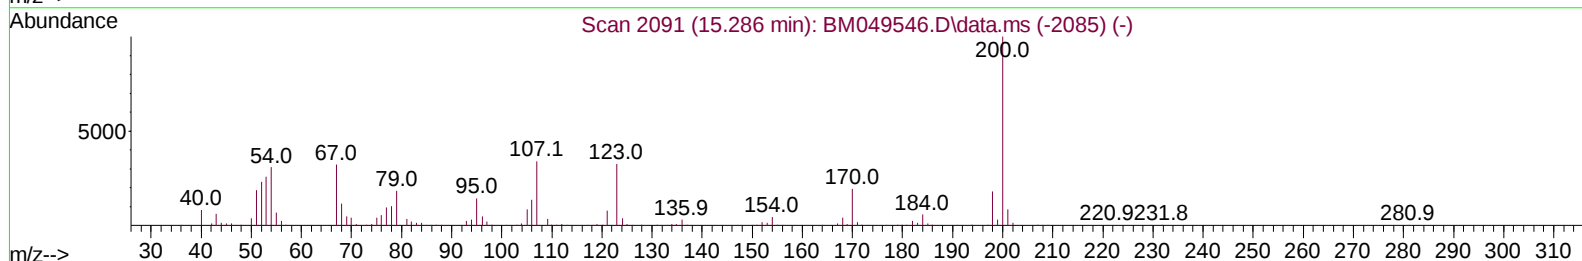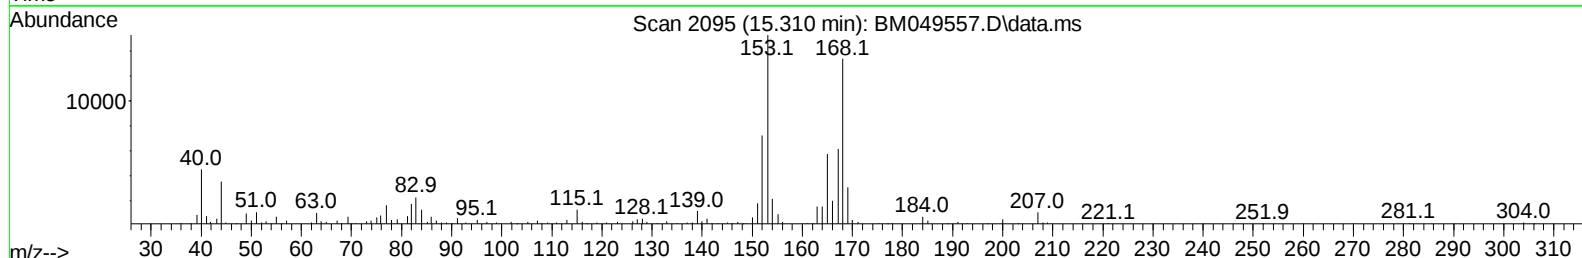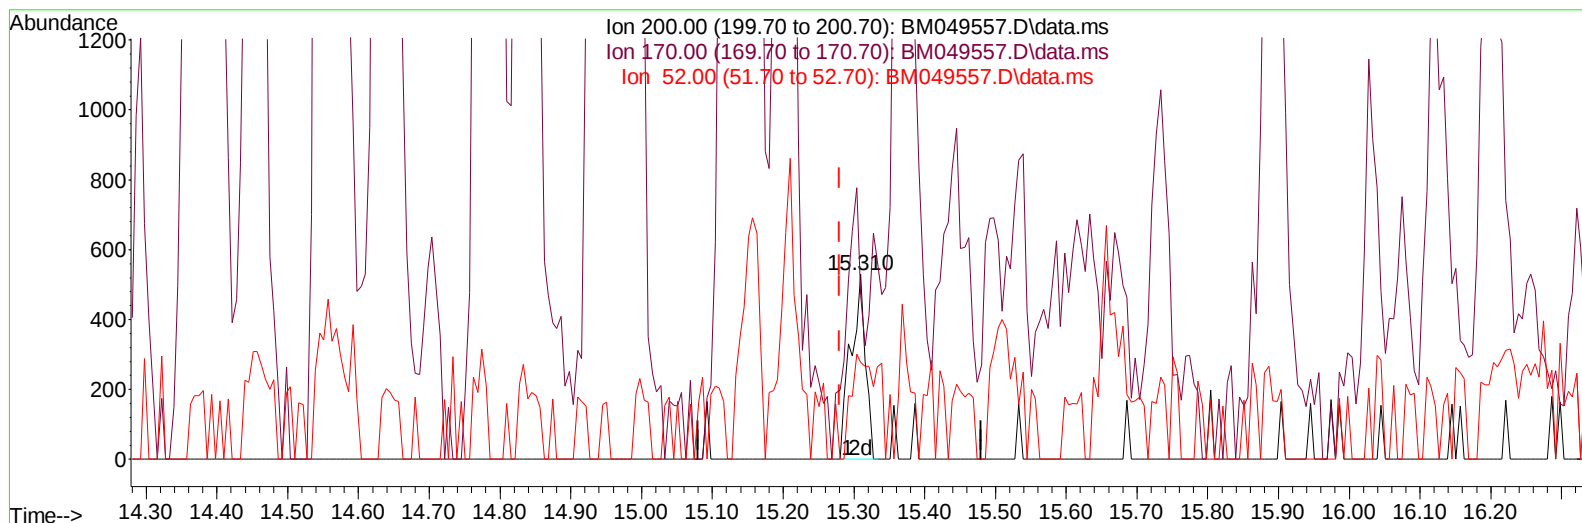

TIC: BM049557.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.310min (+ 0.029) 0.10 ng/ul m

response 764

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	19.40	88.68#
52.00	38.90	52.45#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:17:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

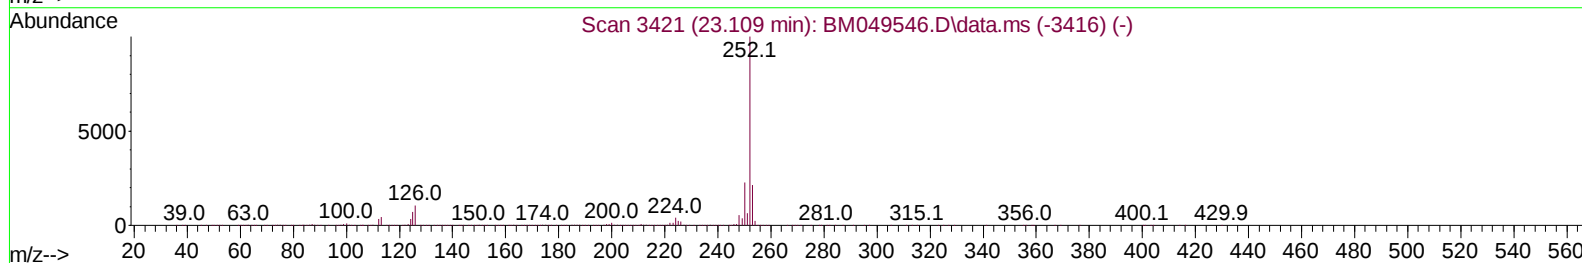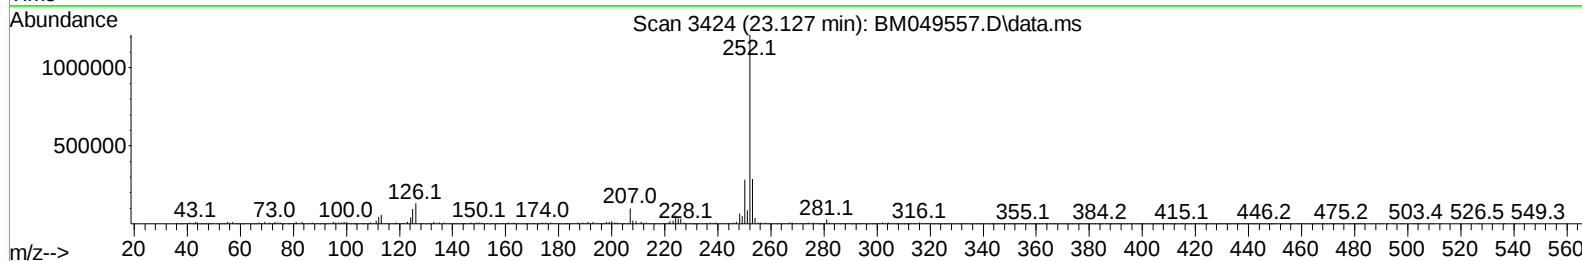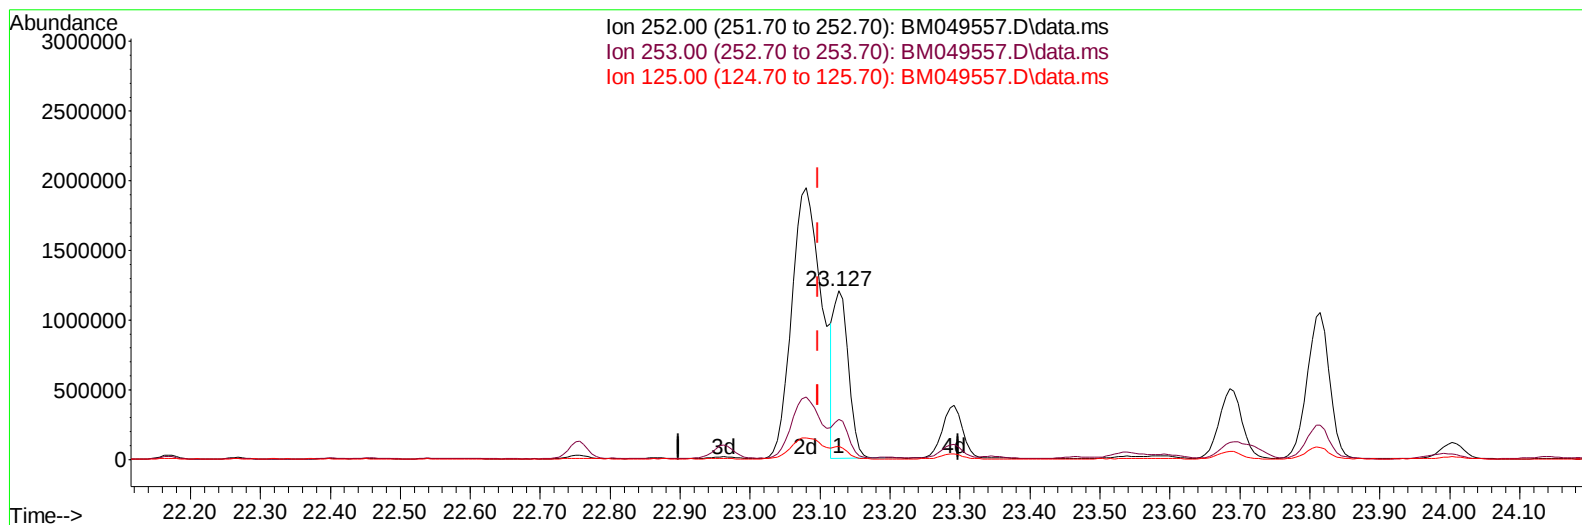

TIC: BM049557.D\data.ms

(91) Benzo(k)fluoranthene

23.127min (+ 0.029) 21.25 ng/u1

response 1753010

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	23.78
125.00	8.10	7.73
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:17:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

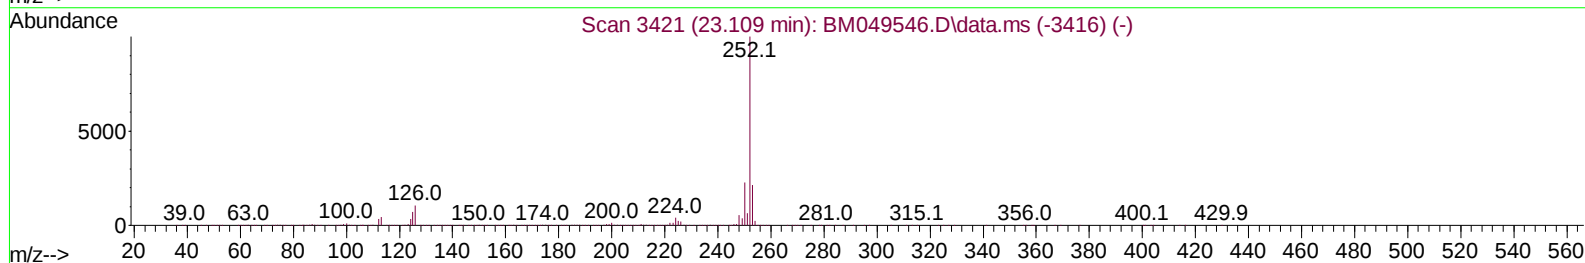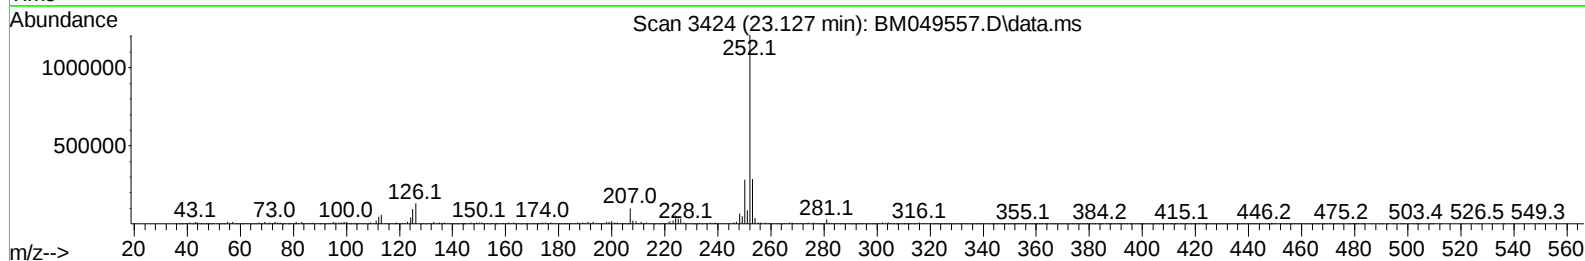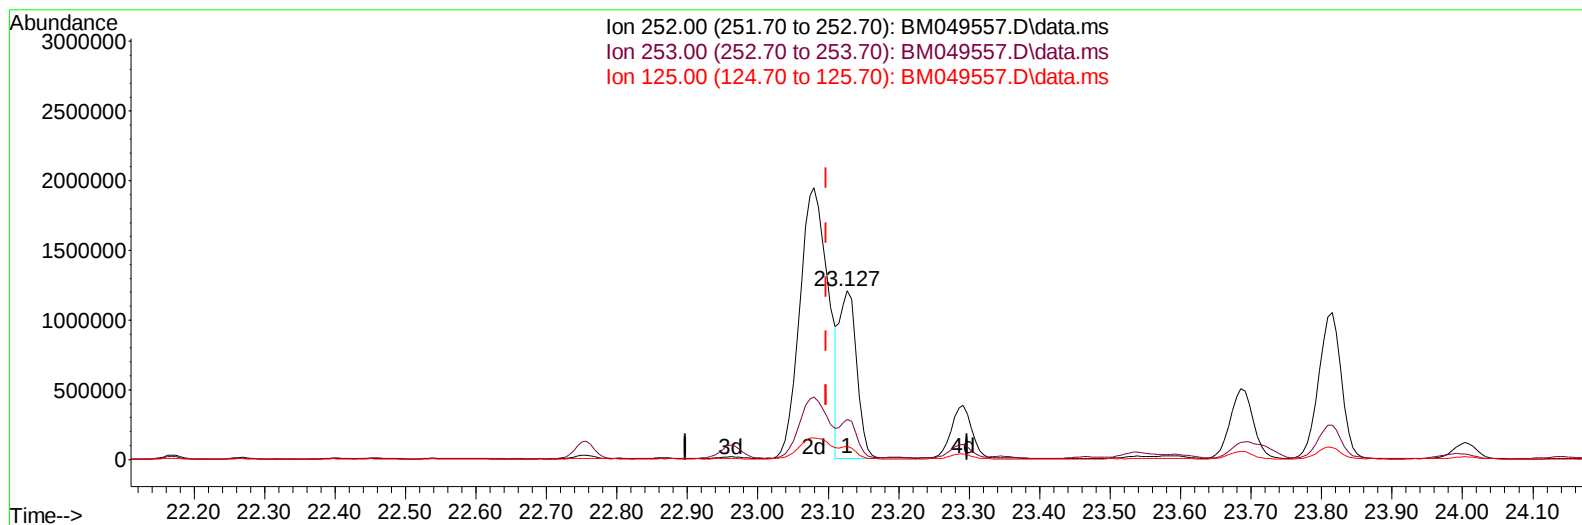

TIC: BM049557.D\data.ms

(91) Benzo(k)fluoranthene

23.127min (+ 0.029) 25.46 ng/ul m

response 2099936

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	23.78
125.00	8.10	7.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
 Data File : BM049557.D
 Acq On : 31 Jan 2025 14:38
 Operator : RC/JU
 Sample : Q1190-02 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:20:48 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 28 14:45:18 2025
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
 Supervised By :mohammad ahmed 02/04/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	217828	20.000	ng/ul	0.00
20) Naphthalene-d8	10.269	136	855684	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.157	164	578155	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.910	188	1181308	20.000	ng/ul	0.00
79) Chrysene-d12	21.151	240	1151728	20.000	ng/ul	0.02
88) Perylene-d12	23.944	264	1259201	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	1136m	0.193	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.728	99	20484m	1.159	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.863	67	12203m	1.010	ng/ul	0.00
11) 2-Chlorophenol-d4	7.057	132	16919	1.237	ng/ul	0.00
15) 4-Methylphenol-d8	8.245	113	13817m	1.067	ng/ul	0.02
21) Nitrobenzene-d5	8.663	128	7014	1.071	ng/ul	0.00
24) 2-Nitrophenol-d4	9.375	143	7548m	1.057	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.928	165	17192m	1.180	ng/ul	0.02
31) 4-Chloroaniline-d4	10.445	131	3531m	0.189	ng/ul	0.02
46) Dimethylphthalate-d6	13.575	166	56314	1.328	ng/ul	0.00
49) Acenaphthylene-d8	13.839	160	55581	1.116	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	5447m	0.783	ng/ul	0.08
60) Fluorene-d10	15.157	176	41322	1.108	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.310	200	764m	0.103	ng/ul	0.03
73) Anthracene-d10	17.010	188	70183	1.190	ng/ul	0.00
81) Pyrene-d10	19.321	212	66049	0.981	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.750	264	39431	0.587	ng/ul	0.02
Target Compounds				Qvalue		
16) Acetophenone	8.334	105	44466	2.065	ng/ul	97
30) Naphthalene	10.322	128	110597	2.428	ng/ul	97
36) 2-Methylnaphthalene	11.945	142	46096	1.484	ng/ul	99
37) 1-Methylnaphthalene	12.169	142	41511	1.355	ng/ul	100
50) Acenaphthylene	13.874	152	138140	2.700	ng/ul	97
52) Acenaphthene	14.216	153	255718	7.000	ng/ul	99
56) Dibenzofuran	14.557	168	202329	3.884	ng/ul	98
61) Fluorene	15.210	166	311448	7.399	ng/ul	96
72) Phenanthrene	16.957	178	4999778	75.188	ng/ul	100
74) Anthracene	17.045	178	1491292	22.265	ng/ul	100
77) Carbazole	17.321	167	425915	7.115	ng/ul	99
80) Fluoranthene	18.986	202	10328954	134.317	ng/ul	98
82) Pyrene	19.351	202	7812100	94.415	ng/ul	99
85) Benzo(a)anthracene	21.133	228	5116859	63.246	ng/ul	98
87) Chrysene	21.192	228	4385074	58.363	ng/ul	97
90) Benzo(b)fluoranthene	23.080	252	5440370	66.655	ng/ul	98
91) Benzo(k)fluoranthene	23.127	252	2099936m	25.461	ng/ul	
93) Benzo(a)pyrene	23.815	252	2344914	30.626	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	27.044	276	1932031	20.358	ng/ul	98
95) Dibenzo(a,h)anthracene	27.080	278	700479	9.109	ng/ul#	92
96) Benzo(g,h,i)perylene	28.003	276	211258	2.928	ng/ul	92

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

Quant Time: Feb 03 08:20:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed								

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049557.D
Acq On : 31 Jan 2025 14:38
Operator : RC/JU
Sample : Q1190-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:20:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 28 14:45:18 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

