

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
 Data File : BM049526.D
 Acq On : 30 Jan 2025 14:23
 Operator : RC/JU
 Sample : PB166284BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK284

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	28	rBV	78124	113330	2.19%	0.192%
2	3.504	84	88	105	rBV	1073891	1760569	34.00%	2.984%
3	3.810	135	140	145	rBV2	18921	29199	0.56%	0.049%
4	6.728	629	636	650	rBV	1201294	1935782	37.38%	3.281%
5	6.857	652	658	673	rVB	975513	1523091	29.41%	2.582%
6	7.057	685	692	702	rBV	1260243	1942777	37.52%	3.293%
7	7.504	762	768	777	rBV	968051	1519088	29.34%	2.575%
8	8.239	885	893	904	rBV	1360194	2217533	42.83%	3.759%
9	8.651	955	963	973	rBV	1042688	1693650	32.71%	2.871%
10	9.363	1078	1084	1094	rBV	843197	1362353	26.31%	2.309%
11	9.916	1171	1178	1193	rBV	1301256	2220971	42.89%	3.765%
12	10.269	1229	1238	1249	rBV	1195380	1956978	37.79%	3.317%
13	10.416	1255	1263	1283	rBV	1060612	1962244	37.90%	3.326%
14	11.875	1505	1511	1520	rVB	15087	29220	0.56%	0.050%
15	13.569	1793	1799	1810	rBV	1910858	2764849	53.40%	4.687%
16	13.839	1838	1845	1857	rBV	2393126	3582738	69.19%	6.073%
17	14.145	1890	1897	1905	rBV	1672876	2462062	47.55%	4.174%
18	14.421	1937	1944	1961	rBV	553873	1151994	22.25%	1.953%
19	15.151	2058	2068	2081	rBV	3136052	4305443	83.15%	7.298%
20	15.280	2083	2090	2101	rVV	819312	1112176	21.48%	1.885%
21	15.392	2105	2109	2115	rVB2	14484	22405	0.43%	0.038%
22	15.721	2161	2165	2169	rVB5	3663	5347	0.10%	0.009%
23	15.939	2197	2202	2206	rVB8	4910	7052	0.14%	0.012%
24	16.580	2309	2311	2316	rVB6	4390	5684	0.11%	0.010%
25	16.692	2324	2330	2333	rBV2	8542	12775	0.25%	0.022%
26	16.904	2359	2366	2376	rBV2	1998428	2767233	53.44%	4.691%
27	16.998	2376	2382	2397	rVV	3192563	4491656	86.74%	7.614%
28	17.592	2479	2483	2486	rBV5	5080	8775	0.17%	0.015%
29	17.827	2519	2523	2529	rBV6	17842	34279	0.66%	0.058%
30	18.868	2696	2700	2707	rVB2	33350	49576	0.96%	0.084%
31	18.945	2708	2713	2719	rBV	33638	55090	1.06%	0.093%
32	19.121	2740	2743	2747	rBV5	11039	16114	0.31%	0.027%
33	19.309	2766	2775	2786	rBV	3905529	5178074	100.00%	8.778%
34	21.133	3080	3085	3094	rBV	2087373	2804900	54.17%	4.755%
35	23.721	3517	3525	3539	rVB	2175598	4783205	92.37%	8.108%
36	23.909	3549	3557	3571	rBV	1258688	3103600	59.94%	5.261%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049526.D
Acq On : 30 Jan 2025 14:23
Operator : RC/JU
Sample : PB166284BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK284

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 58991812

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049526.D
Acq On : 30 Jan 2025 14:23
Operator : RC/JU
Sample : PB166284BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK284

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

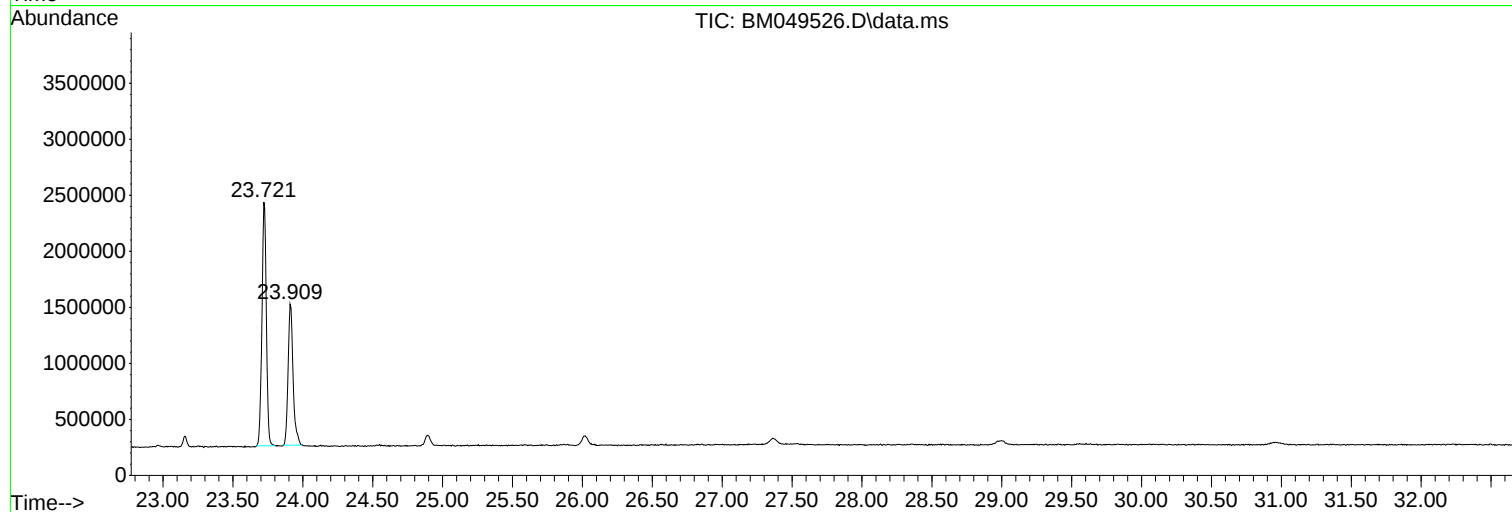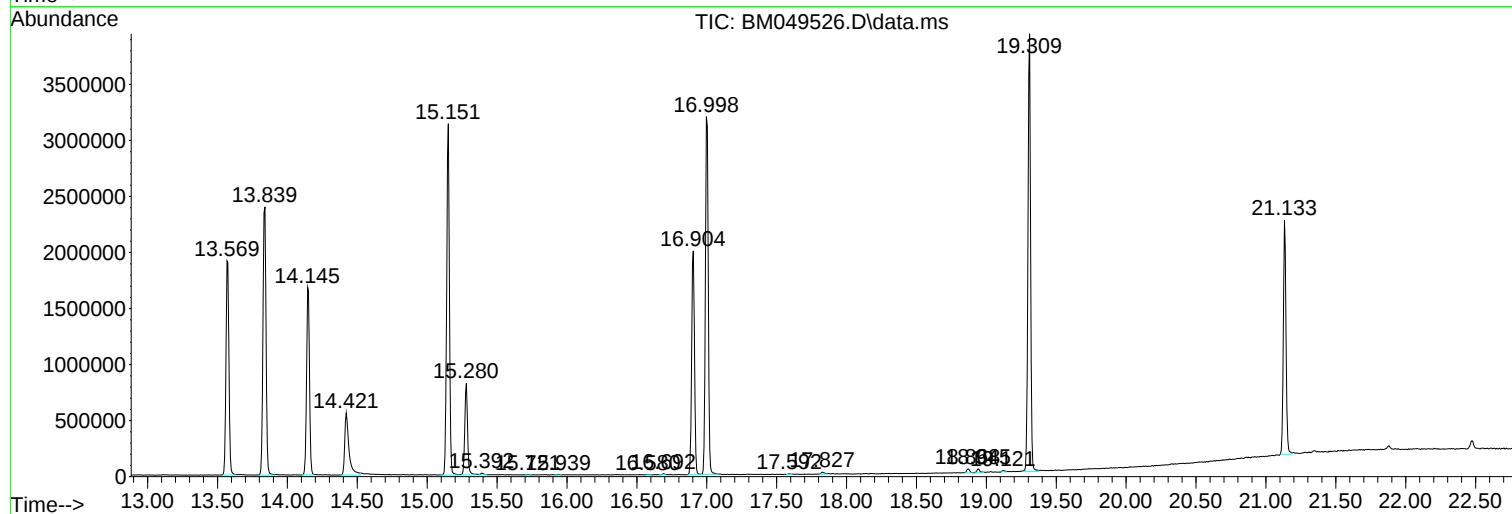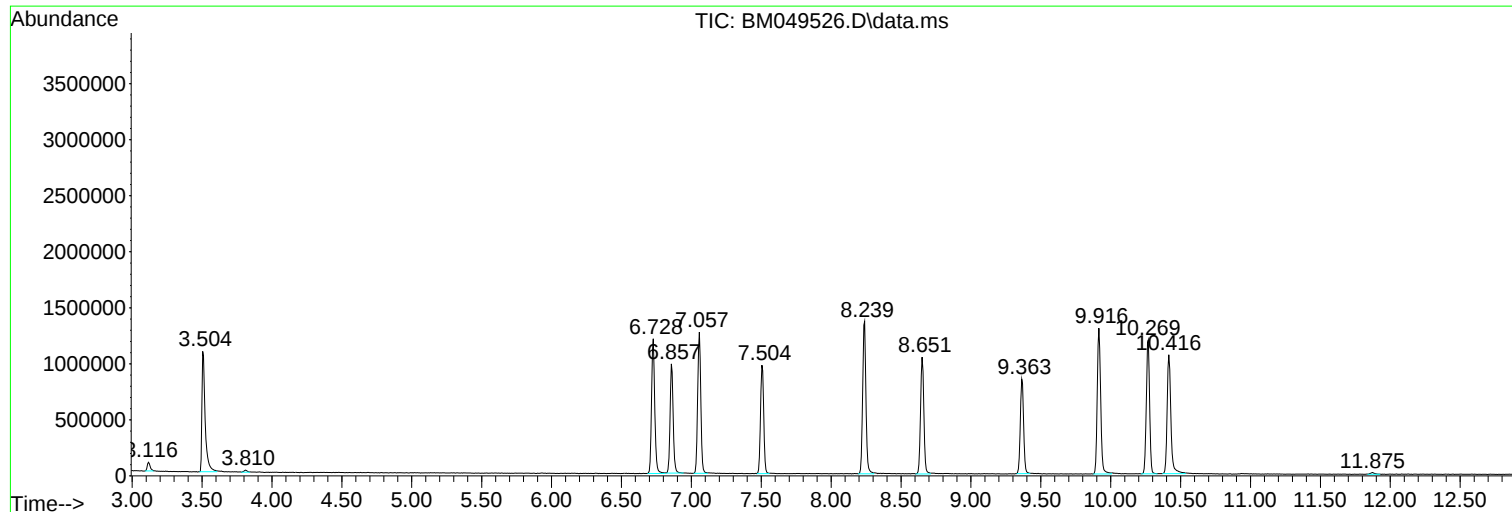

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049526.D
Acq On : 30 Jan 2025 14:23
Operator : RC/JU
Sample : PB166284BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK284

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049526.D
Acq On : 30 Jan 2025 14:23
Operator : RC/JU
Sample : PB166284BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK284

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc