

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
 Data File : BM049558.D
 Acq On : 31 Jan 2025 15:17
 Operator : RC/JU
 Sample : Q1190-08 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A44S7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.804	137	139	144	rVB3	12573	14219	0.38%	0.084%
2	4.693	287	290	291	rBV3	6562	6773	0.18%	0.040%
3	5.563	436	438	441	rVB4	4647	4031	0.11%	0.024%
4	6.728	632	636	646	rBV	38578	77514	2.09%	0.460%
5	6.863	654	659	670	rVB	33822	61388	1.65%	0.364%
6	7.057	687	692	699	rBV	45046	77662	2.09%	0.461%
7	7.510	762	769	778	rBV	781515	1227271	33.08%	7.281%
8	7.910	833	837	841	rBV7	3872	7085	0.19%	0.042%
9	8.022	852	856	860	rVB5	7165	10625	0.29%	0.063%
10	8.116	868	872	877	rVB6	4460	7301	0.20%	0.043%
11	8.245	889	894	902	rBV	36923	74055	2.00%	0.439%
12	8.334	905	909	914	rVB5	8827	16150	0.44%	0.096%
13	8.445	923	928	929	rBV5	3782	3866	0.10%	0.023%
14	8.663	959	965	969	rBV	30810	57378	1.55%	0.340%
15	8.728	973	976	982	rVB7	6491	9276	0.25%	0.055%
16	8.833	987	994	998	rBV10	6211	12656	0.34%	0.075%
17	9.092	1034	1038	1042	rBV6	7036	9164	0.25%	0.054%
18	9.375	1081	1086	1092	rBV3	28325	54671	1.47%	0.324%
19	9.433	1094	1096	1104	rVB9	5700	8857	0.24%	0.053%
20	9.780	1152	1155	1158	rBV5	3044	4681	0.13%	0.028%
21	9.933	1176	1181	1190	rBV	27965	70381	1.90%	0.418%
22	10.275	1230	1239	1248	rBV	1003419	1721679	46.41%	10.214%
23	10.339	1248	1250	1253	rVB4	7264	6672	0.18%	0.040%
24	10.627	1296	1299	1300	rBV3	4593	4261	0.11%	0.025%
25	10.951	1349	1354	1357	rBV7	3681	5965	0.16%	0.035%
26	11.127	1379	1384	1388	rBV7	4418	9799	0.26%	0.058%
27	11.357	1420	1423	1427	rBV6	4496	7764	0.21%	0.046%
28	11.733	1484	1487	1492	rVB5	2799	4652	0.13%	0.028%
29	11.927	1516	1520	1521	rBV4	3751	4813	0.13%	0.029%
30	12.169	1559	1561	1566	rVB5	3311	4242	0.11%	0.025%
31	12.992	1697	1701	1704	rBV6	5799	8880	0.24%	0.053%
32	13.133	1715	1725	1728	rBV9	5926	12192	0.33%	0.072%
33	13.398	1768	1770	1774	rVB5	4664	4054	0.11%	0.024%
34	13.527	1789	1792	1795	rBV5	4000	5391	0.15%	0.032%
35	13.580	1795	1801	1809	rVV	92258	153375	4.13%	0.910%
36	13.639	1809	1811	1814	rVB4	5211	5107	0.14%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
 Data File : BM049558.D
 Acq On : 31 Jan 2025 15:17
 Operator : RC/JU
 Sample : Q1190-08 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A44S7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
 Title : SVOA CALIBRATION

37	13.845	1839	1846	1859	rBV2	117076	212016	5.71%	1.258%
38	14.157	1892	1899	1907	rBV	1611122	2366531	63.79%	14.039%
39	14.215	1907	1909	1915	rVB7	6917	10233	0.28%	0.061%
40	14.380	1933	1937	1939	rBV5	4285	4344	0.12%	0.026%
41	14.451	1948	1949	1951	rBV2	4379	3788	0.10%	0.022%
42	14.774	2000	2004	2005	rBV4	3700	4121	0.11%	0.024%
43	14.915	2026	2028	2033	rBV6	4595	7322	0.20%	0.043%
44	15.157	2064	2069	2075	rBV	144809	221123	5.96%	1.312%
45	15.533	2129	2133	2138	rBV	24285	39085	1.05%	0.232%
46	16.909	2362	2367	2373	rBV2	2005924	2767257	74.59%	16.417%
47	17.009	2380	2384	2389	rBV	155242	206291	5.56%	1.224%
48	21.144	3083	3087	3098	rVB2	2271924	3530374	95.16%	20.944%
49	23.938	3558	3562	3581	rVB	1486181	3710006	100.00%	22.010%




Sum of corrected areas: 16856341

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049558.D
Acq On : 31 Jan 2025 15:17
Operator : RC/JU
Sample : Q1190-08 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

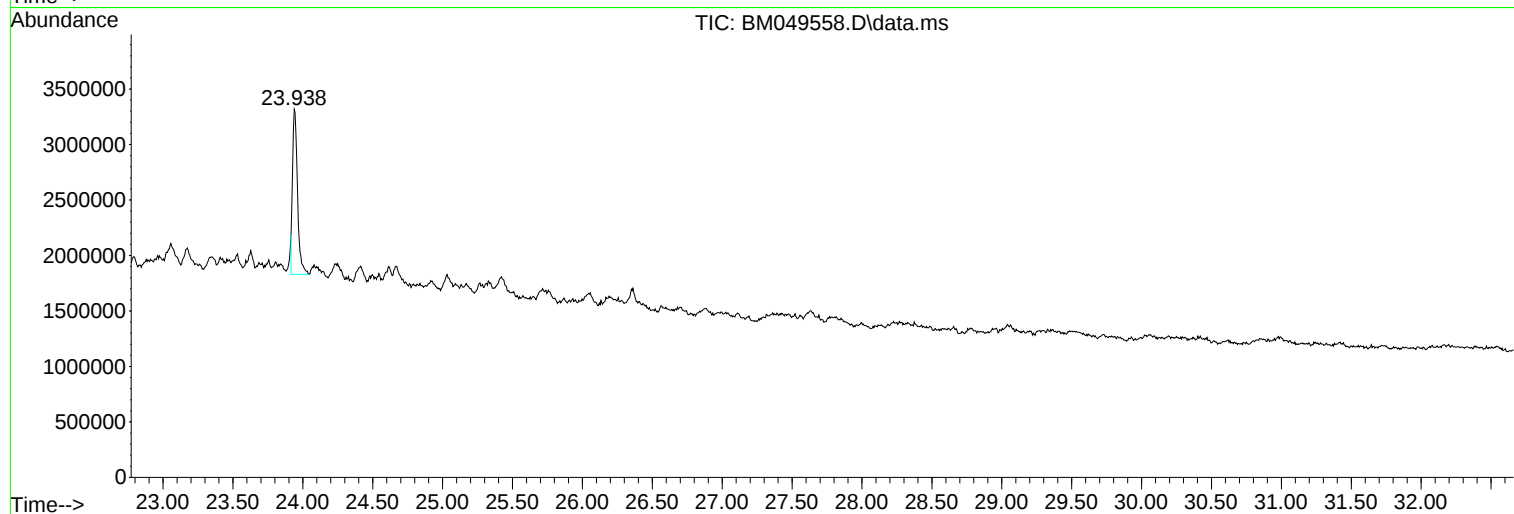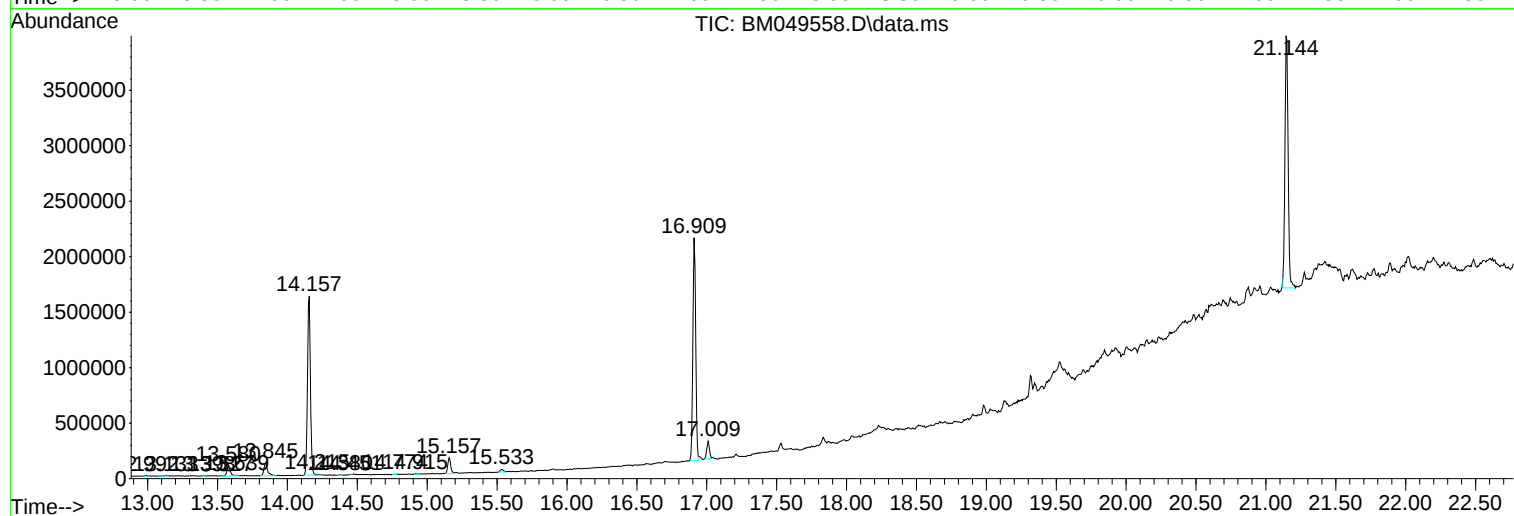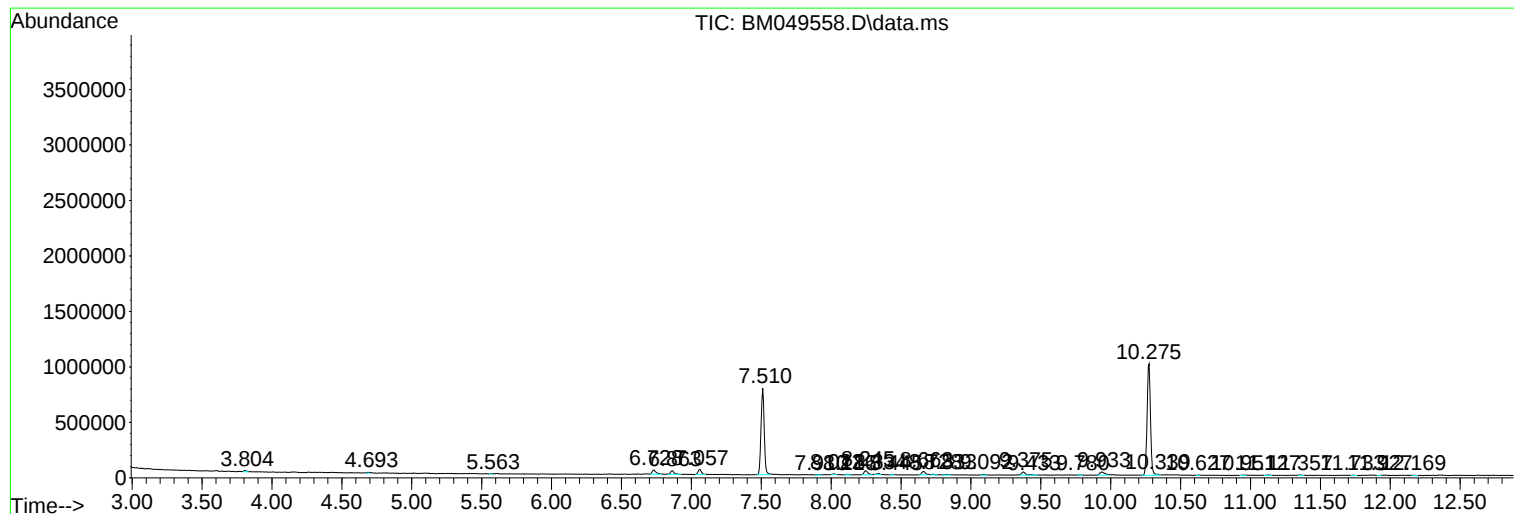

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049558.D
Acq On : 31 Jan 2025 15:17
Operator : RC/JU
Sample : Q1190-08 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013025\
Data File : BM049558.D
Acq On : 31 Jan 2025 15:17
Operator : RC/JU
Sample : Q1190-08 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A44S7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM012825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc