

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013118\
 Data File : BM014051.D
 Acq On : 01 Feb 2018 01:17
 Operator : SJ/JU
 Sample : J1315-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6C63

Quant Time: Feb 01 03:01:00 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 01 01:00:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	113461	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	471873	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	309663	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	759152	20.00	ng/ul	0.00
75) Chrysene-d12	21.18	240	763640	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	738755	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.12	96	11399	4.61	ng/uL	0.00
5) Phenol-d5	6.75	99	199831	23.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	136997	26.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	183990	27.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	187189	26.21	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	95514	28.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	108826	28.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	195326	24.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	242359	35.26	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	788090	30.67	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	947863	30.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	62811	17.74	ng/ul	0.00
57) Fluorene-d10	15.22	176	702329	30.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	106267	22.80	ng/ul	0.00
70) Anthracene-d10	17.07	188	1095384	29.72	ng/ul	0.00
76) Pyrene-d10	19.37	212	1225705	33.33	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.22	264	1079723	29.78	ng/ul	0.00
Target Compounds						
6) Phenol	6.78	94	9854	1.155	ng/ul#	85
44) Dimethylphthalate	13.69	163	142693	5.760	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013118\
Data File : BM014051.D
Acq On : 01 Feb 2018 01:17
Operator : SJ/JU
Sample : J1315-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6C63

Quant Time: Feb 01 03:01:00 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 01 01:00:18 2018
Response via : Initial Calibration

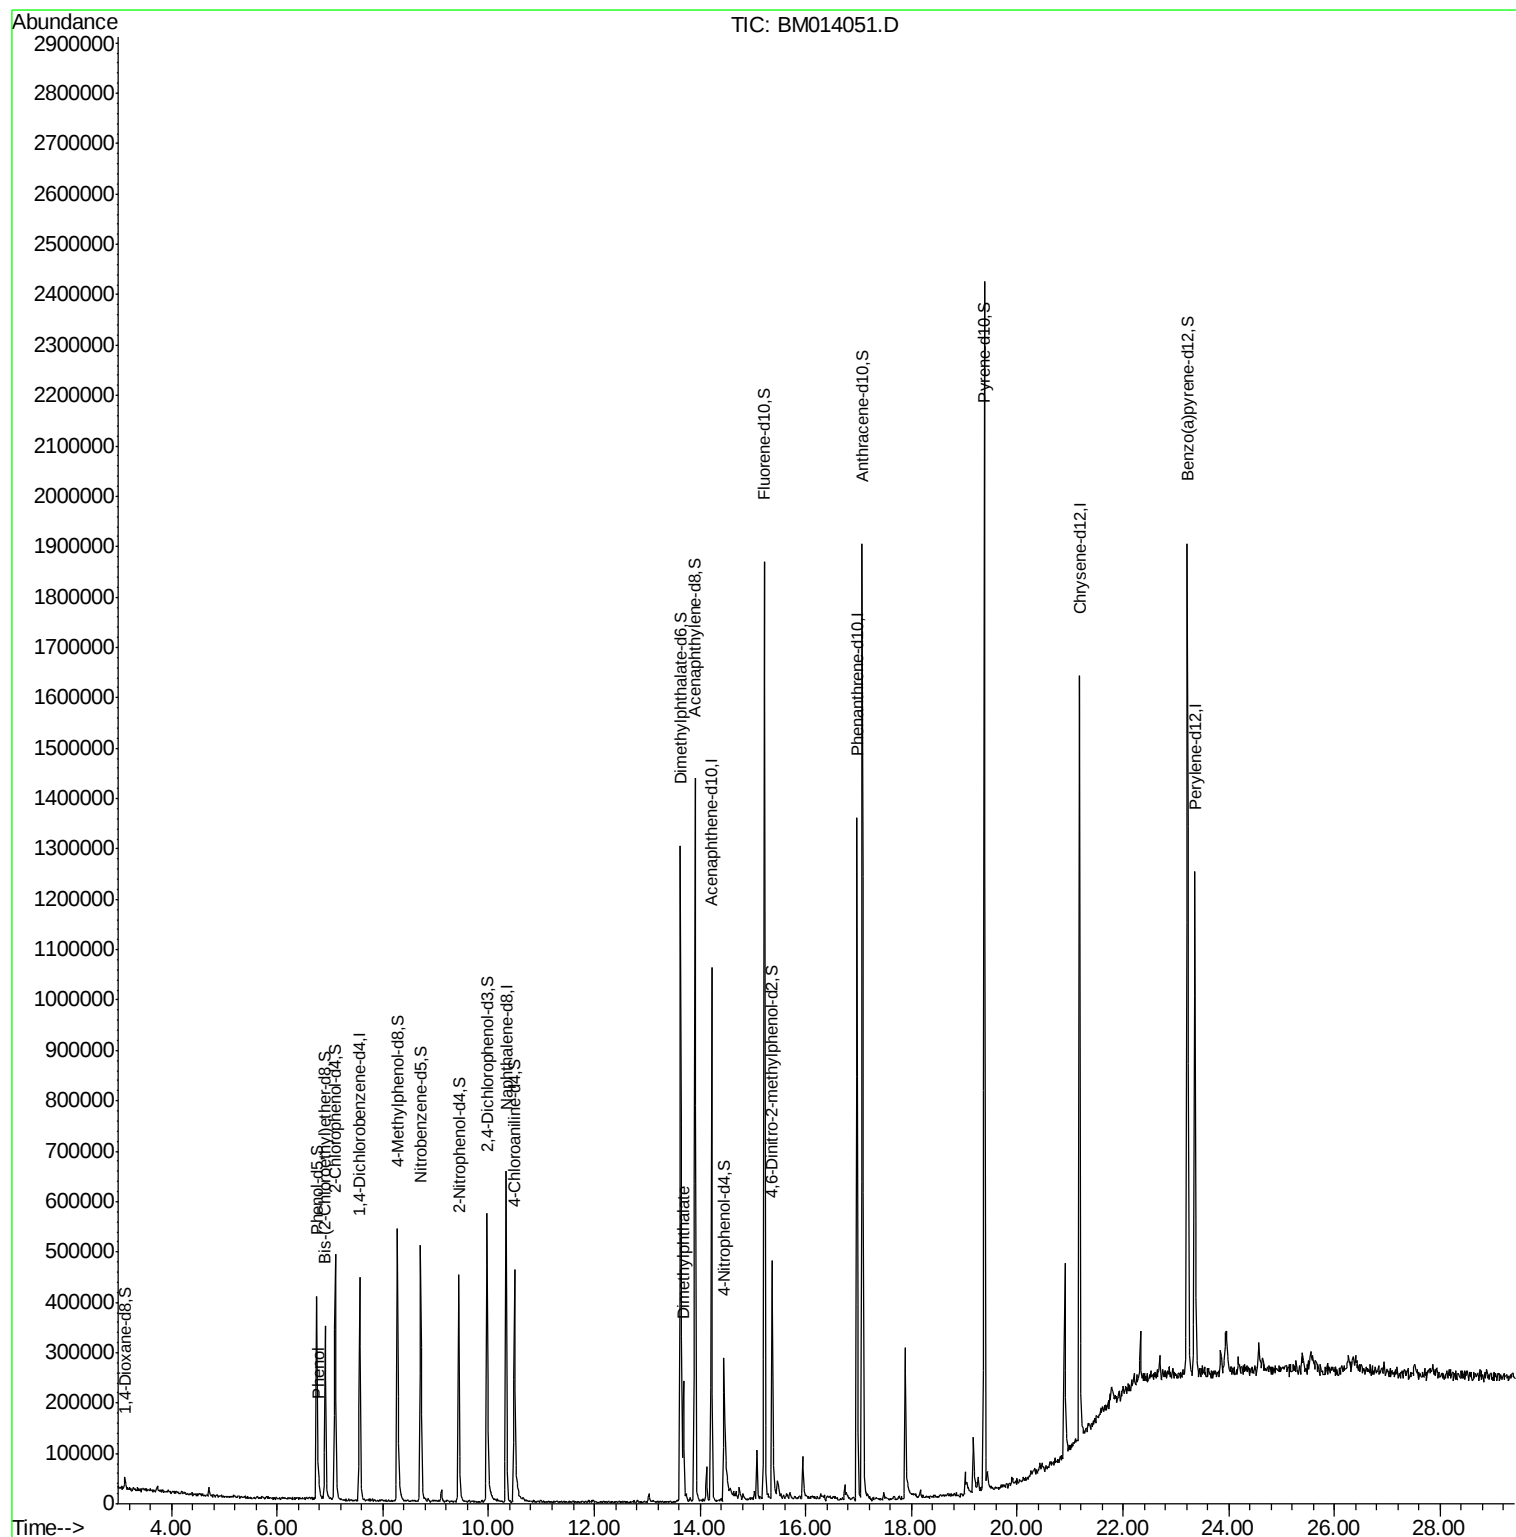

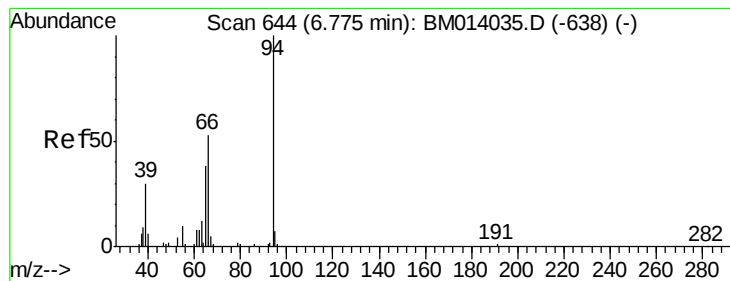





#6

Phenol

Concen: 1.155 ng/ul
 RT: 6.78 min Scan# 645
 Delta R.T. 0.01 min
 Lab File: BM014051.D
 Acq: 01 Feb 2018 01:17

Instrument :
 BNA_M
 ClientSampleId :
 F6C63

Tot Ion: 94 Resp: 9854
 Ion Ratio Lower Upper
 94 100
 65 32.8 28.2 42.4
 66 74.9 47.2 70.8#

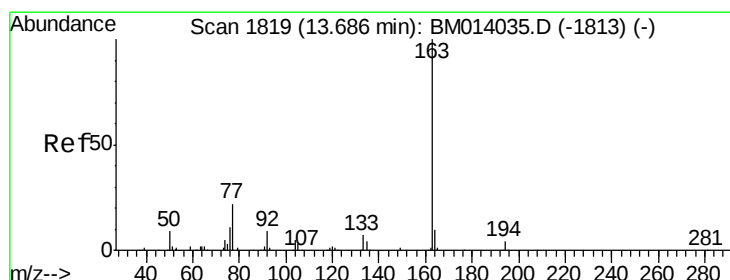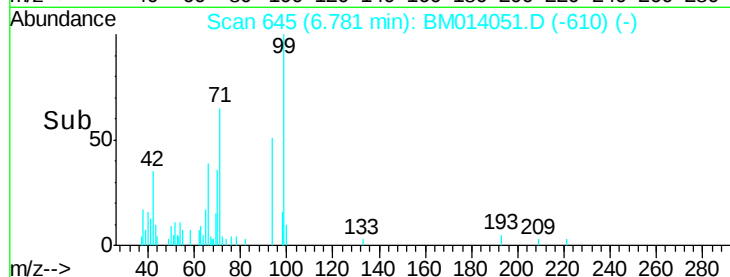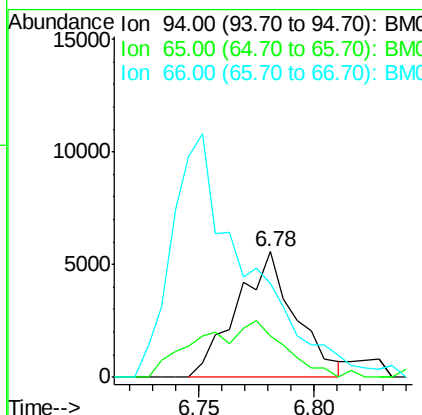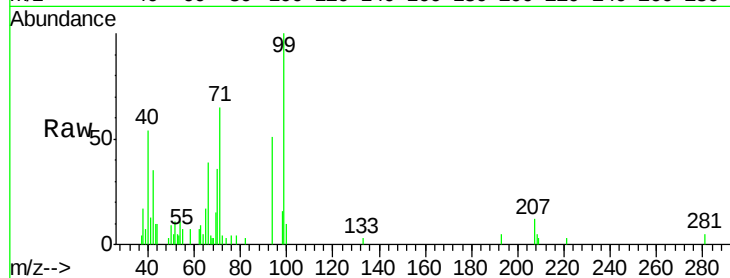

#44

Dimethylphthalate

Concen: 5.760 ng/ul
 RT: 13.69 min Scan# 1819
 Delta R.T. 0.00 min
 Lab File: BM014051.D
 Acq: 01 Feb 2018 01:17

Tgt Ion: 163 Resp: 142693
 Ion Ratio Lower Upper
 163 100
 194 4.5 3.5 5.3
 164 10.3 8.2 12.4

