


Data Path : Z:\HPCHEM1\BNA M\DATA\BM013118\
Data File : BM014068.D
Acq On : 01 Feb 2018 11:49
Operator : SJ/JU
Sample : J1316-09
Misc :
ALS Vial : 34 Sample Multiplier: 1




Quant Time: Feb 01 13:53:51 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 01 12:19:41 2018
Response via : Initial Calibration

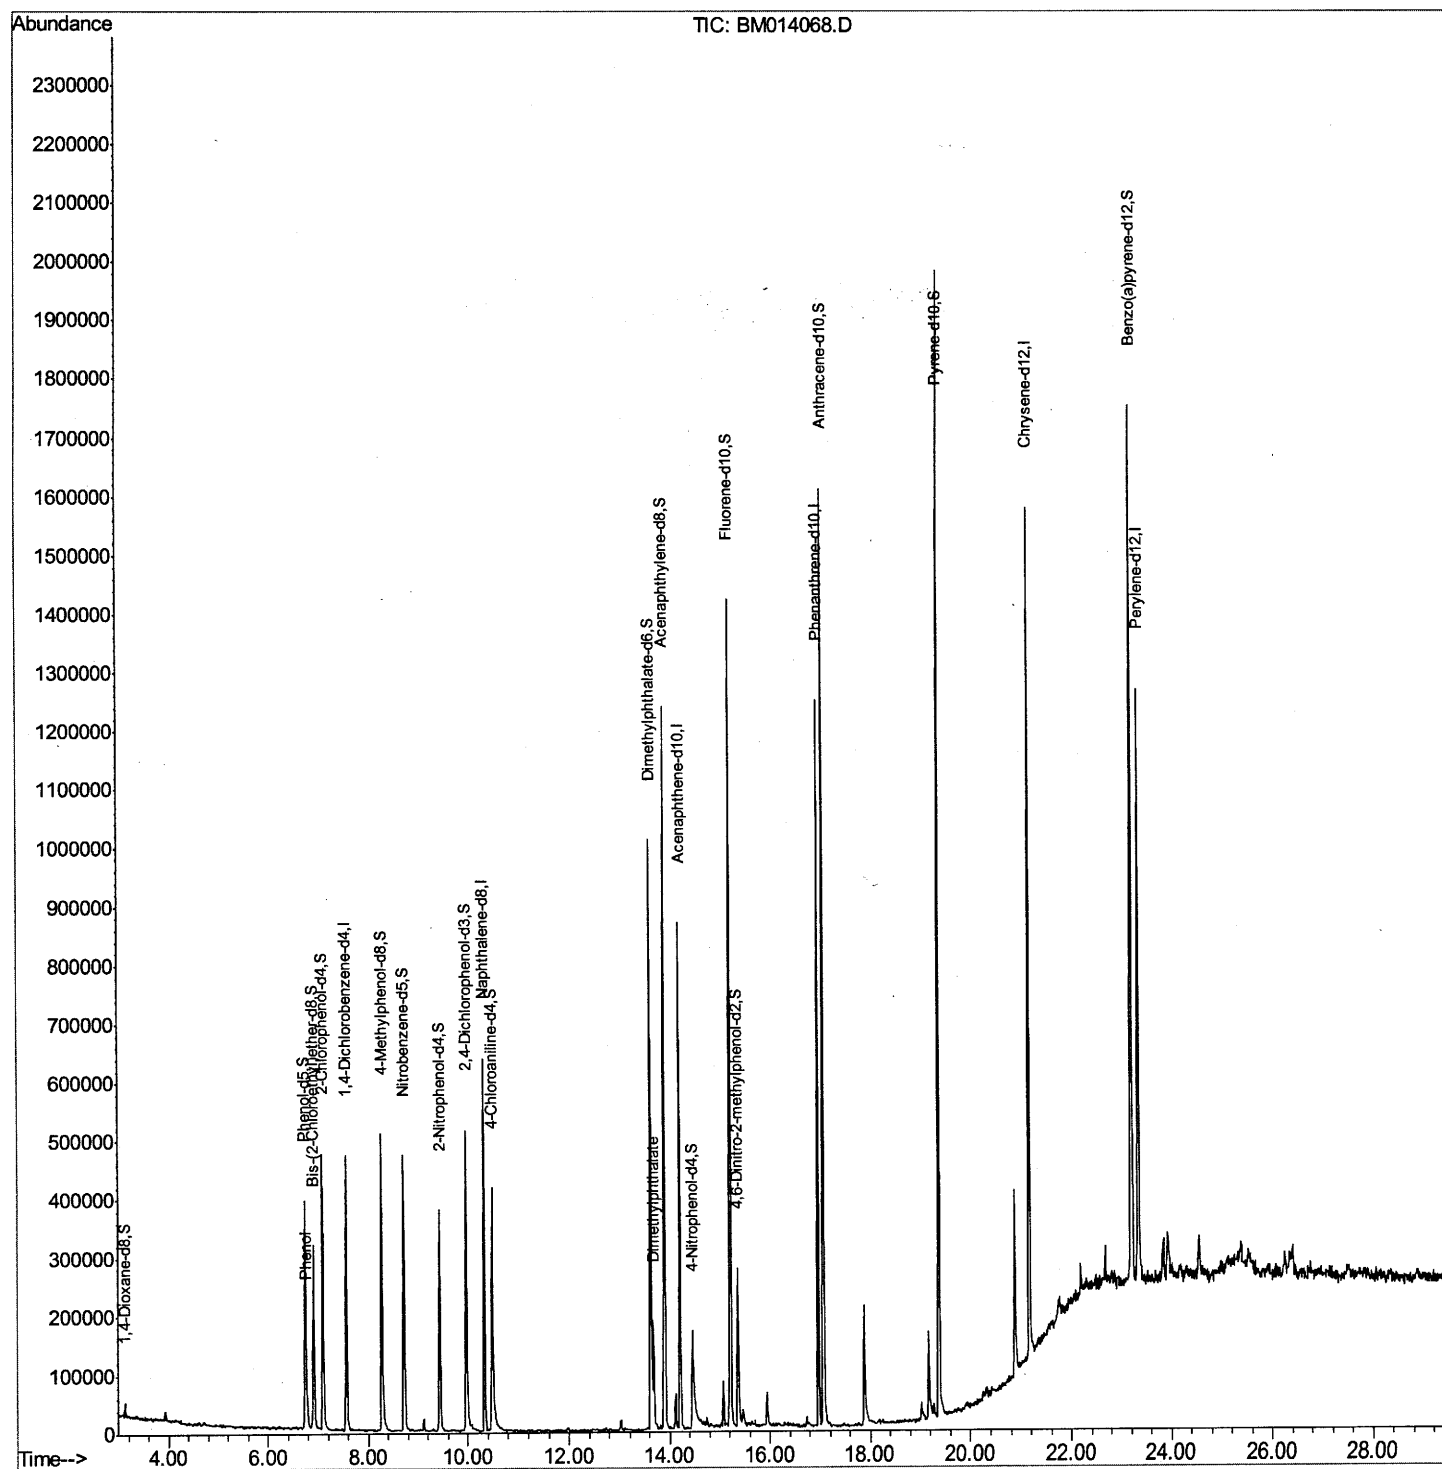

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013118\
Data File : BM014068.D
Acq On : 01 Feb 2018 11:49
Operator : SJ/JU
Sample : J1316-09
Misc :
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Feb 01 13:51:28 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 01 12:19:41 2018
Response via : Initial Calibration

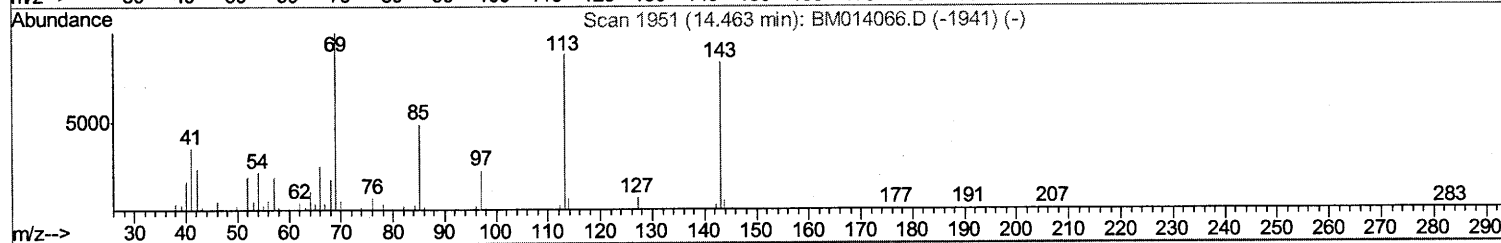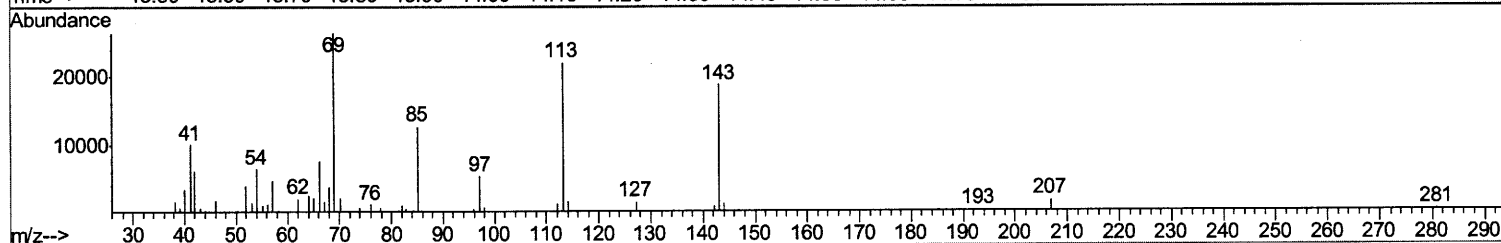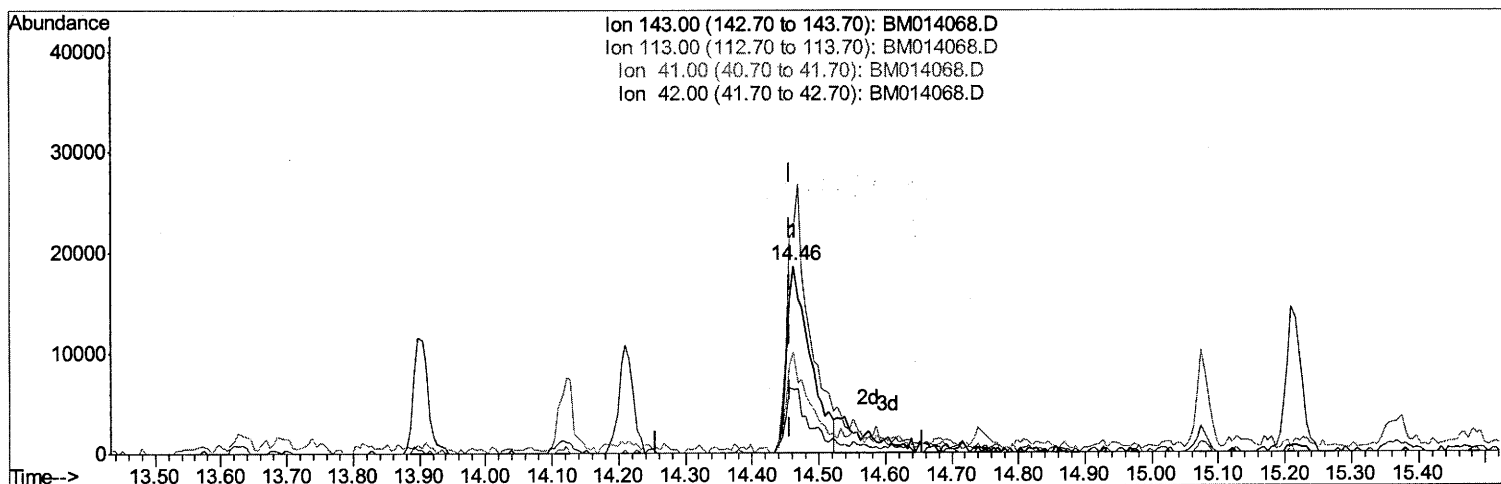

TIC: BM014068.D

(51) 4-Nitrophenol-d4 (S)

14.462min (+0.006) 14.33ng/ul




response 45457

Ion	Exp%	Act%
143.00	100	100
113.00	114.60	117.45
41.00	34.80	53.93#
42.00	20.50	33.65#

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013118\
 Data File : BM014068.D
 Acq On : 01 Feb 2018 11:49
 Operator : SJ/JU
 Sample : J1316-09
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Quant Time: Feb 01 13:51:28 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 01 12:19:41 2018
 Response via : Initial Calibration

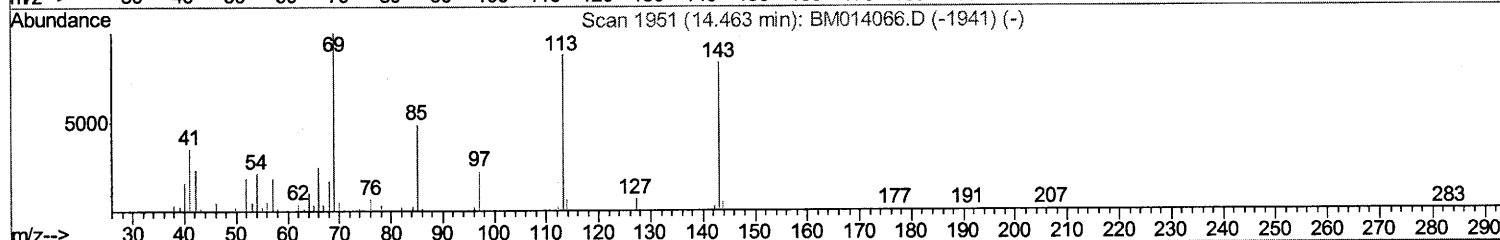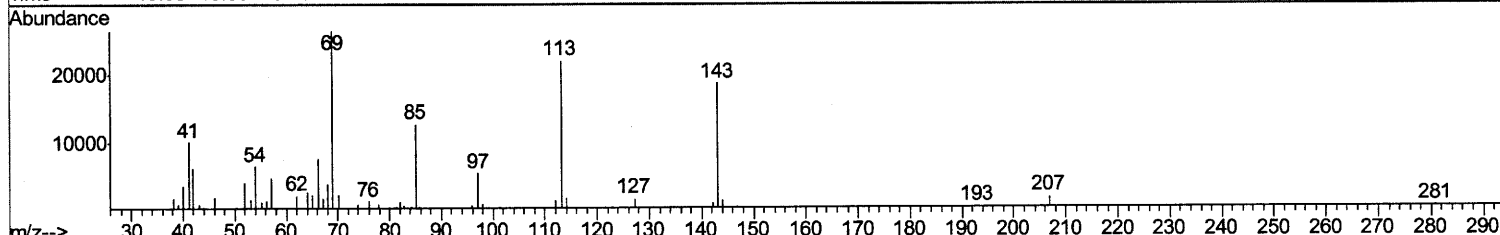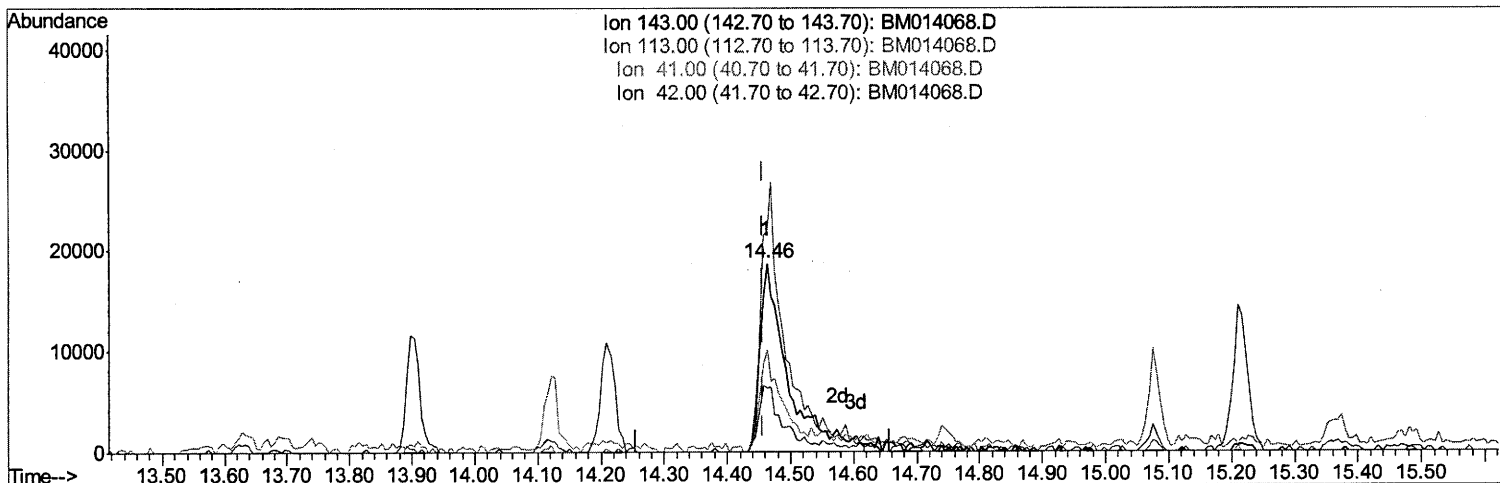

TIC: BM014068.D

(51) 4-Nitrophenol-d4 (S)

14.462min (+0.006) 17.71ng/ul m > SJ 2/8/18

response 56148

Ion	Exp%	Act%
143.00	100	100
113.00	114.60	117.45
41.00	34.80	53.93#
42.00	20.50	33.65#

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013118\
 Data File : BM014068.D
 Acq On : 01 Feb 2018 11:49
 Operator : SJ/JU
 Sample : J1316-09
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Quant Time: Feb 01 13:53:51 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 01 12:19:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	108655	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	446186	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	277276	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	659100	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	740327	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	754297	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	11802	4.98	ng/uL	0.00
5) Phenol-d5	6.75	99	199732	24.46	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	6.90	67	130906	26.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	181003	27.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	174416	25.51	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	90274	28.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	96986	27.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	179478	23.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	205702	31.65	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	613918	26.68	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	790186	28.30	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	56148m	17.71	ng/ul	0.00
57) Fluorene-d10	15.22	176	554622	26.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	63066	15.58	ng/ul	0.00
70) Anthracene-d10	17.07	188	882424	27.57	ng/ul	0.00
76) Pyrene-d10	19.37	212	1002031	28.11	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.21	264	1009323	27.26	ng/ul	0.00

SD 2/8/18

Target Compounds

				Ovalue	
6) Phenol	6.77	94	11798	1.444 ng/ul#	89
44) Dimethylphthalate	13.68	163	105766	4.768 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed