

Data Path : Z:\HPCHEM1\BNA M\DATA\BM013118\
 Data File : BM014064.D
 Acq On : 01 Feb 2018 09:26
 Operator : SJ/JU
 Sample : J1316-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6C88

Manual Integrations
 APPROVED

Sohil
 2/1/2018 6:05:31 PM

Quant Time: Feb 12 18:34:37 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 01 03:26:19 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	116015	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	458725	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	288915	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	687598	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	810355	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	808587	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	11855	4.69	ng/uL	0.00
5) Phenol-d5	6.75	99	237230	27.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	146941	27.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	199297	28.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	204901	28.06	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	102040	30.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	110391	30.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	214591	27.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	247965	37.10	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	708355	29.54	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	884462	30.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	77456m	23.44	ng/ul	0.00
57) Fluorene-d10	15.22	176	623381	29.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	92537	21.92	ng/ul	0.00
70) Anthracene-d10	17.07	188	995108	29.81	ng/ul	0.00
76) Pyrene-d10	19.37	212	1149314	29.45	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.22	264	1175883	29.63	ng/ul	0.00

Target Compounds				Ovalue
44) Dimethylphthalate	13.69	163	146397	6.334 ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM013118\
Data File : BM014064.D
Acq On : 01 Feb 2018 09:26
Operator : SJ/JU
Sample : J1316-04
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6C88

Quant Time: Feb 12 18:34:37 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 01 03:26:19 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
2/1/2018 6:05:31 PM

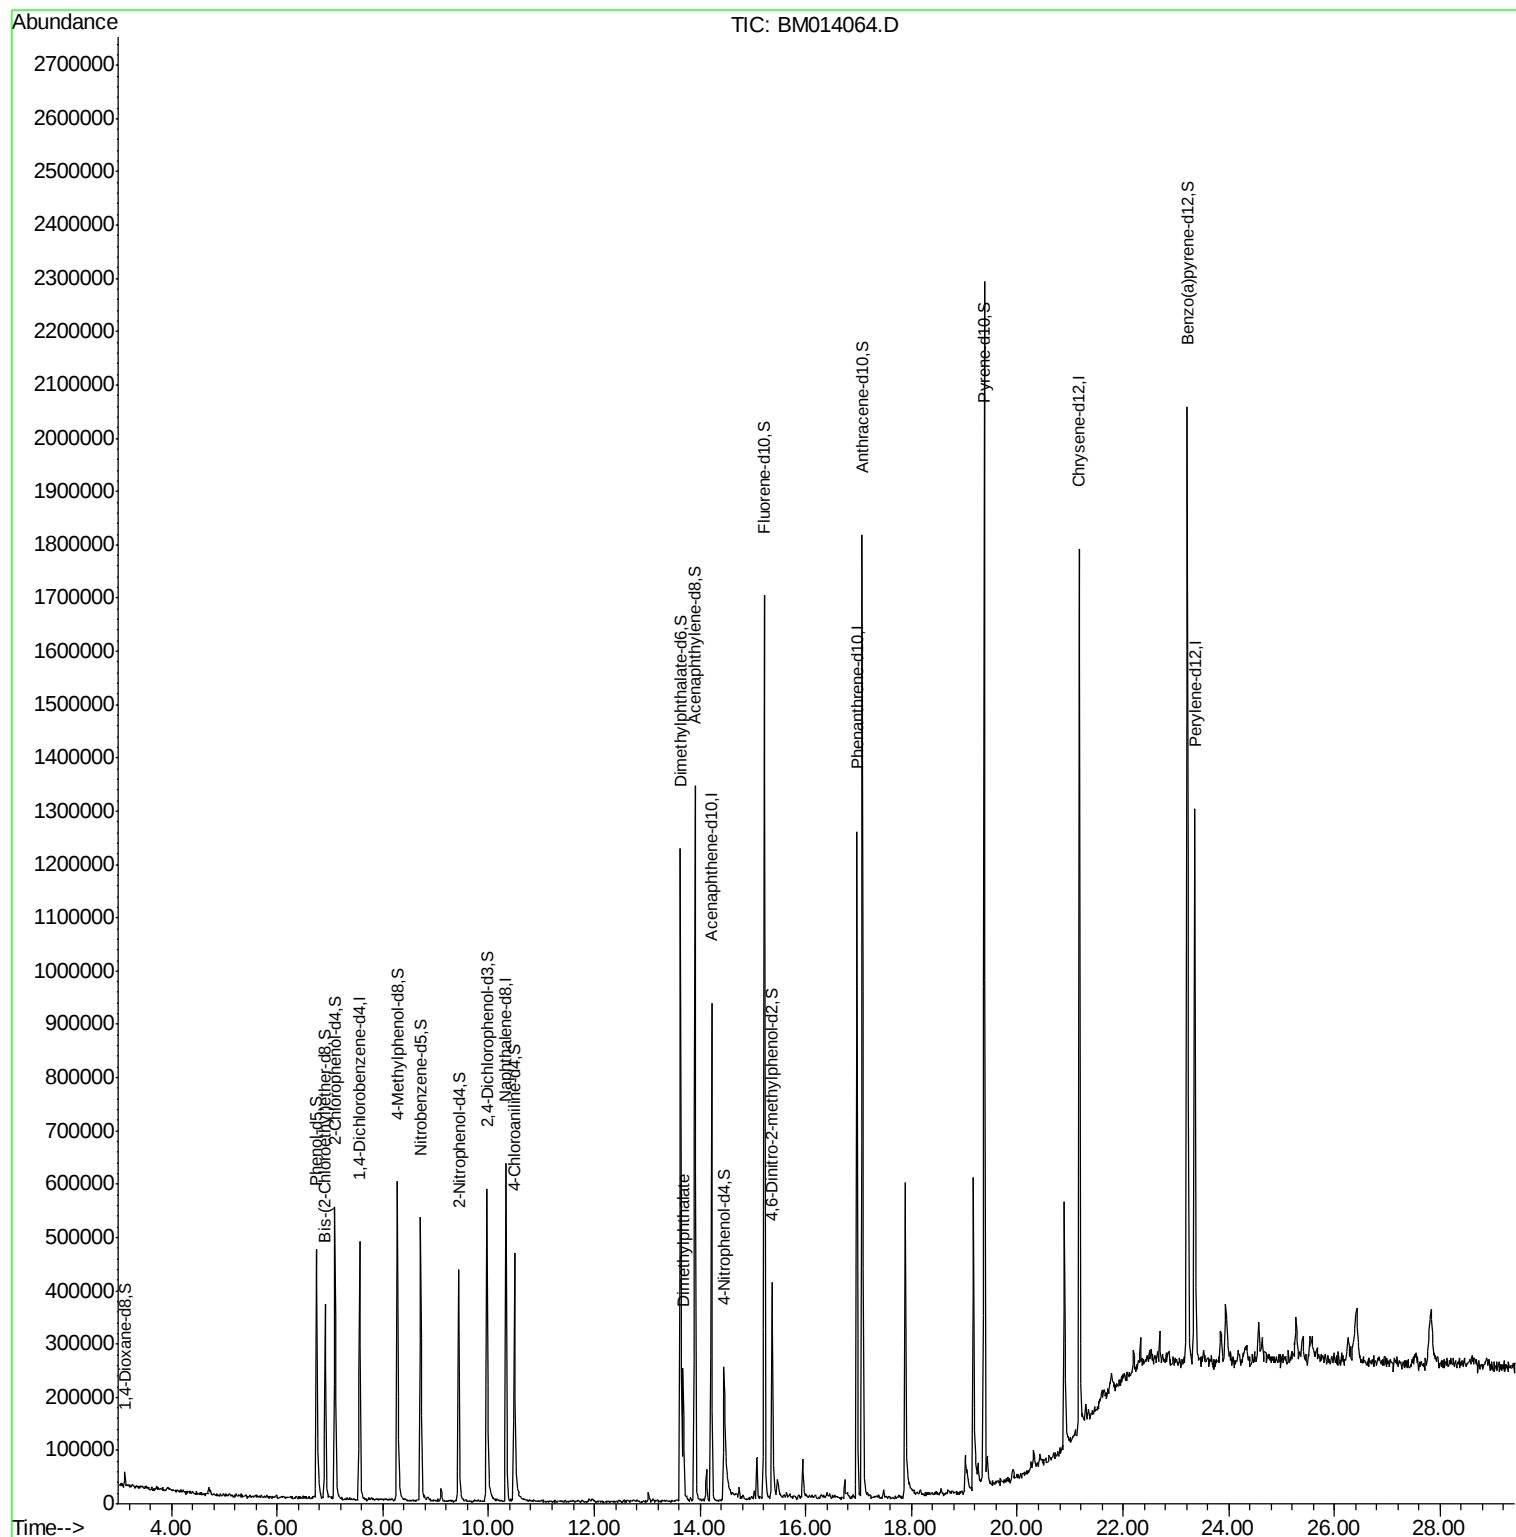

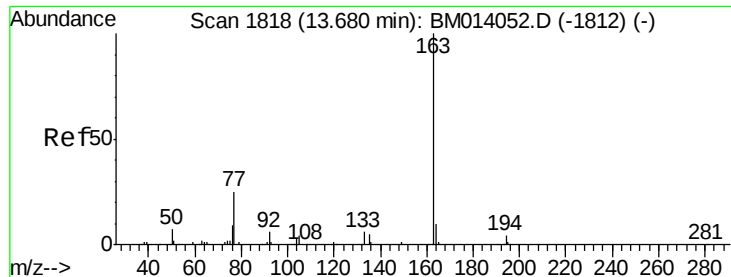

#44
 Dimethylphthalate
 Concen: 6.334 ng/ul
 RT: 13.69 min Scan# 1819
 Delta R.T. 0.01 min
 Lab File: BM014064.D
 Acq: 01 Feb 2018 09:26

Instrument :
 BNA_M
 ClientSampleId :
 F6C88

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.7	3.5	5.3
164	10.8	8.2	12.4

Manual Integrations
 APPROVED

Sohil
 2/1/2018 6:05:31 PM

