
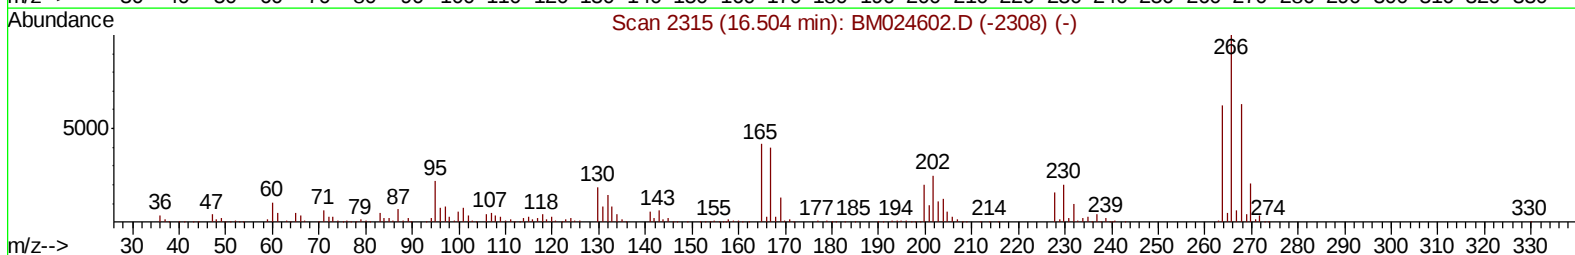
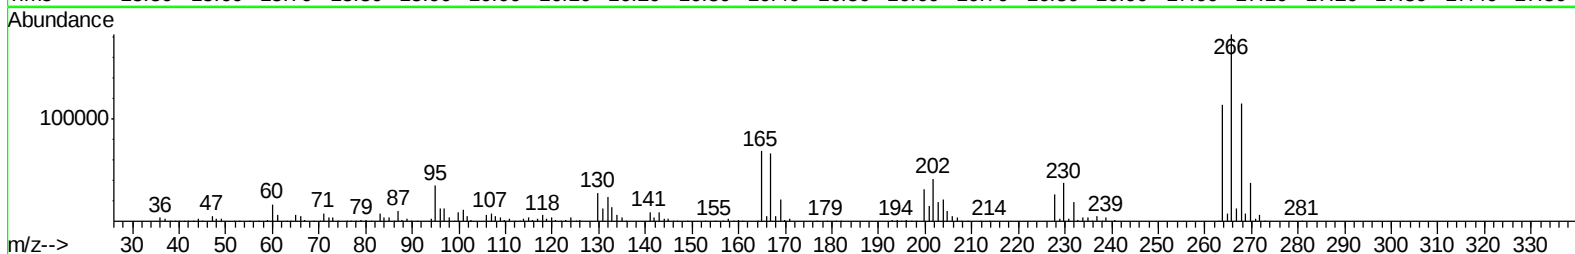


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013120\
 Data File : BM024677.D
 Acq On : 31 Jan 2020 15:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 02:56:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 23 14:57:07 2020
 Response via : Initial Calibration

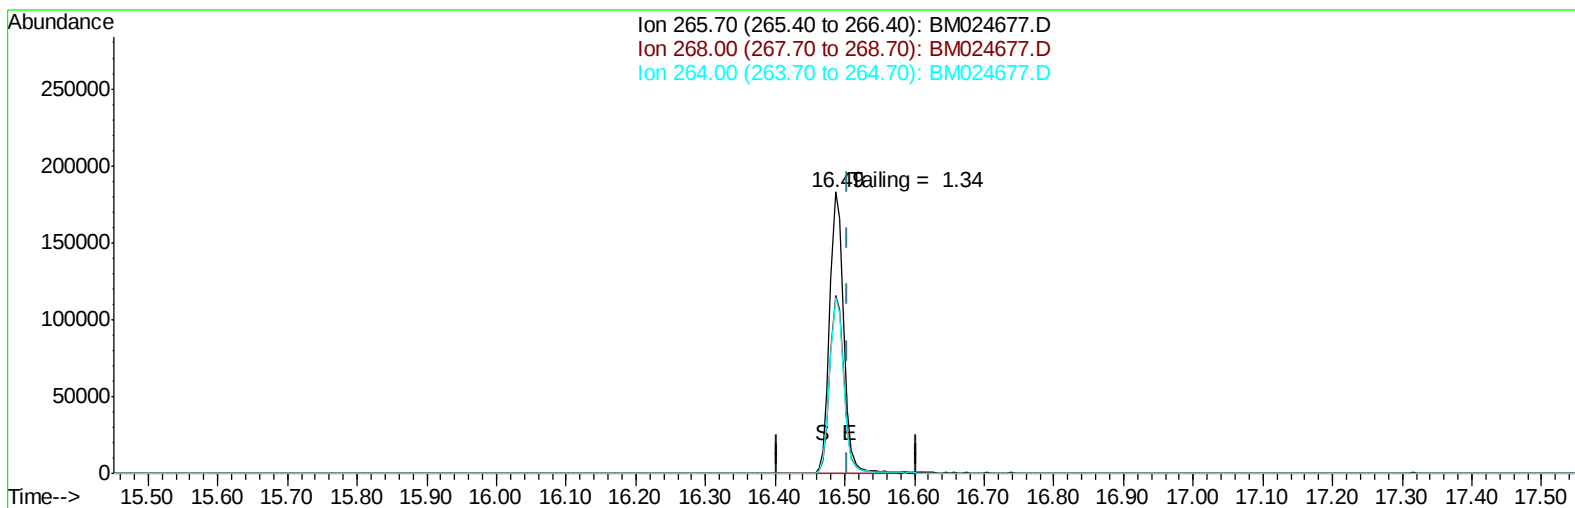

TIC: BM024677.D

(70) Pentachlorophenol (C)




16.486min (-0.018) 13175.58ng

response 254026

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	63.38
264.00	62.40	62.50
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013120\
 Data File : BM024677.D
 Acq On : 31 Jan 2020 15:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 02:56:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 23 14:57:07 2020
 Response via : Initial Calibration

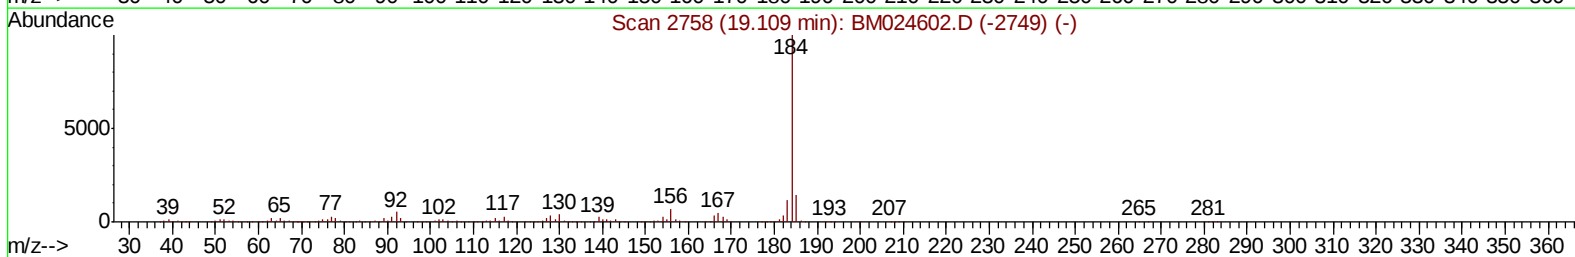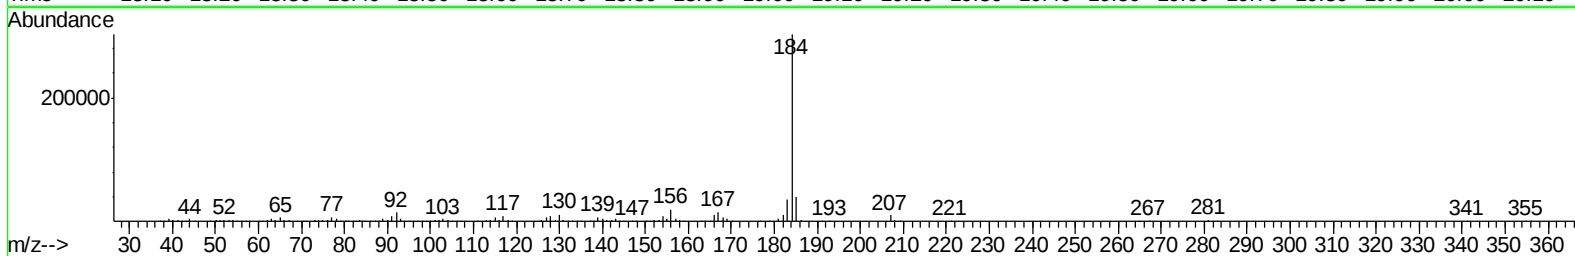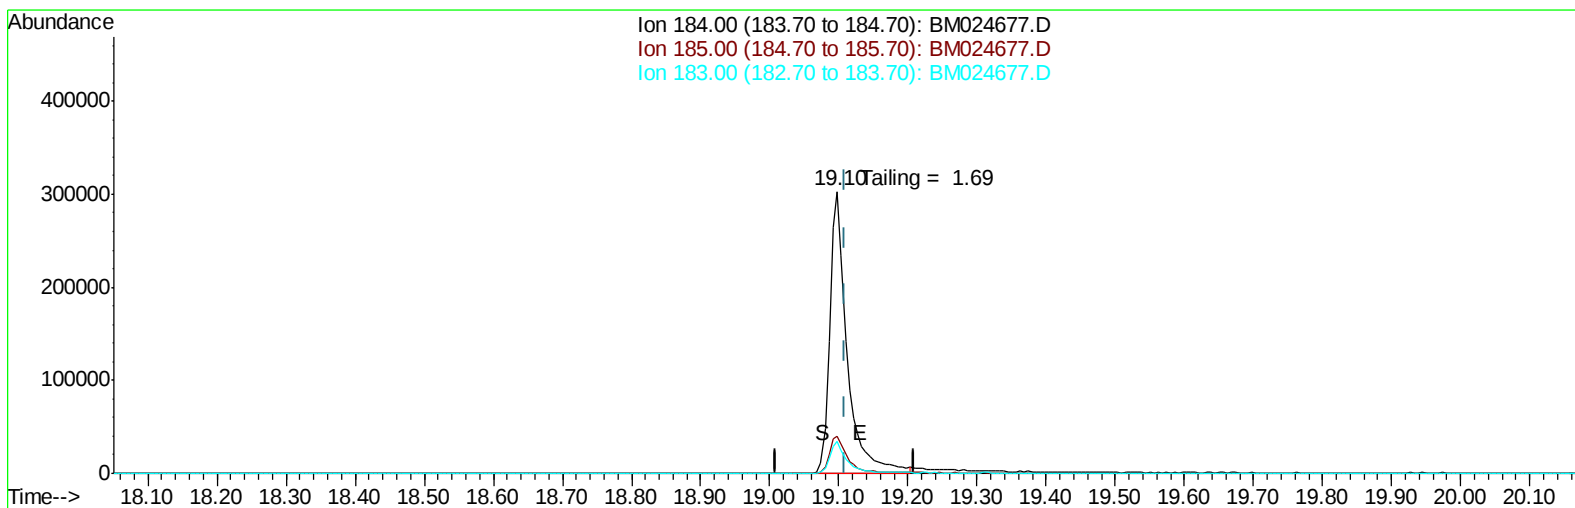

TIC: BM024677.D

(77) Benzidine

19.098min (-0.012) 2912.97ng

response 513542

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.41
183.00	12.00	11.60
0.00	0.00	0.00