


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013120\
 Data File : BM024677.D
 Acq On : 31 Jan 2020 15:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 23 14:57:07 2020

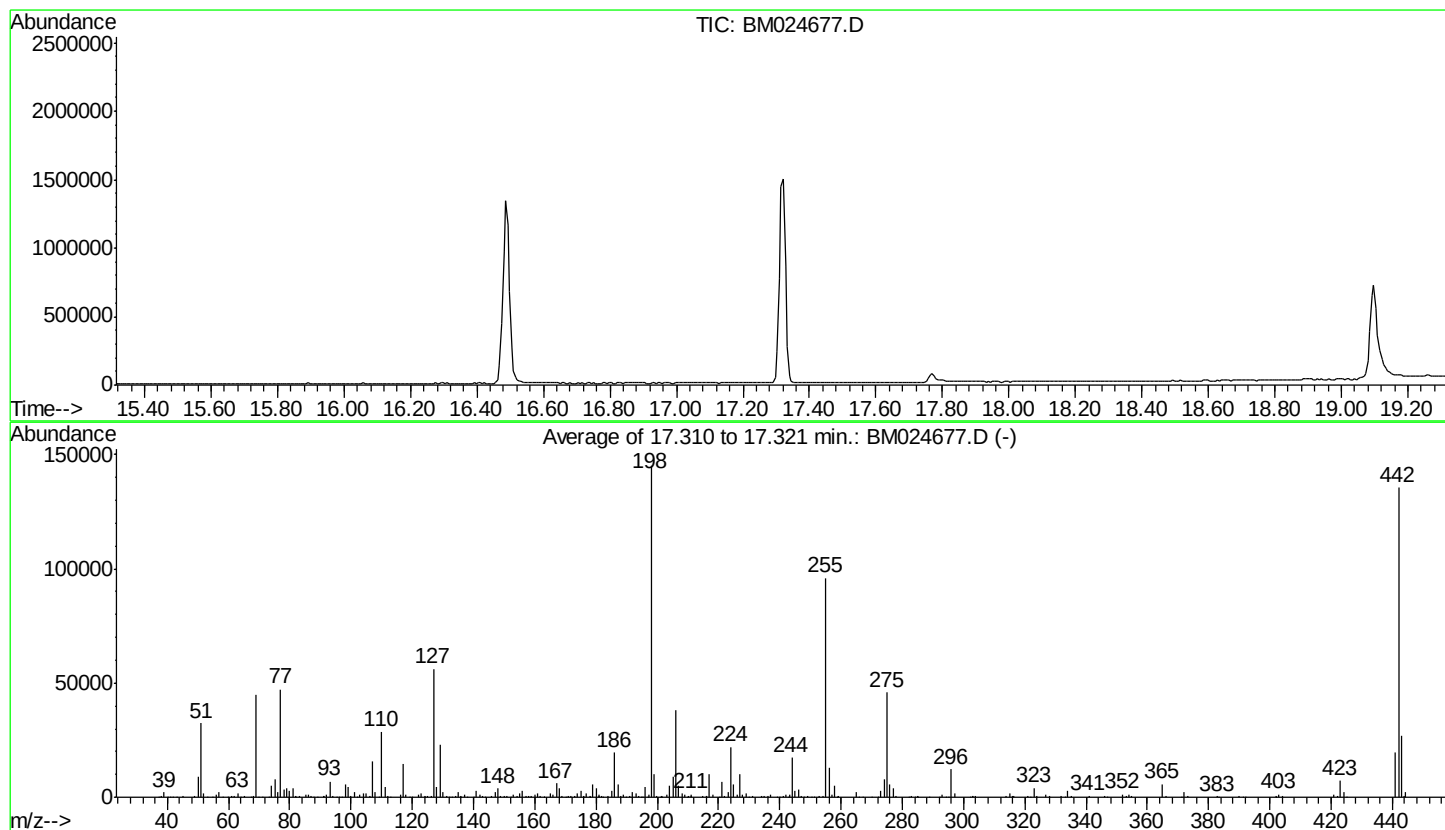

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.2	32298	PASS
68	69	0.00	2	1.7	767	PASS
69	198	0.00	100	31.0	44961	PASS
70	69	0.00	2	0.5	235	PASS
127	198	10	80	38.7	56146	PASS
197	198	0.00	2	0.6	868	PASS
198	198	100	100	100.0	145205	PASS
199	198	5	9	7.0	10121	PASS
275	198	10	60	31.5	45794	PASS
365	198	1	100	4.0	5785	PASS
441	198	0.01	100	13.4	19503	PASS
442	198	50	100	93.4	135645	PASS
443	442	15	24	19.7	26713	PASS