
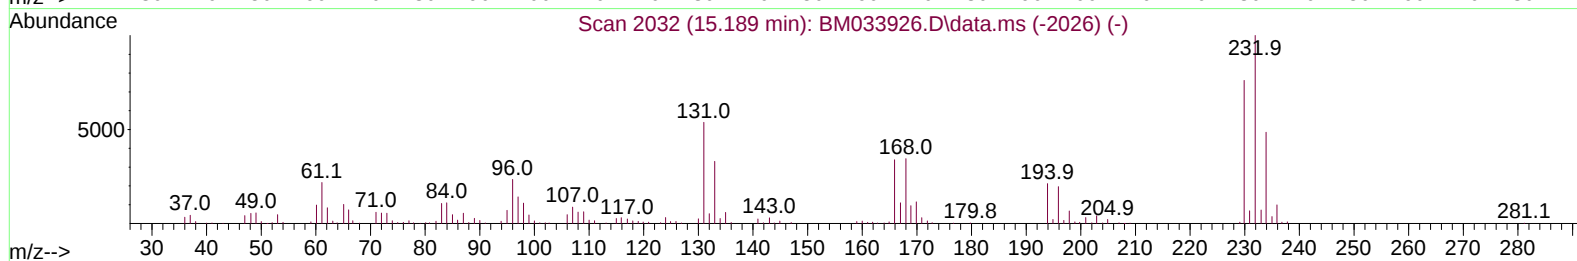
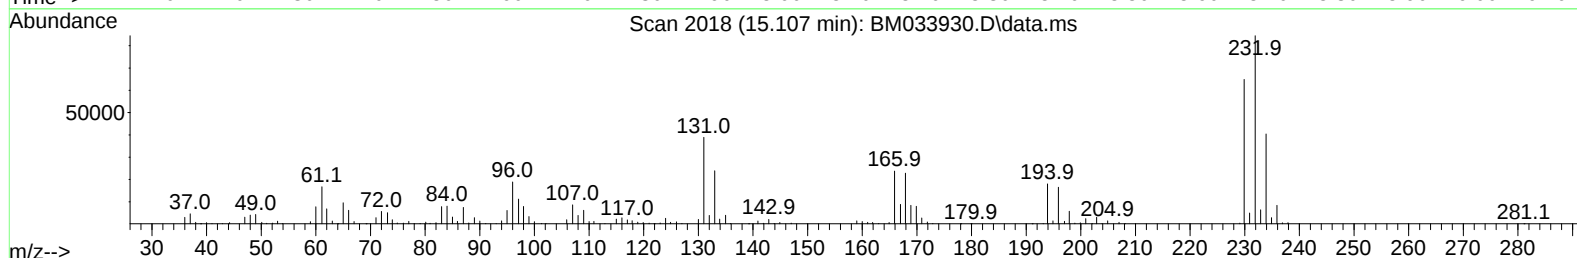


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013122\
Data File : BM033930.D
Acq On : 31 Jan 2022 17:23
Operator : CG/JU
Sample : SSTDICV020
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Feb 01 02:25:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

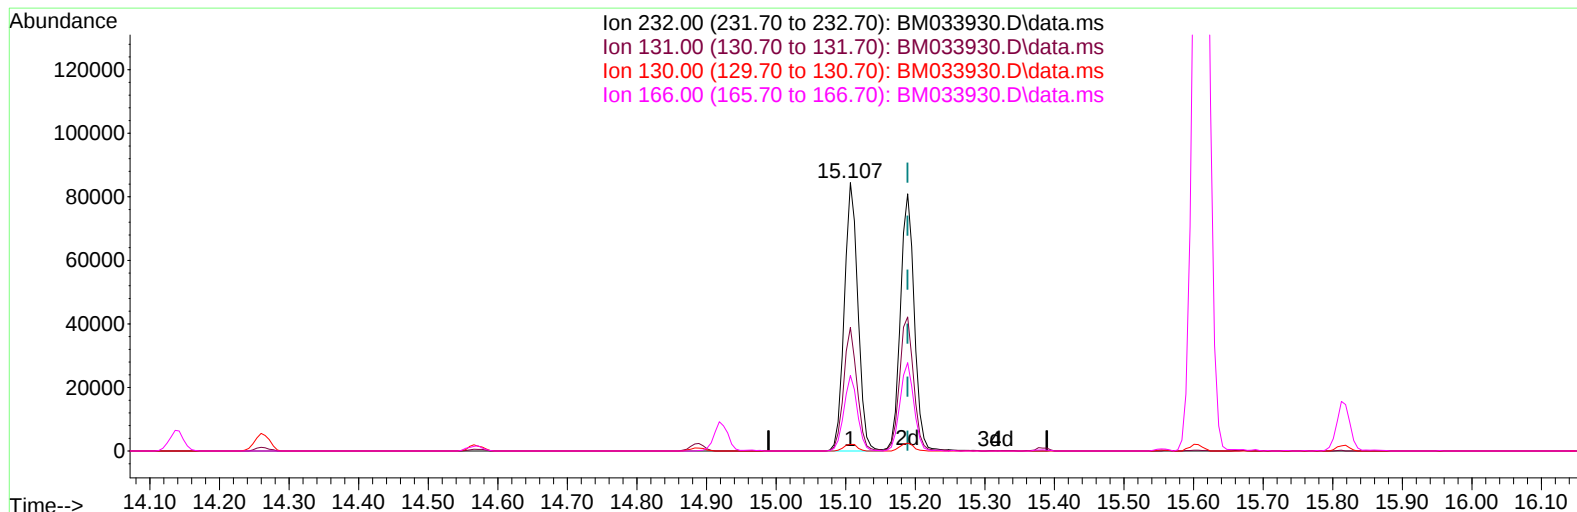

TIC: BM033930.D\data.ms

(58) 2,3,4,6-Tetrachlorophenol

15.107min (-0.082) 22.40 ng/u1

response 114680

Ion	Exp%	Act%
232.00	100.00	100.00
131.00	51.80	46.03
130.00	2.50	2.47
166.00	34.20	28.13