

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013122\
 Data File : BM033926.D
 Acq On : 31 Jan 2022 15:00
 Operator : CG/JU
 Sample : SSTD02027
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020027

Quant Time: Jan 31 16:46:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 16:44:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	117353	20.000	ng/u1	0.00
20) Naphthalene-d8	10.742	136	488605	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.566	164	302798	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.307	188	595115	20.000	ng/u1	0.00
79) Chrysene-d12	21.465	240	509065	20.000	ng/u1	0.00
88) Perylene-d12	23.859	264	467404	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	23966	7.673	ng/uL	0.00
4) Pyridine-d5	3.719	84	168537	19.430	ng/u1	0.00
7) Phenol-d5	7.084	99	201311	19.099	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.254	67	123767	19.282	ng/u1	0.00
11) 2-Chlorophenol-d4	7.460	132	163171	20.248	ng/u1	0.00
15) 4-Methylphenol-d8	8.642	113	159972	18.335	ng/u1	0.00
21) Nitrobenzene-d5	9.095	128	80911	20.969	ng/u1	0.00
24) 2-Nitrophenol-d4	9.819	143	85289	20.856	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	154430	19.698	ng/u1	0.00
31) 4-Chloroaniline-d4	10.872	131	215047	18.453	ng/u1	0.00
46) Dimethylphthalate-d6	13.977	166	455201	19.081	ng/u1	0.00
49) Acenaphthylene-d8	14.260	160	559679	19.886	ng/u1	0.00
54) 4-Nitrophenol-d4	14.754	143	74190	16.204	ng/u1	0.00
60) Fluorene-d10	15.554	176	375529	18.974	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.671	200	69962	19.763	ng/u1	0.00
73) Anthracene-d10	17.401	188	570057	19.741	ng/u1	0.00
81) Pyrene-d10	19.689	212	615719	22.397	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.706	264	505830	20.799	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.325	88	26669	8.179	ng/uL#	88
5) Pyridine	3.737	79	173035	19.452	ng/u1	85
6) Benzaldehyde	7.060	77	133800	21.999	ng/u1	84
8) Phenol	7.113	94	203831	18.824	ng/u1#	84
10) Bis(2-Chloroethyl)ether	7.348	93	163772	19.418	ng/u1	92
12) 2-Chlorophenol	7.490	128	170948	20.195	ng/u1	89
13) 2-Methylphenol	8.372	108	154846	18.597	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.460	45	226212	19.065	ng/u1	97
16) Acetophenone	8.754	105	258743	18.849	ng/u1	89
17) N-Nitroso-di-n-propyla...	8.742	70	131385	18.482	ng/u1#	88
18) 4-Methylphenol	8.701	108	166637	18.310	ng/u1	94
19) Hexachloroethane	9.019	117	73746	20.544	ng/u1#	85
22) Nitrobenzene	9.137	77	195649	19.996	ng/u1#	89
23) Isophorone	9.666	82	356477	19.063	ng/u1	97
25) 2-Nitrophenol	9.848	139	93334	21.154	ng/u1#	83
26) 2,4-Dimethylphenol	9.913	107	203904	19.980	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.148	93	218536	19.498	ng/u1	97
29) 2,4-Dichlorophenol	10.389	162	154681	19.610	ng/u1	95
30) Naphthalene	10.795	128	542662	20.051	ng/u1	99
32) 4-Chloroaniline	10.895	127	217173	18.437	ng/u1	98
33) Hexachlorobutadiene	11.089	225	115000	21.155	ng/u1	99
34) Caprolactam	11.666	113	44951	16.664	ng/u1	84
35) 4-Chloro-3-methylphenol	12.025	107	180479	18.745	ng/u1	88
36) 2-Methylnaphthalene	12.401	142	364436	19.553	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013122\
 Data File : BM033926.D
 Acq On : 31 Jan 2022 15:00
 Operator : CG/JU
 Sample : SST02027
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST020027

Quant Time: Jan 31 16:46:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 16:44:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.619	142	371908	19.370	ng/ul	97
39) 1,2,4,5-Tetrachloroben...	12.772	216	191586	21.174	ng/ul	99
40) Hexachlorocyclopentadiene	12.754	237	130943	22.039	ng/ul	99
41) 2,4,6-Trichlorophenol	13.007	196	120585	20.738	ng/ul	97
42) 2,4,5-Trichlorophenol	13.077	196	128351	19.952	ng/ul	92
43) 1,1'-Biphenyl	13.407	154	479920	20.211	ng/ul	99
44) 2-Chloronaphthalene	13.448	162	364550	20.431	ng/ul	98
45) 2-Nitroaniline	13.642	65	109876	18.928	ng/ul#	83
47) Dimethylphthalate	14.024	163	453975	19.034	ng/ul	99
48) 2,6-Dinitrotoluene	14.142	165	89584	19.595	ng/ul	93
50) Acenaphthylene	14.289	152	594219	19.879	ng/ul	99
51) 3-Nitroaniline	14.466	138	90205	19.200	ng/ul	84
52) Acenaphthene	14.630	153	384571	19.545	ng/ul	98
53) 2,4-Dinitrophenol	14.671	184	48719	17.706	ng/ul	90
55) 4-Nitrophenol	14.766	109	73405	16.549	ng/ul	91
56) Dibenzofuran	14.966	168	545805	19.341	ng/ul	99
57) 2,4-Dinitrotoluene	14.924	165	127131	18.572	ng/ul#	79
58) 2,3,4,6-Tetrachlorophenol	15.189	232	105261	19.306	ng/ul	98
59) Diethylphthalate	15.383	149	464530	18.434	ng/ul	99
61) Fluorene	15.613	166	434108	18.940	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.607	204	221395	19.246	ng/ul	99
63) 4-Nitroaniline	15.618	138	88666	19.589	ng/ul	87
66) 4,6-Dinitro-2-methylph...	15.683	198	69621	19.570	ng/ul	97
67) N-Nitrosodiphenylamine	15.813	169	368236	20.380	ng/ul	98
68) 4-Bromophenyl-phenylether	16.495	248	128315	21.699	ng/ul	96
69) Hexachlorobenzene	16.618	284	147022	20.416	ng/ul	96
70) Atrazine	16.765	200	134198	18.661	ng/ul	99
71) Pentachlorophenol	16.954	266	88939	18.880	ng/ul	97
72) Phenanthrene	17.348	178	666541	19.637	ng/ul	99
74) Anthracene	17.436	178	673654	19.543	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.372	216	205693	22.976	ng/uL	96
76) Pentachlorobenzene	14.889	250	184509	21.942	ng/uL	97
77) Carbazole	17.701	167	588070	19.017	ng/ul	99
78) Di-n-butylphthalate	18.271	149	738673	18.969	ng/ul	99
80) Fluoranthene	19.354	202	732492	22.415	ng/ul	99
82) Pyrene	19.712	202	753034	22.290	ng/ul	99
83) Butylbenzylphthalate	20.606	149	304982	20.868	ng/ul	87
84) 3,3'-Dichlorobenzidine	21.383	252	214531	18.942	ng/ul	97
85) Benzo(a)anthracene	21.453	228	657538	19.729	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.383	149	438518	19.131	ng/ul	100
87) Chrysene	21.506	228	650051	20.090	ng/ul	98
89) Di-n-octyl phthalate	22.300	149	699402	18.246	ng/ul	100
90) Benzo(b)fluoranthene	23.130	252	648775	20.437	ng/ul	100
91) Benzo(k)fluoranthene	23.177	252	605610	20.496	ng/ul	99
93) Benzo(a)pyrene	23.753	252	613453	20.663	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.359	276	712579	23.850	ng/ul	96
95) Dibenzo(a,h)anthracene	26.371	278	622493	24.178	ng/ul	98
96) Benzo(g,h,i)perylene	27.124	276	598589	24.551	ng/ul	98





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 8.179 ng/uL
RT: 3.325 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion: 88 Resp: 26669
Ion Ratio Lower Upper
88 100
43 33.6 36.2 54.4#
58 78.0 68.5 102.7

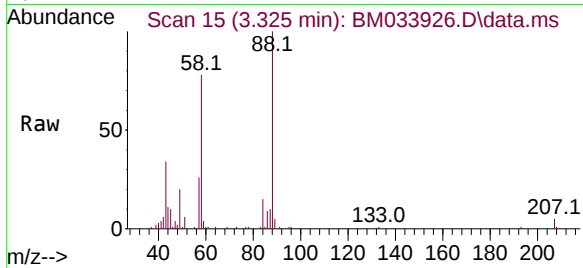

#5
Pyridine
Concen: 19.452 ng/uL
RT: 3.737 min Scan# 85
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion: 79 Resp: 173035
Ion Ratio Lower Upper
79 100
52 79.8 78.1 117.1
51 40.5 36.0 54.0




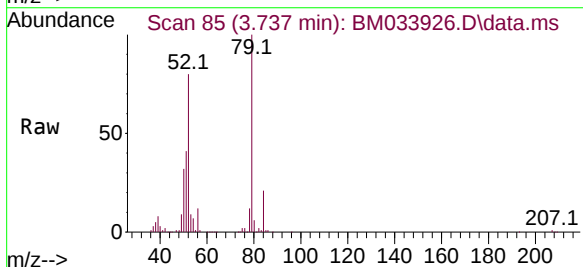




#6
Benzaldehyde
Concen: 21.999 ng/ul
RT: 7.060 min Scan# 650
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion: 77 Resp: 133800
Ion Ratio Lower Upper
77 100
105 96.7 65.6 98.4
106 89.5 60.6 90.8

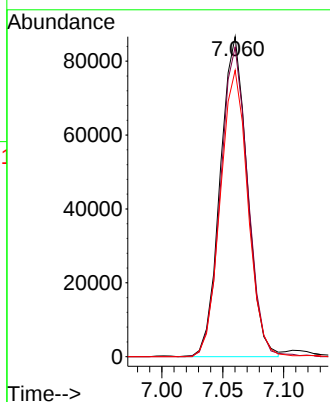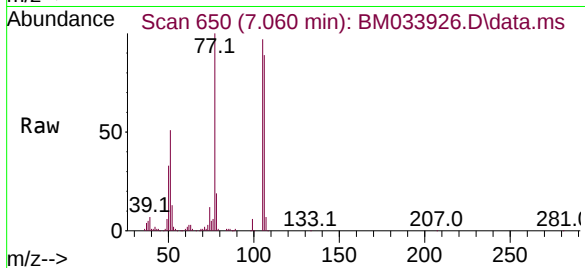

#8
Phenol
Concen: 18.824 ng/ul
RT: 7.113 min Scan# 659
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion: 94 Resp: 203831
Ion Ratio Lower Upper
94 100
65 31.0 31.7 47.5#
66 44.3 45.4 68.0#




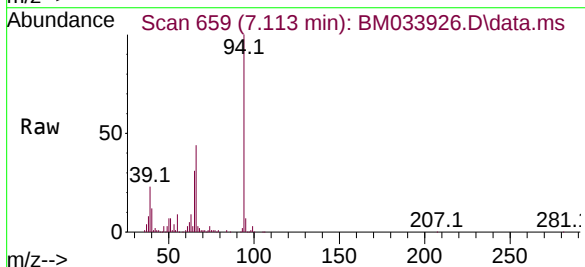




#10
Bis(2-Chloroethyl)ether
Concen: 19.418 ng/ul
RT: 7.348 min Scan# 699
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion: 93 Resp: 163772
Ion Ratio Lower Upper
93 100
63 79.0 71.7 107.5
95 32.4 26.3 39.5

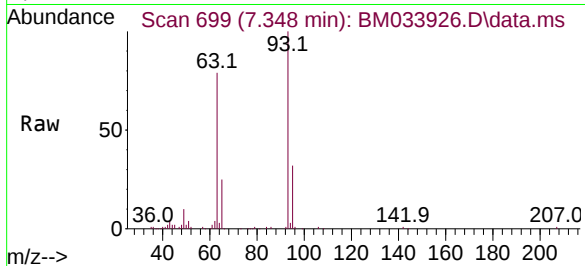

#12
2-Chlorophenol
Concen: 20.195 ng/ul
RT: 7.490 min Scan# 723
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion: 128 Resp: 170948
Ion Ratio Lower Upper
128 100
64 49.9 49.4 74.2
130 31.7 26.8 40.2

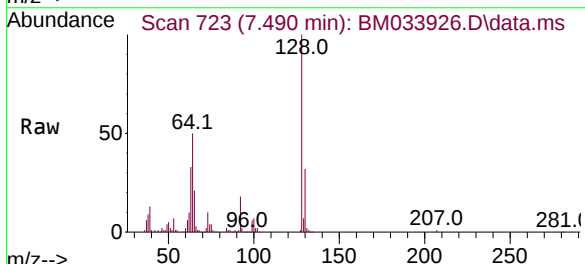



#13

2-Methylphenol

Concen: 18.597 ng/ul

RT: 8.372 min Scan# 873

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00

Instrument :

BNA_M

ClientSampleId :





SSTD020027

Tgt Ion:108 Resp: 154846

Ion Ratio Lower Upper

108 100

107 90.3 70.2 105.4

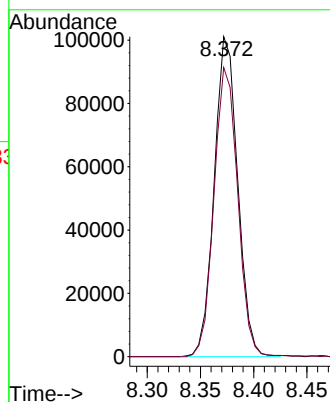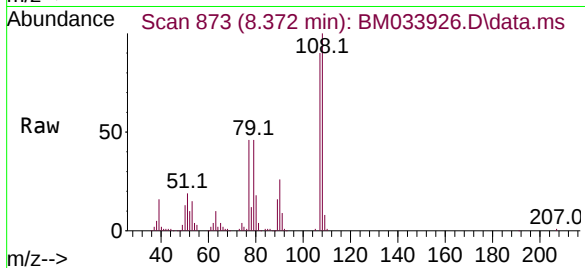

#14

2,2'-oxybis(1-Chloropropane)

Concen: 19.065 ng/ul

RT: 8.460 min Scan# 888

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00




Tgt Ion: 45 Resp: 226212


Ion Ratio Lower Upper

45 100

77 14.5 9.9 14.9

79 10.7 8.3 12.5




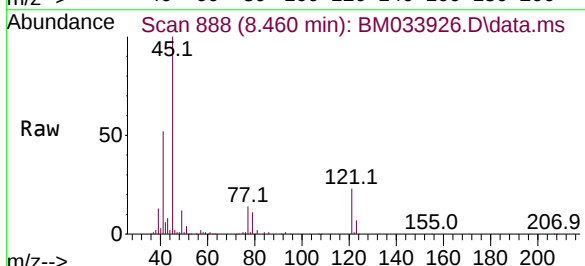




#16
 Acetophenone
 Concen: 18.849 ng/ul
 RT: 8.754 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BM033926.D
 Acq: 31 Jan 2022 15:00




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020027


Tgt Ion:105 Resp: 258743
 Ion Ratio Lower Upper
 105 100
 77 80.9 73.1 109.7
 51 30.7 30.5 45.7

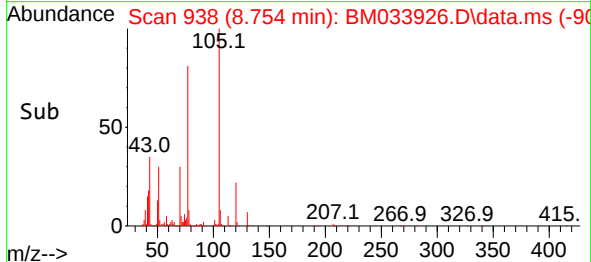

#17
 N-Nitroso-di-n-propylamine
 Concen: 18.482 ng/ul
 RT: 8.742 min Scan# 936
 Delta R.T. 0.000 min
 Lab File: BM033926.D
 Acq: 31 Jan 2022 15:00

Tgt Ion: 70 Resp: 131385
 Ion Ratio Lower Upper
 70 100
 42 60.4 56.9 85.3
 101 10.5 6.9 10.3#
 130 21.3 13.8 20.8#


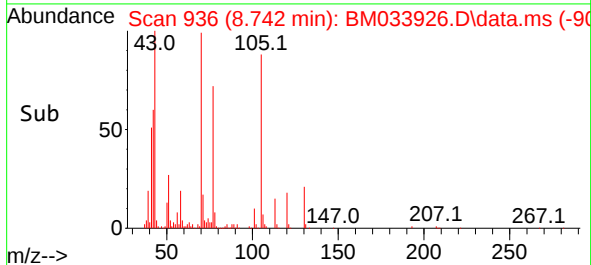






#18
4-Methylphenol
Concen: 18.310 ng/ul
RT: 8.701 min Scan# 91
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:108 Resp: 166637
Ion Ratio Lower Upper
108 100
107 115.3 87.4 131.2

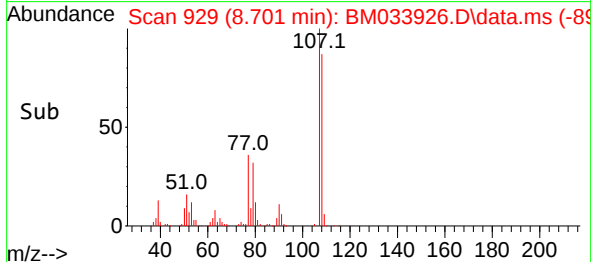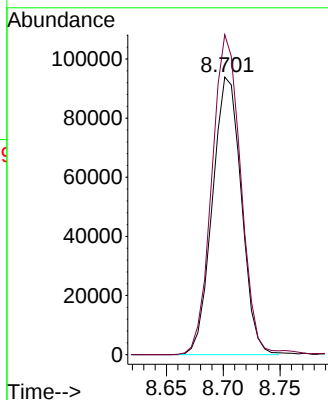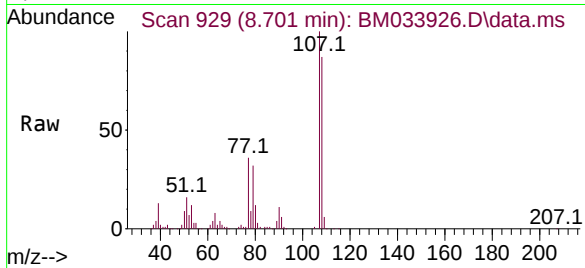

#19
Hexachloroethane
Concen: 20.544 ng/ul
RT: 9.019 min Scan# 983
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:117 Resp: 73746
Ion Ratio Lower Upper
117 100
201 98.6 69.6 104.4
199 63.3 40.6 60.8#



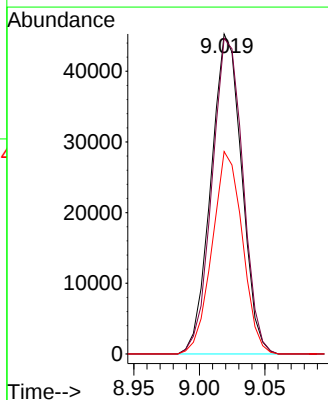
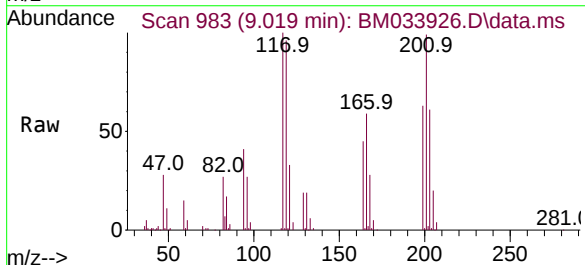




#22
Nitrobenzene
Concen: 19.996 ng/ul
RT: 9.137 min Scan# 1003
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion: 77 Resp: 195649
Ion Ratio Lower Upper
77 100
123 45.2 29.0 43.6#
65 14.5 11.4 17.2



#23
Isophorone
Concen: 19.063 ng/ul
RT: 9.666 min Scan# 1093
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion: 82 Resp: 356477
Ion Ratio Lower Upper
82 100
95 7.8 6.5 9.7
138 16.4 11.8 17.8







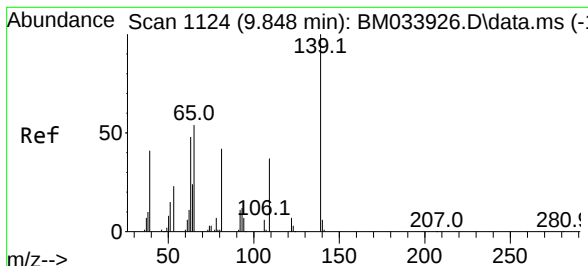

#25
2-Nitrophenol
Concen: 21.154 ng/ul
RT: 9.848 min Scan# 1124
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:139 Resp: 93334
Ion Ratio Lower Upper
139 100
65 56.8 59.0 88.6#
109 37.7 37.2 55.8

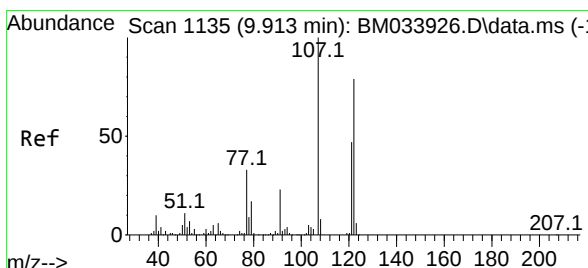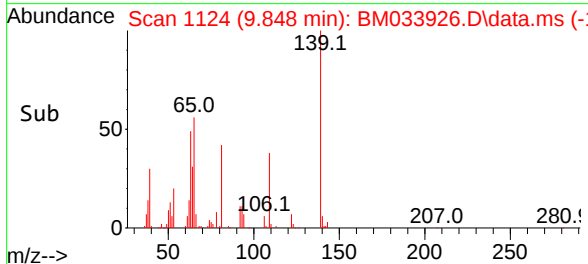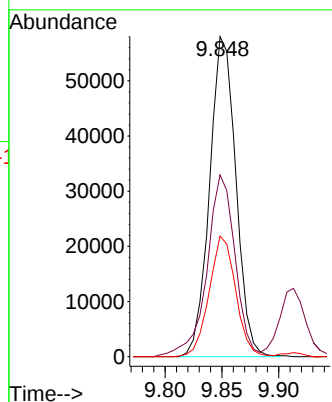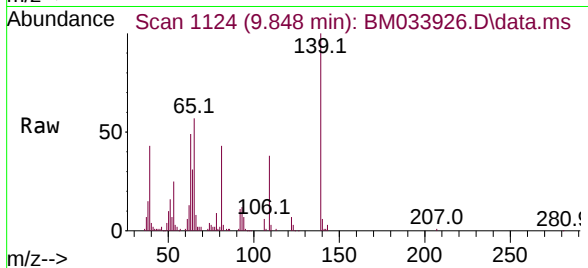

#26
2,4-Dimethylphenol
Concen: 19.980 ng/ul
RT: 9.913 min Scan# 1135
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:107 Resp: 203904
Ion Ratio Lower Upper
107 100
121 46.6 34.8 52.2
122 79.9 60.0 90.0


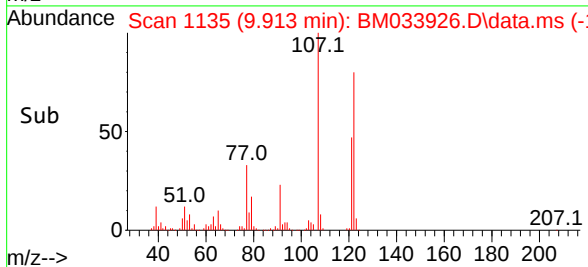
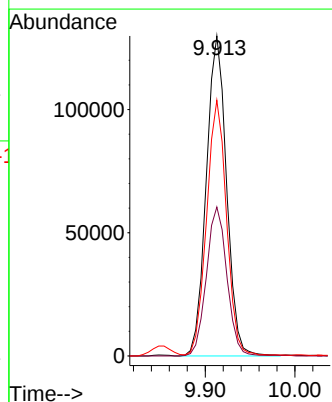
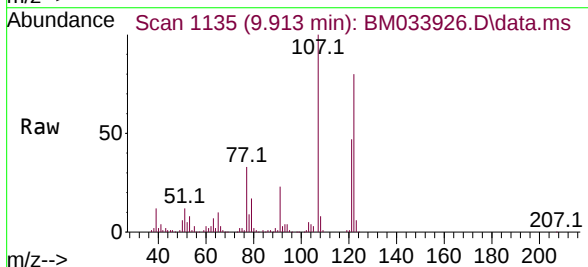




#27
 Bis(2-Chloroethoxy)methane
 Concen: 19.498 ng/ul
 RT: 10.148 min Scan# 1175
 Delta R.T. 0.000 min
 Lab File: BM033926.D
 Acq: 31 Jan 2022 15:00




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020027


Tgt Ion:	93	Resp:	218536
Ion	Ratio	Lower	Upper
93	100		
95	33.6	25.3	37.9
123	11.0	7.9	11.9

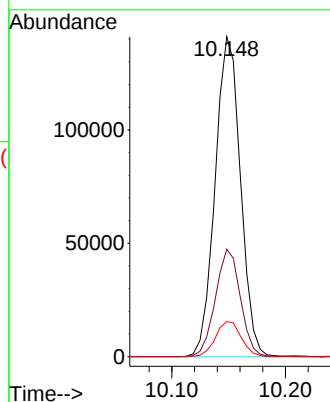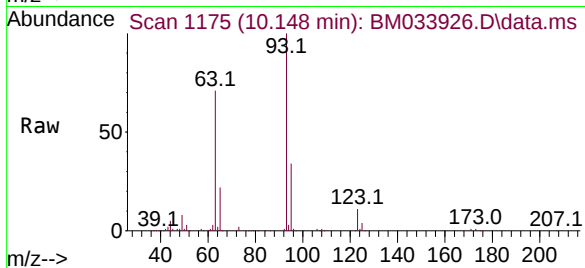

#29
 2,4-Dichlorophenol
 Concen: 19.610 ng/ul
 RT: 10.389 min Scan# 1216
 Delta R.T. 0.000 min
 Lab File: BM033926.D
 Acq: 31 Jan 2022 15:00

Tgt Ion:	162	Resp:	154681
Ion	Ratio	Lower	Upper
162	100		
164	68.1	50.0	75.0
98	39.1	30.6	45.8


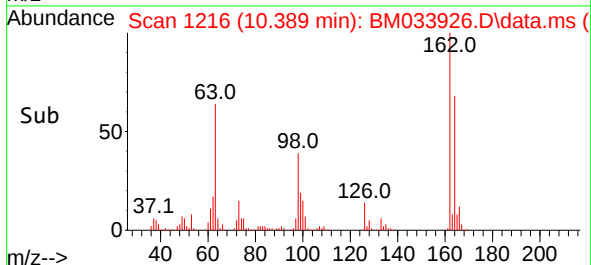

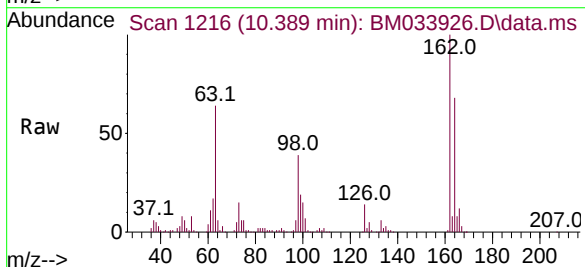




#30
Naphthalene
Concen: 20.051 ng/ul
RT: 10.795 min Scan# 1285
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:128 Resp: 542662
Ion Ratio Lower Upper
128 100
129 10.8 9.1 13.7
127 13.3 10.2 15.4

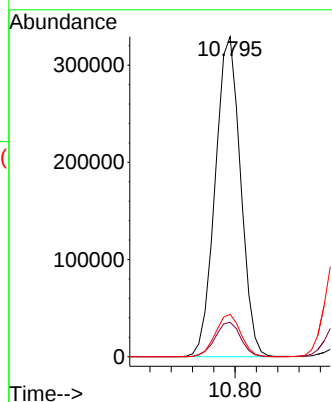

#32
4-Chloroaniline
Concen: 18.437 ng/ul
RT: 10.895 min Scan# 1302
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:127 Resp: 217173
Ion Ratio Lower Upper
127 100
129 33.0 25.4 38.0



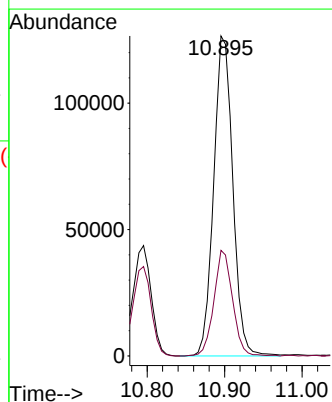





#33
Hexachlorobutadiene
Concen: 21.155 ng/ul
RT: 11.089 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:225 Resp: 115000
Ion Ratio Lower Upper
225 100
223 64.2 52.2 78.2
227 65.0 52.8 79.2

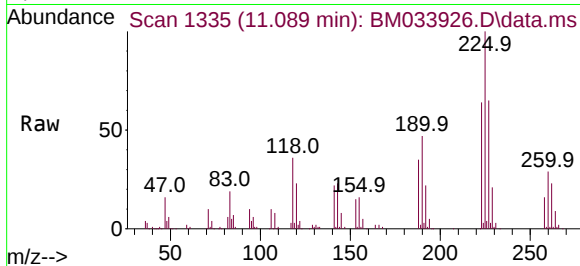

#34
Caprolactam
Concen: 16.664 ng/ul
RT: 11.666 min Scan# 1433
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:113 Resp: 44951
Ion Ratio Lower Upper
113 100
55 173.1 157.9 236.9
56 143.5 131.8 197.6




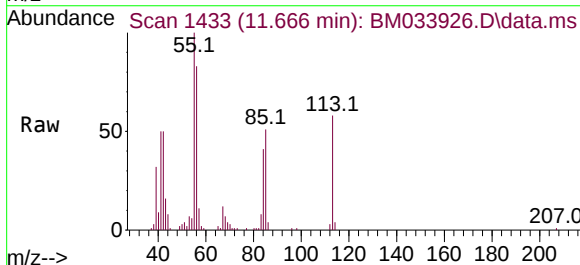




#35
4-Chloro-3-methylphenol
Concen: 18.745 ng/ul
RT: 12.025 min Scan# 1494
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:107 Resp: 180479
Ion Ratio Lower Upper
107 100
144 24.3 17.1 25.7
142 72.7 49.4 74.2

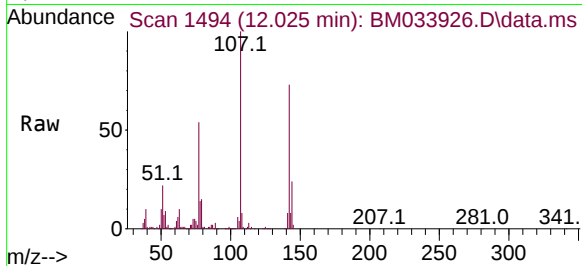

#36
2-Methylnaphthalene
Concen: 19.553 ng/ul
RT: 12.401 min Scan# 1558
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:142 Resp: 364436
Ion Ratio Lower Upper
142 100
141 89.6 71.1 106.7

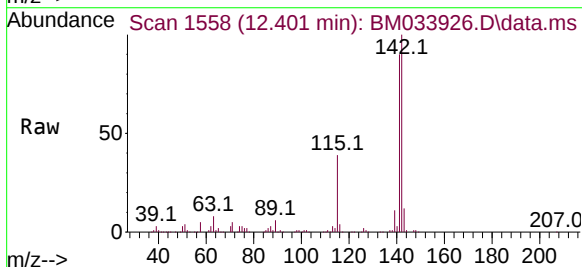



#37

1-Methylnaphthalene

Concen: 19.370 ng/ul

RT: 12.619 min Scan# 1595

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00

Instrument :

BNA_M

ClientSampleId :

SSTD020027





Tgt Ion:142 Resp: 371908

Ion Ratio Lower Upper

142 100

141 91.3 75.5 113.3

116 4.5 4.0 6.0

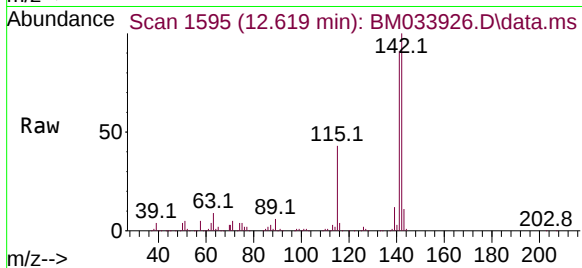

#39

1,2,4,5-Tetrachlorobenzene

Concen: 21.174 ng/ul

RT: 12.772 min Scan# 1621

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00

Tgt Ion:216 Resp: 191586




Ion Ratio Lower Upper


216 100

214 76.9 61.3 91.9

179 21.5 18.0 27.0

108 18.6 16.6 25.0



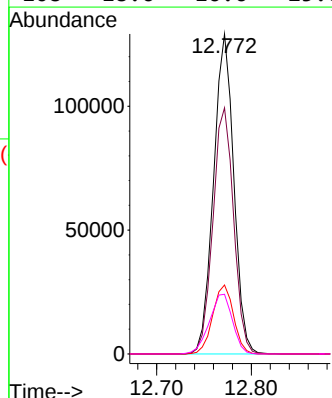
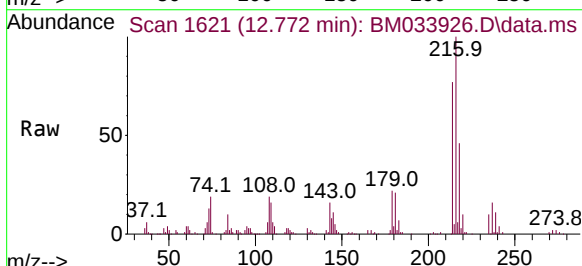




#40
Hexachlorocyclopentadiene
Concen: 22.039 ng/ul
RT: 12.754 min Scan# 1618
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:237 Resp: 130943
Ion Ratio Lower Upper
237 100
235 62.8 50.6 76.0
272 12.9 9.6 14.4

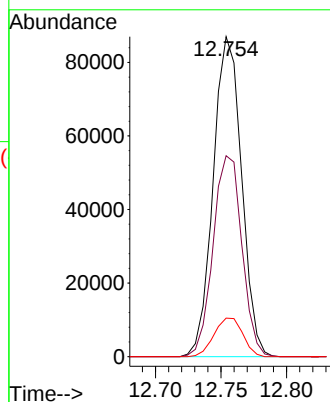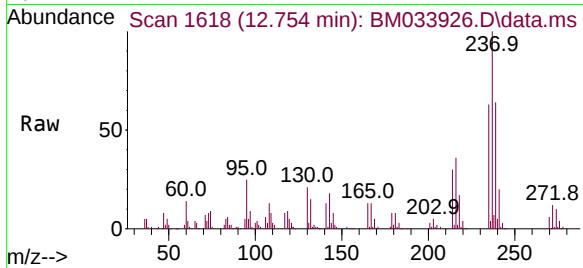

#41
2,4,6-Trichlorophenol
Concen: 20.738 ng/ul
RT: 13.007 min Scan# 1661
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:196 Resp: 120585
Ion Ratio Lower Upper
196 100
198 96.0 78.9 118.3
200 31.0 23.7 35.5




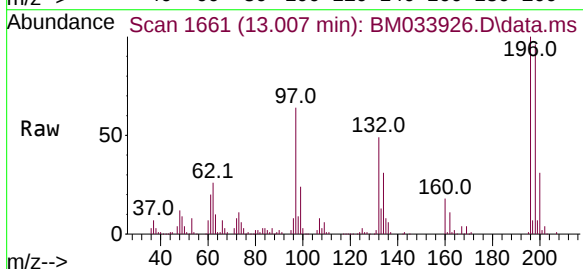




#42
2,4,5-Trichlorophenol
Concen: 19.952 ng/ul
RT: 13.077 min Scan# 1
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:196 Resp: 128351
Ion Ratio Lower Upper
196 100
198 95.5 82.2 123.2
200 29.6 27.9 41.9

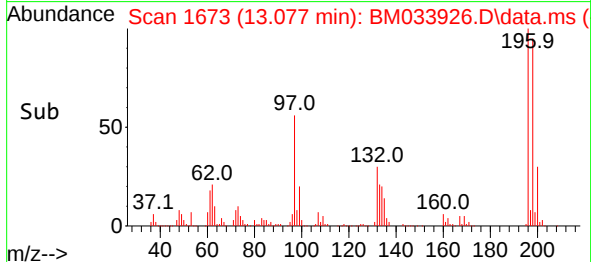

#43
1,1'-Biphenyl
Concen: 20.211 ng/ul
RT: 13.407 min Scan# 1729
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:154 Resp: 479920
Ion Ratio Lower Upper
154 100
153 41.0 33.1 49.7
76 12.6 10.7 16.1



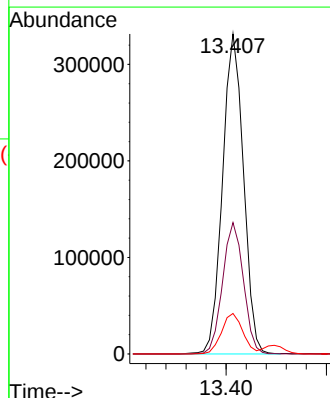





#44
2-Chloronaphthalene
Concen: 20.431 ng/ul
RT: 13.448 min Scan# 1736
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:162 Resp: 364550
Ion Ratio Lower Upper
162 100
164 32.9 26.2 39.4
127 44.0 33.7 50.5

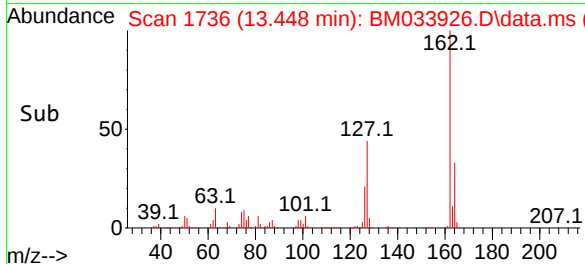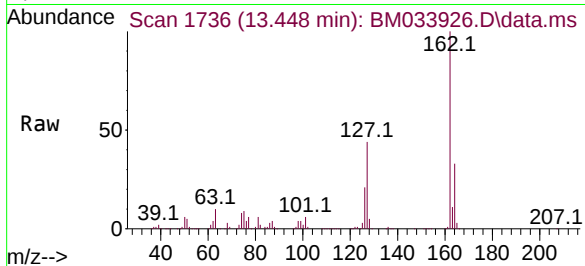

#45
2-Nitroaniline
Concen: 18.928 ng/ul
RT: 13.642 min Scan# 1769
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion: 65 Resp: 109876
Ion Ratio Lower Upper
65 100
92 66.8 47.8 71.6
138 95.5 61.0 91.6#


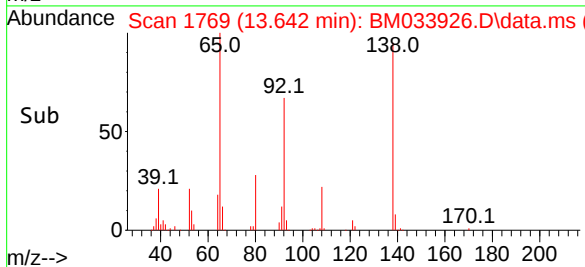

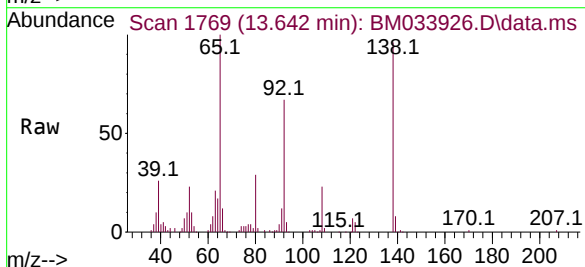




#47
Dimethylphthalate
Concen: 19.034 ng/ul
RT: 14.024 min Scan# 1834
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:163 Resp: 453975
Ion Ratio Lower Upper
163 100
194 3.8 3.3 4.9
164 10.0 8.2 12.2



#48
2,6-Dinitrotoluene
Concen: 19.595 ng/ul
RT: 14.142 min Scan# 1854
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:165 Resp: 89584
Ion Ratio Lower Upper
165 100
89 62.9 55.7 83.5
121 22.5 20.0 30.0









#50
Acenaphthylene
Concen: 19.879 ng/ul
RT: 14.289 min Scan# 1879
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:152 Resp: 594219
Ion Ratio Lower Upper
152 100
151 19.9 15.8 23.8
153 13.1 10.1 15.1

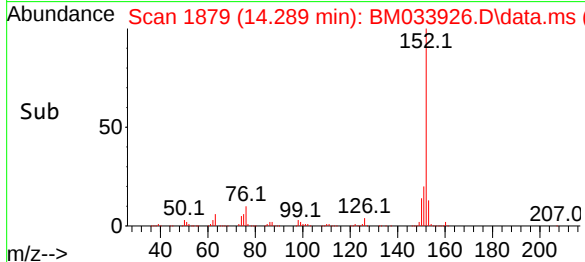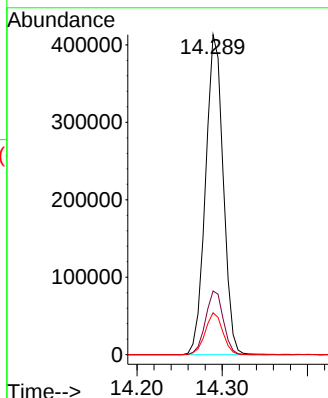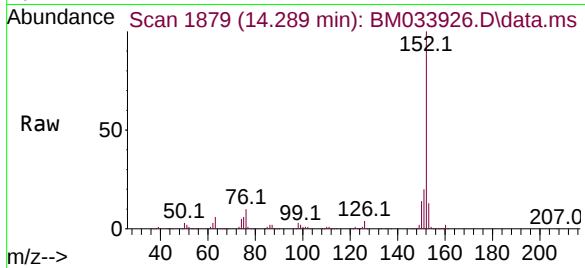

#51
3-Nitroaniline
Concen: 19.200 ng/ul
RT: 14.466 min Scan# 1909
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:138 Resp: 90205
Ion Ratio Lower Upper
138 100
108 11.9 10.8 16.2
92 117.1 110.6 166.0


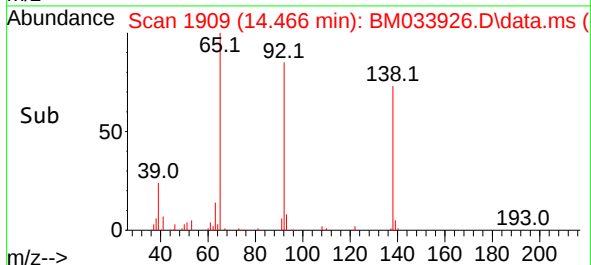
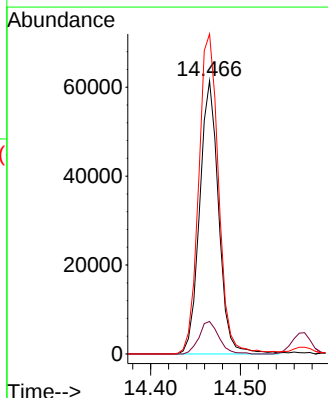
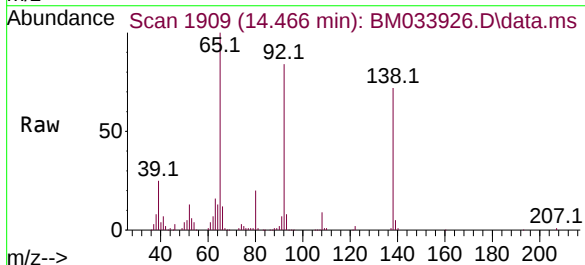




#52
Acenaphthene
Concen: 19.545 ng/ul
RT: 14.630 min Scan# 1937
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:153 Resp: 384571
Ion Ratio Lower Upper
153 100
152 47.8 39.4 59.2
154 89.3 72.7 109.1

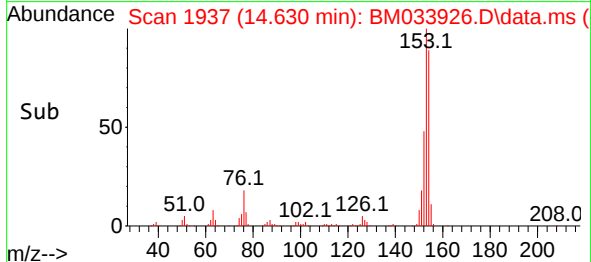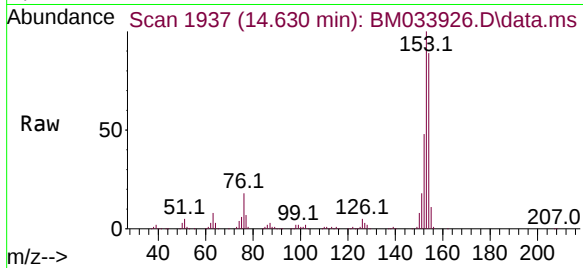

#53
2,4-Dinitrophenol
Concen: 17.706 ng/ul
RT: 14.671 min Scan# 1944
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:184 Resp: 48719
Ion Ratio Lower Upper
184 100
63 78.5 73.8 110.8
154 75.9 63.5 95.3




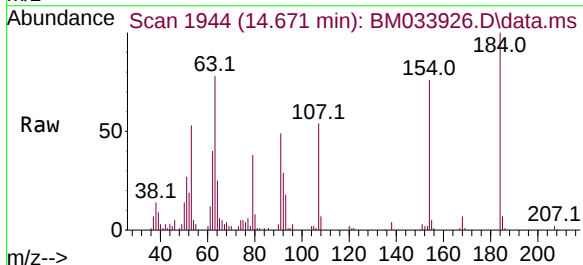




#55
4-Nitrophenol
Concen: 16.549 ng/ul
RT: 14.766 min Scan# 1960
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:109 Resp: 73405
Ion Ratio Lower Upper
109 100
139 102.0 77.6 116.4
65 125.2 112.2 168.4

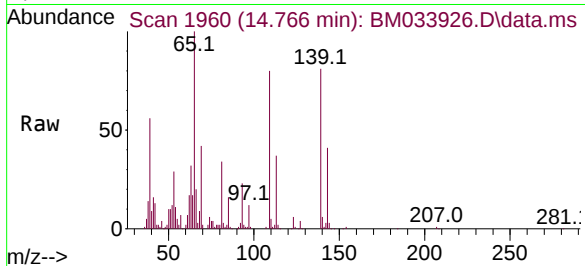

#56
Dibenzofuran
Concen: 19.341 ng/ul
RT: 14.966 min Scan# 1994
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:168 Resp: 545805
Ion Ratio Lower Upper
168 100
139 42.0 34.0 51.0




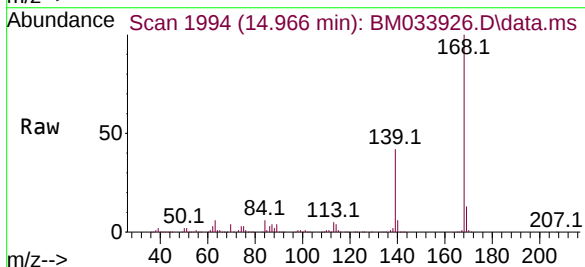




#57
2,4-Dinitrotoluene
Concen: 18.572 ng/ul
RT: 14.924 min Scan# 1987
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:165 Resp: 127131
Ion Ratio Lower Upper
165 100
63 47.2 51.8 77.8#
182 2.6 2.6 4.0#

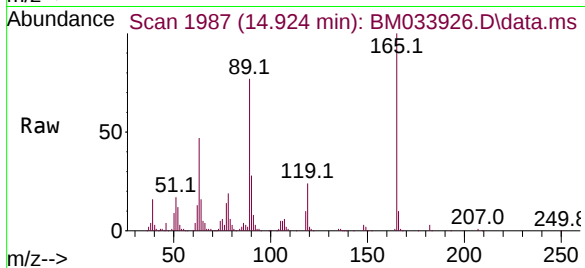

#58
2,3,4,6-Tetrachlorophenol
Concen: 19.306 ng/ul
RT: 15.189 min Scan# 2032
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:232 Resp: 105261
Ion Ratio Lower Upper
232 100
131 53.8 41.4 62.2
130 2.5 2.0 3.0
166 33.9 27.4 41.0




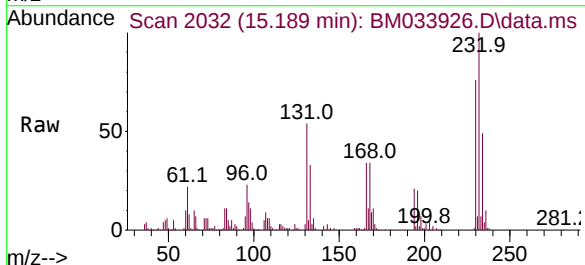




#59
Diethylphthalate
Concen: 18.434 ng/ul
RT: 15.383 min Scan# 2065
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:149 Resp: 464530
Ion Ratio Lower Upper
149 100
177 20.9 17.1 25.7
150 13.0 9.9 14.9

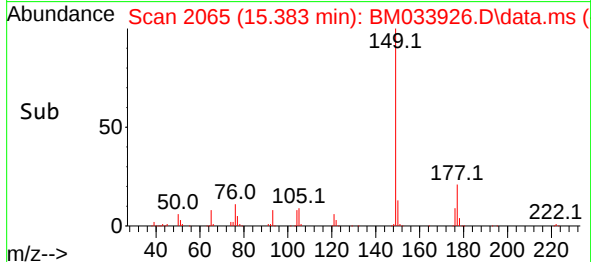

#61
Fluorene
Concen: 18.940 ng/ul
RT: 15.613 min Scan# 2104
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:166 Resp: 434108
Ion Ratio Lower Upper
166 100
165 100.3 77.9 116.9
167 13.9 10.3 15.5




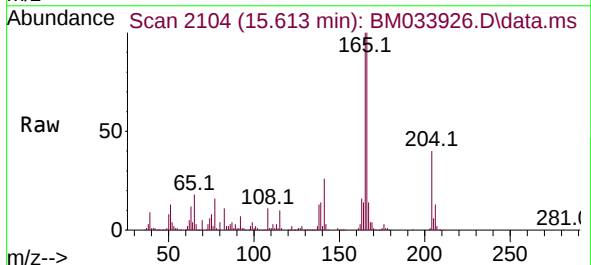




#62
4-Chlorophenyl-phenylether
Concen: 19.246 ng/ul
RT: 15.607 min Scan# 2103
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:204 Resp: 221395
Ion Ratio Lower Upper
204 100
206 32.9 27.8 41.8
141 68.6 54.9 82.3

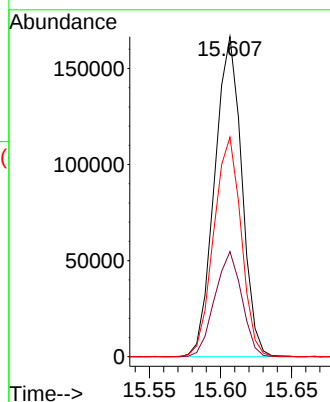

#63
4-Nitroaniline
Concen: 19.589 ng/ul
RT: 15.618 min Scan# 2105
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:138 Resp: 88666
Ion Ratio Lower Upper
138 100
92 53.2 48.0 72.0
108 95.2 89.5 134.3


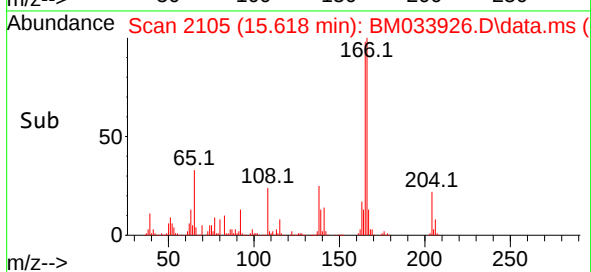
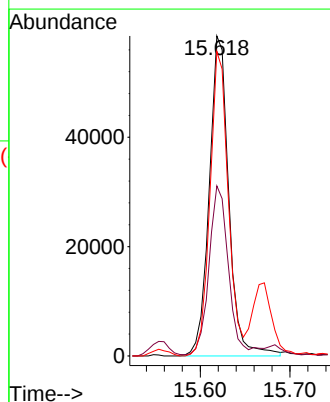
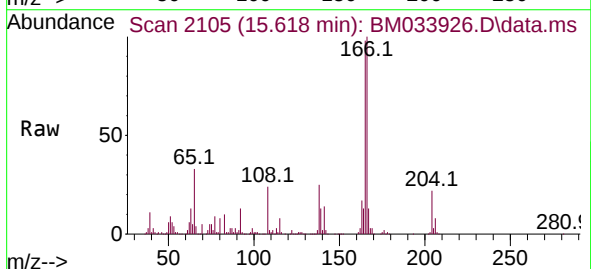




#66
4,6-Dinitro-2-methylphenol
Concen: 19.570 ng/ul
RT: 15.683 min Scan# 2116
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:198 Resp: 69621
Ion Ratio Lower Upper
198 100
182 5.0 4.2 6.2
77 30.9 26.3 39.5

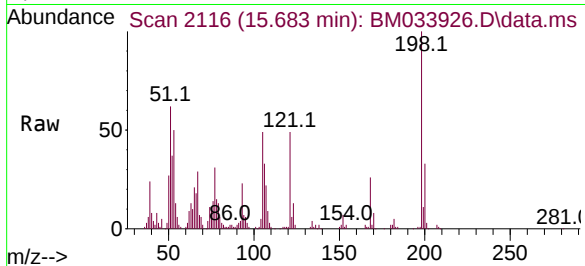

#67
N-Nitrosodiphenylamine
Concen: 20.380 ng/ul
RT: 15.813 min Scan# 2138
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:169 Resp: 368236
Ion Ratio Lower Upper
169 100
168 64.9 52.9 79.3
167 35.0 29.9 44.9




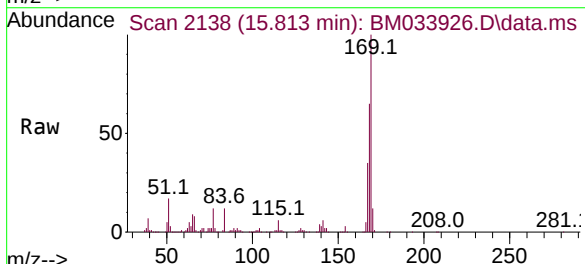




#68
4-Bromophenyl-phenylether
Concen: 21.699 ng/ul
RT: 16.495 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:248 Resp: 128315
Ion Ratio Lower Upper
248 100
250 99.0 79.0 118.4
141 94.6 69.7 104.5

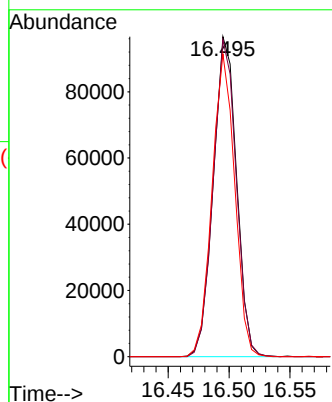

#69
Hexachlorobenzene
Concen: 20.416 ng/ul
RT: 16.618 min Scan# 2275
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:284 Resp: 147022
Ion Ratio Lower Upper
284 100
142 39.5 34.3 51.5
249 33.5 26.1 39.1

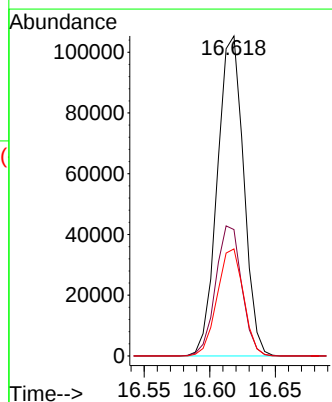



#70

Atrazine

Concen: 18.661 ng/ul

RT: 16.765 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00

Instrument :

BNA_M

ClientSampleId :

SSTD020027





Tgt Ion:200 Resp: 134198

Ion Ratio Lower Upper

200 100

173 26.1 20.6 30.8

215 47.3 36.9 55.3



#71

Pentachlorophenol

Concen: 18.880 ng/ul

RT: 16.954 min Scan# 2332

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00




Tgt Ion:266 Resp: 88939


Ion Ratio Lower Upper

266 100

264 63.5 49.1 73.7

268 62.8 47.8 71.8



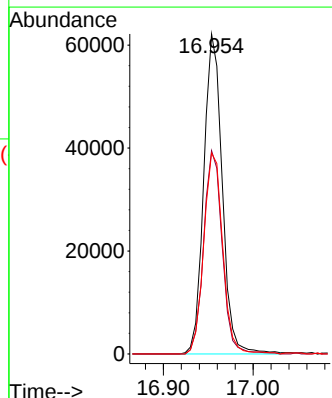





#72
Phenanthrene
Concen: 19.637 ng/u1
RT: 17.348 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:178 Resp: 666541
Ion Ratio Lower Upper
178 100
179 15.1 11.7 17.5
176 18.6 15.1 22.7

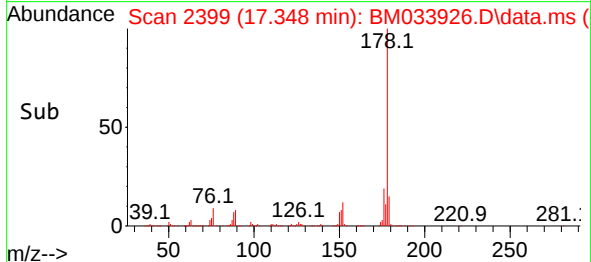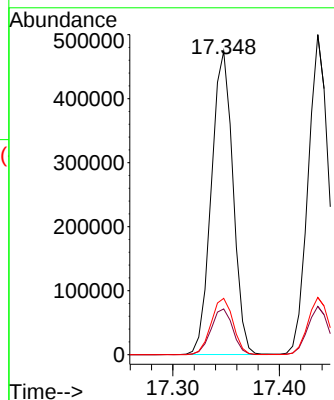

#74
Anthracene
Concen: 19.543 ng/u1
RT: 17.436 min Scan# 2414
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:178 Resp: 673654
Ion Ratio Lower Upper
178 100
179 15.1 12.3 18.5
176 17.9 14.5 21.7



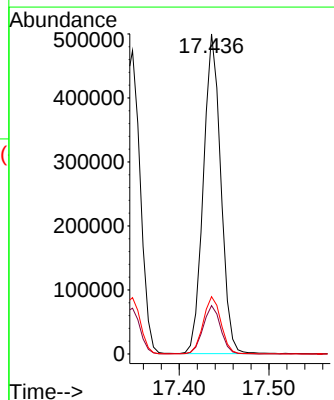
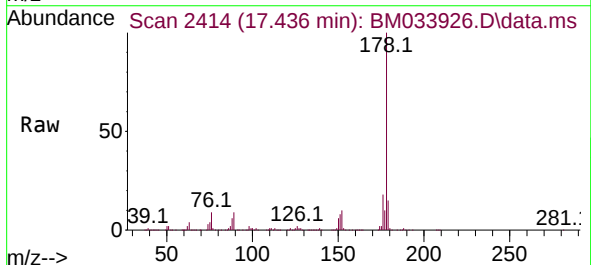




#75
1,2,3,4-Tetrachlorobenzene
Concen: 22.976 ng/uL
RT: 13.372 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:216 Resp: 205693
Ion Ratio Lower Upper
216 100
214 76.5 65.4 98.0
218 48.3 38.8 58.2

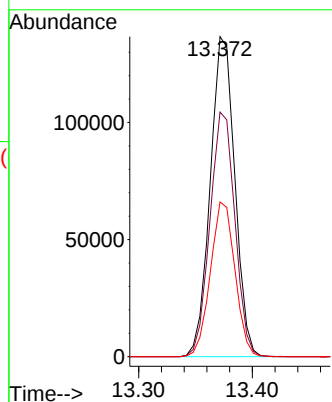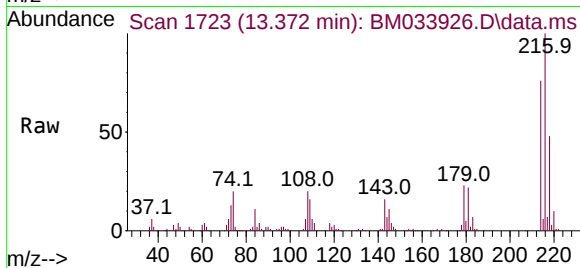

#76
Pentachlorobenzene
Concen: 21.942 ng/uL
RT: 14.889 min Scan# 1981
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:250 Resp: 184509
Ion Ratio Lower Upper
250 100
248 62.6 51.6 77.4
252 62.3 52.0 78.0


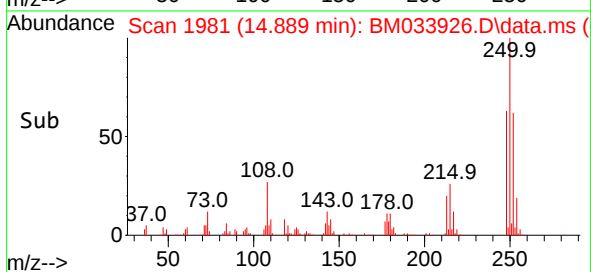
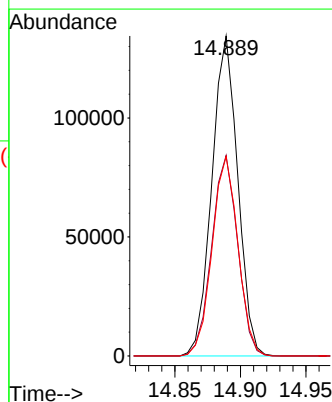
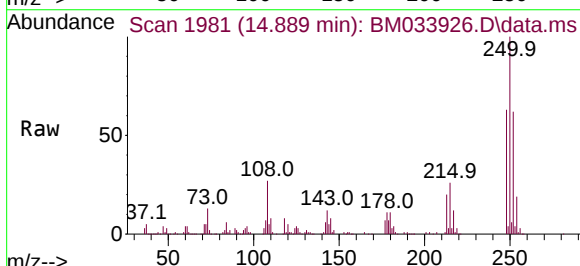


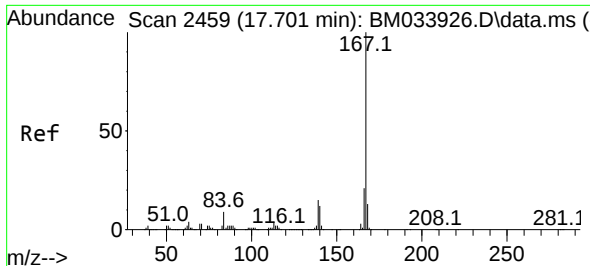

#77
 Carbazole
 Concen: 19.017 ng/ul
 RT: 17.701 min Scan# 2459
 Delta R.T. 0.000 min
 Lab File: BM033926.D
 Acq: 31 Jan 2022 15:00




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020027


Tgt Ion:167 Resp: 588070
 Ion Ratio Lower Upper
 167 100
 166 21.1 16.9 25.3
 139 14.6 10.5 15.7

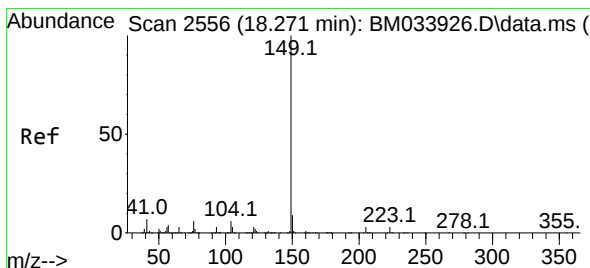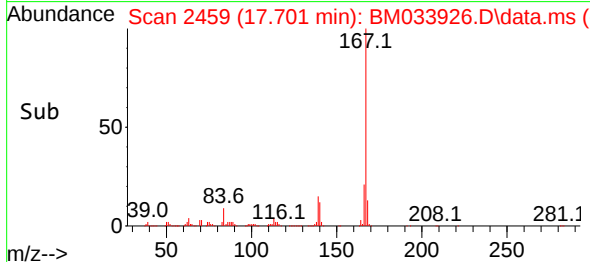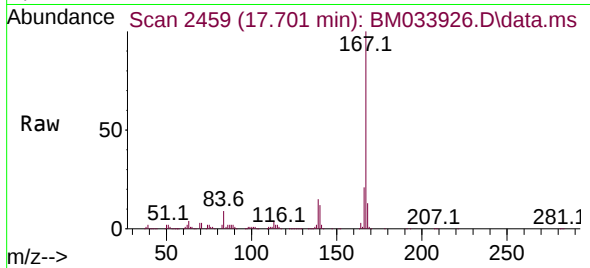

#78
 Di-n-butylphthalate
 Concen: 18.969 ng/ul
 RT: 18.271 min Scan# 2556
 Delta R.T. 0.000 min
 Lab File: BM033926.D
 Acq: 31 Jan 2022 15:00

Tgt Ion:149 Resp: 738673
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.0 10.6
 104 5.6 5.1 7.7

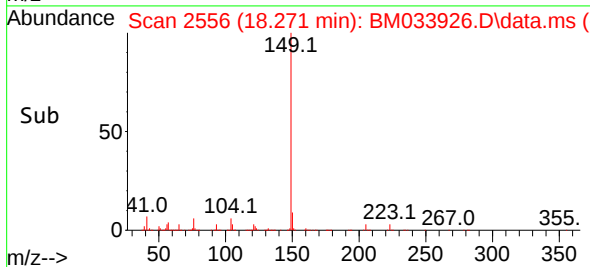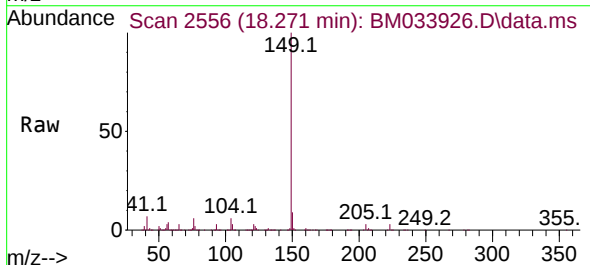



#80

Fluoranthene

Concen: 22.415 ng/u1

RT: 19.354 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00

Instrument :

BNA_M

ClientSampleId :

SSTD020027





Tgt Ion:202 Resp: 732492

Ion Ratio Lower Upper

202 100

101 10.9 8.2 12.4

100 8.2 6.9 10.3



#82

Pyrene

Concen: 22.290 ng/u1

RT: 19.712 min Scan# 2801

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00




Tgt Ion:202 Resp: 753034


Ion Ratio Lower Upper

202 100

101 12.7 9.8 14.6

100 11.0 8.6 13.0





#83

Butylbenzylphthalate

Concen: 20.868 ng/ul

RT: 20.606 min Scan# 2953

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00

Instrument :

BNA_M

ClientSampleId :

SSTD020027





Tgt Ion:149 Resp: 304982

Ion Ratio Lower Upper

149 100

91 72.5 69.3 103.9

206 19.5 16.1 24.1

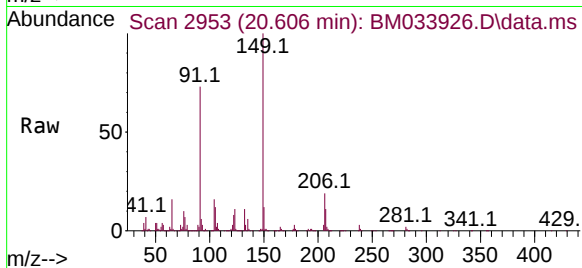

#84

3,3'-Dichlorobenzidine

Concen: 18.942 ng/ul

RT: 21.383 min Scan# 3085

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00




Tgt Ion:252 Resp: 214531


Ion Ratio Lower Upper

252 100

254 64.1 49.4 74.2

126 11.7 8.2 12.4




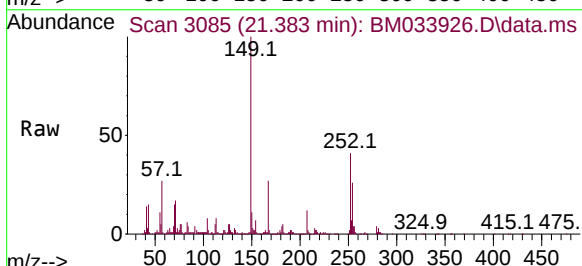




#85
Benzo(a)anthracene
Concen: 19.729 ng/ul
RT: 21.453 min Scan# 3097
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:228 Resp: 657538
Ion Ratio Lower Upper
228 100
229 20.3 15.0 22.4
226 27.4 21.4 32.0

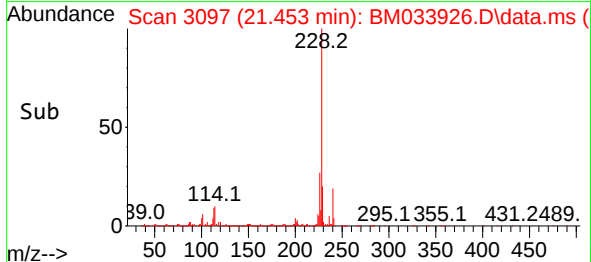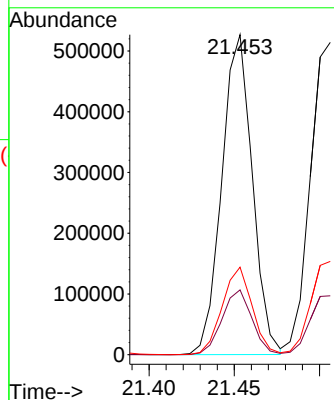

#86
Bis(2-ethylhexyl)phthalate
Concen: 19.131 ng/ul
RT: 21.383 min Scan# 3085
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:149 Resp: 438518
Ion Ratio Lower Upper
149 100
167 27.4 21.8 32.8
279 4.1 3.2 4.8



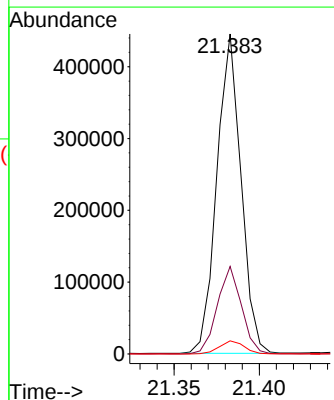





#87
Chrysene
Concen: 20.090 ng/u1
RT: 21.506 min Scan# 3106
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:228 Resp: 650051
Ion Ratio Lower Upper
228 100
226 29.9 24.5 36.7
229 18.9 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 18.246 ng/u1
RT: 22.300 min Scan# 3241
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:149 Resp: 699402




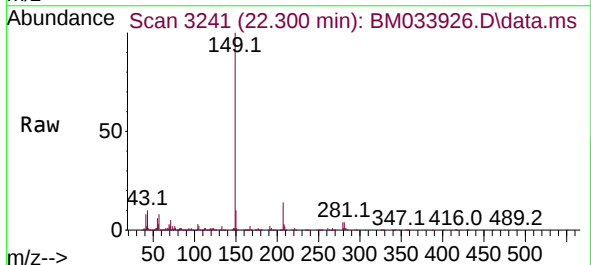




#90
Benzo(b)fluoranthene
Concen: 20.437 ng/ul
RT: 23.130 min Scan# 3382
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:252 Resp: 648775
Ion Ratio Lower Upper
252 100
253 21.9 17.7 26.5
125 9.9 7.8 11.6



#91
Benzo(k)fluoranthene
Concen: 20.496 ng/ul
RT: 23.177 min Scan# 3390
Delta R.T. 0.000 min
Lab File: BM033926.D
Acq: 31 Jan 2022 15:00

Tgt Ion:252 Resp: 605610
Ion Ratio Lower Upper
252 100
253 22.3 17.6 26.4
125 9.4 7.4 11.2





#93

Benzo(a)pyrene

Concen: 20.663 ng/ul

RT: 23.753 min Scan# 3488

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00

Instrument :

BNA_M

ClientSampleId :

SSTD020027





Tgt Ion:252 Resp: 613453

Ion Ratio Lower Upper

252 100

253 21.6 17.4 26.0

125 10.3 7.8 11.6



#94

Indeno(1,2,3-cd)pyrene

Concen: 23.850 ng/ul

RT: 26.359 min Scan# 3931

Delta R.T. 0.000 min

Lab File: BM033926.D

Acq: 31 Jan 2022 15:00




Tgt Ion:276 Resp: 712579


Ion Ratio Lower Upper

276 100

138 23.7 16.5 24.7

277 24.9 20.6 31.0









#95
 Dibenzo(a,h)anthracene
 Concen: 24.178 ng/ul
 RT: 26.371 min Scan# 3933
 Delta R.T. 0.000 min
 Lab File: BM033926.D
 Acq: 31 Jan 2022 15:00

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020027

Tgt Ion:278 Resp: 622493
 Ion Ratio Lower Upper
 278 100
 139 14.3 11.0 16.4
 279 23.8 18.1 27.1

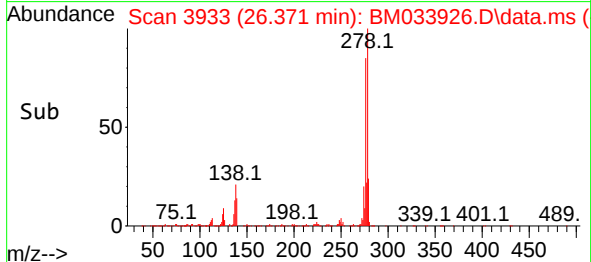

#96
 Benzo(g,h,i)perylene
 Concen: 24.551 ng/ul
 RT: 27.124 min Scan# 4061
 Delta R.T. 0.000 min
 Lab File: BM033926.D
 Acq: 31 Jan 2022 15:00

Tgt Ion:276 Resp: 598589
 Ion Ratio Lower Upper
 276 100
 138 20.8 15.6 23.4
 277 23.7 18.7 28.1

