

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013122\
 Data File : BM033929.D
 Acq On : 31 Jan 2022 16:47
 Operator : CG/JU
 Sample : SSTD16030
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160030

Quant Time: Jan 31 17:18:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 16:44:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	105195	20.000	ng/ul	0.00
20) Naphthalene-d8	10.748	136	408152	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.572	164	235899	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.307	188	443694	20.000	ng/ul	0.00
79) Chrysene-d12	21.477	240	418380	20.000	ng/ul	0.01
88) Perylene-d12	23.871	264	438498	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	165491	59.105	ng/uL	0.00
4) Pyridine-d5	3.714	84	1184077	152.287	ng/ul	0.00
7) Phenol-d5	7.102	99	1381736	146.242	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.260	67	815426	141.723	ng/ul	0.00
11) 2-Chlorophenol-d4	7.466	132	1152499	159.546	ng/ul	0.00
15) 4-Methylphenol-d8	8.654	113	1086043	138.859	ng/ul	0.01
21) Nitrobenzene-d5	9.101	128	551319	171.043	ng/ul	0.00
24) 2-Nitrophenol-d4	9.831	143	625272	183.037	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.372	165	1054722	161.050	ng/ul	0.01
31) 4-Chloroaniline-d4	10.884	131	1370081	140.738	ng/ul	0.01
46) Dimethylphthalate-d6	13.989	166	2709469	145.780	ng/ul	0.01
49) Acenaphthylene-d8	14.272	160	3513320	160.230	ng/ul	0.01
54) 4-Nitrophenol-d4	14.778	143	514604	144.266	ng/ul	0.02
60) Fluorene-d10	15.566	176	2309338	149.768	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.683	200	497397	188.461	ng/ul	0.01
73) Anthracene-d10	17.413	188	3426400	159.148	ng/ul	0.01
81) Pyrene-d10	19.695	212	3759356	166.388	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.724	264	3766021	165.063	ng/ul	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.325	88	180418	61.730	ng/uL#	87
5) Pyridine	3.737	79	1201840	150.726	ng/ul#	83
6) Benzaldehyde	7.066	77	907287	166.411	ng/ul#	83
8) Phenol	7.131	94	1410411	145.309	ng/ul#	83
10) Bis(2-Chloroethyl)ether	7.355	93	1094316	144.746	ng/ul	91
12) 2-Chlorophenol	7.502	128	1176839	155.096	ng/ul#	87
13) 2-Methylphenol	8.384	108	1061308	142.198	ng/ul	95
14) 2,2'-oxybis(1-Chloropr...	8.472	45	1411138	132.674	ng/ul#	95
16) Acetophenone	8.766	105	1673607	136.009	ng/ul#	87
17) N-Nitroso-di-n-propyla...	8.778	70	833835	130.855	ng/ul#	86
18) 4-Methylphenol	8.731	108	1119288	137.202	ng/ul	98
19) Hexachloroethane	9.025	117	515519	160.211	ng/ul#	81
22) Nitrobenzene	9.149	77	1293112	158.215	ng/ul#	89
23) Isophorone	9.690	82	2287337	146.429	ng/ul	96
25) 2-Nitrophenol	9.860	139	644227	174.793	ng/ul#	82
26) 2,4-Dimethylphenol	9.925	107	1314621	154.208	ng/ul	94
27) Bis(2-Chloroethoxy)met...	10.160	93	1381964	147.602	ng/ul	99
29) 2,4-Dichlorophenol	10.401	162	1048220	159.084	ng/ul	98
30) Naphthalene	10.801	128	3526296	155.979	ng/ul	99
32) 4-Chloroaniline	10.907	127	1380275	140.276	ng/ul	98
33) Hexachlorobutadiene	11.090	225	772258	170.063	ng/ul	98
34) Caprolactam	11.719	113	172111	76.379	ng/ul	81
35) 4-Chloro-3-methylphenol	12.037	107	1149929	142.979	ng/ul	89
36) 2-Methylnaphthalene	12.407	142	2291998	147.208	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013122\
 Data File : BM033929.D
 Acq On : 31 Jan 2022 16:47
 Operator : CG/JU
 Sample : SSTD16030
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160030


Quant Time: Jan 31 17:18:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 16:44:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.625	142	2311553	144.123	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.778	216	1241321	176.097	ng/ul	97
40) Hexachlorocyclopentadiene	12.760	237	959708	207.337	ng/ul	100
41) 2,4,6-Trichlorophenol	13.013	196	792981	175.051	ng/ul	97
42) 2,4,5-Trichlorophenol	13.089	196	847911	169.184	ng/ul	94
43) 1,1'-Biphenyl	13.413	154	2992904	161.783	ng/ul	99
44) 2-Chloronaphthalene	13.454	162	2298680	165.364	ng/ul	98
45) 2-Nitroaniline	13.660	65	736089	162.763	ng/ul#	74
47) Dimethylphthalate	14.036	163	2710741	145.882	ng/ul	100
48) 2,6-Dinitrotoluene	14.154	165	588845	165.325	ng/ul	91
50) Acenaphthylene	14.301	152	3667950	157.508	ng/ul	99
51) 3-Nitroaniline	14.478	138	486280	132.854	ng/ul	84
52) Acenaphthene	14.636	153	2370003	154.609	ng/ul	97
53) 2,4-Dinitrophenol	14.683	184	386450	180.282	ng/ul#	85
55) 4-Nitrophenol	14.795	109	481027	139.197	ng/ul	83
56) Dibenzofuran	14.972	168	3309607	150.536	ng/ul	99
57) 2,4-Dinitrotoluene	14.936	165	821912	154.124	ng/ul#	79
58) 2,3,4,6-Tetrachlorophenol	15.195	232	679735	160.022	ng/ul	99
59) Diethylphthalate	15.395	149	2756201	140.394	ng/ul	100
61) Fluorene	15.619	166	2619735	146.713	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.613	204	1343173	149.875	ng/ul	94
63) 4-Nitroaniline	15.642	138	435428	123.481	ng/ul	85
66) 4,6-Dinitro-2-methylph...	15.701	198	490649	184.985	ng/ul#	89
67) N-Nitrosodiphenylamine	15.825	169	2226542	165.281	ng/ul	98
68) 4-Bromophenyl-phenylether	16.501	248	792165	179.679	ng/ul	100
69) Hexachlorobenzene	16.625	284	902472	168.088	ng/ul	94
70) Atrazine	16.777	200	833467	155.449	ng/ul	99
71) Pentachlorophenol	16.960	266	603199	171.744	ng/ul	98
72) Phenanthrene	17.354	178	3910523	154.525	ng/ul	98
74) Anthracene	17.448	178	4007366	155.927	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.378	216	1300541	194.846	ng/ul	97
76) Pentachlorobenzene	14.895	250	1139508	181.756	ng/ul	98
77) Carbazole	17.713	167	3540988	153.591	ng/ul	98
78) Di-n-butylphthalate	18.277	149	4442268	153.008	ng/ul	98
80) Fluoranthene	19.360	202	4439552	165.302	ng/ul	99
82) Pyrene	19.724	202	4510297	162.444	ng/ul	99
83) Butylbenzylphthalate	20.613	149	2016148	167.850	ng/ul#	84
84) 3,3'-Dichlorobenzidine	21.389	252	1088802	116.972	ng/ul	97
85) Benzo(a)anthracene	21.460	228	4330652	158.102	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.389	149	2903587	154.131	ng/ul#	99
87) Chrysene	21.512	228	4194290	157.720	ng/ul	99
89) Di-n-octyl phthalate	22.307	149	5025285	139.744	ng/ul	100
90) Benzo(b)fluoranthene	23.148	252	4614190	154.931	ng/ul	99
91) Benzo(k)fluoranthene	23.195	252	4448118	160.463	ng/ul	100
93) Benzo(a)pyrene	23.777	252	4592905	164.901	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.400	276	5482517	195.595	ng/ul	96
95) Dibenzo(a,h)anthracene	26.412	278	4783433	198.038	ng/ul	99
96) Benzo(g,h,i)perylene	27.171	276	4589860	200.661	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 31 17:18:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 16:44:50 2022
Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 61.730 ng/uL
RT: 3.325 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion: 88 Resp: 180418
Ion Ratio Lower Upper
88 100
43 29.9 36.2 54.4#
58 78.3 68.5 102.7

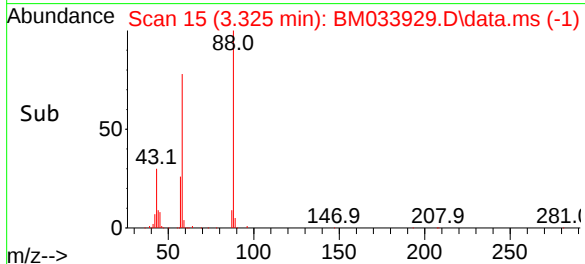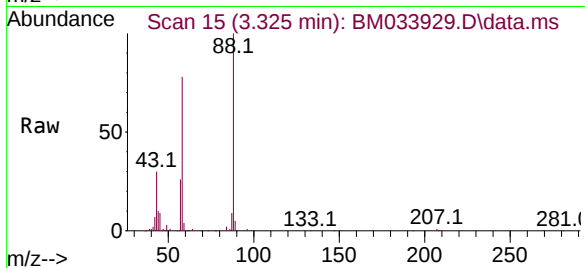

#5
Pyridine
Concen: 150.726 ng/uL
RT: 3.737 min Scan# 85
Delta R.T. 0.000 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion: 79 Resp: 1201840
Ion Ratio Lower Upper
79 100
52 77.7 78.1 117.1#
51 38.9 36.0 54.0




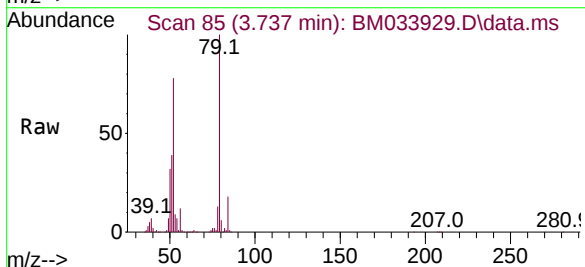




#6
Benzaldehyde
Concen: 166.411 ng/ul
RT: 7.066 min Scan# 61
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion: 77 Resp: 907287
Ion Ratio Lower Upper
77 100
105 97.2 65.6 98.4
106 91.1 60.6 90.8#

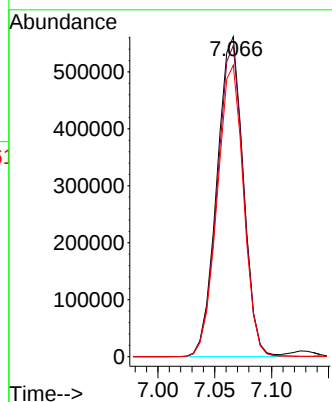

#8
Phenol
Concen: 145.309 ng/ul
RT: 7.131 min Scan# 662
Delta R.T. 0.018 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion: 94 Resp: 1410411
Ion Ratio Lower Upper
94 100
65 30.0 31.7 47.5#
66 43.8 45.4 68.0#









#10
Bis(2-Chloroethyl)ether
Concen: 144.746 ng/ul
RT: 7.355 min Scan# 700
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Instrument :
BNA_M
ClientSampleId :
SSTD160030

Tgt Ion: 93 Resp: 1094316




Ion	Ratio	Lower	Upper
93	100		
63	78.4	71.7	107.5
95	32.3	26.3	39.5




#12
2-Chlorophenol
Concen: 155.096 ng/ul
RT: 7.502 min Scan# 725
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion: 128 Resp: 1176839

Ion	Ratio	Lower	Upper
128	100		
64	47.9	49.4	74.2#
130	32.1	26.8	40.2

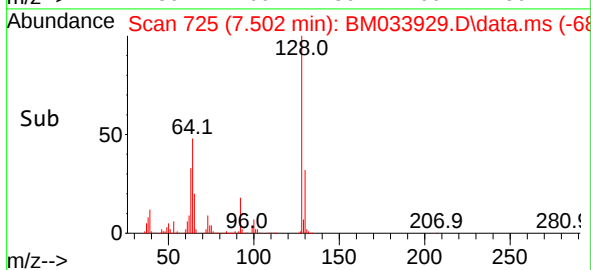



#13

2-Methylphenol

Concen: 142.198 ng/ul

RT: 8.384 min Scan# 81

Delta R.T. 0.012 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Instrument :

BNA_M

ClientSampleId :





SSTD160030

Tgt Ion:108 Resp: 1061308

Ion Ratio Lower Upper

108 100

107 92.2 70.2 105.4

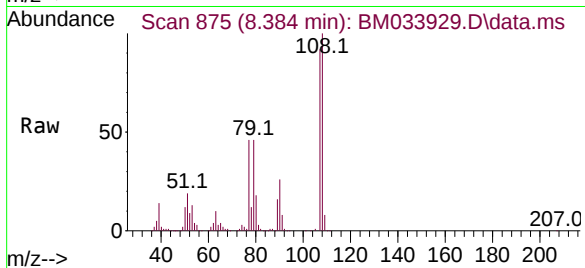

#14

2,2'-oxybis(1-Chloropropane)

Concen: 132.674 ng/ul

RT: 8.472 min Scan# 890

Delta R.T. 0.012 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47




Tgt Ion: 45 Resp: 1411138


Ion Ratio Lower Upper

45 100

77 15.3 9.9 14.9#

79 11.4 8.3 12.5


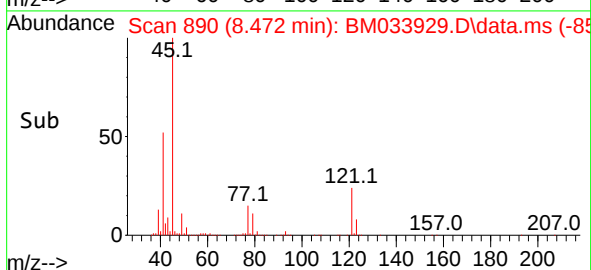

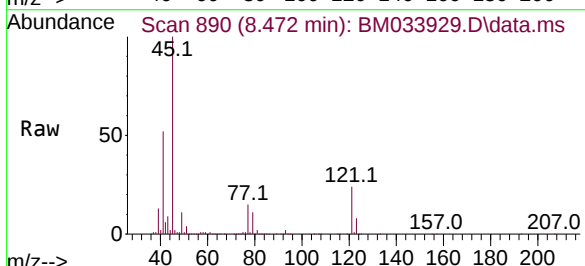




#16
Acetophenone
Concen: 136.009 ng/ul
RT: 8.766 min Scan# 941
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:105 Resp: 1673607
Ion Ratio Lower Upper
105 100
77 79.3 73.1 109.7
51 29.2 30.5 45.7#



#17
N-Nitroso-di-n-propylamine
Concen: 130.855 ng/ul
RT: 8.778 min Scan# 942
Delta R.T. 0.036 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion: 70 Resp: 833835
Ion Ratio Lower Upper
70 100
42 57.7 56.9 85.3
101 10.5 6.9 10.3#
130 21.9 13.8 20.8#


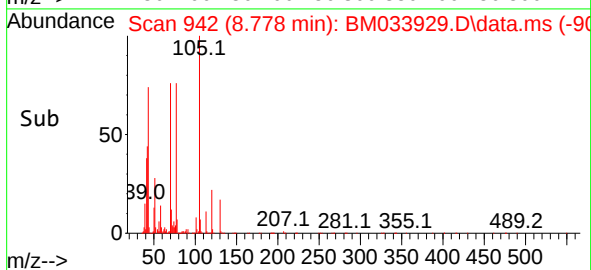






#18
4-Methylphenol
Concen: 137.202 ng/ul
RT: 8.731 min Scan# 911
Delta R.T. 0.030 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:108 Resp: 1119288
Ion Ratio Lower Upper
108 100
107 111.7 87.4 131.2



#19
Hexachloroethane
Concen: 160.211 ng/ul
RT: 9.025 min Scan# 984
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:117 Resp: 515519
Ion Ratio Lower Upper
117 100
201 104.3 69.6 104.4
199 64.9 40.6 60.8#









#22
Nitrobenzene
Concen: 158.215 ng/ul
RT: 9.149 min Scan# 1005
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion: 77 Resp: 1293112
Ion Ratio Lower Upper
77 100
123 45.1 29.0 43.6#
65 14.8 11.4 17.2

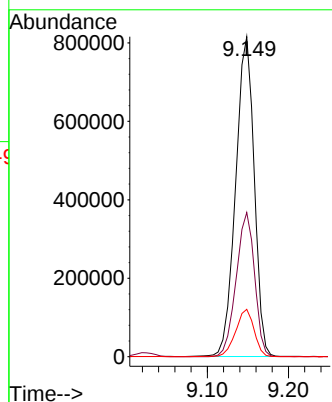

#23
Isophorone
Concen: 146.429 ng/ul
RT: 9.690 min Scan# 1097
Delta R.T. 0.024 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion: 82 Resp: 2287337
Ion Ratio Lower Upper
82 100
95 8.1 6.5 9.7
138 17.3 11.8 17.8


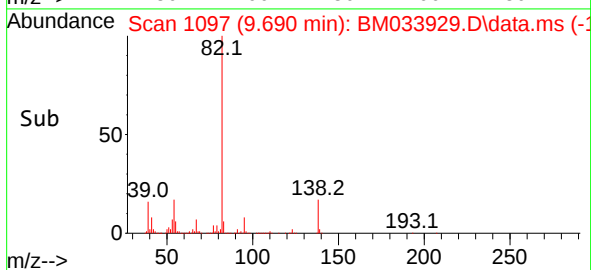




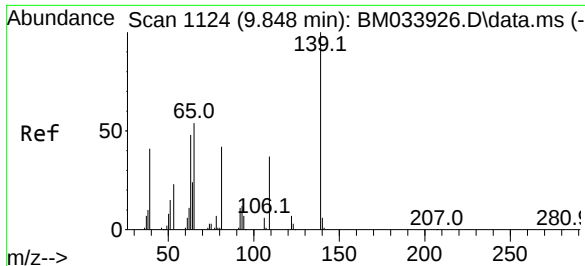

#25
2-Nitrophenol
Concen: 174.793 ng/ul
RT: 9.860 min Scan# 1126
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:139 Resp: 644227
Ion Ratio Lower Upper
139 100
65 55.7 59.0 88.6#
109 37.9 37.2 55.8

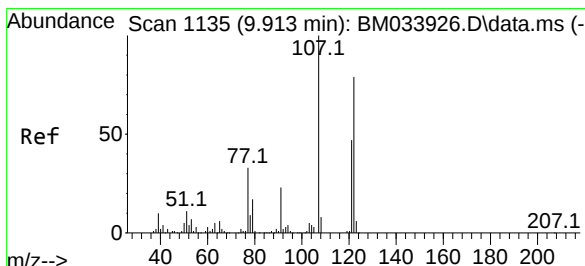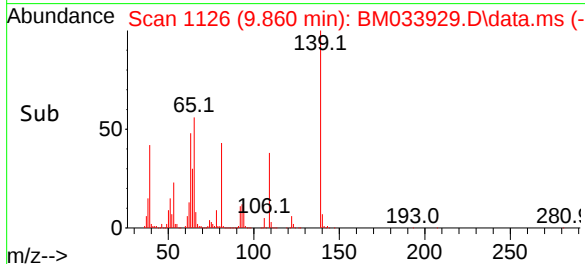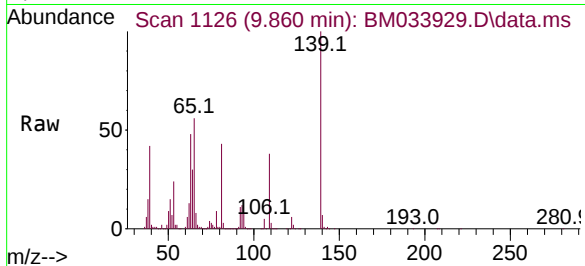

#26
2,4-Dimethylphenol
Concen: 154.208 ng/ul
RT: 9.925 min Scan# 1137
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:107 Resp: 1314621
Ion Ratio Lower Upper
107 100
121 47.9 34.8 52.2
122 79.2 60.0 90.0

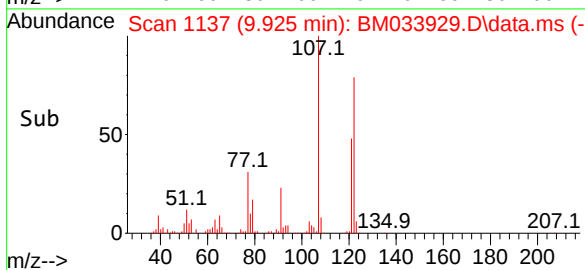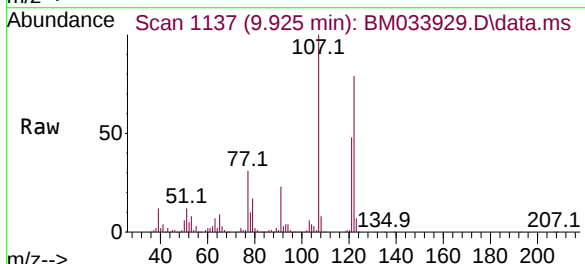



#27

Bis(2-Chloroethoxy)methane

Concen: 147.602 ng/ul

RT: 10.160 min Scan# 1177

Delta R.T. 0.012 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Instrument :





BNA_M

ClientSampleId :

SSTD160030

Tgt Ion: 93 Resp: 1381964

Ion	Ratio	Lower	Upper
93	100		
95	32.1	25.3	37.9
123	11.0	7.9	11.9

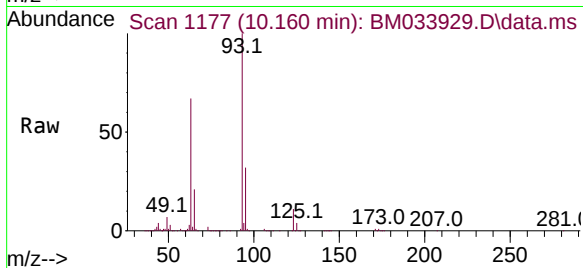

#29

2,4-Dichlorophenol

Concen: 159.084 ng/ul

RT: 10.401 min Scan# 1218




Delta R.T. 0.012 min


Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Tgt Ion:162 Resp: 1048220

Ion	Ratio	Lower	Upper
162	100		
164	64.7	50.0	75.0
98	37.8	30.6	45.8




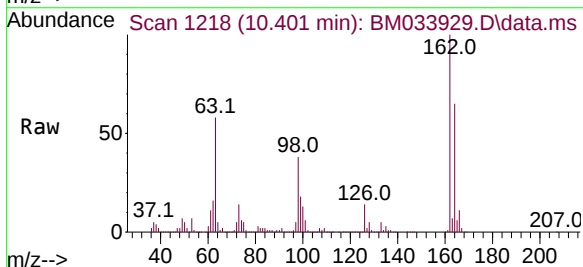




#30
Naphthalene
Concen: 155.979 ng/ul
RT: 10.801 min Scan# 11
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:128 Resp: 3526296
Ion Ratio Lower Upper
128 100
129 10.9 9.1 13.7
127 13.3 10.2 15.4



#32
4-Chloroaniline
Concen: 140.276 ng/ul
RT: 10.907 min Scan# 1304
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:127 Resp: 1380275
Ion Ratio Lower Upper
127 100
129 32.6 25.4 38.0









#33
Hexachlorobutadiene
Concen: 170.063 ng/ul
RT: 11.090 min Scan# 111
Delta R.T. 0.000 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:225 Resp: 772258
Ion Ratio Lower Upper
225 100
223 63.4 52.2 78.2
227 64.1 52.8 79.2



#34
Caprolactam
Concen: 76.379 ng/ul
RT: 11.719 min Scan# 1442
Delta R.T. 0.053 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:113 Resp: 172111
Ion Ratio Lower Upper
113 100
55 170.1 157.9 236.9
56 136.4 131.8 197.6









#35
4-Chloro-3-methylphenol
Concen: 142.979 ng/ul
RT: 12.037 min Scan# 1494
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:107 Resp: 1149929
Ion Ratio Lower Upper
107 100
144 23.4 17.1 25.7
142 72.4 49.4 74.2

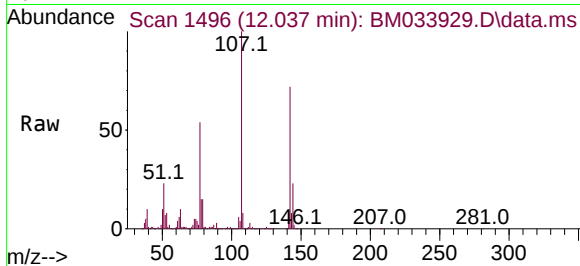

#36
2-Methylnaphthalene
Concen: 147.208 ng/ul
RT: 12.407 min Scan# 1559
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:142 Resp: 2291998
Ion Ratio Lower Upper
142 100
141 89.9 71.1 106.7

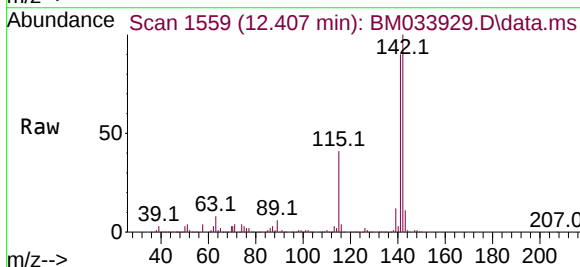



#37

1-Methylnaphthalene

Concen: 144.123 ng/ul

RT: 12.625 min Scan# 1

Delta R.T. 0.006 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Instrument :

BNA_M

ClientSampleId :

SSTD160030





Tgt Ion:142 Resp: 2311553

Ion Ratio Lower Upper

142 100

141 93.8 75.5 113.3

116 4.5 4.0 6.0

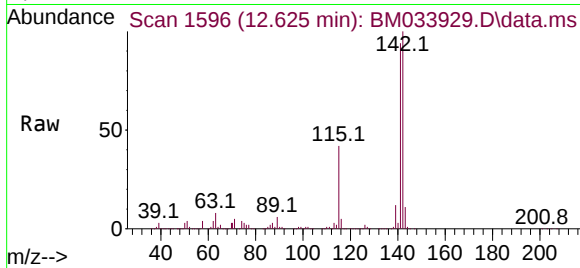

#39

1,2,4,5-Tetrachlorobenzene

Concen: 176.097 ng/ul

RT: 12.778 min Scan# 1622

Delta R.T. 0.006 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Tgt Ion:216 Resp: 1241321




Ion Ratio Lower Upper


216 100

214 79.5 61.3 91.9

179 22.4 18.0 27.0

108 18.4 16.6 25.0




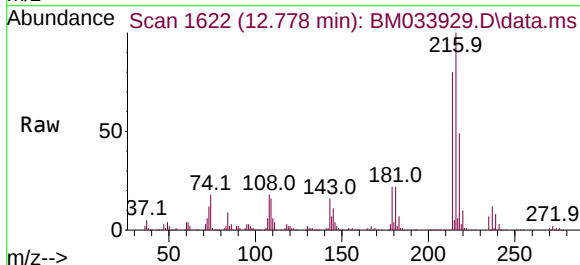




#40
Hexachlorocyclopentadiene
Concen: 207.337 ng/ul
RT: 12.760 min Scan# 1618
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:237 Resp: 959708
Ion Ratio Lower Upper
237 100
235 63.0 50.6 76.0
272 11.9 9.6 14.4

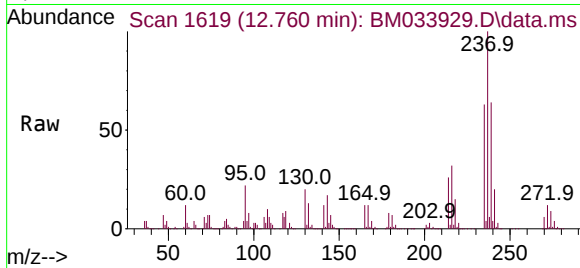

#41
2,4,6-Trichlorophenol
Concen: 175.051 ng/ul
RT: 13.013 min Scan# 1662
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:196 Resp: 792981
Ion Ratio Lower Upper
196 100
198 96.2 78.9 118.3
200 31.2 23.7 35.5




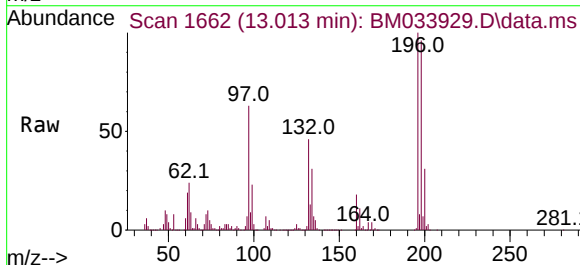




#42
2,4,5-Trichlorophenol
Concen: 169.184 ng/ul
RT: 13.089 min Scan# 1
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:196 Resp: 847911
Ion Ratio Lower Upper
196 100
198 97.2 82.2 123.2
200 30.9 27.9 41.9

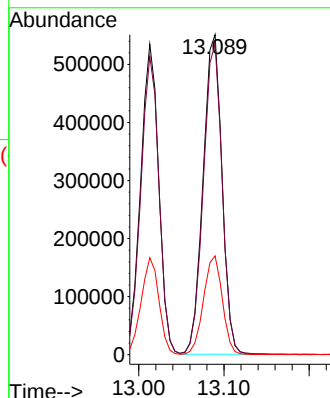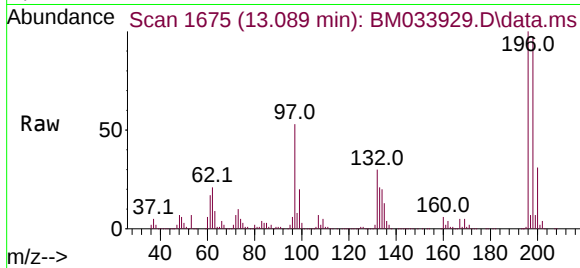

#43
1,1'-Biphenyl
Concen: 161.783 ng/ul
RT: 13.413 min Scan# 1730
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:154 Resp: 2992904
Ion Ratio Lower Upper
154 100
153 41.2 33.1 49.7
76 12.2 10.7 16.1

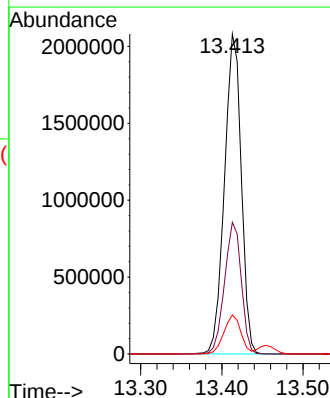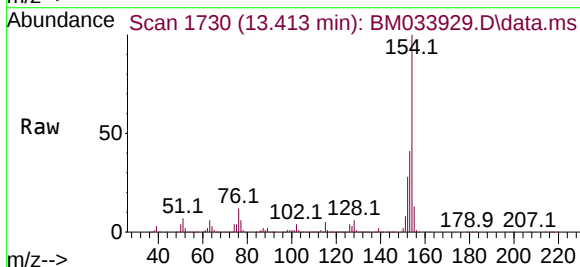



#44

2-Chloronaphthalene

Concen: 165.364 ng/ul

RT: 13.454 min Scan# 1

Delta R.T. 0.006 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Instrument :

BNA_M

ClientSampleId :

SSTD160030





Tgt Ion:162 Resp: 2298680

Ion Ratio Lower Upper

162 100

164 32.7 26.2 39.4

127 44.1 33.7 50.5

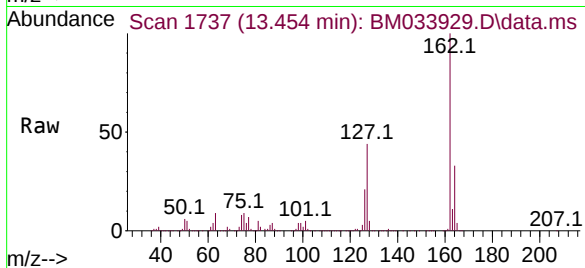

#45

2-Nitroaniline

Concen: 162.763 ng/ul

RT: 13.660 min Scan# 1772

Delta R.T. 0.018 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47




Tgt Ion: 65 Resp: 736089


Ion Ratio Lower Upper

65 100

92 69.9 47.8 71.6

138 106.5 61.0 91.6#

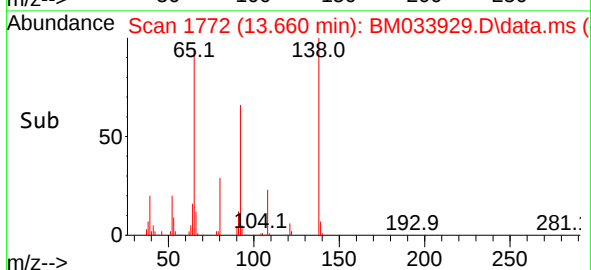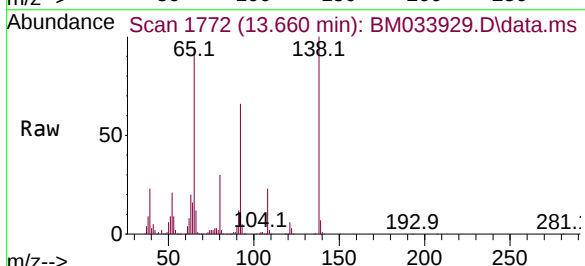



#47

Dimethylphthalate

Concen: 145.882 ng/ul

RT: 14.036 min Scan# 1836

Delta R.T. 0.012 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Instrument :

BNA_M

ClientSampleId :

SSTD160030





Tgt Ion:163 Resp: 2710741

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.1 8.2 12.2



#48

2,6-Dinitrotoluene

Concen: 165.325 ng/ul

RT: 14.154 min Scan# 1856

Delta R.T. 0.012 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47




Tgt Ion:165 Resp: 588845


Ion Ratio Lower Upper

165 100

89 61.2 55.7 83.5

121 21.9 20.0 30.0









#50
Acenaphthylene
Concen: 157.508 ng/ul
RT: 14.301 min Scan# 1881
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:152 Resp: 3667950
Ion Ratio Lower Upper
152 100
151 20.2 15.8 23.8
153 13.0 10.1 15.1

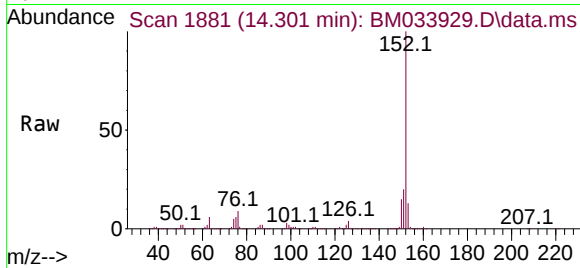

#51
3-Nitroaniline
Concen: 132.854 ng/ul
RT: 14.478 min Scan# 1911
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:138 Resp: 486280
Ion Ratio Lower Upper
138 100
108 11.6 10.8 16.2
92 118.2 110.6 166.0




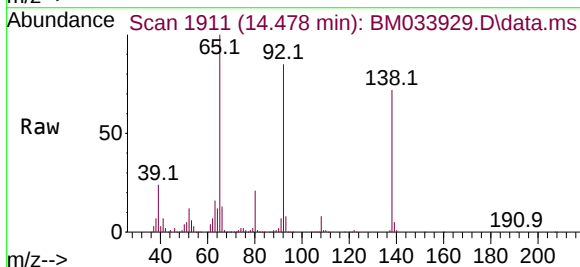


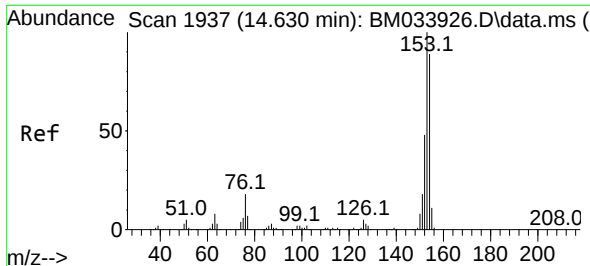

#52
Acenaphthene
Concen: 154.609 ng/ul
RT: 14.636 min Scan# 1937
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:153 Resp: 2370003
Ion Ratio Lower Upper
153 100
152 47.0 39.4 59.2
154 87.6 72.7 109.1

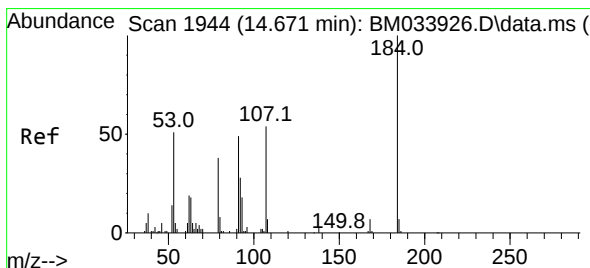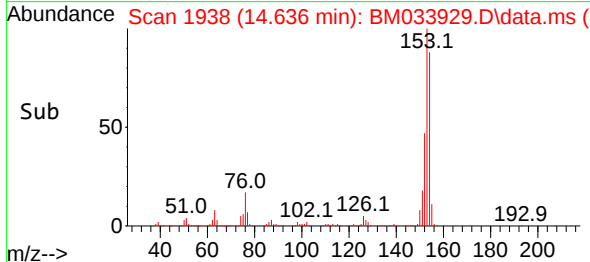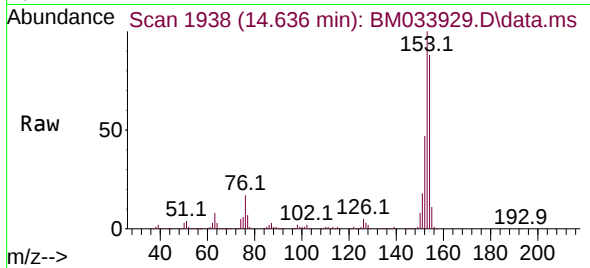

#53
2,4-Dinitrophenol
Concen: 180.282 ng/ul
RT: 14.683 min Scan# 1946
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:184 Resp: 386450
Ion Ratio Lower Upper
184 100
63 71.2 73.8 110.8#
154 73.3 63.5 95.3


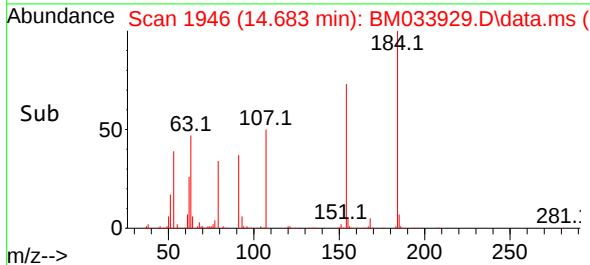

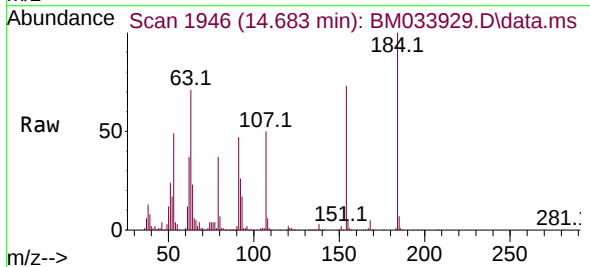




#55
4-Nitrophenol
Concen: 139.197 ng/ul
RT: 14.795 min Scan# 1965
Delta R.T. 0.030 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:109 Resp: 481027
Ion Ratio Lower Upper
109 100
139 111.1 77.6 116.4
65 116.4 112.2 168.4



#56
Dibenzofuran
Concen: 150.536 ng/ul
RT: 14.972 min Scan# 1995
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:168 Resp: 3309607
Ion Ratio Lower Upper
168 100
139 41.7 34.0 51.0





#57

2,4-Dinitrotoluene

Concen: 154.124 ng/ul

RT: 14.936 min Scan# 1989

Delta R.T. 0.012 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Instrument :

BNA_M

ClientSampleId :

SSTD160030





Tgt Ion:165 Resp: 821912

Ion Ratio Lower Upper

165 100

63 47.8 51.8 77.8#

182 2.6 2.6 4.0#

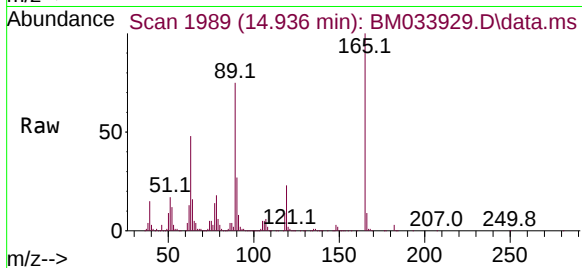

#58

2,3,4,6-Tetrachlorophenol

Concen: 160.022 ng/ul

RT: 15.195 min Scan# 2033

Delta R.T. 0.006 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Tgt Ion:232 Resp: 679735




Ion Ratio Lower Upper


232 100

131 52.5 41.4 62.2

130 2.8 2.0 3.0

166 33.9 27.4 41.0

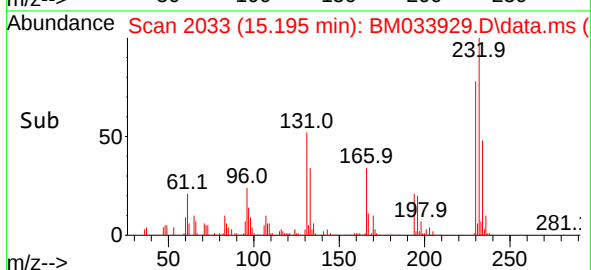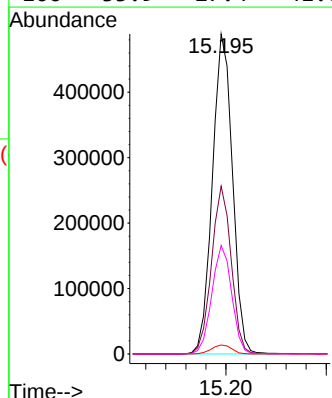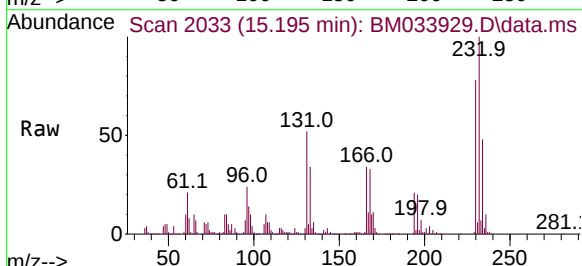



#59

Diethylphthalate

Concen: 140.394 ng/ul

RT: 15.395 min Scan# 2067

Delta R.T. 0.012 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Instrument :

BNA_M

ClientSampleId :

SSTD160030





Tgt Ion:149 Resp: 2756201

Ion Ratio Lower Upper

149 100

177 21.4 17.1 25.7

150 12.7 9.9 14.9



#61

Fluorene

Concen: 146.713 ng/ul

RT: 15.619 min Scan# 2105

Delta R.T. 0.006 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47




Tgt Ion:166 Resp: 2619735


Ion Ratio Lower Upper

166 100

165 98.5 77.9 116.9

167 13.6 10.3 15.5









#62
4-Chlorophenyl-phenylether
Concen: 149.875 ng/ul
RT: 15.613 min Scan# 2104
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:204 Resp: 1343173
Ion Ratio Lower Upper
204 100
206 32.5 27.8 41.8
141 63.2 54.9 82.3



#63
4-Nitroaniline
Concen: 123.481 ng/ul
RT: 15.642 min Scan# 2109
Delta R.T. 0.024 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:138 Resp: 435428
Ion Ratio Lower Upper
138 100
92 52.0 48.0 72.0
108 93.5 89.5 134.3









#66
4,6-Dinitro-2-methylphenol
Concen: 184.985 ng/ul
RT: 15.701 min Scan# 2116
Delta R.T. 0.018 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:198 Resp: 490649
Ion Ratio Lower Upper
198 100
182 3.4 4.2 6.2#
77 26.5 26.3 39.5



#67
N-Nitrosodiphenylamine
Concen: 165.281 ng/ul
RT: 15.825 min Scan# 2140
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:169 Resp: 2226542
Ion Ratio Lower Upper
169 100
168 67.2 52.9 79.3
167 36.3 29.9 44.9









#68
4-Bromophenyl-phenylether
Concen: 179.679 ng/ul
RT: 16.501 min Scan# 21
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:248 Resp: 792165
Ion Ratio Lower Upper
248 100
250 98.9 79.0 118.4
141 86.9 69.7 104.5



#69
Hexachlorobenzene
Concen: 168.088 ng/ul
RT: 16.625 min Scan# 2276
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:284 Resp: 902472
Ion Ratio Lower Upper
284 100
142 36.4 34.3 51.5
249 33.4 26.1 39.1


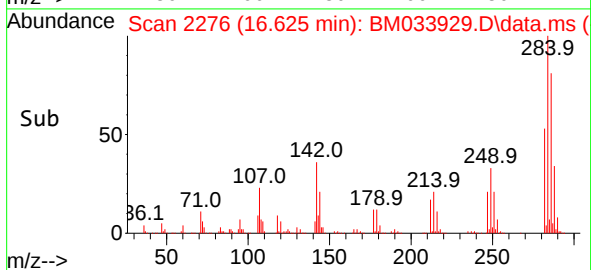






#70
Atrazine
Concen: 155.449 ng/ul
RT: 16.777 min Scan# 21
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:200 Resp: 833467
Ion Ratio Lower Upper
200 100
173 26.0 20.6 30.8
215 45.4 36.9 55.3



#71
Pentachlorophenol
Concen: 171.744 ng/ul
RT: 16.960 min Scan# 2333
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:266 Resp: 603199
Ion Ratio Lower Upper
266 100
264 62.0 49.1 73.7
268 63.0 47.8 71.8









#72
Phenanthrene
Concen: 154.525 ng/ul
RT: 17.354 min Scan# 2410
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:178 Resp: 3910523
Ion Ratio Lower Upper
178 100
179 15.3 11.7 17.5
176 19.5 15.1 22.7



#74
Anthracene
Concen: 155.927 ng/ul
RT: 17.448 min Scan# 2416
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:178 Resp: 4007366
Ion Ratio Lower Upper
178 100
179 15.6 12.3 18.5
176 18.8 14.5 21.7









#75
1,2,3,4-Tetrachlorobenzene
Concen: 194.846 ng/uL
RT: 13.378 min Scan# 1724
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:216 Resp: 1300541
Ion Ratio Lower Upper
216 100
214 78.1 65.4 98.0
218 47.9 38.8 58.2



#76
Pentachlorobenzene
Concen: 181.756 ng/uL
RT: 14.895 min Scan# 1982
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:250 Resp: 1139508
Ion Ratio Lower Upper
250 100
248 63.3 51.6 77.4
252 63.9 52.0 78.0









#77
 Carbazole
 Concen: 153.591 ng/ul
 RT: 17.713 min Scan# 2459
 Delta R.T. 0.012 min
 Lab File: BM033929.D
 Acq: 31 Jan 2022 16:47




Instrument :
 BNA_M
 ClientSampleId :
 SSTD160030


Tgt Ion:167 Resp: 3540988
 Ion Ratio Lower Upper
 167 100
 166 22.1 16.9 25.3
 139 14.2 10.5 15.7

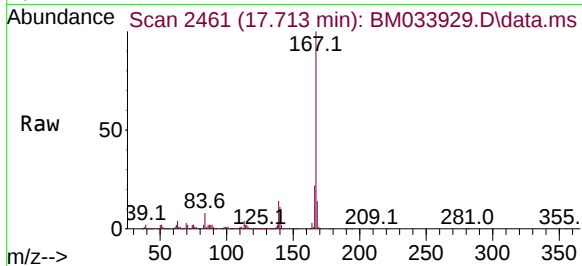

#78
 Di-n-butylphthalate
 Concen: 153.008 ng/ul
 RT: 18.277 min Scan# 2557
 Delta R.T. 0.006 min
 Lab File: BM033929.D
 Acq: 31 Jan 2022 16:47

Tgt Ion:149 Resp: 4442268
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.0 10.6
 104 5.5 5.1 7.7


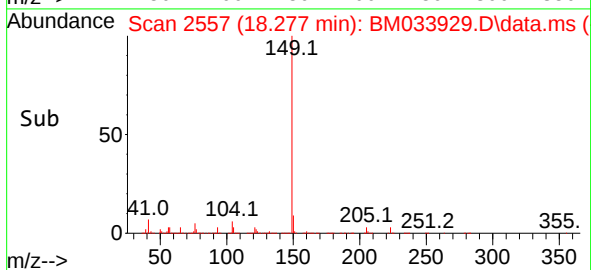

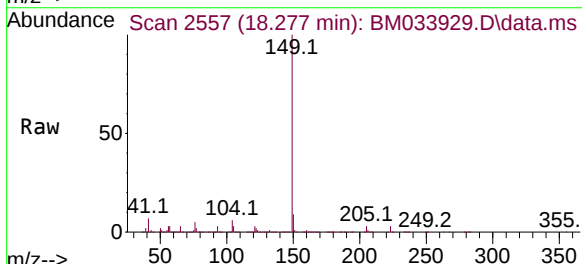




#80
Fluoranthene
Concen: 165.302 ng/u1
RT: 19.360 min Scan# 21
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:202 Resp: 4439552
Ion Ratio Lower Upper
202 100
101 10.7 8.2 12.4
100 8.2 6.9 10.3



#82
Pyrene
Concen: 162.444 ng/u1
RT: 19.724 min Scan# 2803
Delta R.T. 0.012 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:202 Resp: 4510297
Ion Ratio Lower Upper
202 100
101 12.1 9.8 14.6
100 10.2 8.6 13.0



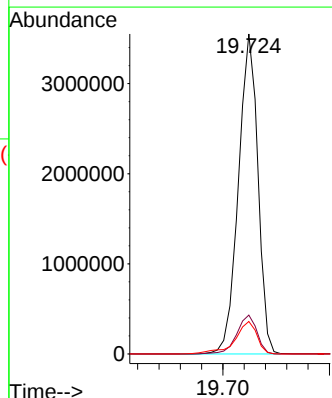





#83
Butylbenzylphthalate
Concen: 167.850 ng/ul
RT: 20.613 min Scan# 2954
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:149 Resp: 2016148
Ion Ratio Lower Upper
149 100
91 68.6 69.3 103.9#
206 20.8 16.1 24.1

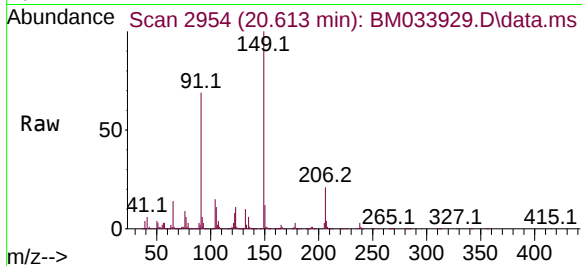

#84
3,3'-Dichlorobenzidine
Concen: 116.972 ng/ul
RT: 21.389 min Scan# 3086
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:252 Resp: 1088802
Ion Ratio Lower Upper
252 100
254 64.7 49.4 74.2
126 10.2 8.2 12.4



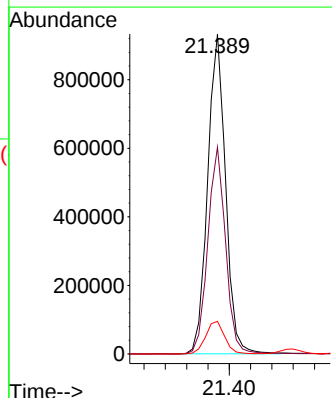
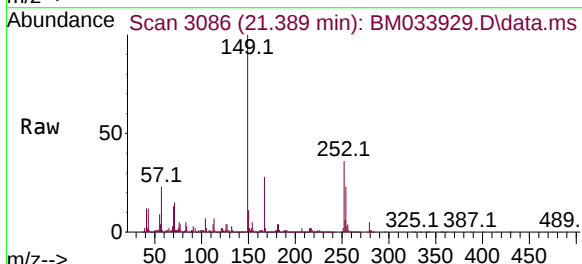




#85
Benzo(a)anthracene
Concen: 158.102 ng/ul
RT: 21.460 min Scan# 3097
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:228 Resp: 4330652
Ion Ratio Lower Upper
228 100
229 20.1 15.0 22.4
226 27.4 21.4 32.0

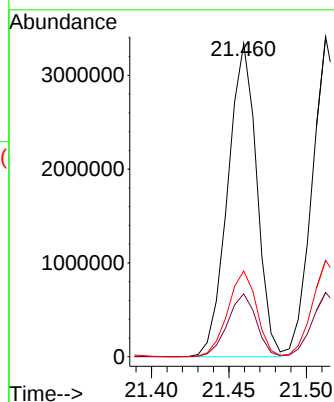

#86
Bis(2-ethylhexyl)phthalate
Concen: 154.131 ng/ul
RT: 21.389 min Scan# 3086
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:149 Resp: 2903587
Ion Ratio Lower Upper
149 100
167 27.7 21.8 32.8
279 4.9 3.2 4.8#



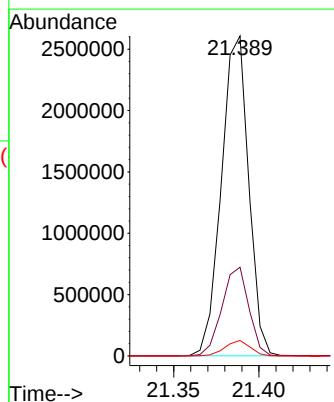





#87
Chrysene
Concen: 157.720 ng/ul
RT: 21.512 min Scan# 3106
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:228 Resp: 4194290
Ion Ratio Lower Upper
228 100
226 30.1 24.5 36.7
229 20.0 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 139.744 ng/ul
RT: 22.307 min Scan# 3242
Delta R.T. 0.006 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:149 Resp: 5025285









#90
Benzo(b)fluoranthene
Concen: 154.931 ng/ul
RT: 23.148 min Scan# 31
Delta R.T. 0.018 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47




Instrument :
BNA_M
ClientSampleId :
SSTD160030


Tgt Ion:252 Resp: 4614190
Ion Ratio Lower Upper
252 100
253 21.5 17.7 26.5
125 9.1 7.8 11.6



#91
Benzo(k)fluoranthene
Concen: 160.463 ng/ul
RT: 23.195 min Scan# 3393
Delta R.T. 0.018 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:252 Resp: 4448118
Ion Ratio Lower Upper
252 100
253 22.2 17.6 26.4
125 9.1 7.4 11.2

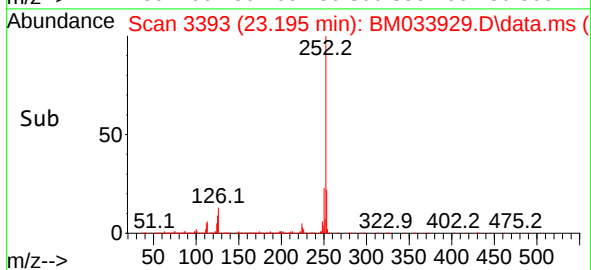



#93

Benzo(a)pyrene

Concen: 164.901 ng/ul

RT: 23.777 min Scan# 34

Delta R.T. 0.024 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47

Instrument :

BNA_M

ClientSampleId :

SSTD160030





Tgt Ion:252 Resp: 4592905

Ion Ratio Lower Upper

252 100

253 21.7 17.4 26.0

125 10.3 7.8 11.6

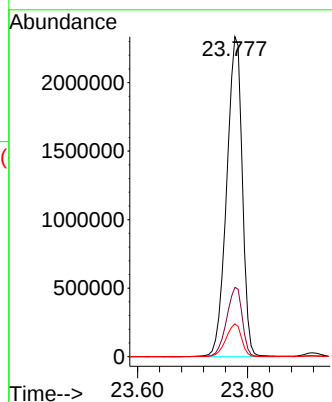

#94

Indeno(1,2,3-cd)pyrene

Concen: 195.595 ng/ul

RT: 26.400 min Scan# 3938

Delta R.T. 0.041 min

Lab File: BM033929.D

Acq: 31 Jan 2022 16:47




Tgt Ion:276 Resp: 5482517


Ion Ratio Lower Upper

276 100

138 24.5 16.5 24.7

277 26.0 20.6 31.0


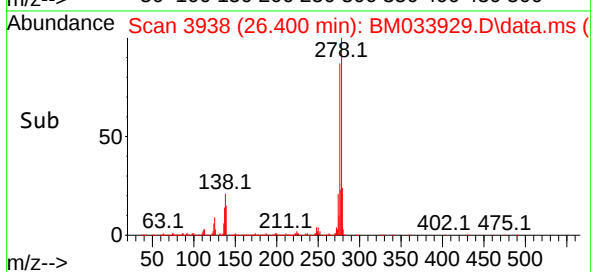
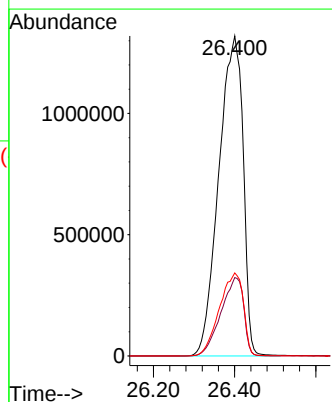





#95
Dibenzo(a,h)anthracene
Concen: 198.038 ng/ul
RT: 26.412 min Scan# 3933
Delta R.T. 0.041 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Instrument :
BNA_M
ClientSampleId :
SSTD160030

Tgt Ion:278 Resp: 4783433
Ion Ratio Lower Upper
278 100
139 14.0 11.0 16.4
279 23.5 18.1 27.1



#96
Benzo(g,h,i)perylene
Concen: 200.661 ng/ul
RT: 27.171 min Scan# 4069
Delta R.T. 0.047 min
Lab File: BM033929.D
Acq: 31 Jan 2022 16:47

Tgt Ion:276 Resp: 4589860
Ion Ratio Lower Upper
276 100
138 19.7 15.6 23.4
277 23.9 18.7 28.1

