

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013122\
 Data File : BM033930.D
 Acq On : 31 Jan 2022 17:23
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SICV031

Quant Time: Feb 01 02:25:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	116443	20.000	ng/ul	0.00
20) Naphthalene-d8	10.742	136	487457	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.566	164	296210	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.307	188	578969	20.000	ng/ul	0.00
79) Chrysene-d12	21.471	240	492432	20.000	ng/ul	0.00
88) Perylene-d12	23.859	264	471673	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	22211	7.523	ng/uL	0.00
4) Pyridine-d5	3.719	84	153813	18.664	ng/ul	0.00
7) Phenol-d5	7.084	99	190642	19.543	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.254	67	127908	21.507	ng/ul	0.00
11) 2-Chlorophenol-d4	7.460	132	157096	20.100	ng/ul	0.00
15) 4-Methylphenol-d8	8.642	113	153143	19.811	ng/ul	0.00
21) Nitrobenzene-d5	9.089	128	76071	19.449	ng/ul	0.00
24) 2-Nitrophenol-d4	9.819	143	84302	19.959	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	150341	19.669	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131	206995	19.611	ng/ul	0.00
46) Dimethylphthalate-d6	13.977	166	434773	19.642	ng/ul	0.00
49) Acenaphthylene-d8	14.260	160	543195	20.033	ng/ul	0.00
54) 4-Nitrophenol-d4	14.754	143	70673	18.688	ng/ul	0.00
60) Fluorene-d10	15.554	176	354463	19.178	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.671	200	64019	17.613	ng/ul	0.00
73) Anthracene-d10	17.401	188	537919	19.401	ng/ul	0.00
81) Pyrene-d10	19.689	212	574222	19.752	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.706	264	472843	19.086	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.325	88	23613	7.329	ng/uL#	91
5) Pyridine	3.737	79	136614	16.060	ng/ul	91
6) Benzaldehyde	7.060	77	143520	24.366	ng/ul	83
8) Phenol	7.113	94	209945	20.986	ng/ul#	82
10) Bis(2-Chloroethyl)ether	7.348	93	164389	20.804	ng/ul	92
12) 2-Chlorophenol	7.490	128	173397	21.176	ng/ul#	88
13) 2-Methylphenol	8.372	108	160367	21.224	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.466	45	229963	21.619	ng/ul#	94
16) Acetophenone	8.754	105	265822	21.662	ng/ul#	86
17) N-Nitroso-di-n-propyla...	8.742	70	136241	21.868	ng/ul	87
18) 4-Methylphenol	8.701	108	170465	21.147	ng/ul	94
19) Hexachloroethane	9.019	117	74386	20.937	ng/ul	87
22) Nitrobenzene	9.136	77	199466	20.599	ng/ul#	89
23) Isophorone	9.666	82	342967	19.735	ng/ul	97
25) 2-Nitrophenol	9.848	139	96358	21.263	ng/ul#	82
26) 2,4-Dimethylphenol	9.913	107	208034	21.044	ng/ul	96
27) Bis(2-Chloroethoxy)met...	10.148	93	216120	20.004	ng/ul	97
29) 2,4-Dichlorophenol	10.389	162	160565	21.025	ng/ul	98
30) Naphthalene	10.795	128	561160	20.812	ng/ul	99
32) 4-Chloroaniline	10.895	127	227238	21.203	ng/ul	100
33) Hexachlorobutadiene	11.089	225	115455	20.430	ng/ul	96
34) Caprolactam	11.672	113	42782	19.684	ng/ul	79
35) 4-Chloro-3-methylphenol	12.019	107	181681	20.761	ng/ul	88
36) 2-Methylnaphthalene	12.401	142	392287	22.083	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013122\
 Data File : BM033930.D
 Acq On : 31 Jan 2022 17:23
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SICV031

Quant Time: Feb 01 02:25:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.619	142	364217	20.001	ng/ul	97
39) 1,2,4,5-Tetrachloroben...	12.772	216	193549	20.545	ng/ul	97
40) Hexachlorocyclopentadiene	12.754	237	140712	20.247	ng/ul	99
41) 2,4,6-Trichlorophenol	13.007	196	123475	21.048	ng/ul	99
42) 2,4,5-Trichlorophenol	13.077	196	131640	21.153	ng/ul	94
43) 1,1'-Biphenyl	13.407	154	483960	20.382	ng/ul	99
44) 2-Chloronaphthalene	13.448	162	372454	20.804	ng/ul	98
45) 2-Nitroaniline	13.648	65	115584	21.939	ng/ul#	82
47) Dimethylphthalate	14.024	163	460838	20.729	ng/ul	99
48) 2,6-Dinitrotoluene	14.142	165	97224	22.913	ng/ul	90
50) Acenaphthylene	14.289	152	588890	20.369	ng/ul	99
51) 3-Nitroaniline	14.466	138	98830	23.593	ng/ul	86
52) Acenaphthene	14.630	153	395493	20.895	ng/ul	97
53) 2,4-Dinitrophenol	14.671	184	48226	18.625	ng/ul#	86
55) 4-Nitrophenol	14.766	109	72411	19.835	ng/ul	85
56) Dibenzofuran	14.966	168	552971	20.760	ng/ul	100
57) 2,4-Dinitrotoluene	14.924	165	131510	21.722	ng/ul#	78
58) 2,3,4,6-Tetrachlorophenol	15.107	232	114680	22.398	ng/ul	91
59) Diethylphthalate	15.383	149	462994	20.447	ng/ul	100
61) Fluorene	15.613	166	446288	20.936	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.607	204	223178	20.497	ng/ul	98
63) 4-Nitroaniline	15.618	138	99795	24.697	ng/ul	83
66) 4,6-Dinitro-2-methylph...	15.683	198	69780	19.214	ng/ul#	94
67) N-Nitrosodiphenylamine	15.813	169	376666	20.965	ng/ul	99
68) 4-Bromophenyl-phenylether	16.495	248	128986	20.619	ng/ul	96
69) Hexachlorobenzene	16.618	284	147270	20.589	ng/ul	94
70) Atrazine	16.765	200	124085	18.355	ng/ul	99
71) Pentachlorophenol	16.954	266	88423	19.274	ng/ul	95
72) Phenanthrene	17.348	178	673252	20.679	ng/ul	100
74) Anthracene	17.436	178	686573	20.984	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.371	216	187343	18.515	ng/uL	98
76) Pentachlorobenzene	14.889	250	174348	19.329	ng/uL	99
77) Carbazole	17.701	167	590683	20.396	ng/ul	99
78) Di-n-butylphthalate	18.271	149	733108	20.357	ng/ul	98
80) Fluoranthene	19.353	202	721840	20.743	ng/ul	99
82) Pyrene	19.718	202	745450	20.959	ng/ul	99
83) Butylbenzylphthalate	20.606	149	297260	20.512	ng/ul	90
84) 3,3'-Dichlorobenzidine	21.383	252	229031	23.372	ng/ul	98
85) Benzo(a)anthracene	21.453	228	654557	20.518	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.383	149	434044	20.538	ng/ul	99
87) Chrysene	21.506	228	640023	20.530	ng/ul	98
89) Di-n-octyl phthalate	22.300	149	699046	20.467	ng/ul	100
90) Benzo(b)fluoranthene	23.130	252	641533	20.023	ng/ul	100
91) Benzo(k)fluoranthene	23.177	252	625923	21.279	ng/ul	99
93) Benzo(a)pyrene	23.753	252	612061	20.202	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.359	276	721416	20.600	ng/ul	97
95) Dibenzo(a,h)anthracene	26.377	278	618582	20.408	ng/ul	98
96) Benzo(g,h,i)perylene	27.124	276	607320	20.625	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013122\
 Data File : BM033930.D
 Acq On : 31 Jan 2022 17:23
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SICV031

Quant Time: Feb 01 02:25:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration




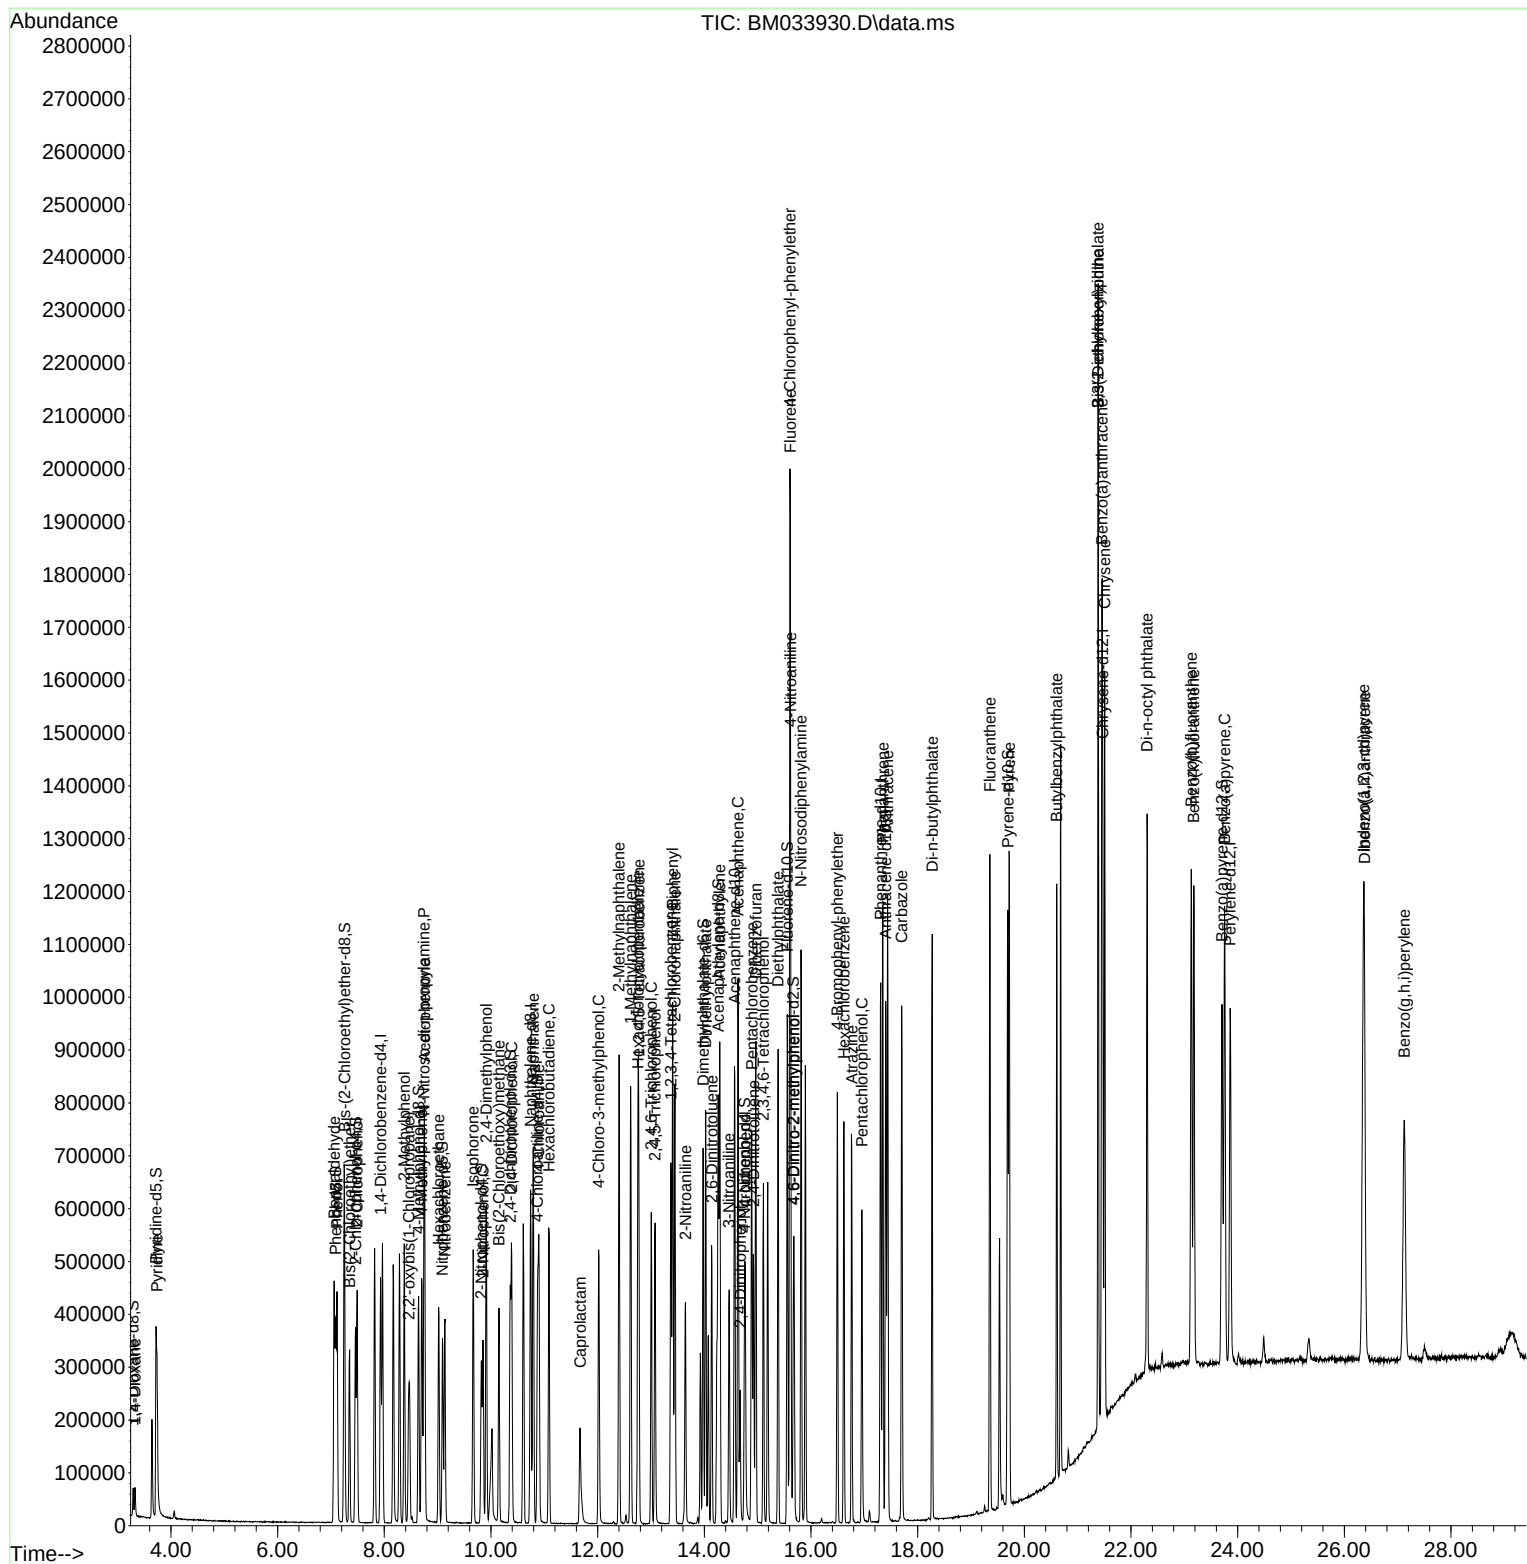


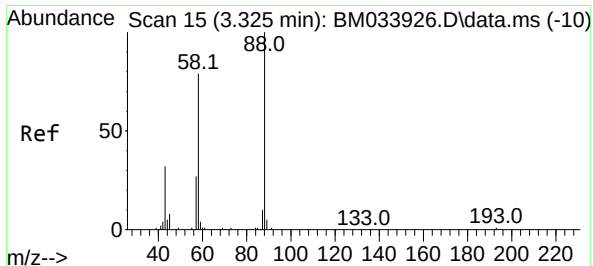

#2
1,4-Dioxane
Concen: 7.329 ng/uL
RT: 3.325 min Scan# 15
Delta R.T. 0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion: 88 Resp: 23613
Ion Ratio Lower Upper
88 100
43 29.8 36.2 54.4#
58 84.6 68.5 102.7

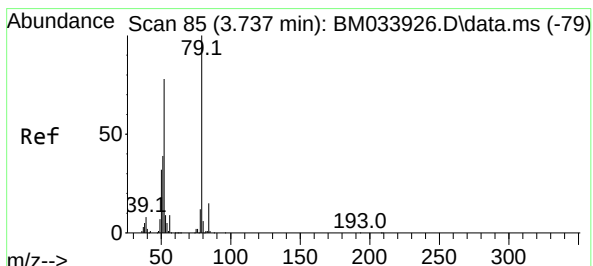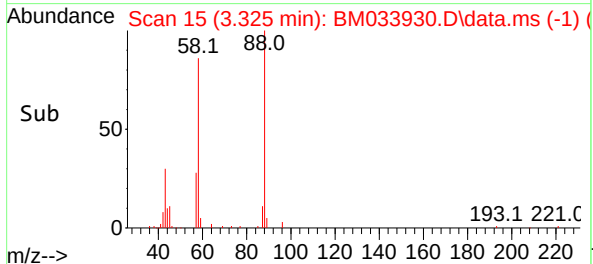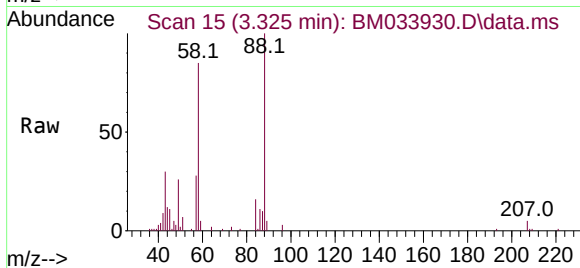

#5
Pyridine
Concen: 16.060 ng/uL
RT: 3.737 min Scan# 85
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion: 79 Resp: 136614
Ion Ratio Lower Upper
79 100
52 87.0 78.1 117.1
51 41.6 36.0 54.0


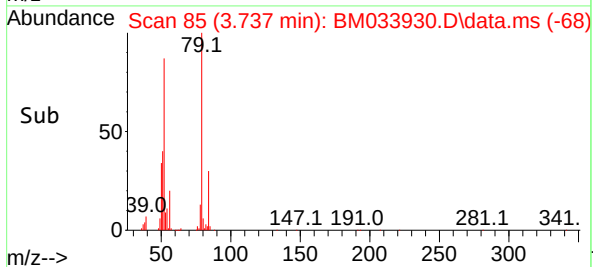

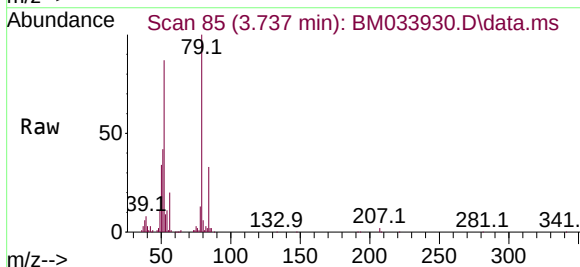




#6
Benzaldehyde
Concen: 24.366 ng/ul
RT: 7.060 min Scan# 610
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion: 77 Resp: 143520
Ion Ratio Lower Upper
77 100
105 98.3 65.6 98.4
106 90.0 60.6 90.8

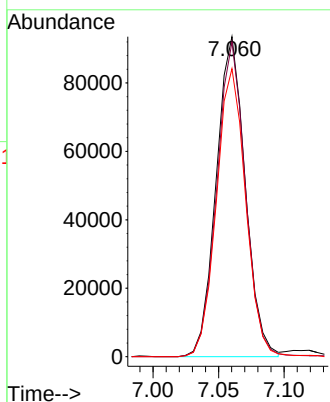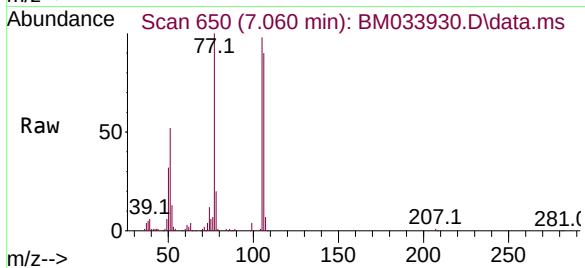

#8
Phenol
Concen: 20.986 ng/ul
RT: 7.113 min Scan# 659
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion: 94 Resp: 209945
Ion Ratio Lower Upper
94 100
65 29.5 31.7 47.5#
66 43.2 45.4 68.0#




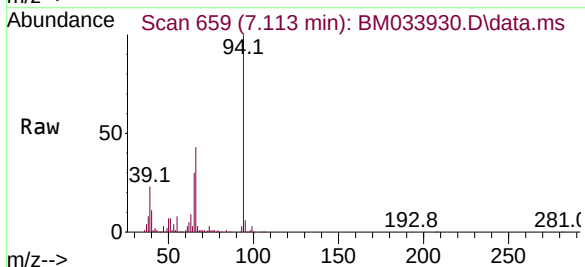




#10
Bis(2-Chloroethyl)ether
Concen: 20.804 ng/ul
RT: 7.348 min Scan# 699
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion: 93 Resp: 164389
Ion Ratio Lower Upper
93 100
63 79.7 71.7 107.5
95 34.0 26.3 39.5



#12
2-Chlorophenol
Concen: 21.176 ng/ul
RT: 7.490 min Scan# 723
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:128 Resp: 173397
Ion Ratio Lower Upper
128 100
64 48.2 49.4 74.2#
130 32.2 26.8 40.2





#13

2-Methylphenol

Concen: 21.224 ng/ul

RT: 8.372 min Scan# 81

Delta R.T. -0.000 min

Lab File: BM033930.D

Acq: 31 Jan 2022 17:23

Instrument :

BNA_M

ClientSampleId :





SICV031

Tgt Ion:108 Resp: 160367

Ion Ratio Lower Upper

108 100

107 88.3 70.2 105.4

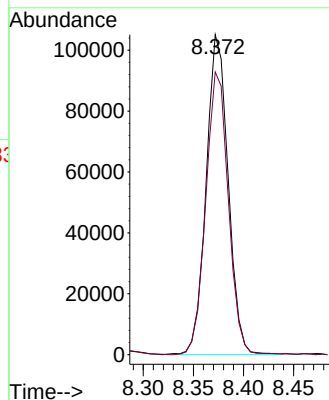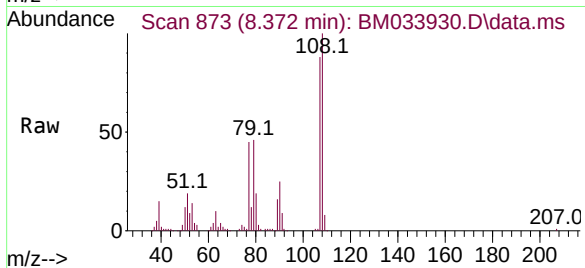

#14

2,2'-oxybis(1-Chloropropane)

Concen: 21.619 ng/ul

RT: 8.466 min Scan# 889

Delta R.T. 0.006 min

Lab File: BM033930.D

Acq: 31 Jan 2022 17:23




Tgt Ion: 45 Resp: 229963


Ion Ratio Lower Upper

45 100

77 15.6 9.9 14.9#

79 11.8 8.3 12.5



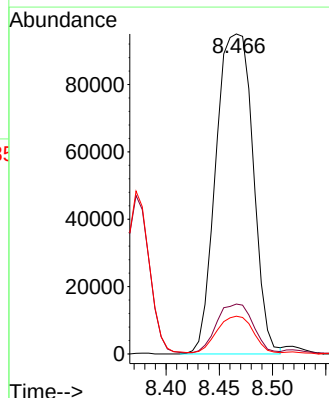
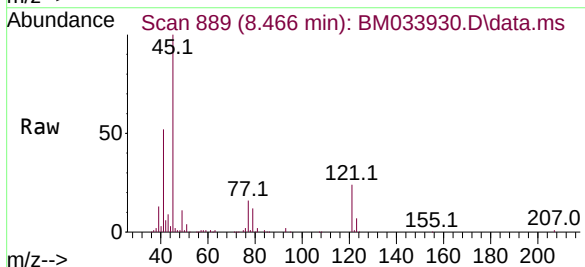




#16
Acetophenone
Concen: 21.662 ng/ul
RT: 8.754 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:105 Resp: 265822
Ion Ratio Lower Upper
105 100
77 78.0 73.1 109.7
51 28.9 30.5 45.7#



#17
N-Nitroso-di-n-propylamine
Concen: 21.868 ng/ul
RT: 8.742 min Scan# 936
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion: 70 Resp: 136241
Ion Ratio Lower Upper
70 100
42 58.2 56.9 85.3
101 9.8 6.9 10.3
130 20.3 13.8 20.8



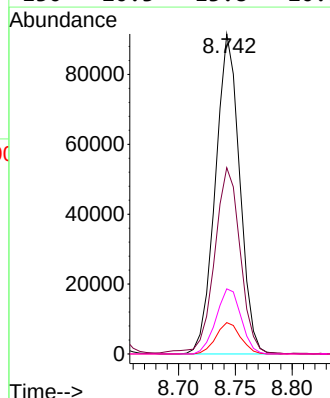





#18
4-Methylphenol
Concen: 21.147 ng/ul
RT: 8.701 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:108 Resp: 170465
Ion Ratio Lower Upper
108 100
107 115.9 87.4 131.2



#19
Hexachloroethane
Concen: 20.937 ng/ul
RT: 9.019 min Scan# 983
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:117 Resp: 74386
Ion Ratio Lower Upper
117 100
201 98.3 69.6 104.4
199 60.8 40.6 60.8









#22
Nitrobenzene
Concen: 20.599 ng/ul
RT: 9.136 min Scan# 1003
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion: 77 Resp: 199466
Ion Ratio Lower Upper
77 100
123 45.6 29.0 43.6#
65 14.0 11.4 17.2



#23
Isophorone
Concen: 19.735 ng/ul
RT: 9.666 min Scan# 1093
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion: 82 Resp: 342967
Ion Ratio Lower Upper
82 100
95 8.1 6.5 9.7
138 16.9 11.8 17.8









#25
2-Nitrophenol
Concen: 21.263 ng/ul
RT: 9.848 min Scan# 1124
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:139 Resp: 96358
Ion Ratio Lower Upper
139 100
65 56.5 59.0 88.6#
109 37.7 37.2 55.8



#26
2,4-Dimethylphenol
Concen: 21.044 ng/ul
RT: 9.913 min Scan# 1135
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:107 Resp: 208034
Ion Ratio Lower Upper
107 100
121 47.7 34.8 52.2
122 77.6 60.0 90.0





#27

Bis(2-Chloroethoxy)methane

Concen: 20.004 ng/ul

RT: 10.148 min Scan# 1175

Delta R.T. -0.000 min

Lab File: BM033930.D

Acq: 31 Jan 2022 17:23

Instrument :

BNA_M

ClientSampleId :

SICV031





Tgt Ion: 93 Resp: 216120

Ion Ratio Lower Upper

93 100

95 33.2 25.3 37.9

123 11.0 7.9 11.9

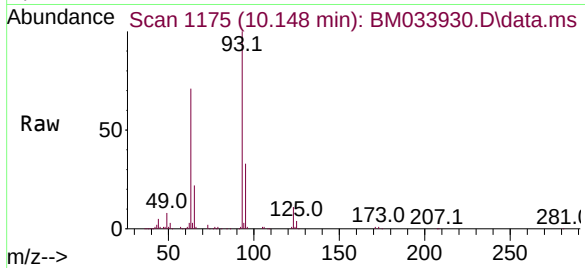

#29

2,4-Dichlorophenol

Concen: 21.025 ng/ul

RT: 10.389 min Scan# 1216

Delta R.T. -0.000 min

Lab File: BM033930.D

Acq: 31 Jan 2022 17:23




Tgt Ion:162 Resp: 160565


Ion Ratio Lower Upper

162 100

164 65.0 50.0 75.0

98 38.8 30.6 45.8



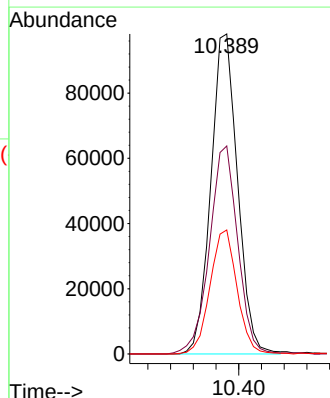
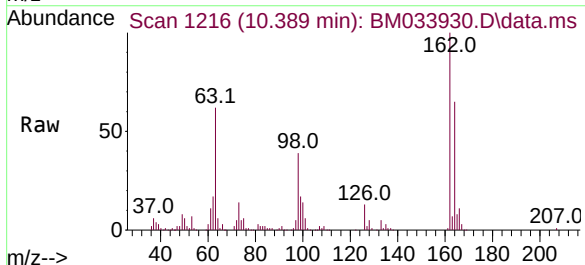




#30
Naphthalene
Concen: 20.812 ng/ul
RT: 10.795 min Scan# 1285
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:128 Resp: 561160
Ion Ratio Lower Upper
128 100
129 10.5 9.1 13.7
127 12.8 10.2 15.4



#32
4-Chloroaniline
Concen: 21.203 ng/ul
RT: 10.895 min Scan# 1302
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:127 Resp: 227238
Ion Ratio Lower Upper
127 100
129 31.8 25.4 38.0


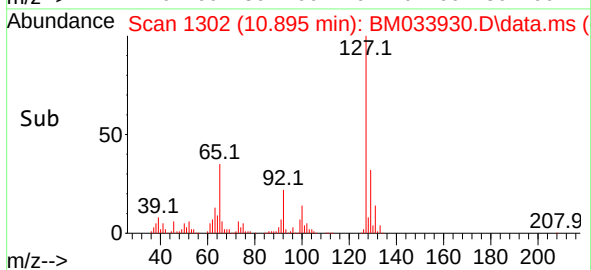






#33
Hexachlorobutadiene
Concen: 20.430 ng/ul
RT: 11.089 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:225 Resp: 115455
Ion Ratio Lower Upper
225 100
223 62.4 52.2 78.2
227 63.1 52.8 79.2



#34
Caprolactam
Concen: 19.684 ng/ul
RT: 11.672 min Scan# 1434
Delta R.T. 0.006 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:113 Resp: 42782
Ion Ratio Lower Upper
113 100
55 165.7 157.9 236.9
56 136.4 131.8 197.6









#35
4-Chloro-3-methylphenol
Concen: 20.761 ng/ul
RT: 12.019 min Scan# 1493
Delta R.T. -0.006 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:107 Resp: 181681
Ion Ratio Lower Upper
107 100
144 22.7 17.1 25.7
142 73.1 49.4 74.2



#36
2-Methylnaphthalene
Concen: 22.083 ng/ul
RT: 12.401 min Scan# 1558
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:142 Resp: 392287
Ion Ratio Lower Upper
142 100
141 89.3 71.1 106.7

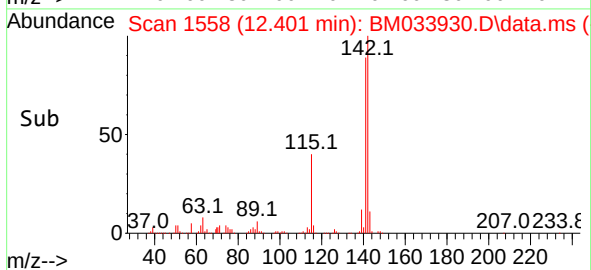



#37

1-Methylnaphthalene

Concen: 20.001 ng/ul

RT: 12.619 min Scan# 1595

Delta R.T. -0.000 min

Lab File: BM033930.D

Acq: 31 Jan 2022 17:23

Instrument :

BNA_M

ClientSampleId :

SICV031





Tgt Ion:142 Resp: 364217

Ion Ratio Lower Upper

142 100

141 91.8 75.5 113.3

116 4.2 4.0 6.0

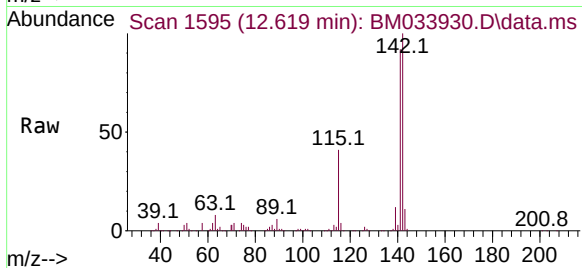

#39

1,2,4,5-Tetrachlorobenzene

Concen: 20.545 ng/ul

RT: 12.772 min Scan# 1621

Delta R.T. -0.000 min

Lab File: BM033930.D

Acq: 31 Jan 2022 17:23

Tgt Ion:216 Resp: 193549




Ion Ratio Lower Upper


216 100

214 78.9 61.3 91.9

179 23.0 18.0 27.0


108 19.1 16.6 25.0

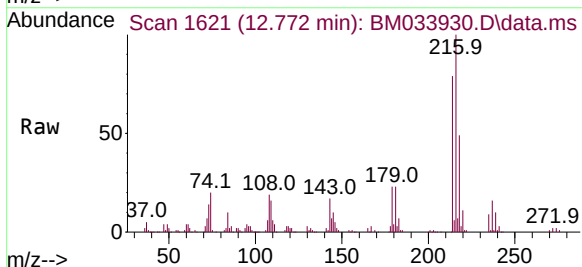






#40
Hexachlorocyclopentadiene
Concen: 20.247 ng/ul
RT: 12.754 min Scan# 1618
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Instrument :
BNA_M
ClientSampleId :
SICV031



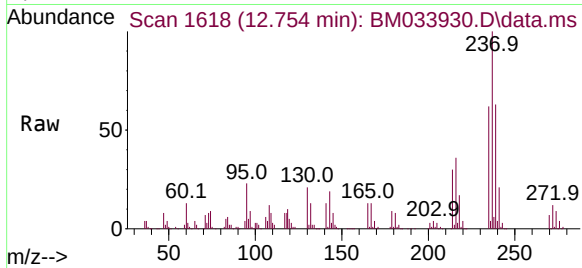



Tgt Ion:237 Resp: 140712
Ion Ratio Lower Upper
237 100
235 62.2 50.6 76.0
272 12.0 9.6 14.4



#41
2,4,6-Trichlorophenol
Concen: 21.048 ng/ul
RT: 13.007 min Scan# 1661
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:196 Resp: 123475
Ion Ratio Lower Upper
196 100
198 98.2 78.9 118.3
200 31.1 23.7 35.5




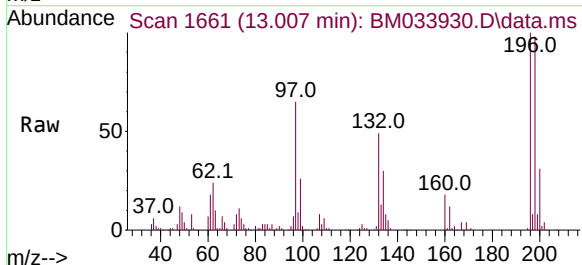




#42
2,4,5-Trichlorophenol
Concen: 21.153 ng/ul
RT: 13.077 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:196 Resp: 131640
Ion Ratio Lower Upper
196 100
198 97.4 82.2 123.2
200 31.1 27.9 41.9



#43
1,1'-Biphenyl
Concen: 20.382 ng/ul
RT: 13.407 min Scan# 1729
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:154 Resp: 483960
Ion Ratio Lower Upper
154 100
153 41.0 33.1 49.7
76 12.1 10.7 16.1


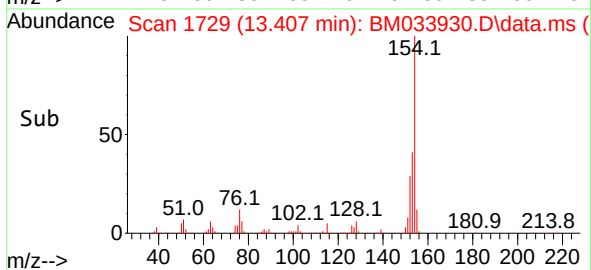






#44
2-Chloronaphthalene
Concen: 20.804 ng/ul
RT: 13.448 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:162 Resp: 372454
Ion Ratio Lower Upper
162 100
164 33.0 26.2 39.4
127 44.5 33.7 50.5

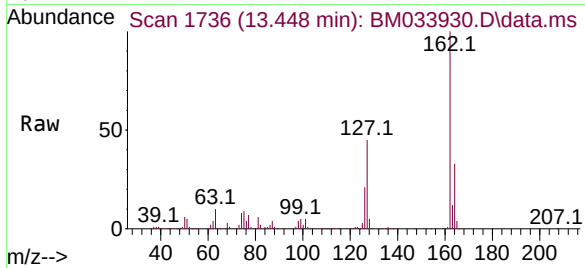

#45
2-Nitroaniline
Concen: 21.939 ng/ul
RT: 13.648 min Scan# 1770
Delta R.T. 0.006 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion: 65 Resp: 115584
Ion Ratio Lower Upper
65 100
92 65.0 47.8 71.6
138 98.5 61.0 91.6#

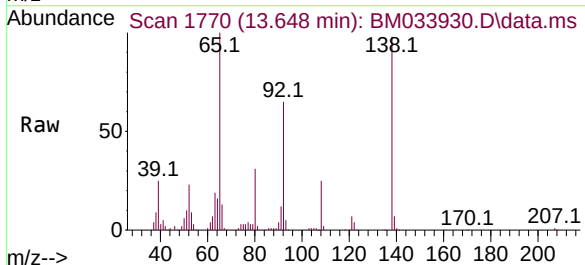



#47

Dimethylphthalate

Concen: 20.729 ng/ul

RT: 14.024 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM033930.D

Acq: 31 Jan 2022 17:23

Instrument :

BNA_M

ClientSampleId :

SICV031





Tgt Ion:163 Resp: 460838

Ion Ratio Lower Upper

163 100

194 3.8 3.3 4.9

164 9.9 8.2 12.2



#48

2,6-Dinitrotoluene

Concen: 22.913 ng/ul

RT: 14.142 min Scan# 1854

Delta R.T. -0.000 min

Lab File: BM033930.D

Acq: 31 Jan 2022 17:23




Tgt Ion:165 Resp: 97224


Ion Ratio Lower Upper

165 100

89 59.3 55.7 83.5

121 22.8 20.0 30.0









#50
Acenaphthylene
Concen: 20.369 ng/ul
RT: 14.289 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:152 Resp: 588890
Ion Ratio Lower Upper
152 100
151 20.3 15.8 23.8
153 13.4 10.1 15.1

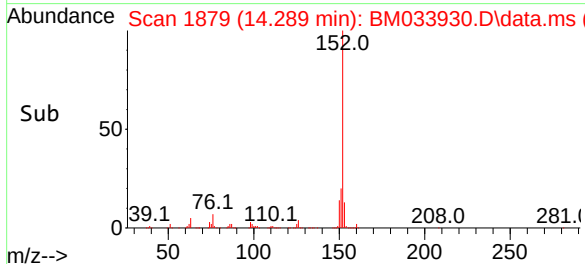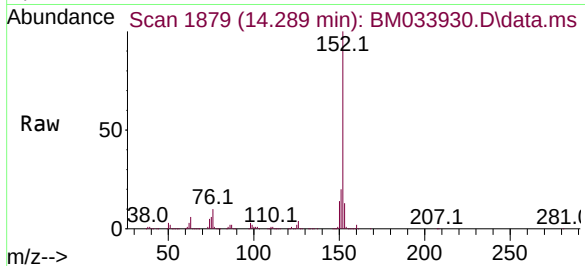

#51
3-Nitroaniline
Concen: 23.593 ng/ul
RT: 14.466 min Scan# 1909
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:138 Resp: 98830
Ion Ratio Lower Upper
138 100
108 11.6 10.8 16.2
92 120.2 110.6 166.0




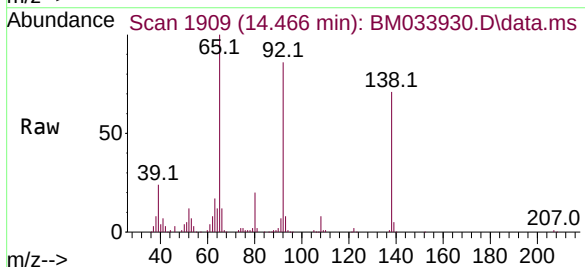




#52
Acenaphthene
Concen: 20.895 ng/ul
RT: 14.630 min Scan# 1937
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:153 Resp: 395493
Ion Ratio Lower Upper
153 100
152 46.9 39.4 59.2
154 88.9 72.7 109.1



#53
2,4-Dinitrophenol
Concen: 18.625 ng/ul
RT: 14.671 min Scan# 1944
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:184 Resp: 48226
Ion Ratio Lower Upper
184 100
63 72.8 73.8 110.8#
154 73.1 63.5 95.3









#55
4-Nitrophenol
Concen: 19.835 ng/ul
RT: 14.766 min Scan# 1960
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:109 Resp: 72411
Ion Ratio Lower Upper
109 100
139 112.8 77.6 116.4
65 123.5 112.2 168.4

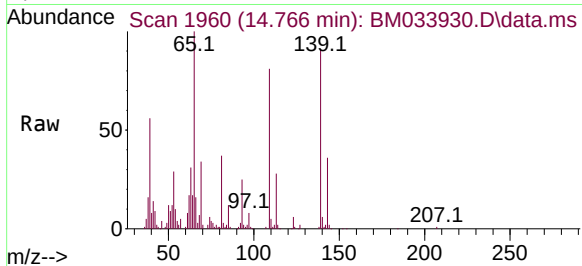

#56
Dibenzofuran
Concen: 20.760 ng/ul
RT: 14.966 min Scan# 1994
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:168 Resp: 552971
Ion Ratio Lower Upper
168 100
139 42.8 34.0 51.0




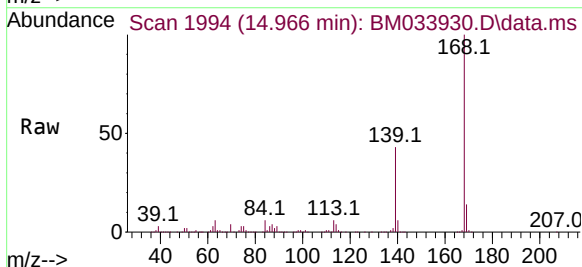




#57
2,4-Dinitrotoluene
Concen: 21.722 ng/ul
RT: 14.924 min Scan# 1987
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:165 Resp: 131510
Ion Ratio Lower Upper
165 100
63 47.0 51.8 77.8#
182 3.3 2.6 4.0

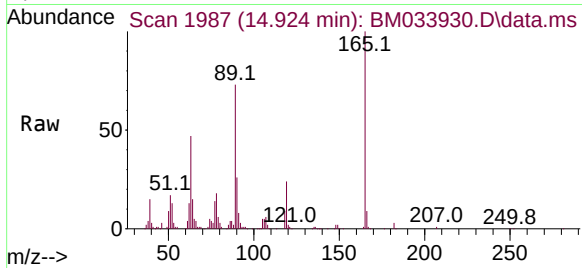

#58
2,3,4,6-Tetrachlorophenol
Concen: 22.398 ng/ul
RT: 15.107 min Scan# 2018
Delta R.T. -0.082 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:232 Resp: 114680
Ion Ratio Lower Upper
232 100
131 46.0 41.4 62.2
130 2.5 2.0 3.0
166 28.1 27.4 41.0



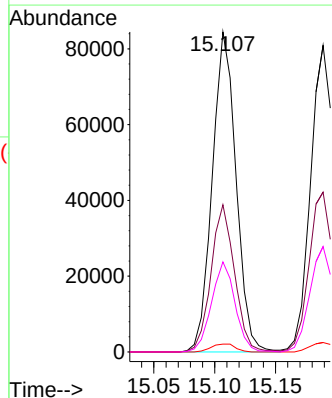
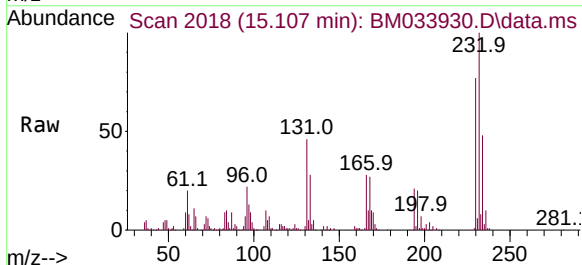




#59
Diethylphthalate
Concen: 20.447 ng/ul
RT: 15.383 min Scan# 2065
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:149 Resp: 462994
Ion Ratio Lower Upper
149 100
177 21.5 17.1 25.7
150 12.6 9.9 14.9



#61
Fluorene
Concen: 20.936 ng/ul
RT: 15.613 min Scan# 2104
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:166 Resp: 446288
Ion Ratio Lower Upper
166 100
165 97.9 77.9 116.9
167 12.7 10.3 15.5









#62
4-Chlorophenyl-phenylether
Concen: 20.497 ng/ul
RT: 15.607 min Scan# 2103
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:204 Resp: 223178
Ion Ratio Lower Upper
204 100
206 32.4 27.8 41.8
141 67.8 54.9 82.3



#63
4-Nitroaniline
Concen: 24.697 ng/ul
RT: 15.618 min Scan# 2105
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:138 Resp: 99795
Ion Ratio Lower Upper
138 100
92 52.6 48.0 72.0
108 90.4 89.5 134.3









#66
4,6-Dinitro-2-methylphenol
Concen: 19.214 ng/ul
RT: 15.683 min Scan# 2116
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:198 Resp: 69780
Ion Ratio Lower Upper
198 100
182 3.9 4.2 6.2#
77 29.3 26.3 39.5

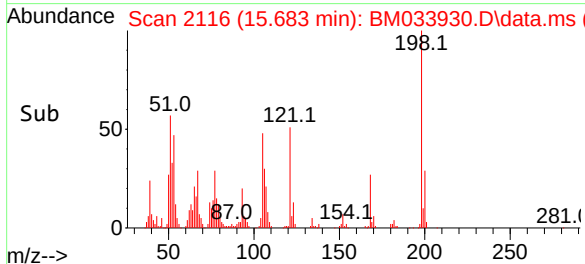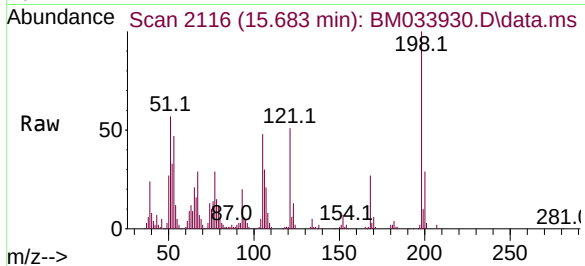

#67
N-Nitrosodiphenylamine
Concen: 20.965 ng/ul
RT: 15.813 min Scan# 2138
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:169 Resp: 376666
Ion Ratio Lower Upper
169 100
168 65.6 52.9 79.3
167 36.4 29.9 44.9


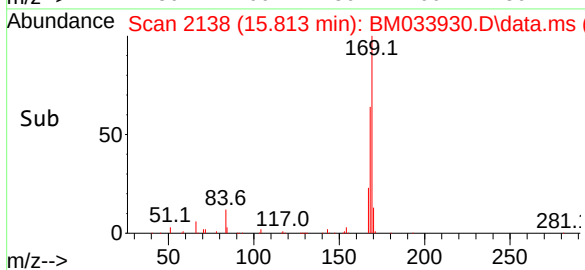

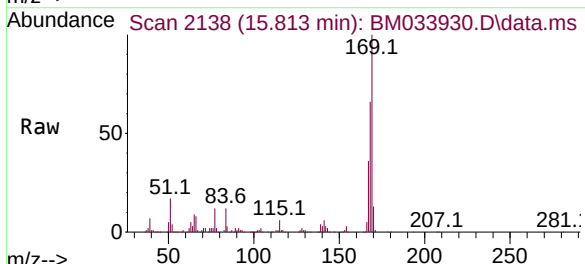




#68
4-Bromophenyl-phenylether
Concen: 20.619 ng/ul
RT: 16.495 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:248	Resp:	128986
Ion Ratio	Lower	Upper
248	100	
250	99.2	79.0 118.4
141	94.4	69.7 104.5



#69
Hexachlorobenzene
Concen: 20.589 ng/ul
RT: 16.618 min Scan# 2275
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:284	Resp:	147270
Ion Ratio	Lower	Upper
284	100	
142	36.6	34.3 51.5
249	32.5	26.1 39.1









#70
Atrazine
Concen: 18.355 ng/ul
RT: 16.765 min Scan# 2300
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:200 Resp: 124085
Ion Ratio Lower Upper
200 100
173 26.0 20.6 30.8
215 45.4 36.9 55.3

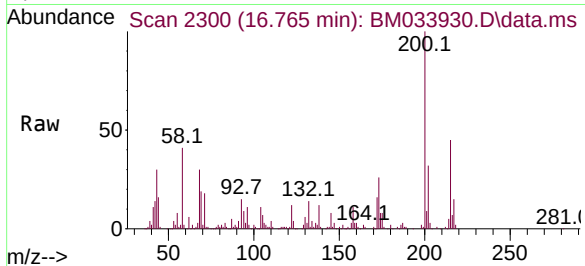

#71
Pentachlorophenol
Concen: 19.274 ng/ul
RT: 16.954 min Scan# 2332
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:266 Resp: 88423
Ion Ratio Lower Upper
266 100
264 64.0 49.1 73.7
268 64.7 47.8 71.8




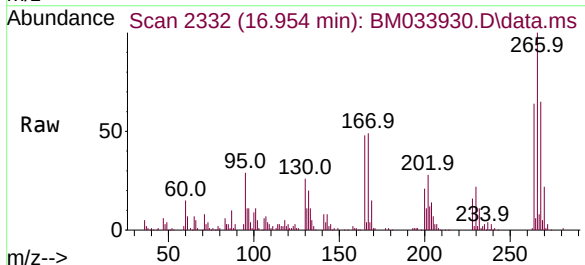




#72
Phenanthrene
Concen: 20.679 ng/u1
RT: 17.348 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:178 Resp: 673252
Ion Ratio Lower Upper
178 100
179 14.7 11.7 17.5
176 19.0 15.1 22.7



#74
Anthracene
Concen: 20.984 ng/u1
RT: 17.436 min Scan# 2414
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:178 Resp: 686573
Ion Ratio Lower Upper
178 100
179 15.2 12.3 18.5
176 18.0 14.5 21.7









#75
1,2,3,4-Tetrachlorobenzene
Concen: 18.515 ng/uL
RT: 13.371 min Scan# 1723
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:216 Resp: 187343
Ion Ratio Lower Upper
216 100
214 78.9 65.4 98.0
218 47.9 38.8 58.2



#76
Pentachlorobenzene
Concen: 19.329 ng/uL
RT: 14.889 min Scan# 1981
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:250 Resp: 174348
Ion Ratio Lower Upper
250 100
248 63.4 51.6 77.4
252 64.0 52.0 78.0


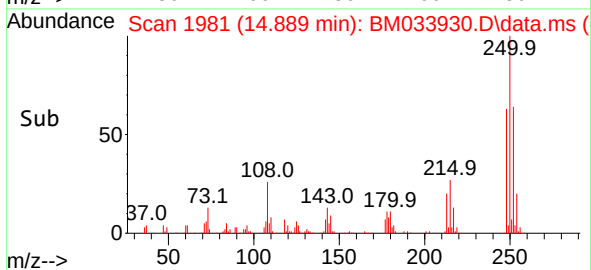






#77
 Carbazole
 Concen: 20.396 ng/ul
 RT: 17.701 min Scan# 2459
 Delta R.T. -0.000 min
 Lab File: BM033930.D
 Acq: 31 Jan 2022 17:23




Instrument :
 BNA_M
 ClientSampleId :
 SICV031


Tgt Ion:167 Resp: 590683
 Ion Ratio Lower Upper
 167 100
 166 21.3 16.9 25.3
 139 14.3 10.5 15.7

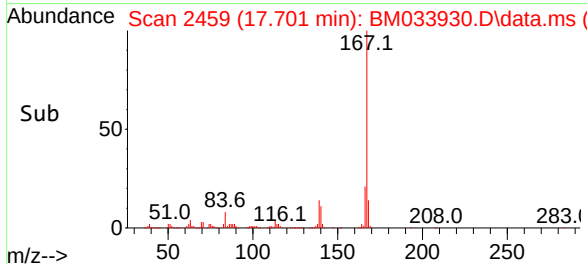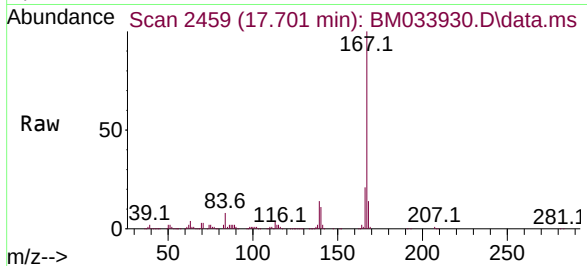

#78
 Di-n-butylphthalate
 Concen: 20.357 ng/ul
 RT: 18.271 min Scan# 2556
 Delta R.T. -0.000 min
 Lab File: BM033930.D
 Acq: 31 Jan 2022 17:23

Tgt Ion:149 Resp: 733108
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.0 10.6
 104 5.4 5.1 7.7


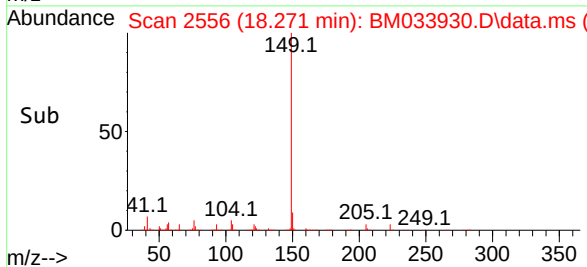

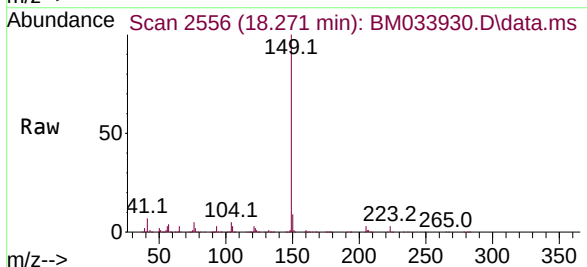




#80
 Fluoranthene
 Concen: 20.743 ng/u1
 RT: 19.353 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BM033930.D
 Acq: 31 Jan 2022 17:23




Instrument :
 BNA_M
 ClientSampleId :
 SICV031


Tgt Ion:202 Resp: 721840
 Ion Ratio Lower Upper
 202 100
 101 10.9 8.2 12.4
 100 8.8 6.9 10.3

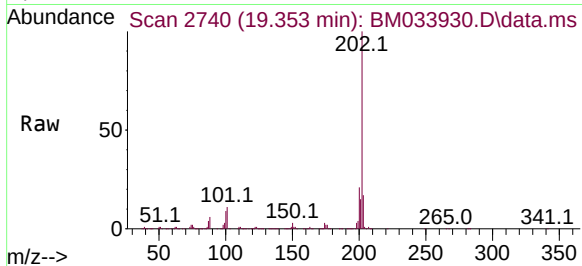

#82
 Pyrene
 Concen: 20.959 ng/u1
 RT: 19.718 min Scan# 2802
 Delta R.T. 0.006 min
 Lab File: BM033930.D
 Acq: 31 Jan 2022 17:23

Tgt Ion:202 Resp: 745450
 Ion Ratio Lower Upper
 202 100
 101 12.1 9.8 14.6
 100 10.2 8.6 13.0


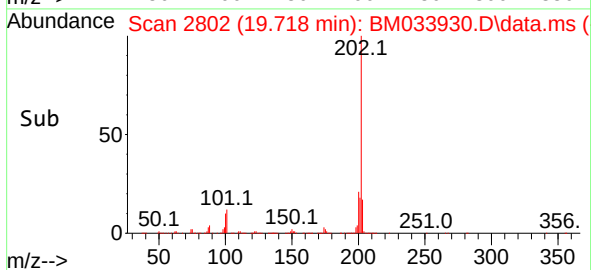

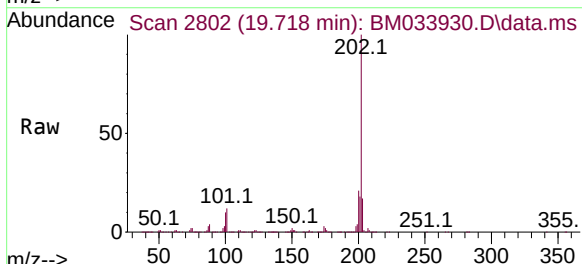




#83
Butylbenzylphthalate
Concen: 20.512 ng/ul
RT: 20.606 min Scan# 2953
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:149 Resp: 297260
Ion Ratio Lower Upper
149 100
91 75.0 69.3 103.9
206 19.5 16.1 24.1

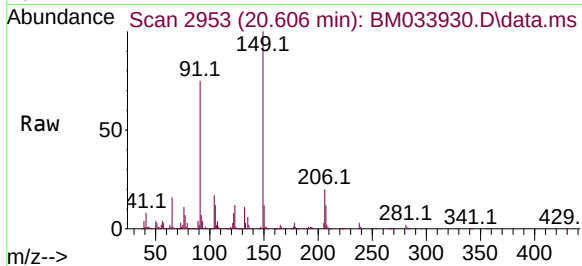

#84
3,3'-Dichlorobenzidine
Concen: 23.372 ng/ul
RT: 21.383 min Scan# 3085
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:252 Resp: 229031
Ion Ratio Lower Upper
252 100
254 63.6 49.4 74.2
126 11.2 8.2 12.4




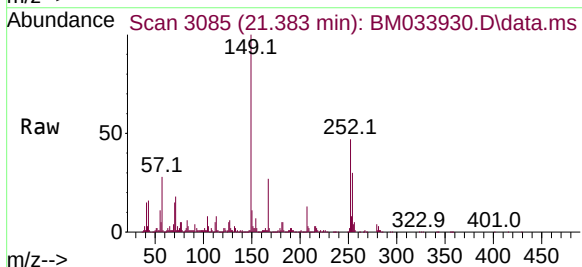




#85
Benzo(a)anthracene
Concen: 20.518 ng/ul
RT: 21.453 min Scan# 3097
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:228 Resp: 654557
Ion Ratio Lower Upper
228 100
229 19.6 15.0 22.4
226 27.2 21.4 32.0



#86
Bis(2-ethylhexyl)phthalate
Concen: 20.538 ng/ul
RT: 21.383 min Scan# 3085
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:149 Resp: 434044
Ion Ratio Lower Upper
149 100
167 26.8 21.8 32.8
279 4.0 3.2 4.8









#87
Chrysene
Concen: 20.530 ng/ul
RT: 21.506 min Scan# 3106
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:228 Resp: 640023
Ion Ratio Lower Upper
228 100
226 29.5 24.5 36.7
229 19.3 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 20.467 ng/ul
RT: 22.300 min Scan# 3241
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:149 Resp: 699046









#90
Benzo(b)fluoranthene
Concen: 20.023 ng/u1
RT: 23.130 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:252 Resp: 641533
Ion Ratio Lower Upper
252 100
253 21.9 17.7 26.5
125 9.8 7.8 11.6

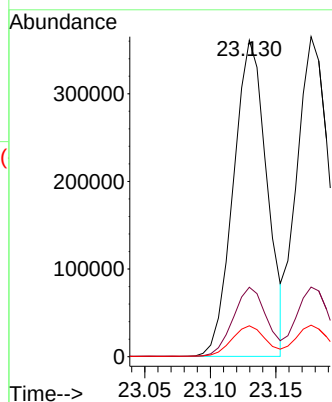

#91
Benzo(k)fluoranthene
Concen: 21.279 ng/u1
RT: 23.177 min Scan# 3390
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:252 Resp: 625923
Ion Ratio Lower Upper
252 100
253 21.8 17.6 26.4
125 9.9 7.4 11.2


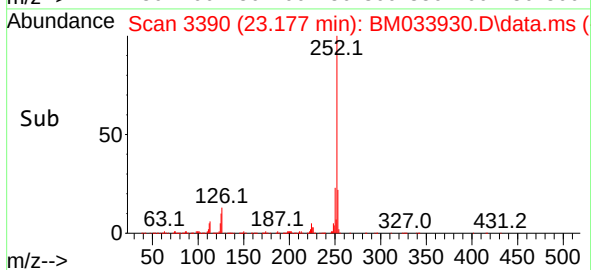






#93
Benzo(a)pyrene
Concen: 20.202 ng/ul
RT: 23.753 min Scan# 3488
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23




Instrument :
BNA_M
ClientSampleId :
SICV031


Tgt Ion:252 Resp: 612061
Ion Ratio Lower Upper
252 100
253 22.4 17.4 26.0
125 10.9 7.8 11.6



#94
Indeno(1,2,3-cd)pyrene
Concen: 20.600 ng/ul
RT: 26.359 min Scan# 3931
Delta R.T. -0.000 min
Lab File: BM033930.D
Acq: 31 Jan 2022 17:23

Tgt Ion:276 Resp: 721416
Ion Ratio Lower Upper
276 100
138 22.9 16.5 24.7
277 25.4 20.6 31.0


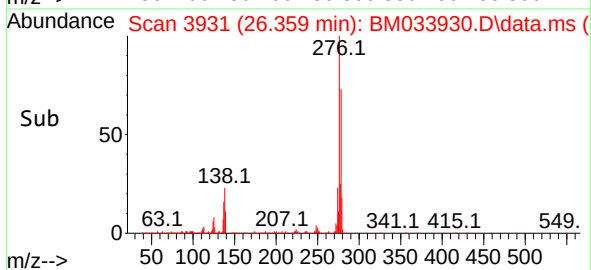






#95
 Dibenzo(a,h)anthracene
 Concen: 20.408 ng/ul
 RT: 26.377 min Scan# 3933
 Delta R.T. 0.006 min
 Lab File: BM033930.D
 Acq: 31 Jan 2022 17:23

Instrument :
 BNA_M
 ClientSampleId :
 SICV031

Tgt Ion:278 Resp: 618582
 Ion Ratio Lower Upper
 278 100
 139 14.8 11.0 16.4
 279 23.1 18.1 27.1

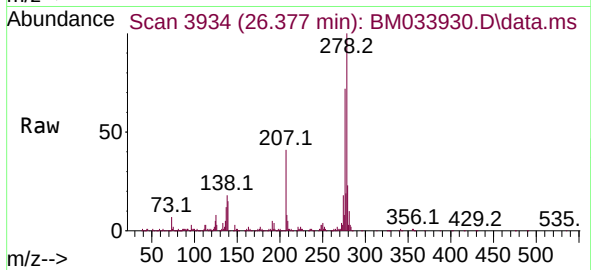

#96
 Benzo(g,h,i)perylene
 Concen: 20.625 ng/ul
 RT: 27.124 min Scan# 4061
 Delta R.T. -0.000 min
 Lab File: BM033930.D
 Acq: 31 Jan 2022 17:23

Tgt Ion:276 Resp: 607320
 Ion Ratio Lower Upper
 276 100
 138 20.2 15.6 23.4
 277 23.6 18.7 28.1

