


Data Path : Z:\HPCHEM1\BNA M\DATA\BM020116\
Data File : BM004157.D
Acq On : 01 Feb 2016 09:02
Operator : SJ/IZ
Sample : DFTPP46
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP46

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM012916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 02 01:18:17 2016

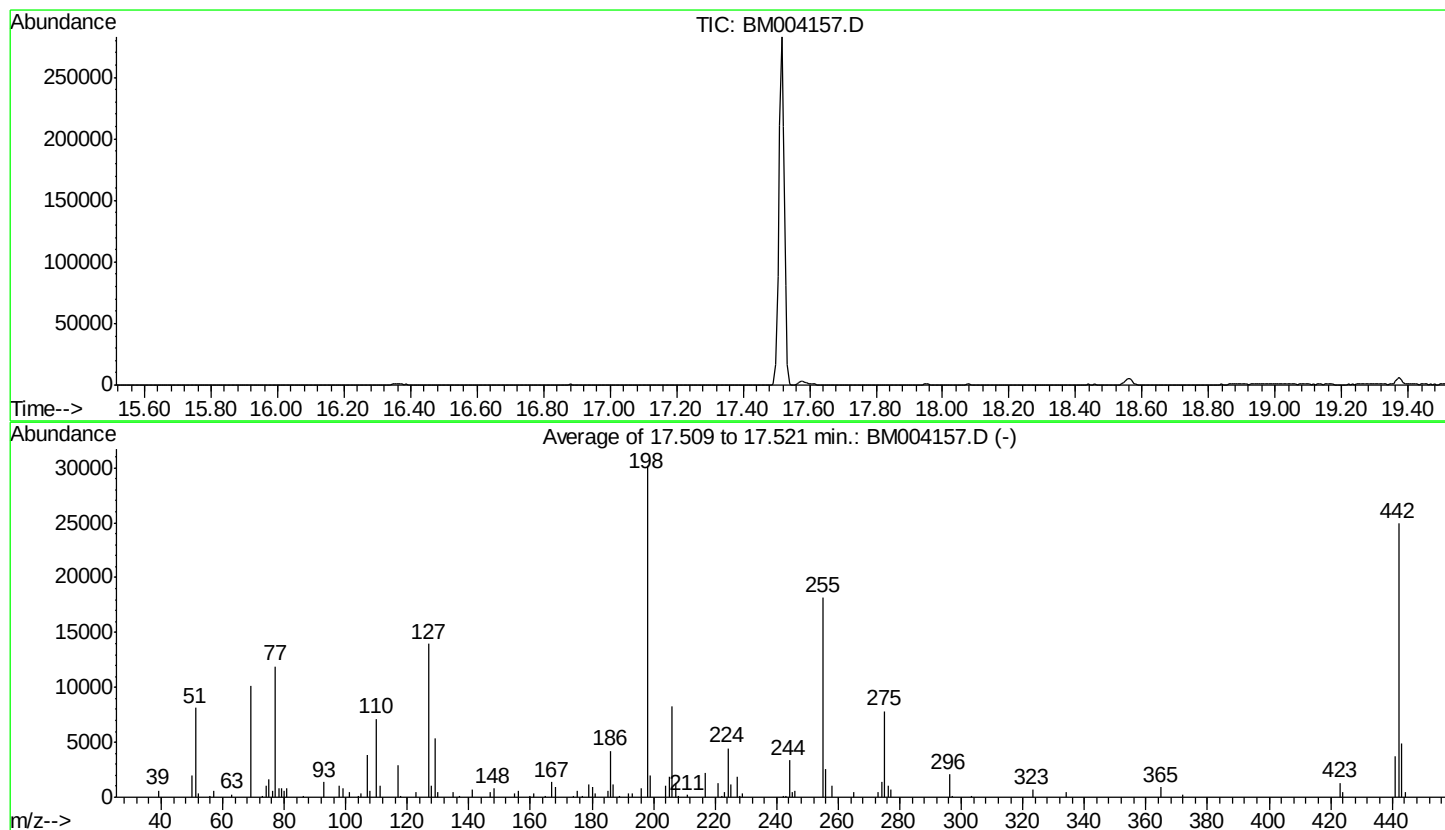

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	8130	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.5	10112	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	13960	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	30200	PASS
199	198	5	9	6.7	2019	PASS
275	198	10	60	25.9	7822	PASS
365	198	1	100	3.1	927	PASS
441	443	0.01	100	76.7	3763	PASS
442	198	50	100	82.6	24941	PASS
443	442	15	24	19.7	4906	PASS

m/z	Abundance
39.00	655.0
50.10	2155.0
51.10	8527.0
52.00	449.0
57.00	605.0
63.00	378.0
69.00	10673.0
74.00	1081.0
75.10	1706.0
76.10	544.0
77.10	12409.0
78.10	917.0
79.00	756.0
80.00	676.0
81.00	808.0
93.00	1388.0
98.00	1026.0
99.00	886.0
101.00	551.0
105.00	318.0
107.00	3862.0
108.00	603.0
110.00	7165.0
111.00	1107.0
117.00	2865.0
123.00	443.0
127.10	13441.0
128.00	1166.0
129.00	5180.0
130.00	442.0
135.00	489.0
141.00	688.0
147.00	462.0
148.00	747.0
155.00	398.0
156.00	610.0
161.00	342.0
167.00	1254.0
168.00	943.0
175.00	577.0
179.00	1044.0
180.00	788.0
181.00	412.0
185.00	499.0
186.10	3840.0
187.00	1108.0
191.90	313.0
193.10	403.0
196.10	760.0
198.00	27464.0
199.00	1854.0
204.00	969.0
205.10	1735.0
206.10	7513.0
207.10	1132.0
217.00	1938.0
221.10	1058.0
223.00	383.0
224.10	4022.0
225.10	1050.0
227.00	1697.0
229.00	361.0
244.10	2835.0
245.00	379.0
246.00	616.0
255.10	15896.0
256.00	2257.0
258.00	838.0
265.00	348.0
273.00	440.0
274.10	1226.0
275.10	6773.0
276.10	886.0
277.00	604.0
296.10	1710.0
323.00	520.0
334.00	340.0
365.00	742.0
423.10	956.0
424.10	354.0
441.10	2658.0
442.20	17568.0
443.10	3473.0
444.10	344.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z	Abundance
39.10	640.0
50.10	2431.0
51.10	9625.0
52.10	478.0
56.00	322.0
57.00	686.0
63.00	450.0
69.00	11985.0
73.10	360.0
74.00	1194.0
75.00	1878.0
76.10	615.0
77.10	14149.0
78.10	964.0
79.00	880.0
80.00	760.0
81.00	1033.0
86.00	301.0
93.00	1665.0
98.00	1208.0
99.00	1071.0
101.00	509.0
104.00	328.0
105.00	404.0
107.10	4501.0
108.00	683.0
110.00	8421.0
111.00	1344.0
117.00	3517.0
118.00	306.0
123.00	513.0
127.10	16720.0
128.00	1236.0
129.00	6508.0
130.00	516.0
135.00	550.0
137.00	344.0
141.00	812.0
147.00	519.0
148.00	1052.0
155.00	483.0
156.00	752.0
159.90	336.0
160.90	405.0
164.90	388.0
167.00	1623.0
168.00	1044.0
174.00	336.0
175.10	676.0
177.00	393.0
179.00	1319.0
180.10	1074.0
181.10	404.0
185.00	648.0
186.10	5094.0
187.00	1460.0
188.90	311.0
192.00	434.0
193.10	447.0
196.00	965.0
198.00	36264.0
199.00	2421.0
204.10	1286.0
205.10	2259.0
206.10	9980.0
207.10	1482.0
208.00	368.0
211.10	316.0
217.00	2613.0
221.10	1395.0
222.00	354.0
223.00	614.0
224.10	5247.0
225.10	1449.0
227.00	2173.0
228.00	322.0
229.00	429.0
242.00	303.0
243.00	320.0
244.10	3933.0
245.10	590.0
246.10	717.0
255.10	21616.0
256.10	3113.0
258.00	1204.0
265.00	488.0
273.10	603.0
274.10	1618.0
275.10	9398.0
276.10	1268.0
277.00	766.0
296.10	2525.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

297.10	362.0
303.10	323.0
323.10	764.0
334.10	465.0
365.10	1110.0
372.10	363.0
423.10	1573.0
424.10	544.0
441.20	4298.0
442.10	29064.0
443.10	5903.0
444.10	542.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z	Abundance
39.00	469.0
50.10	1503.0
51.10	6238.0
57.00	467.0
69.00	7680.0
74.00	788.0
75.00	1317.0
76.00	503.0
77.10	9236.0
78.10	593.0
79.00	650.0
80.00	495.0
81.00	658.0
93.00	1024.0
98.00	808.0
99.00	668.0
101.00	395.0
105.00	332.0
107.00	3147.0
108.00	493.0
110.00	5796.0
111.00	854.0
117.00	2403.0
123.00	331.0
127.00	11721.0
128.00	820.0
129.00	4578.0
130.00	368.0
135.00	349.0
141.00	590.0
147.00	370.0
148.00	643.0
155.00	331.0
156.10	556.0
161.00	306.0
167.10	1285.0
168.00	730.0
175.00	495.0
179.00	1000.0
180.00	793.0
181.00	322.0
185.00	484.0
186.10	3717.0
187.00	1078.0
192.00	337.0
193.00	374.0
196.00	743.0
198.00	26872.0
199.00	1784.0
204.00	957.0
205.00	1659.0
206.10	7371.0
207.10	1099.0
211.10	362.0
217.00	1975.0
221.10	1250.0
223.00	411.0
224.10	4026.0
225.10	964.0
227.00	1690.0
229.00	370.0
244.10	3226.0
245.10	396.0
246.00	592.0
255.10	17024.0
256.10	2420.0
258.00	999.0
265.10	409.0
273.00	502.0
274.00	1339.0
275.10	7297.0
276.10	943.0
277.00	623.0
296.10	2044.0
323.10	706.0
334.10	434.0
365.00	931.0
372.10	390.0
423.10	1432.0
424.10	408.0
441.20	4333.0
442.20	28192.0
443.10	5343.0
444.10	460.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z

Abundance

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z Abundance

Instrument :
BNA_M
ClientSampleId :
DFTPP46